

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121724\
 Data File : VX044356.D
 Acq On : 17 Dec 2024 17:04
 Operator : JC/MD
 Sample : VX1217WBL02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK741

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
 Title : VOC Analysis

Signal : TIC: VX044356.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	23	26	27	rBV	2431	2564	0.23%	0.032%
2	1.368	43	46	55	rVB	128153	140865	12.40%	1.784%
3	1.642	88	91	100	rVB	111548	159028	14.00%	2.014%
4	2.294	192	198	210	rVB	211368	328783	28.95%	4.163%
5	2.495	228	231	233	rBV4	999	1439	0.13%	0.018%
6	2.788	273	279	281	rBV4	1342	1854	0.16%	0.023%
7	2.849	287	289	291	rVB2	789	503	0.04%	0.006%
8	2.940	297	304	311	rVV5	3137	7773	0.68%	0.098%
9	3.014	315	316	320	rVB	1136	890	0.08%	0.011%
10	3.434	380	385	391	rBV5	1833	3612	0.32%	0.046%
11	3.520	396	399	404	rVB3	432	653	0.06%	0.008%
12	3.696	426	428	431	rVB2	885	746	0.07%	0.009%
13	3.757	436	438	440	rVV3	962	943	0.08%	0.012%
14	3.782	440	442	444	rVV3	860	800	0.07%	0.010%
15	3.800	444	445	449	rVV3	856	929	0.08%	0.012%
16	3.837	449	451	454	rVV3	504	493	0.04%	0.006%
17	3.891	456	460	463	rVB3	503	665	0.06%	0.008%
18	3.983	473	475	479	rVB4	418	556	0.05%	0.007%
19	4.032	479	483	486	rBV4	699	1329	0.12%	0.017%
20	4.062	486	488	490	rVV	656	576	0.05%	0.007%
21	4.288	524	525	528	rBV2	632	604	0.05%	0.008%
22	4.373	535	539	542	rBV2	329	709	0.06%	0.009%
23	4.458	545	553	569	rBV	85495	260809	22.96%	3.302%
24	4.885	622	623	626	rBV2	453	460	0.04%	0.006%
25	5.050	637	650	665	rBV2	151914	481749	42.42%	6.100%
26	5.342	695	698	700	rBV2	601	746	0.07%	0.009%
27	5.385	704	705	710	rVB3	704	773	0.07%	0.010%
28	5.867	783	784	787	rBV3	671	557	0.05%	0.007%
29	5.958	787	799	817	rBV2	379489	1135707	100.00%	14.380%
30	6.220	841	842	844	rBV2	833	594	0.05%	0.008%
31	6.354	862	864	865	rVV	749	494	0.04%	0.006%
32	6.562	896	898	901	rVB2	632	554	0.05%	0.007%
33	6.635	908	910	913	rBV2	558	571	0.05%	0.007%
34	6.757	921	930	945	rBV	227709	559507	49.27%	7.084%
35	6.958	960	963	964	rVB2	891	813	0.07%	0.010%
36	7.086	983	984	985	rBV	959	522	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121724\
 Data File : VX044356.D
 Acq On : 17 Dec 2024 17:04
 Operator : JC/MD
 Sample : VX1217WBL02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK741

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
 Title : VOC Analysis

37	7.116	985	989	1000	rVV6	3338	7998	0.70%	0.101%
38	7.305	1011	1020	1033	rBV	239506	530790	46.74%	6.721%
39	7.793	1098	1100	1102	rVV3	748	642	0.06%	0.008%
40	7.811	1102	1103	1109	rVV2	695	651	0.06%	0.008%
41	7.891	1114	1116	1118	rVB2	672	541	0.05%	0.007%
42	8.031	1136	1139	1140	rVB2	646	567	0.05%	0.007%
43	8.208	1166	1168	1171	rBV	841	782	0.07%	0.010%
44	8.324	1181	1187	1198	rBV	136550	231408	20.38%	2.930%
45	8.580	1226	1229	1232	rBV3	563	709	0.06%	0.009%
46	8.647	1234	1240	1257	rVB	507042	811846	71.48%	10.279%
47	8.952	1284	1290	1299	rBV	98376	149896	13.20%	1.898%
48	9.262	1340	1341	1345	rVB2	629	641	0.06%	0.008%
49	9.384	1356	1361	1383	rBV	356120	558893	49.21%	7.077%
50	9.695	1409	1412	1413	rBV2	495	470	0.04%	0.006%
51	10.049	1465	1470	1483	rBV	444282	650169	57.25%	8.232%
52	10.207	1495	1496	1499	rVB3	1091	643	0.06%	0.008%
53	10.463	1537	1538	1541	rVB2	776	582	0.05%	0.007%
54	10.512	1544	1546	1548	rBV2	447	563	0.05%	0.007%
55	10.591	1554	1559	1560	rBV3	681	1070	0.09%	0.014%
56	10.646	1565	1568	1572	rVV3	893	1586	0.14%	0.020%
57	10.908	1609	1611	1613	rBV2	517	516	0.05%	0.007%
58	10.969	1618	1621	1623	rBV4	947	1297	0.11%	0.016%
59	11.097	1641	1642	1644	rBV2	719	602	0.05%	0.008%
60	11.189	1652	1657	1669	rVB	445320	569258	50.12%	7.208%
61	11.451	1697	1700	1702	rBV3	645	910	0.08%	0.012%
62	11.634	1728	1730	1733	rVB3	526	462	0.04%	0.006%
63	11.707	1739	1742	1745	rVB4	737	1039	0.09%	0.013%
64	11.750	1745	1749	1751	rBV3	808	990	0.09%	0.013%
65	11.817	1759	1760	1765	rBV4	386	522	0.05%	0.007%
66	11.939	1778	1780	1782	rBV2	937	888	0.08%	0.011%
67	11.975	1784	1786	1788	rVV2	1373	909	0.08%	0.012%
68	12.018	1788	1793	1806	rVV	417560	540871	47.62%	6.848%
69	12.317	1837	1842	1853	rBV	549332	701138	61.74%	8.878%
70	12.481	1867	1869	1871	rBV2	503	552	0.05%	0.007%
71	12.567	1880	1883	1886	rBV3	570	754	0.07%	0.010%
72	12.609	1886	1890	1891	rBV2	670	548	0.05%	0.007%
73	12.658	1897	1898	1901	rBV3	551	704	0.06%	0.009%
74	12.762	1912	1915	1918	rBV3	1443	1575	0.14%	0.020%
75	12.853	1929	1930	1933	rBV3	594	514	0.05%	0.007%
76	13.042	1959	1961	1964	rVB3	520	596	0.05%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121724\
 Data File : VX044356.D
 Acq On : 17 Dec 2024 17:04
 Operator : JC/MD
 Sample : VX1217WBL02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK741

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
 Title : VOC Analysis

77	13.073	1964	1966	1968	rBV	746	633	0.06%	0.008%
78	13.115	1971	1973	1976	rVB3	621	639	0.06%	0.008%
79	13.378	2012	2016	2017	rBV2	566	635	0.06%	0.008%
80	13.530	2038	2041	2045	rBV4	437	674	0.06%	0.009%
81	13.597	2049	2052	2054	rBV3	949	977	0.09%	0.012%
82	13.786	2079	2083	2087	rBV4	995	1500	0.13%	0.019%
83	13.932	2104	2107	2110	rBV3	664	892	0.08%	0.011%
84	13.963	2110	2112	2116	rVB4	1320	1442	0.13%	0.018%
85	14.134	2136	2140	2144	rVB4	2562	4047	0.36%	0.051%
86	14.524	2201	2204	2206	rVB2	818	623	0.05%	0.008%
87	14.560	2209	2210	2213	rBV2	383	530	0.05%	0.007%
88	14.700	2232	2233	2235	rBV2	533	464	0.04%	0.006%
89	14.920	2267	2269	2274	rVB2	637	569	0.05%	0.007%
90	14.963	2274	2276	2279	rVB4	755	738	0.06%	0.009%
91	15.206	2313	2316	2317	rBV2	628	545	0.05%	0.007%
92	15.286	2327	2329	2330	rBV2	711	586	0.05%	0.007%
93	15.395	2344	2347	2351	rVB4	1650	2272	0.20%	0.029%
94	15.682	2393	2394	2396	rBV2	595	508	0.04%	0.006%
95	15.847	2419	2421	2423	rBV	487	481	0.04%	0.006%
96	16.030	2449	2451	2454	rVB3	995	942	0.08%	0.012%
97	16.218	2480	2482	2483	rVB2	929	539	0.05%	0.007%
98	16.231	2483	2484	2488	rBV3	636	863	0.08%	0.011%
99	16.529	2531	2533	2536	rVB3	608	618	0.05%	0.008%
100	16.590	2541	2543	2546	rBV3	796	821	0.07%	0.010%

Sum of corrected areas: 7897800




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121724\
Data File : VX044356.D
Acq On : 17 Dec 2024 17:04
Operator : JC/MD
Sample : VX1217WBL02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK741

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

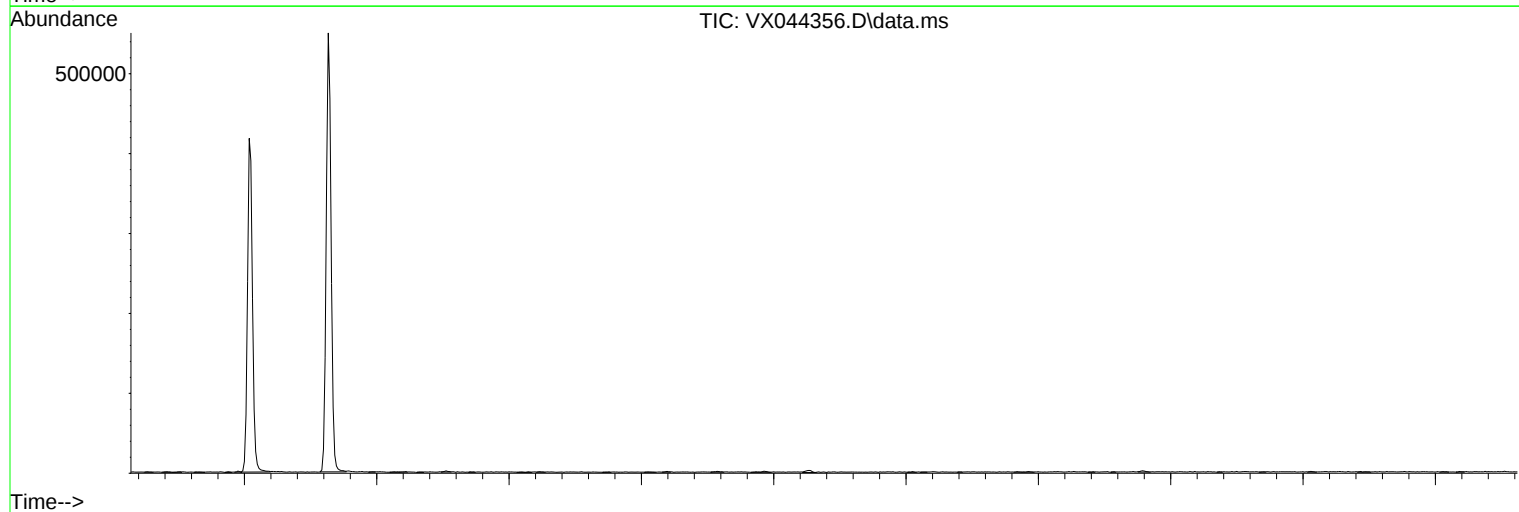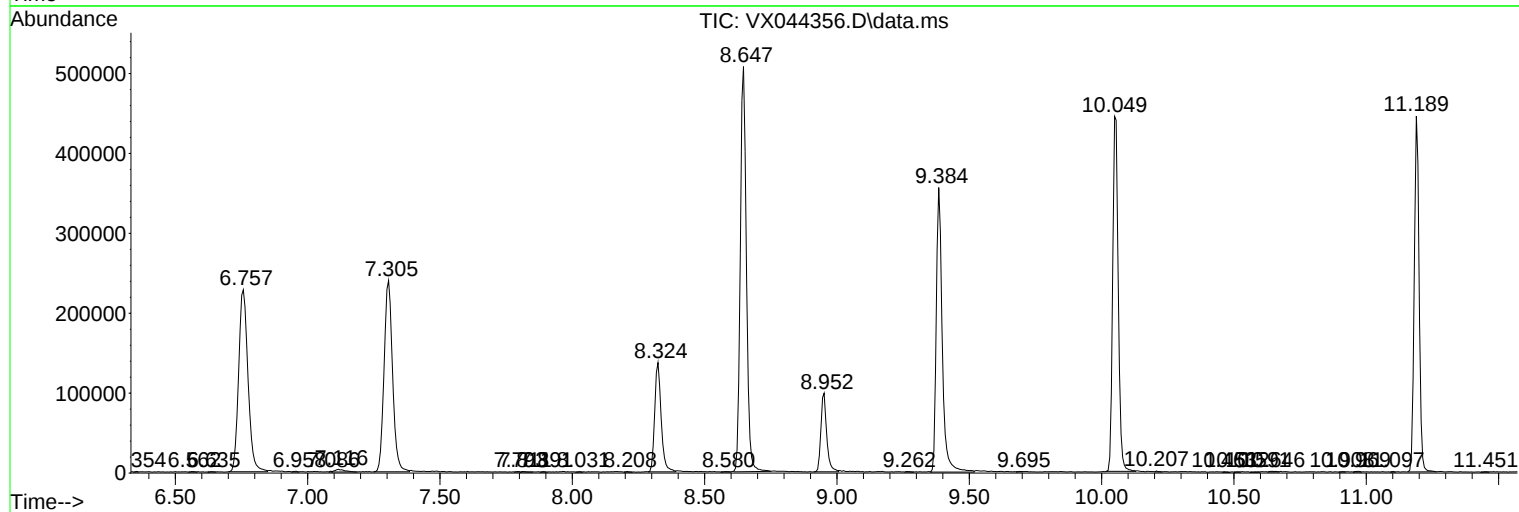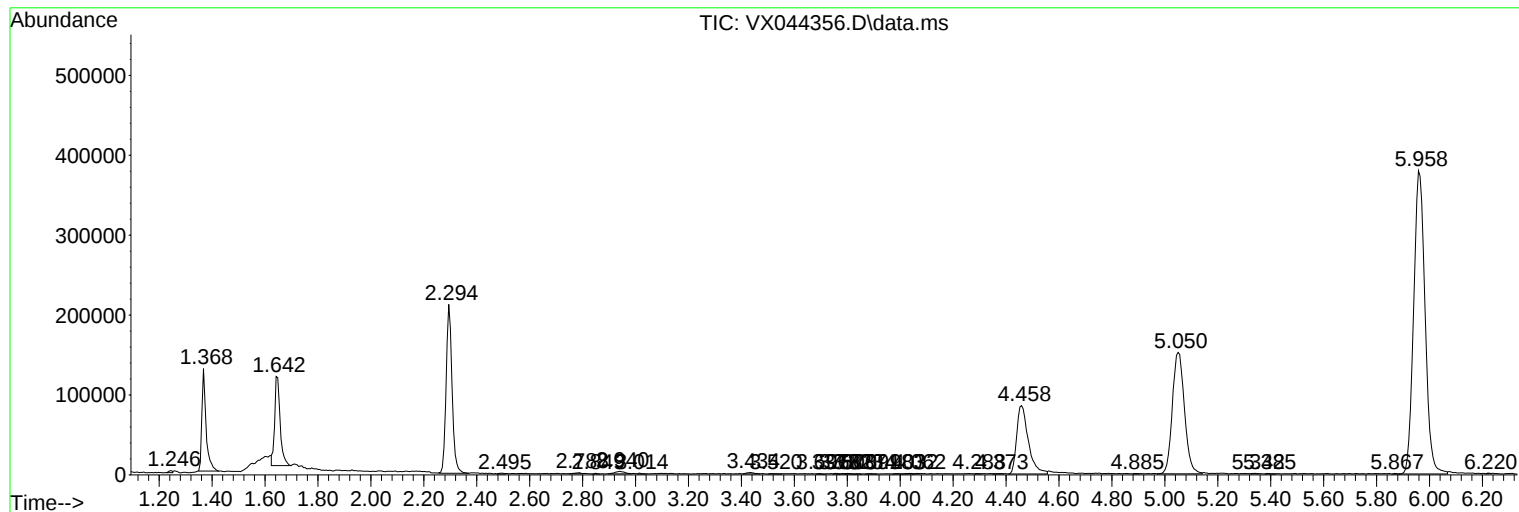

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121724\
Data File : VX044356.D
Acq On : 17 Dec 2024 17:04
Operator : JC/MD
Sample : VX1217WBL02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK741

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121724\
Data File : VX044356.D
Acq On : 17 Dec 2024 17:04
Operator : JC/MD
Sample : VX1217WBL02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK741

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120524WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc
