
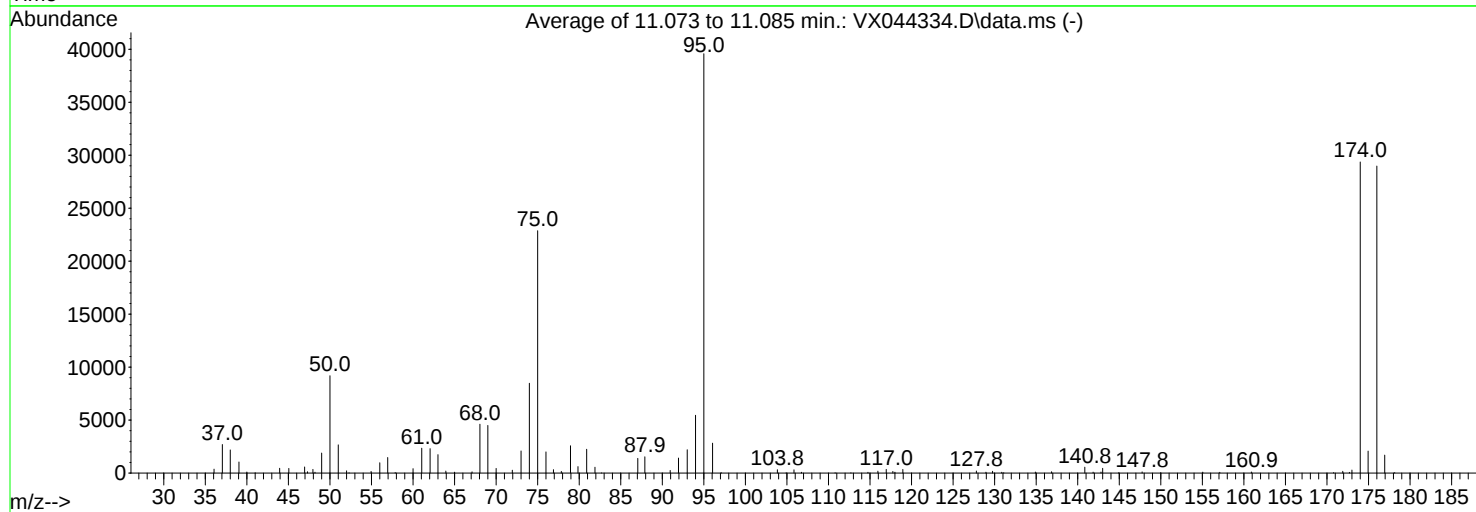


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121724\
Data File : VX044334.D
Acq On : 17 Dec 2024 08:23
Operator : JC/MD
Sample : BFB706
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB706

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120524WMA.M
Title : VOC Analysis
Last Update : Wed Dec 18 04:40:20 2024

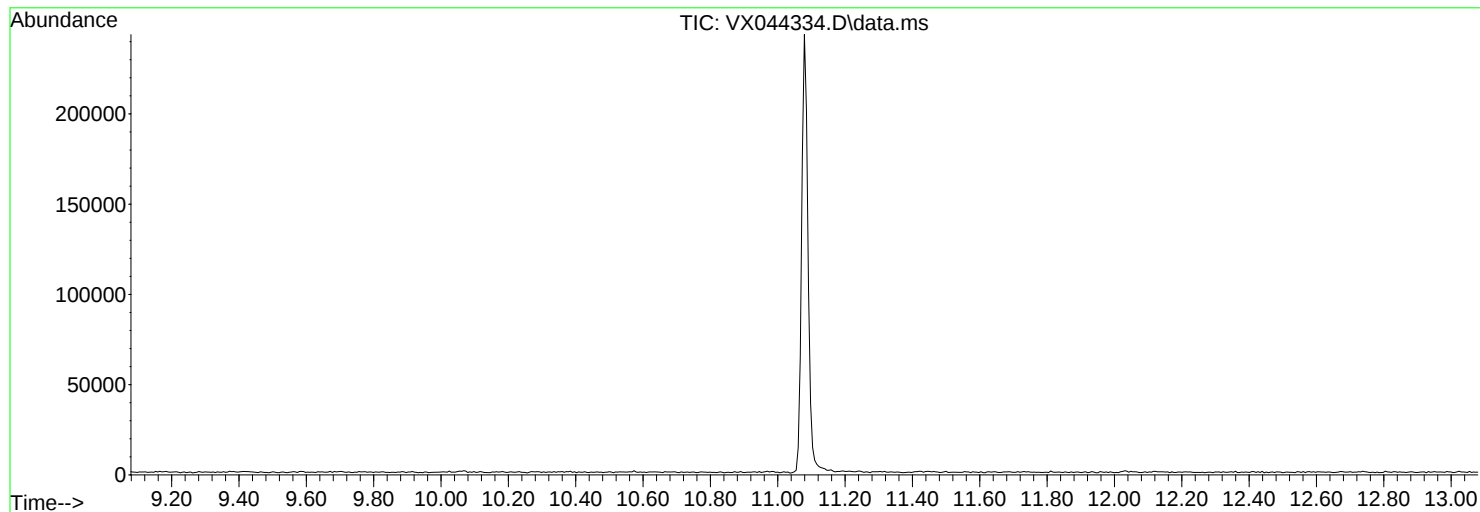

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.2	9188	PASS
75	95	30	80	57.8	22875	PASS
95	95	100	100	100.0	39579	PASS
96	95	5	9	7.1	2822	PASS
173	174	0.00	2	1.0	287	PASS
174	95	50	120	74.2	29365	PASS
175	174	5	9	7.1	2077	PASS
176	174	95	101	98.7	28976	PASS
177	176	5	9	5.9	1697	PASS

m/z	Abundance
38.00	166.0
39.10	312.0
40.00	525.0
43.90	216.0

Instrument :
MSVOA_X
ClientSampleId :
BFB706

m/z	Abundance
36.10	418.0
37.10	3113.0
38.00	2336.0
39.00	1454.0
40.00	382.0
44.00	845.0
45.10	467.0
47.00	499.0
47.90	441.0
49.00	1974.0
50.00	8826.0
51.00	2553.0
52.10	225.0
54.90	113.0
56.00	956.0
57.00	1447.0
60.00	296.0
61.00	2163.0
62.10	1821.0
63.00	1669.0
63.90	216.0
65.00	99.0
67.10	169.0
68.10	4273.0
69.00	4146.0
69.90	341.0
72.00	275.0
73.00	1935.0
74.00	7641.0
75.00	20632.0
76.00	1619.0
76.90	191.0
77.90	145.0
78.90	2154.0
79.90	474.0
80.90	1914.0
81.90	502.0
87.10	1128.0
87.90	1436.0
91.00	214.0
91.90	1168.0
93.10	2100.0
94.00	4810.0
95.00	34536.0
96.10	2437.0
103.80	225.0
105.90	177.0
106.80	67.0
114.80	58.0
115.90	118.0
117.00	304.0
117.70	186.0
119.00	292.0
127.80	124.0
129.70	175.0
130.80	170.0
134.90	109.0
137.00	104.0
140.90	440.0
141.80	79.0
142.80	300.0
147.80	112.0
155.00	78.0
157.10	100.0
160.90	82.0
171.90	74.0
172.70	205.0
174.00	21016.0
175.00	1598.0
176.00	21464.0
176.90	1475.0

Instrument :
MSVOA_X
ClientSampleId :
BFB706

m/z	Abundance
36.00	386.0
37.00	2848.0
38.00	3078.0
39.00	1441.0
40.00	683.0
41.00	58.0
44.00	685.0
45.00	451.0
46.90	470.0
47.30	387.0
48.00	399.0
49.00	2192.0
50.00	10884.0
51.00	3027.0
52.00	289.0
55.00	149.0
56.00	1280.0
57.00	1545.0
57.90	70.0
60.00	513.0
61.00	2738.0
62.00	2782.0
63.00	2313.0
63.90	192.0
65.00	57.0
67.10	92.0
68.00	5190.0
69.00	5229.0
70.00	522.0
72.00	299.0
73.00	2445.0
74.00	10502.0
75.00	27088.0
76.00	2401.0
76.90	300.0
77.90	207.0
78.90	3175.0
79.90	897.0
80.90	3047.0
81.90	681.0
87.00	1701.0
88.00	1672.0
91.00	301.0
92.00	1642.0
92.90	2507.0
94.00	6439.0
95.00	47192.0
96.00	3317.0
97.10	96.0
103.90	354.0
105.90	467.0
106.70	106.0
114.70	113.0
115.90	176.0
117.00	563.0
117.80	294.0
118.90	415.0
127.90	299.0
128.90	98.0
129.80	183.0
131.10	101.0
134.90	184.0
136.80	120.0
140.90	731.0
141.80	99.0
143.00	757.0
144.90	78.0
147.80	119.0
150.00	91.0
155.00	103.0
157.10	117.0
160.90	96.0
170.80	87.0
172.00	201.0
173.00	414.0
174.00	34096.0
174.90	2464.0
176.00	33200.0
176.90	1898.0
178.20	54.0

Instrument :
MSVOA_X
ClientSampleId :
BFB706

m/z	Abundance
36.10	312.0
37.10	2134.0
38.00	1635.0
39.10	1181.0
40.00	818.0
44.00	473.0
45.00	398.0
47.00	763.0
47.90	213.0
48.20	243.0
49.00	1498.0
50.00	7854.0
51.00	2416.0
51.90	128.0
52.30	87.0
55.00	217.0
56.10	686.0
56.90	1407.0
57.80	82.0
60.00	446.0
61.10	2140.0
62.00	2318.0
63.00	1231.0
64.00	161.0
65.00	96.0
67.00	86.0
68.00	4374.0
69.00	4112.0
70.10	451.0
71.80	250.0
73.00	1886.0
74.00	7287.0
75.00	20904.0
76.00	1978.0
76.90	473.0
77.80	122.0
79.00	2414.0
79.80	460.0
80.90	1778.0
81.90	475.0
82.70	56.0
87.00	1335.0
87.80	1498.0
90.90	238.0
92.00	1447.0
93.00	2000.0
94.00	5120.0
95.00	37008.0
96.00	2712.0
103.80	373.0
104.90	60.0
105.80	276.0
106.80	63.0
110.80	89.0
112.70	80.0
114.70	62.0
116.00	256.0
116.80	181.0
118.00	257.0
118.90	324.0
127.70	160.0
129.00	167.0
129.80	157.0
130.90	59.0
136.80	160.0
140.80	497.0
141.90	91.0
143.00	597.0
147.70	115.0
155.10	95.0
160.90	135.0
170.80	52.0
171.80	222.0
173.00	446.0
174.00	32984.0
174.90	2168.0
176.00	32264.0
177.00	1719.0
178.10	85.0

Instrument :
MSVOA_X
ClientSampleId :
BFB706