




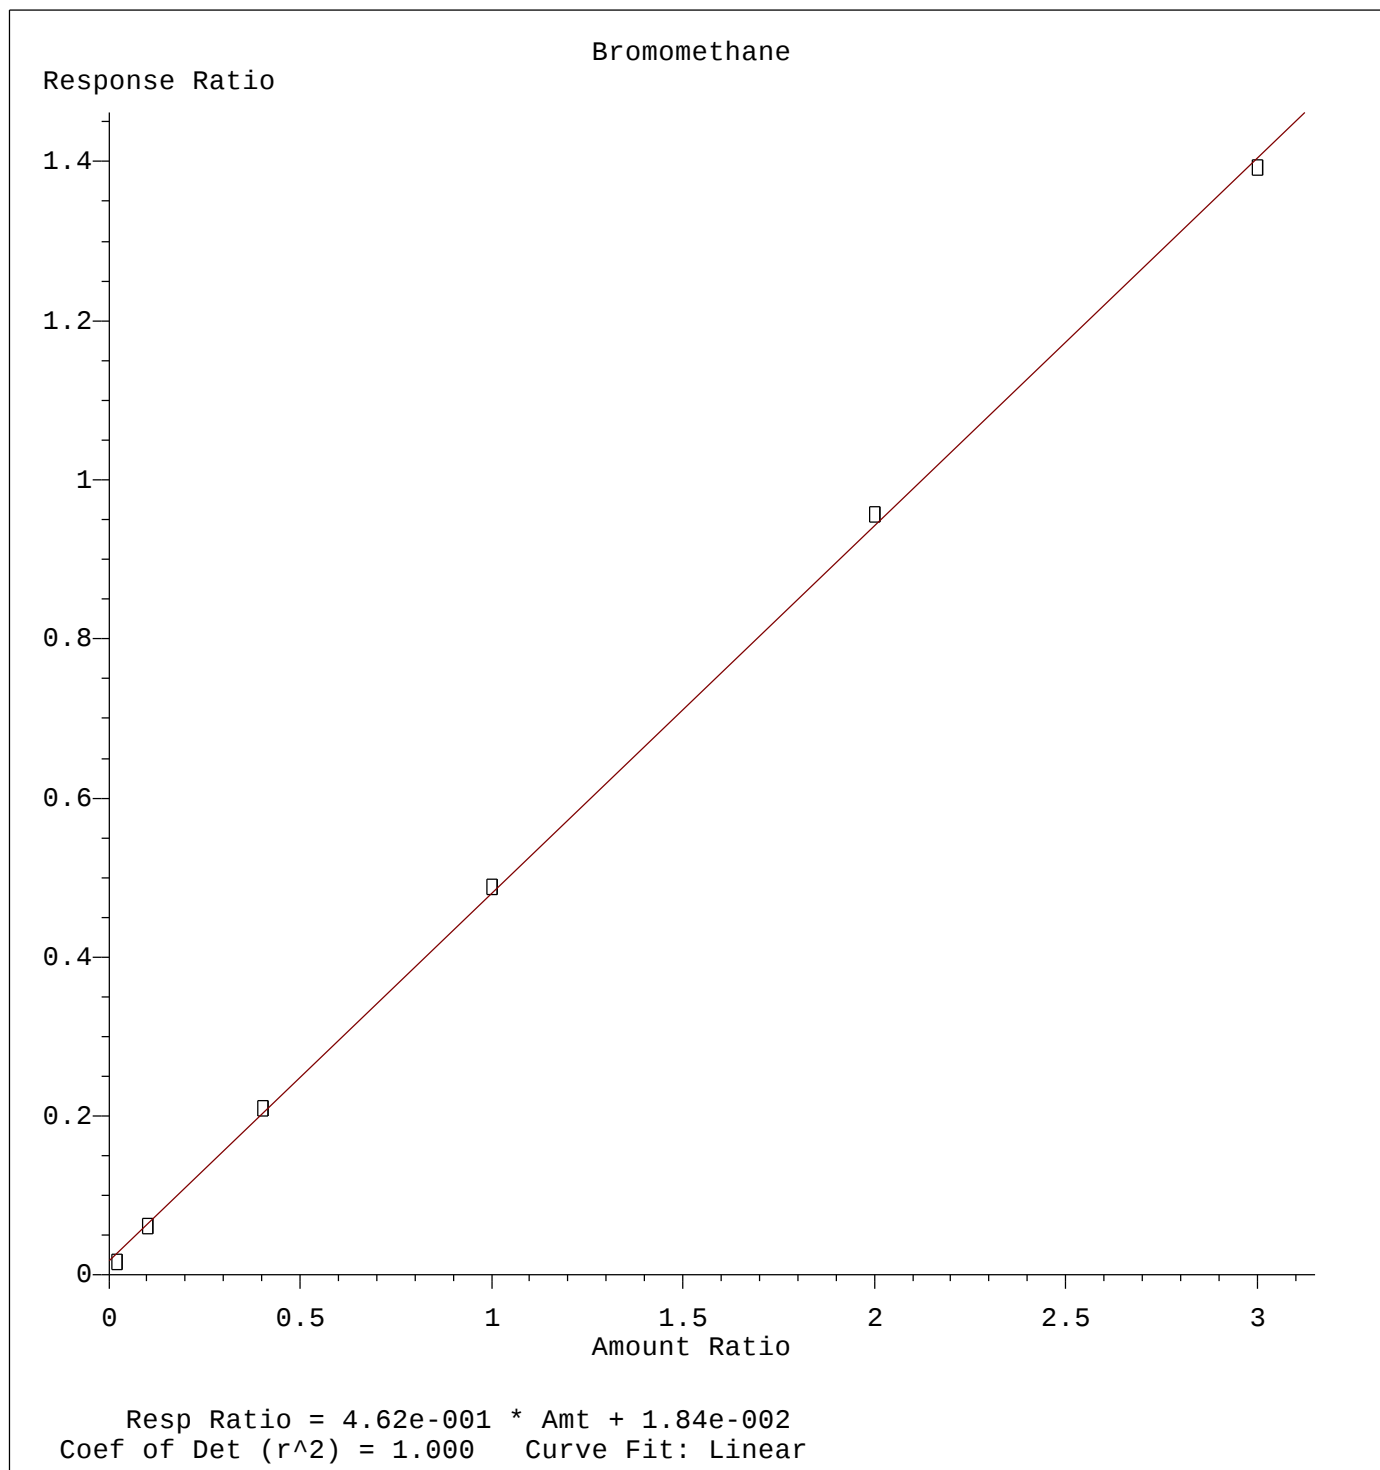

Method Name: Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82X121818W.M  
Calibration Table Last Updated: Wed Dec 19 00:58:54 2018

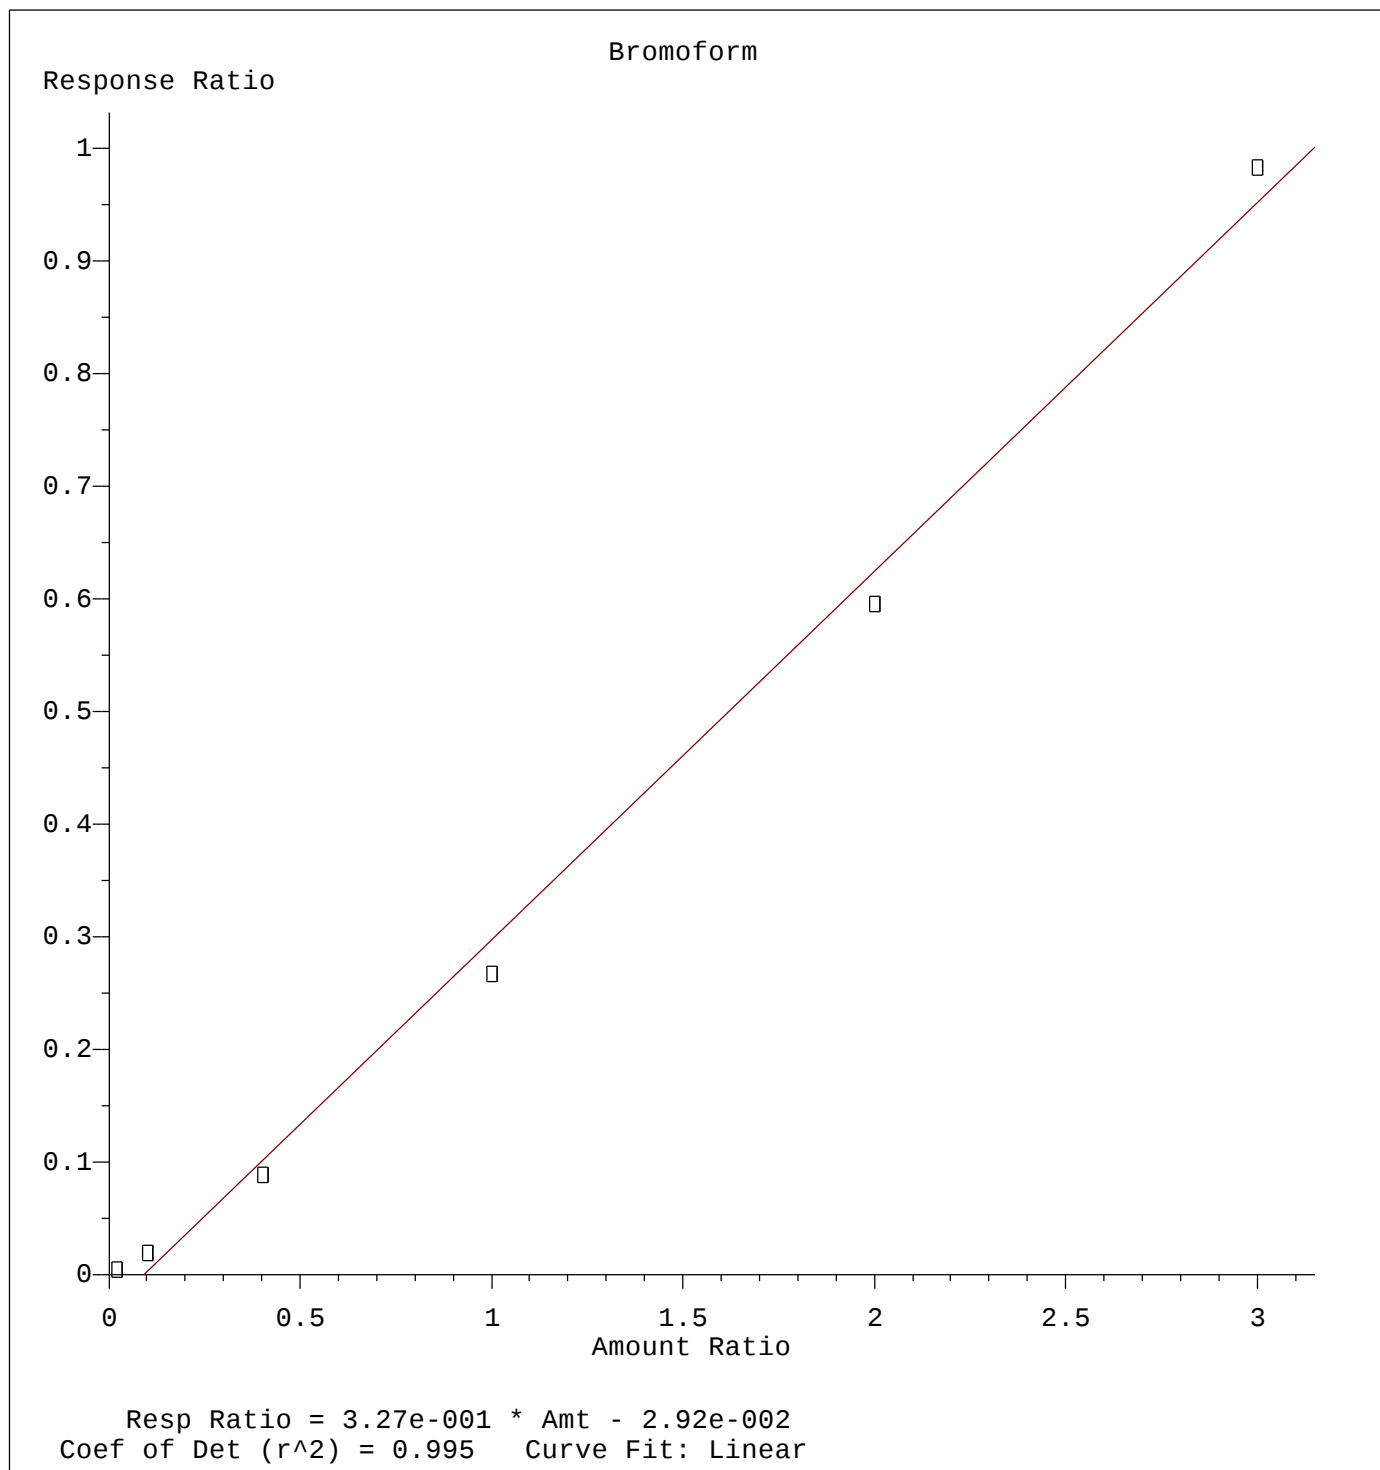


Method Name: Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82X121818W.M  
Calibration Table Last Updated: Wed Dec 19 00:58:54 2018

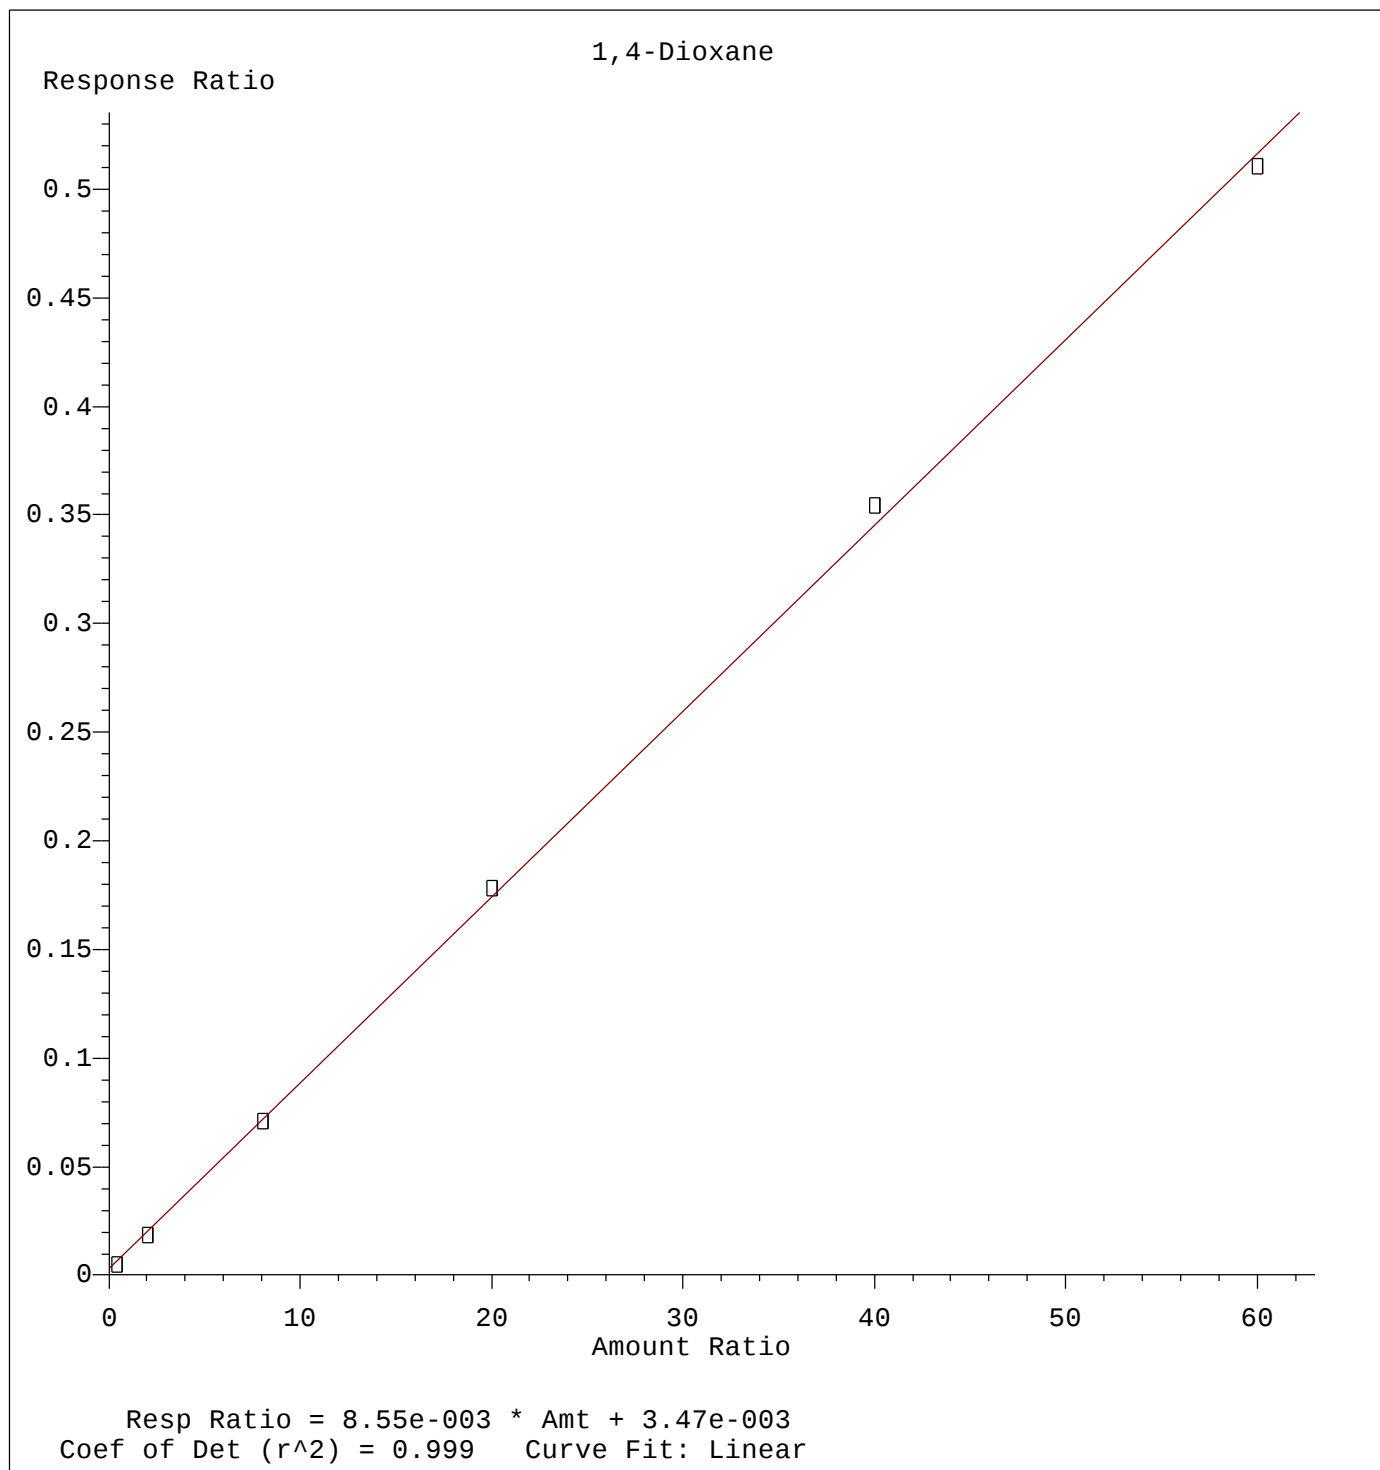

Method Name: Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82X121818W.M  
Calibration Table Last Updated: Wed Dec 19 00:58:54 2018


# Bromochloromethane

Response Ratio

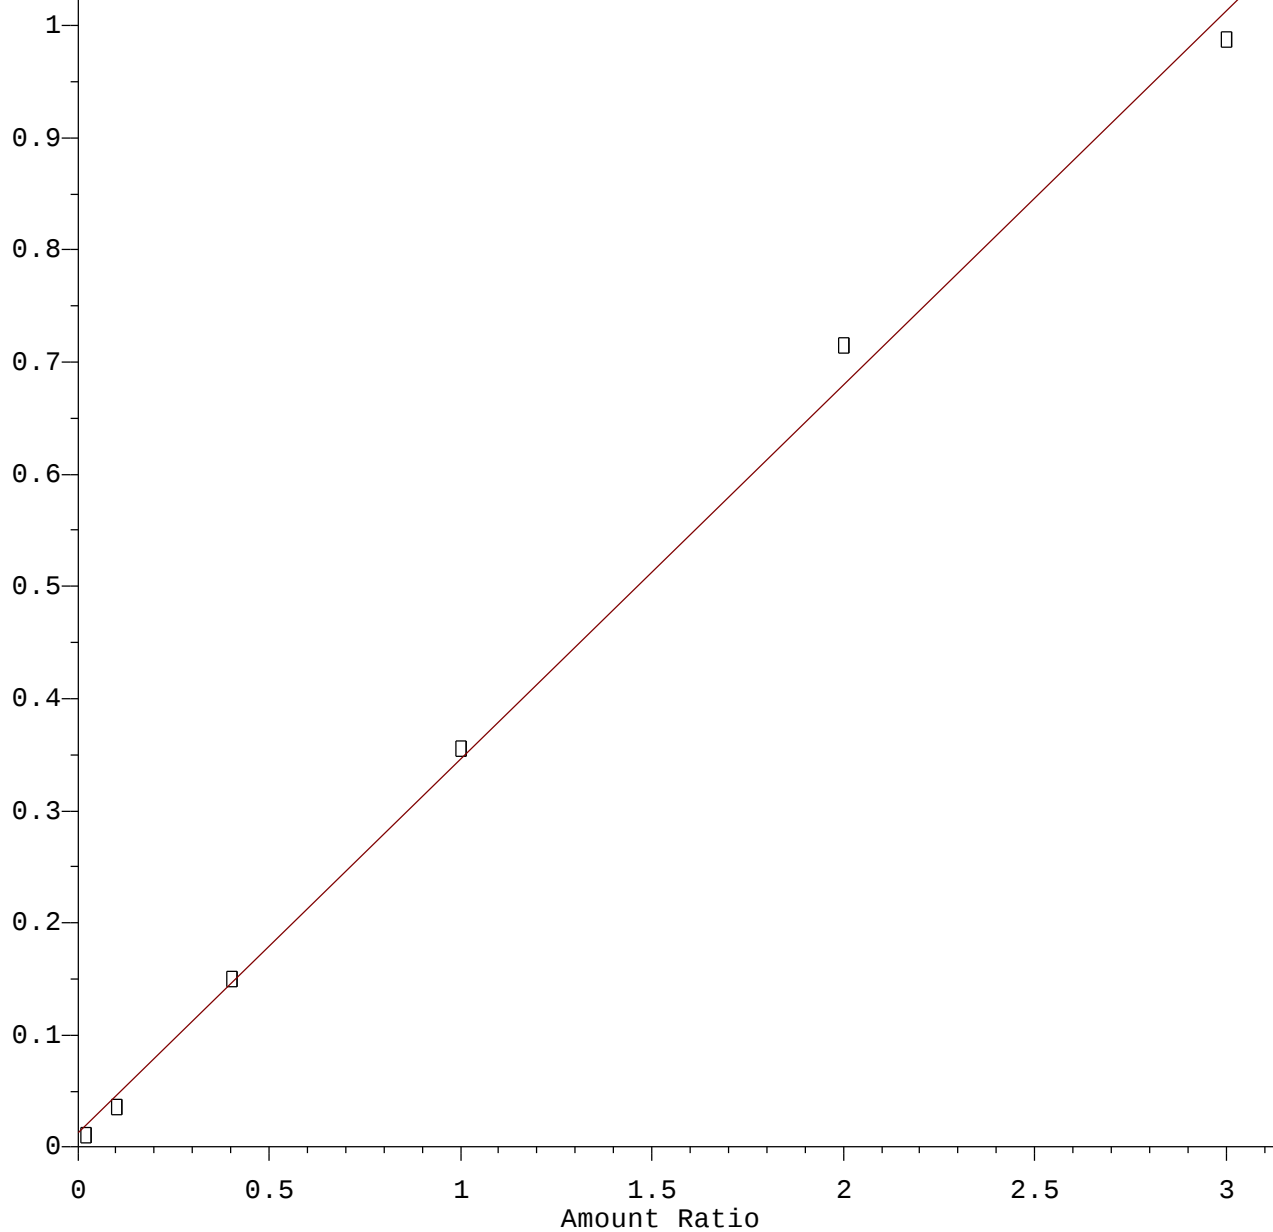


Resp Ratio =  $3.33 \times 10^{-1} \times \text{Amt} + 1.28 \times 10^{-2}$   
Coef of Det ( $r^2$ ) = 0.997    Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82X121818W.M  
Calibration Table Last Updated: Wed Dec 19 00:58:54 2018

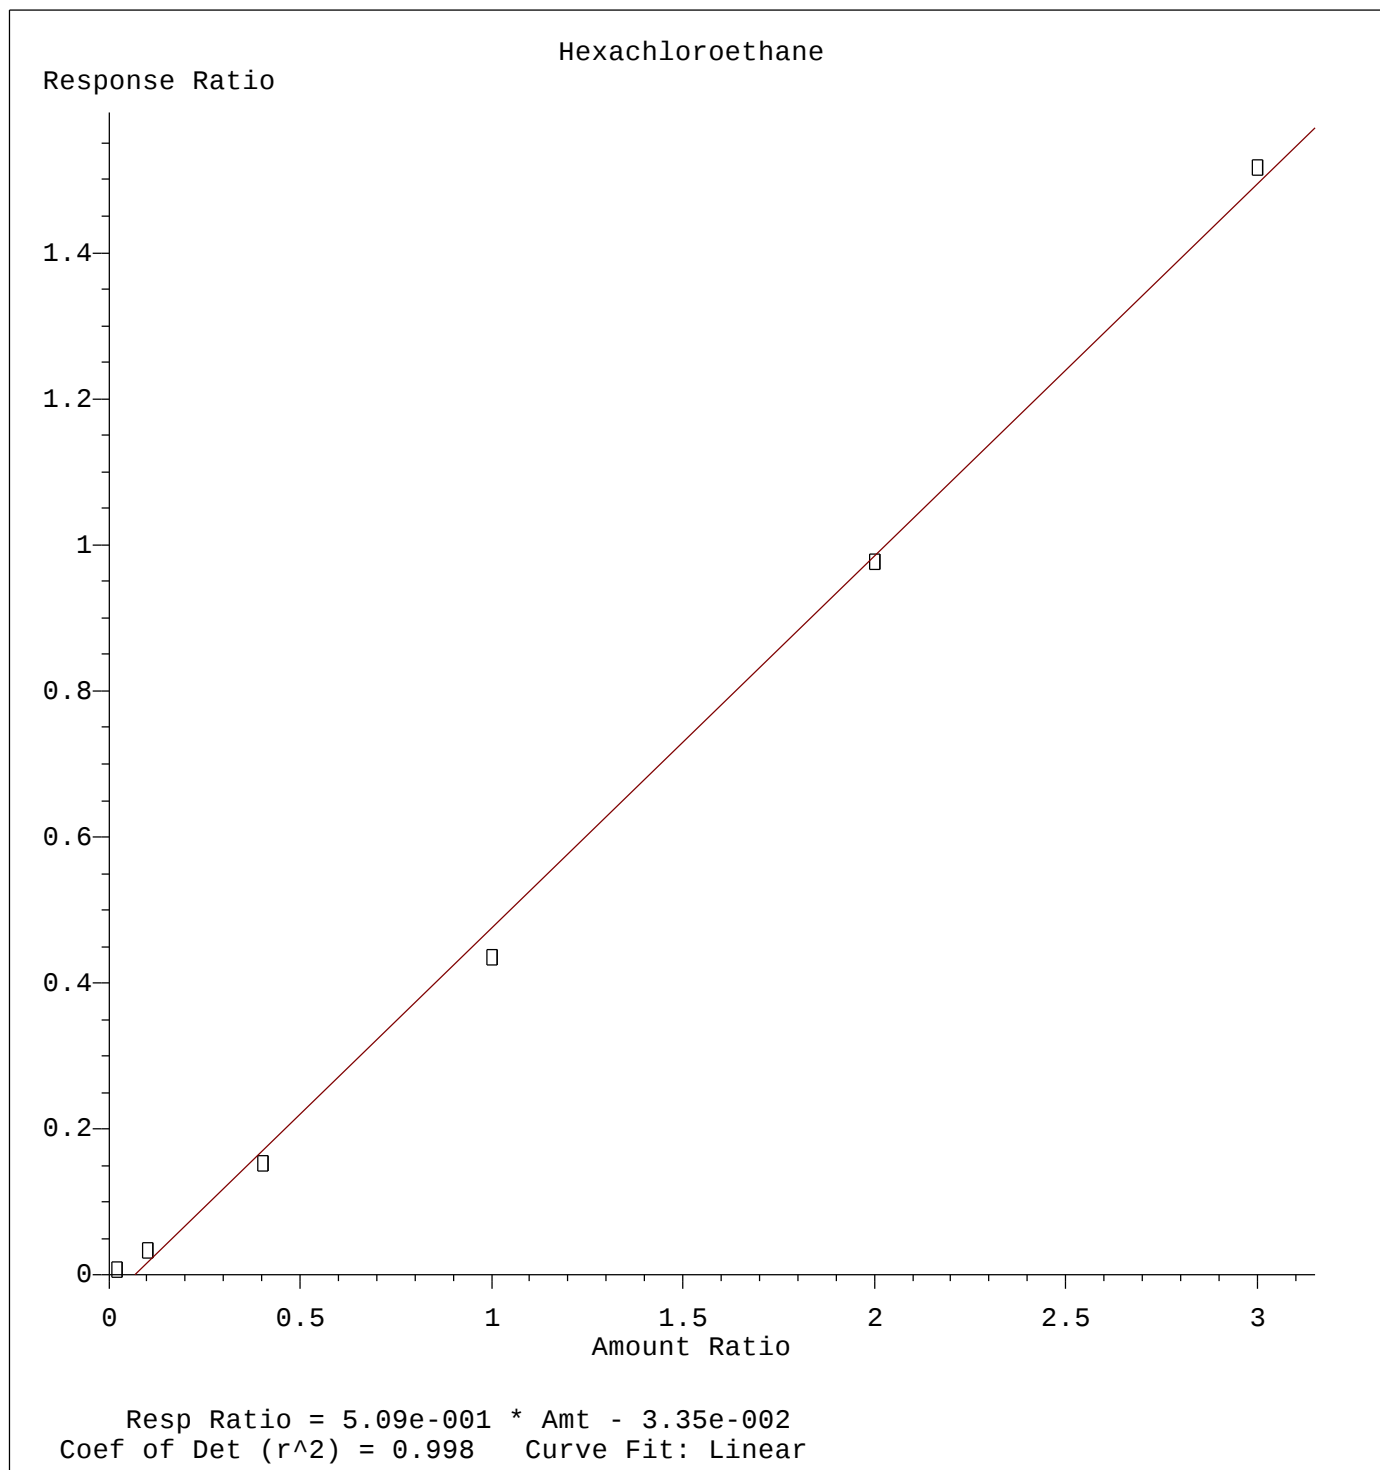


Method Name: Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82X121818W.M  
Calibration Table Last Updated: Wed Dec 19 00:58:54 2018

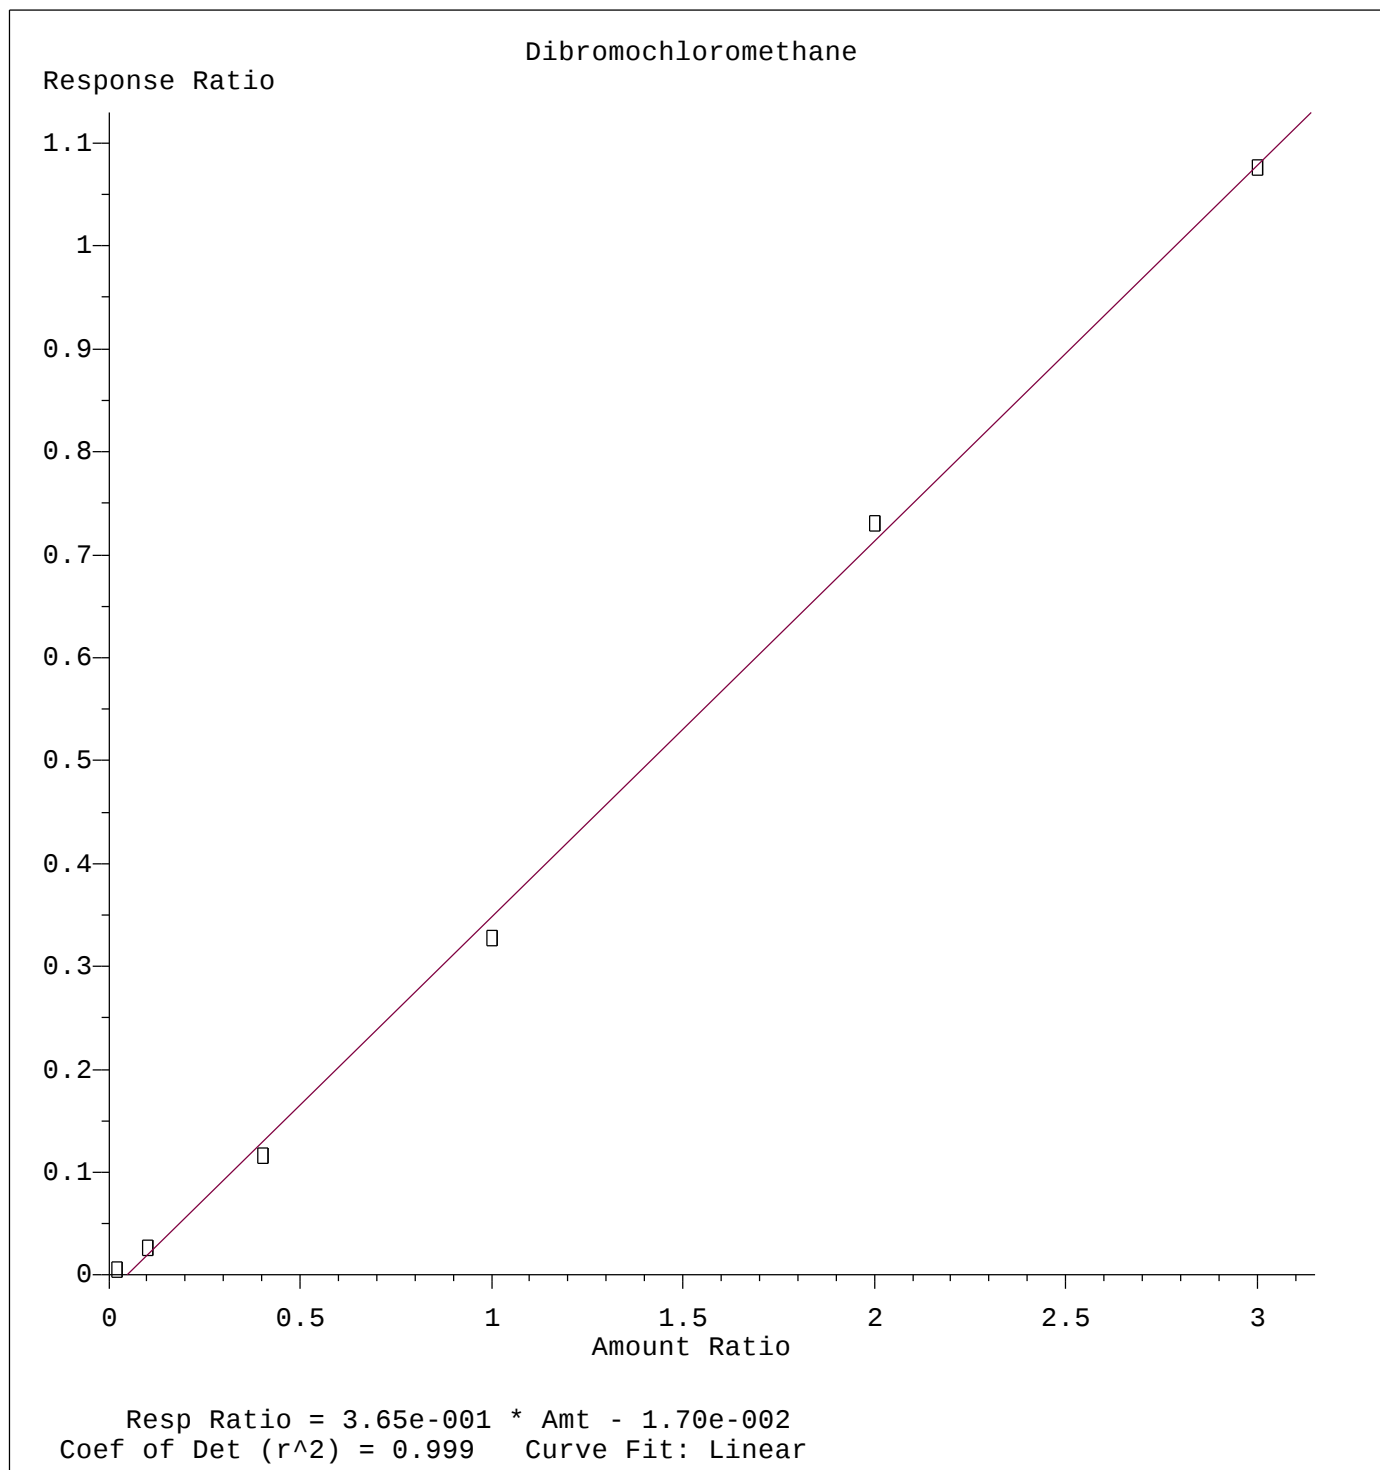

Method Name: Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82X121818W.M  
Calibration Table Last Updated: Wed Dec 19 15:20:58 2018

trans-1,4-Dichloro-2-butene

Response Ratio

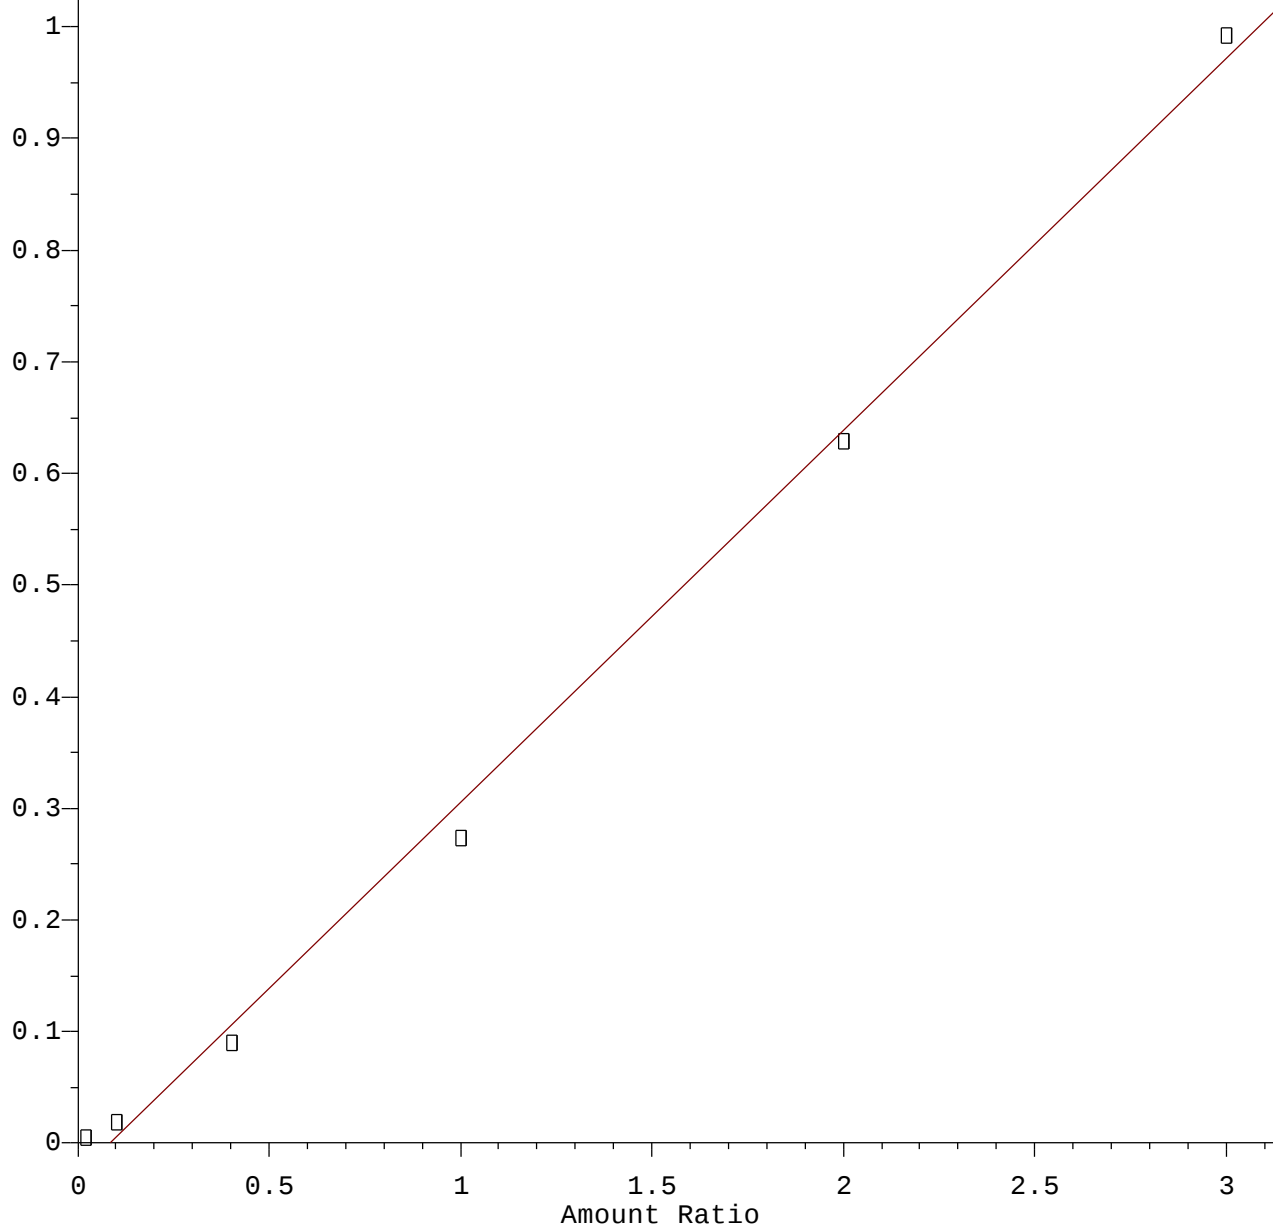

Resp Ratio =  $3.34 \times 10^{-1} \times \text{Amt} - 2.82 \times 10^{-2}$   
Coef of Det ( $r^2$ ) = 0.997    Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82X121818W.M  
Calibration Table Last Updated: Wed Dec 19 00:58:54 2018