


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX121818\
Data File : VX006586.D
Acq On : 18 Dec 2018 08:18
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X121818W.M
Title : SW846 8260
Last Update : Wed Dec 19 15:20:58 2018

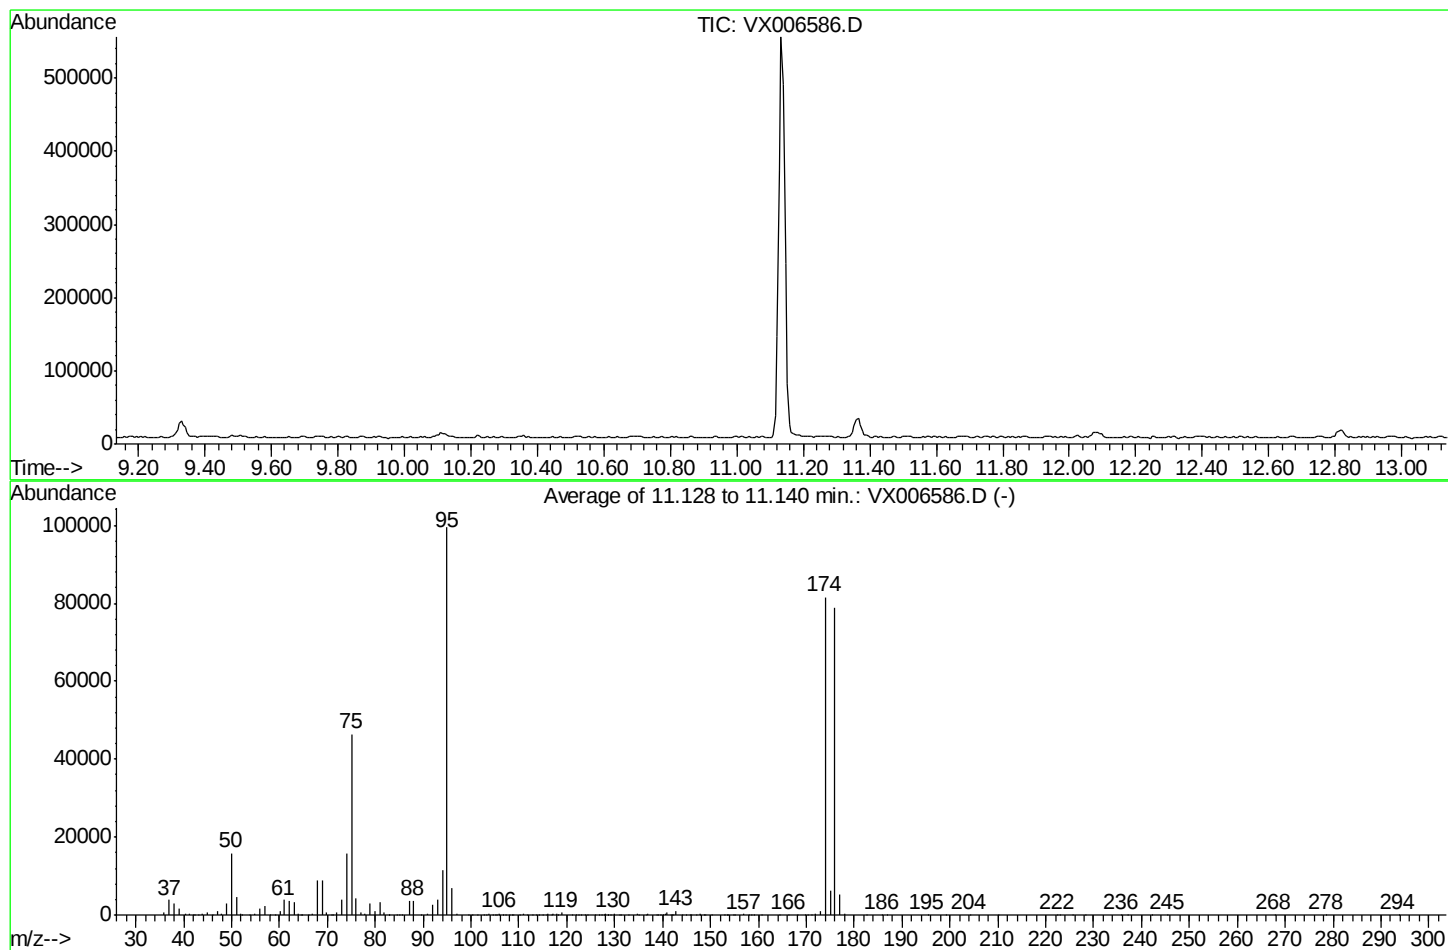

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1625

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.9	15849	PASS
75	95	30	60	46.6	46384	PASS
95	95	100	100	100.0	99496	PASS
96	95	5	9	6.9	6824	PASS
173	174	0.00	2	1.4	1125	PASS
174	95	50	100	81.9	81509	PASS
175	174	5	9	7.5	6107	PASS
176	174	95	101	96.8	78928	PASS
177	176	5	9	6.6	5230	PASS