


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX121818\
 Data File : VX006609.D
 Acq On : 18 Dec 2018 20:18
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X121818W.M
 Title : SW846 8260
 Last Update : Wed Dec 19 15:20:58 2018

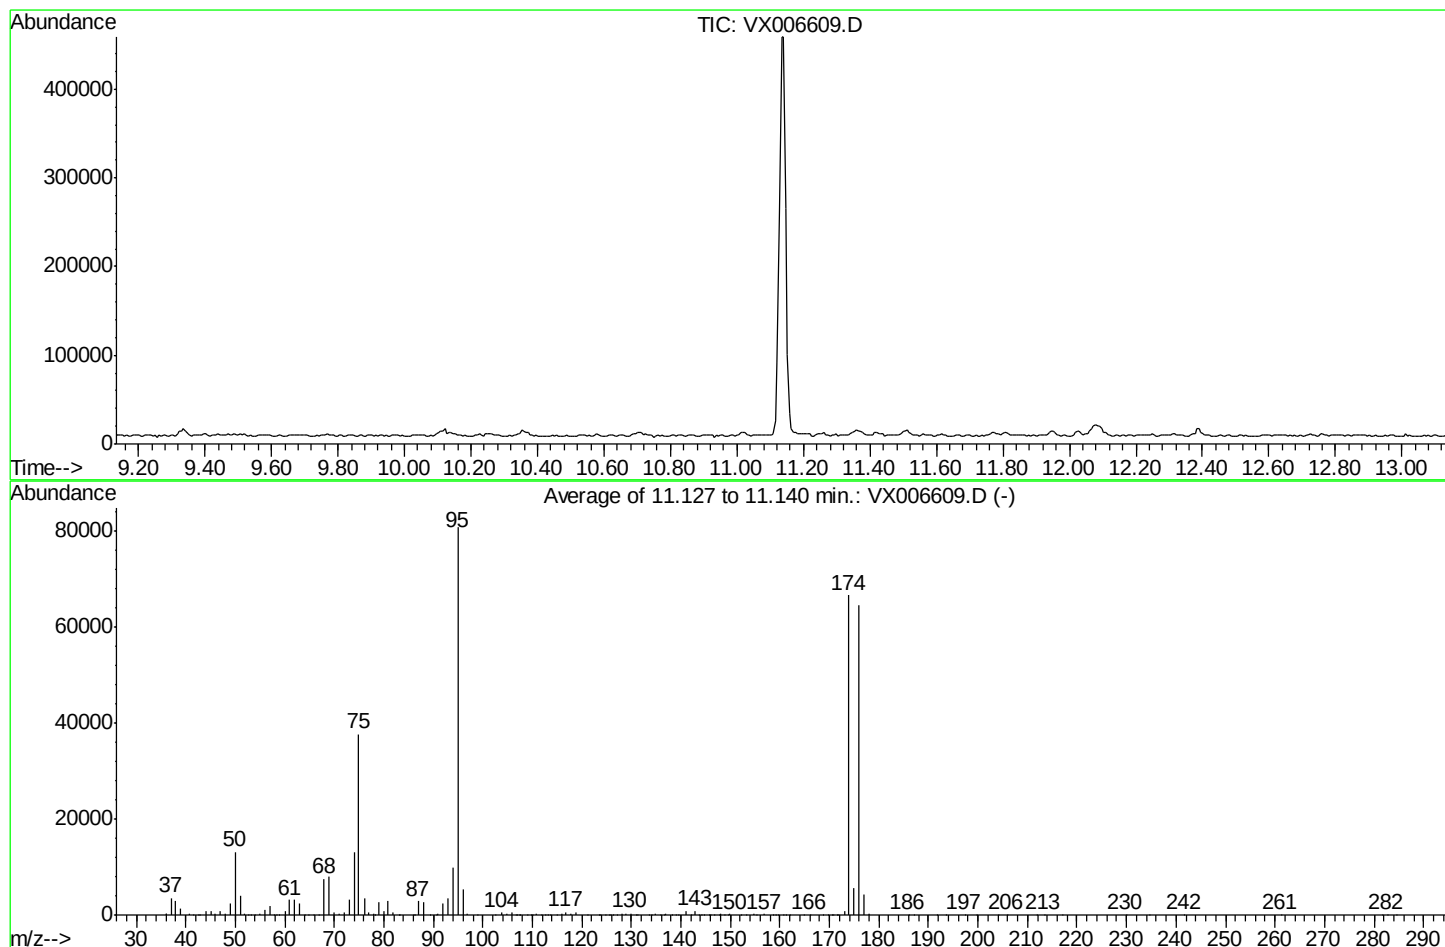

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1627

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.3	13130	PASS
75	95	30	60	46.7	37664	PASS
95	95	100	100	100.0	80673	PASS
96	95	5	9	6.7	5375	PASS
173	174	0.00	2	1.3	861	PASS
174	95	50	100	82.5	66549	PASS
175	174	5	9	8.5	5689	PASS
176	174	95	101	96.8	64402	PASS
177	176	5	9	6.8	4388	PASS