


Methyl Iodide

Response Ratio

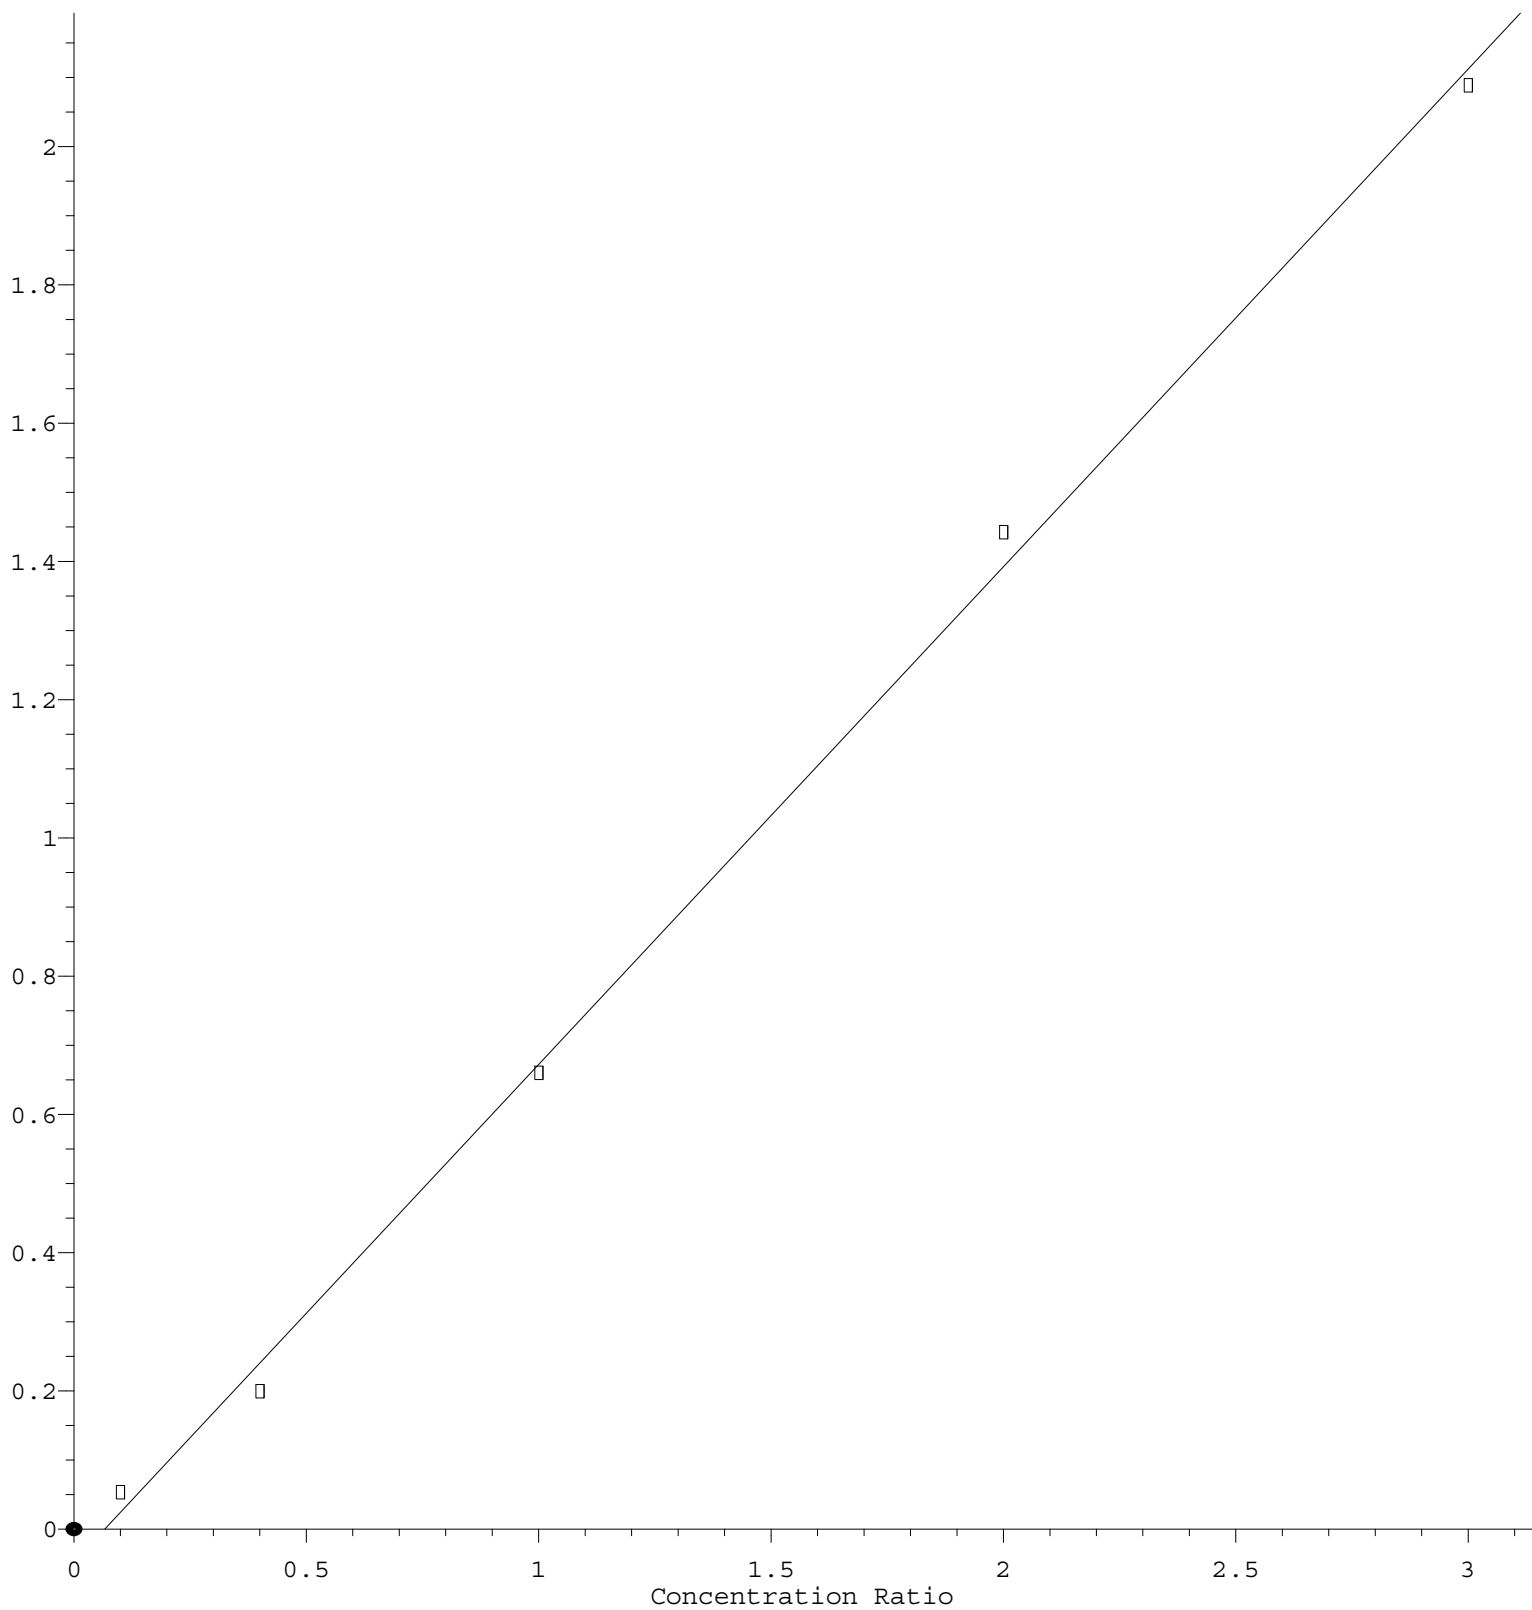

$$\text{Response} = 7.200\text{e-}001 * \text{Amt} - 4.732\text{e-}002$$


Coef of Det (r^2) = 0.998079 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA X\METHOD\82X121820W.M

Calibration Table Last Updated: Fri Dec 18 13:09:49 2020

Hexachlorobutadiene

Response Ratio

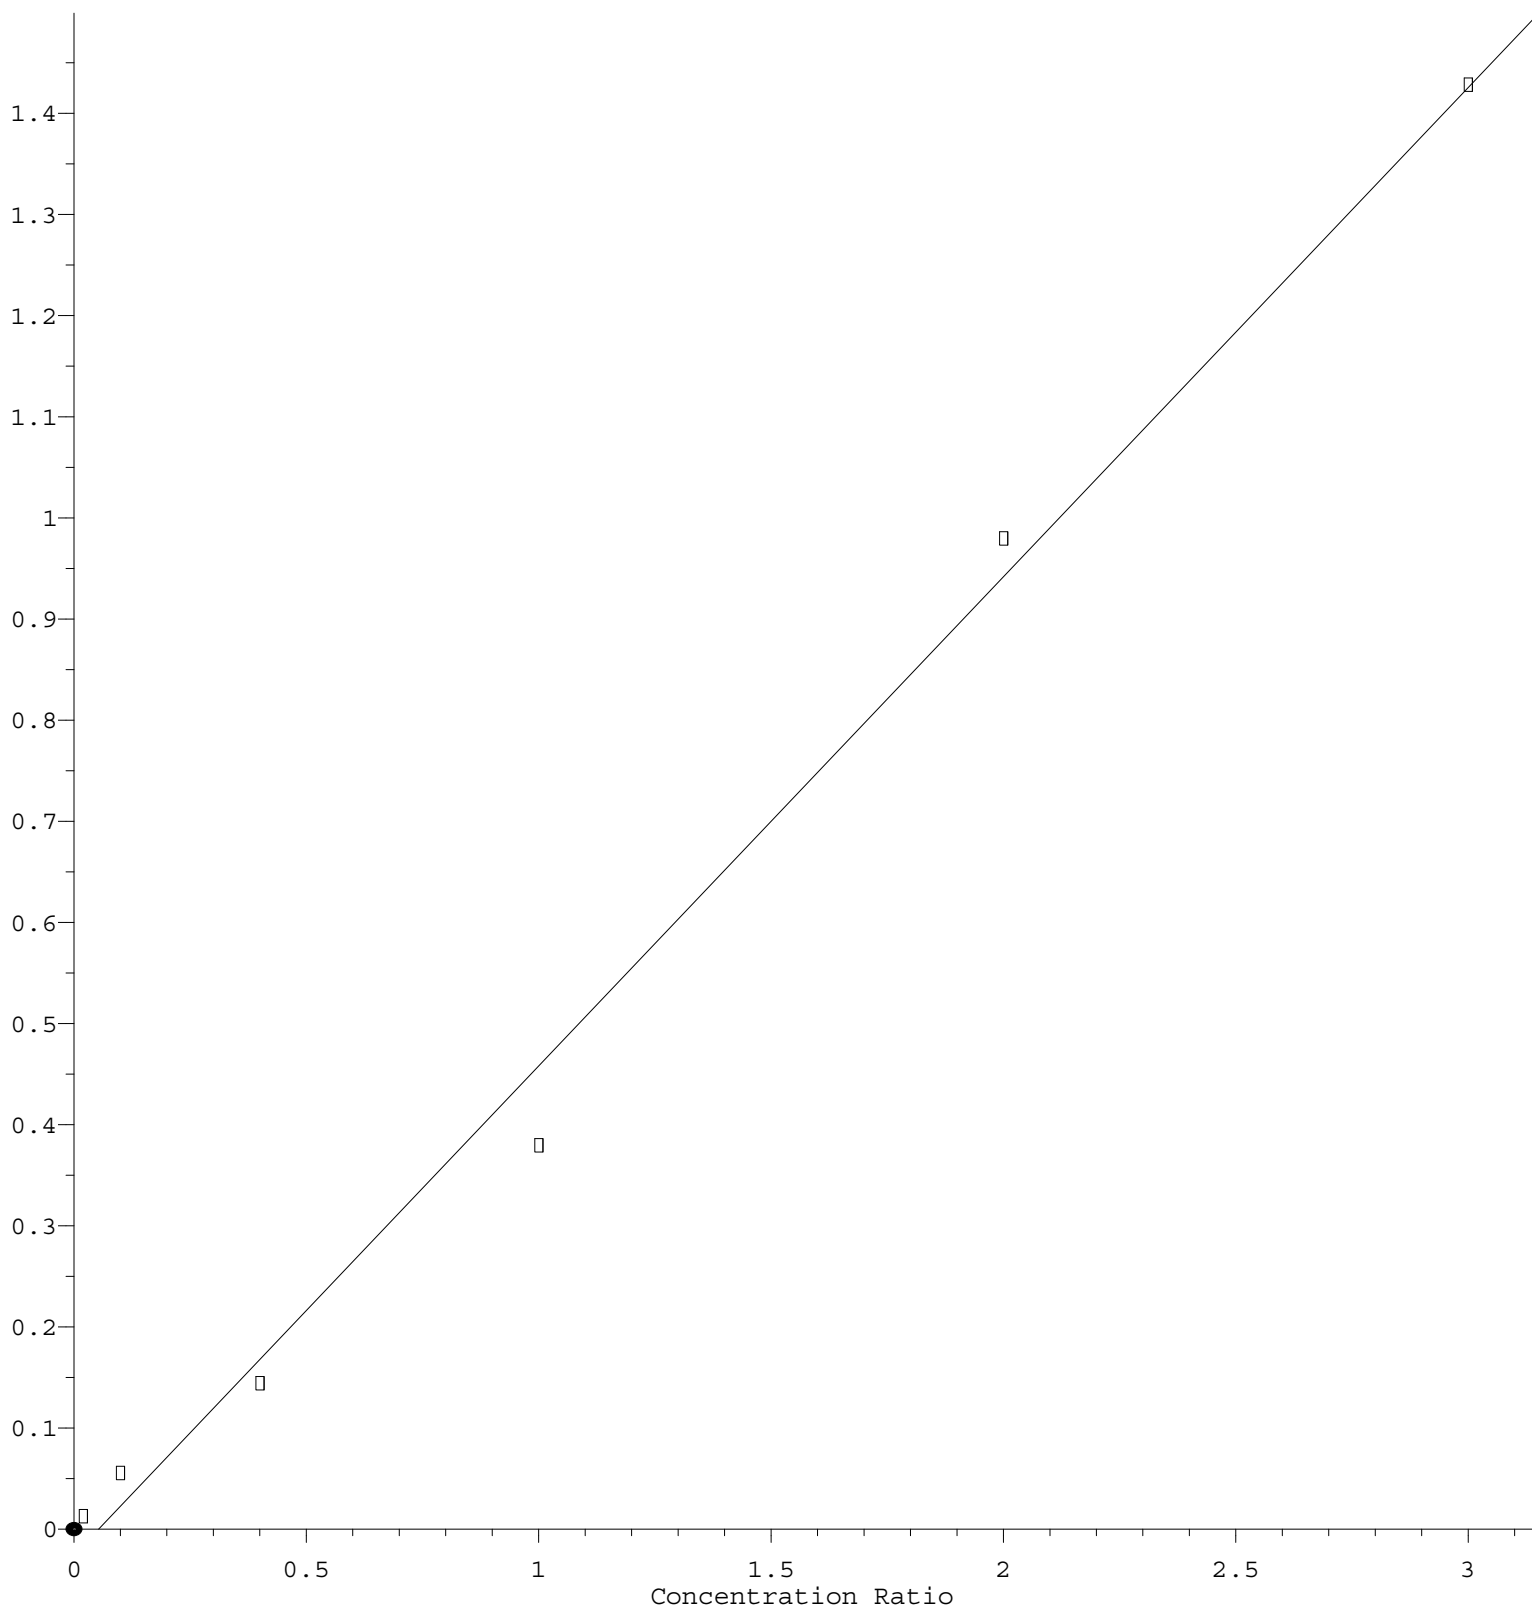

$$\text{Response} = 4.837\text{e-}001 * \text{Amt} - 2.557\text{e-}002$$

Coef of Det (r^2) = 0.993964 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA X\METHOD\82X121820W.M

Calibration Table Last Updated: Fri Dec 18 13:09:49 2020