

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\WX121820\  
 Data File : VX020122.D  
 Acq On : 18 Dec 2020 13:07  
 Operator : JC/MD  
 Sample : IBLK  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 9 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 IBLK

Quant Time: Dec 18 13:37:19 2020  
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82X121820W.M  
 Quant Title : SW846 8260  
 QLast Update : Fri Dec 18 13:09:49 2020  
 Response via : Initial Calibration

| Compound                   | R.T.   | QIon | Response | Conc  | Units | Dev(Min) |
|----------------------------|--------|------|----------|-------|-------|----------|
| -----                      |        |      |          |       |       |          |
| Internal Standards         |        |      |          |       |       |          |
| 1) Pentafluorobenzene      | 5.629  | 168  | 328087   | 50.00 | ug/l  | 0.01     |
| 34) 1,4-Difluorobenzene    | 6.830  | 114  | 536515   | 50.00 | ug/l  | 0.00     |
| 63) Chlorobenzene-d5       | 10.097 | 117  | 486388   | 50.00 | ug/l  | 0.00     |
| 72) 1,4-Dichlorobenzene-d4 | 12.060 | 152  | 212581   | 50.00 | ug/l  | 0.00     |

|                             |        |       |          |          |      |        |
|-----------------------------|--------|-------|----------|----------|------|--------|
| System Monitoring Compounds |        |       |          |          |      |        |
| 33) 1,2-Dichloroethane-d4   | 6.031  | 65    | 201228   | 45.76    | ug/l | 0.00   |
| Spiked Amount               | 50.000 | Range | 61 - 141 | Recovery | =    | 91.52% |
| 35) Dibromofluoromethane    | 5.458  | 113   | 162016   | 47.21    | ug/l | 0.00   |
| Spiked Amount               | 50.000 | Range | 69 - 133 | Recovery | =    | 94.42% |
| 50) Toluene-d8              | 8.695  | 98    | 639137   | 48.38    | ug/l | 0.00   |
| Spiked Amount               | 50.000 | Range | 65 - 126 | Recovery | =    | 96.76% |
| 62) 4-Bromofluorobenzene    | 11.122 | 95    | 228272   | 45.15    | ug/l | 0.00   |
| Spiked Amount               | 50.000 | Range | 58 - 135 | Recovery | =    | 90.30% |

|                               |        |     |        |              |        |
|-------------------------------|--------|-----|--------|--------------|--------|
| Target Compounds              |        |     |        |              | Qvalue |
| 2) Dichlorodifluoromethane    | 1.184  | 85  | 976    | 0.27 ug/l    | 94     |
| 3) Chloromethane              | 1.312  | 50  | 1418   | 0.34 ug/l #  | 88     |
| 4) Vinyl Chloride             | 1.392  | 62  | 947    | 0.21 ug/l    | 97     |
| 5) Bromomethane               | 1.629  | 94  | 2112   | 1.46 ug/l    | 94     |
| 6) Chloroethane               | 1.715  | 64  | 620    | 0.22 ug/l #  | 54     |
| 9) 1,1,2-Trichlorotrifluo...  | 2.361  | 101 | 1155   | 0.35 ug/l    | 97     |
| 10) Methyl Iodide             | 2.495  | 142 | 3018   | 3.92 ug/l    | 98     |
| 11) Tert butyl alcohol        | 2.995  | 59  | 3526   | 3.58 ug/l #  | 75     |
| 12) 1,1-Dichloroethene        | 2.355  | 96  | 926    | 0.28 ug/l    | 96     |
| 13) Acrolein                  | 2.276  | 56  | 1023   | 1.66 ug/l #  | 76     |
| 14) Allyl chloride            | 2.708  | 41  | 1230   | 0.21 ug/l #  | 74     |
| 15) Acrylonitrile             | 3.117  | 53  | 2576   | 1.14 ug/l    | 98     |
| 16) Acetone                   | 2.416  | 43  | 2000   | 1.00 ug/l    | 91     |
| 17) Carbon Disulfide          | 2.550  | 76  | 12624  | 1.28 ug/l    | 100    |
| 18) Methyl Acetate            | 2.745  | 43  | 1297   | 0.29 ug/l    | 93     |
| 20) Methylene Chloride        | 2.830  | 84  | 1341   | 0.30 ug/l    | 89     |
| 21) trans-1,2-Dichloroethene  | 3.141  | 96  | 2060   | 0.51 ug/l    | 96     |
| 23) Vinyl Acetate             | 3.781  | 43  | 3233   | 0.31 ug/l    | 94     |
| 25) 2-Butanone                | 4.647  | 43  | 1366   | 0.47 ug/l    | 91     |
| 27) cis-1,2-Dichloroethene    | 4.562  | 96  | 1209   | 0.26 ug/l    | 88     |
| 28) Bromochloromethane        | 4.982  | 49  | 700    | 0.22 ug/l #  | 88     |
| 29) Tetrahydrofuran           | 5.117  | 42  | 1223   | 0.67 ug/l #  | 72     |
| 36) 1,1-Dichloropropene       | 5.763  | 75  | 1961   | 0.37 ug/l    | 94     |
| 38) Carbon Tetrachloride      | 5.623  | 117 | 31775  | 6.30 ug/l #  | 17     |
| 39) Methylcyclohexane         | 7.439  | 83  | 2139   | 0.35 ug/l    | 94     |
| 42) 1,2-Dichloroethane        | 6.165  | 62  | 1171   | 0.21 ug/l    | 84     |
| 44) Trichloroethene           | 7.183  | 130 | 1467   | 0.34 ug/l    | 97     |
| 46) Dibromomethane            | 7.634  | 93  | 696    | 0.24 ug/l    | 95     |
| 49) 1,4-Dioxane               | 7.720  | 88  | 222    | 2.22 ug/l #  | 77     |
| 51) 4-Methyl-2-Pentanone      | 8.622  | 43  | 1198   | 0.22 ug/l #  | 83     |
| 53) t-1,3-Dichloropropene     | 9.018  | 75  | 1286   | 0.21 ug/l    | 91     |
| 58) 2-Chloroethyl Vinyl ether | 8.287  | 63  | 1079   | 0.34 ug/l    | 98     |
| 59) 2-Hexanone                | 9.469  | 43  | 1246   | 0.30 ug/l    | 77     |
| 64) Tetrachloroethene         | 9.317  | 164 | 1281   | 0.35 ug/l    | 96     |
| 65) Chlorobenzene             | 10.122 | 112 | 2156   | 0.21 ug/l    | 98     |
| 68) m/p-Xylenes               | 10.341 | 106 | 2529   | 0.37 ug/l    | 97     |
| 76) 1,2,3-Trichloropropane    | 11.116 | 75  | 110370 | 21.08 ug/l # | 39     |

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX121820\  
 Data File : VX020122.D  
 Acq On : 18 Dec 2020 13:07  
 Operator : JC/MD  
 Sample : IBLK  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 9 Sample Multiplier: 1


Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 IBLK


Quant Time: Dec 18 13:37:19 2020  
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82X121820W.M  
 Quant Title : SW846 8260  
 QLast Update : Fri Dec 18 13:09:49 2020  
 Response via : Initial Calibration

| Compound                      | R.T.   | QIon | Response | Conc  | Units  | Dev(Min) |
|-------------------------------|--------|------|----------|-------|--------|----------|
| -----                         |        |      |          |       |        |          |
| 77) Bromobenzene              | 11.237 | 156  | 1091     | 0.27  | ug/l   | 96       |
| 78) n-propylbenzene           | 11.341 | 91   | 5305     | 0.30  | ug/l   | 97       |
| 79) 2-Chlorotoluene           | 11.402 | 91   | 2517     | 0.23  | ug/l   | 95       |
| 80) 1,3,5-Trimethylbenzene    | 11.487 | 105  | 2788     | 0.21  | ug/l   | 98       |
| 81) trans-1,4-Dichloro-2-b... | 11.116 | 75   | 110370   | 62.53 | ug/l # | 12       |
| 82) 4-Chlorotoluene           | 11.493 | 91   | 4562     | 0.35  | ug/l   | 99       |
| 84) 1,2,4-Trimethylbenzene    | 11.792 | 105  | 3014     | 0.23  | ug/l   | 98       |
| 85) sec-Butylbenzene          | 11.932 | 105  | 4402     | 0.31  | ug/l   | 98       |
| 86) p-Isopropyltoluene        | 12.048 | 119  | 4166     | 0.31  | ug/l # | 81       |
| 87) 1,3-Dichlorobenzene       | 12.006 | 146  | 3267     | 0.45  | ug/l   | 94       |
| 88) 1,4-Dichlorobenzene       | 12.006 | 146  | 3267     | 0.43  | ug/l   | 93       |
| 89) n-Butylbenzene            | 12.371 | 91   | 5660     | 0.49  | ug/l   | 97       |
| 91) 1,2-Dichlorobenzene       | 12.377 | 146  | 2281     | 0.32  | ug/l   | 99       |
| 92) 1,2-Dibromo-3-Chloropr... | 12.981 | 75   | 282      | 0.24  | ug/l # | 58       |
| 93) 1,2,4-Trichlorobenzene    | 13.627 | 180  | 4436     | 0.96  | ug/l   | 98       |
| 94) Hexachlorobutadiene       | 13.767 | 225  | 2622     | 3.92  | ug/l   | 96       |
| 95) Naphthalene               | 13.816 | 128  | 9870     | 0.67  | ug/l   | 99       |
| 96) 1,2,3-Trichlorobenzene    | 13.999 | 180  | 4104     | 0.89  | ug/l   | 97       |
| -----                         |        |      |          |       |        |          |

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Dec 18 13:37:19 2020  
Quant Method : Z:\V\OASRV\HPCHEM1\MSVOA\_X\METHOD\82X121820W.M  
Quant Title : SW846 8260  
QLast Update : Fri Dec 18 13:09:49 2020  
Response via : Initial Calibration




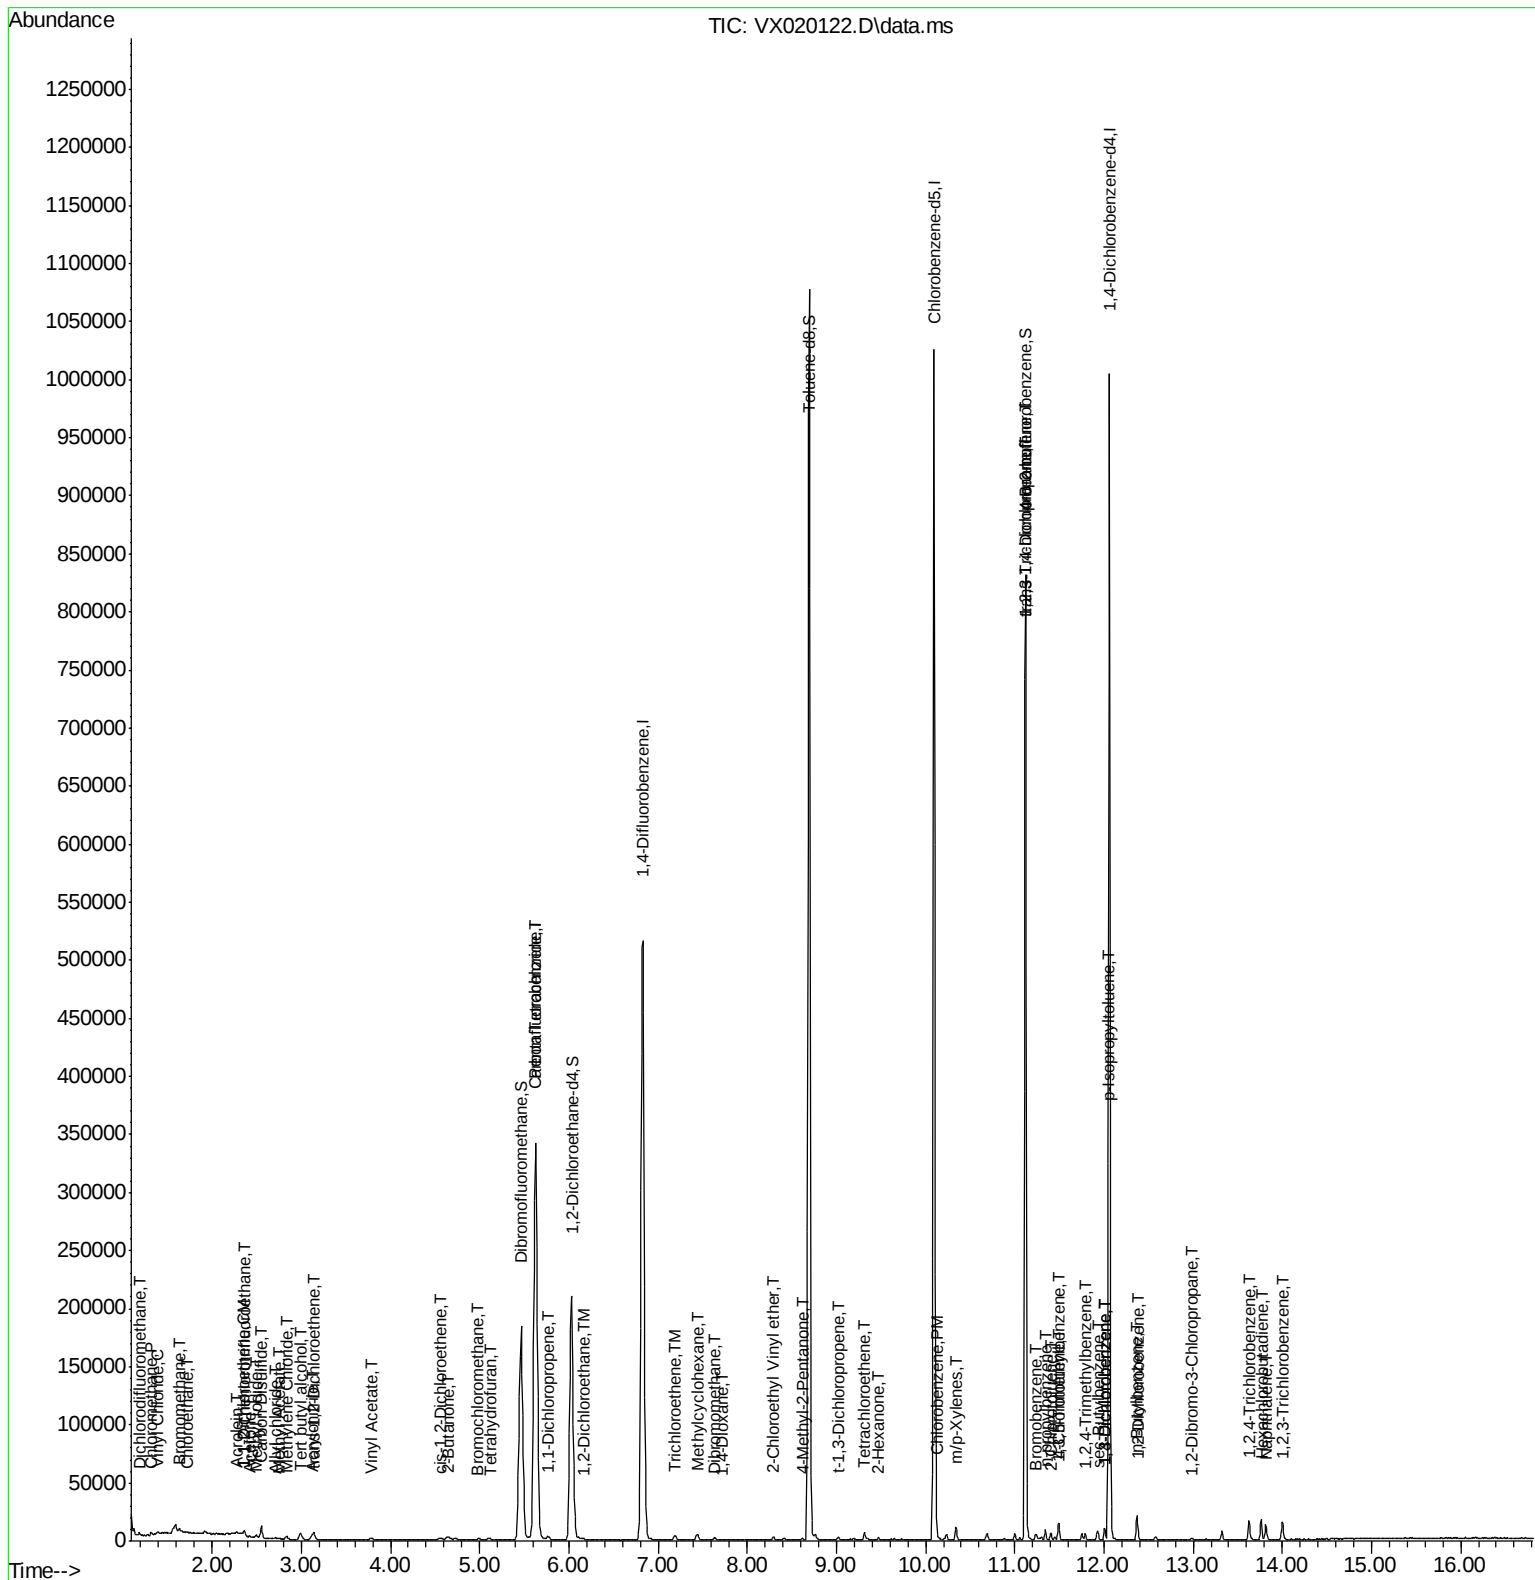




Scan 743 (5.617 min): VX020119.D\data.ms (-743) (-)  
 Pentafluorobenzene  
 Concen: 50.00 ug/l  
 RT: 5.629 min Scan# 745  
 Delta R.T. 0.012 min  
 Lab File: VX020122.D  
 Acq: 18 Dec 2020 13:07




Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 IBLK


Tgt Ion:168 Resp: 328087  
 Ion Ratio Lower Upper  
 168 100  
 99 55.5 45.8 68.6

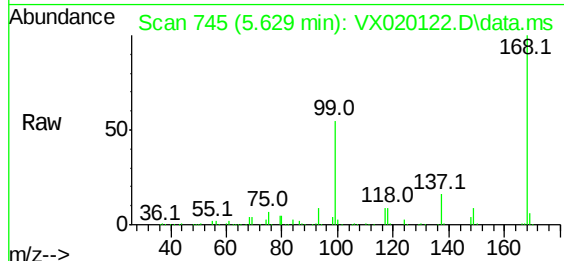

Scan 16 (1.185 min): VX020119.D\data.ms (-1172) (-)  
 Dichlorodifluoromethane  
 Concen: 0.27 ug/l  
 RT: 1.184 min Scan# 16  
 Delta R.T. -0.001 min  
 Lab File: VX020122.D  
 Acq: 18 Dec 2020 13:07

Tgt Ion: 85 Resp: 976  
 Ion Ratio Lower Upper  
 85 100  
 87 29.4 16.4 49.2


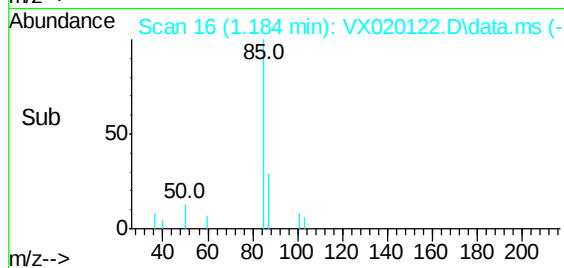




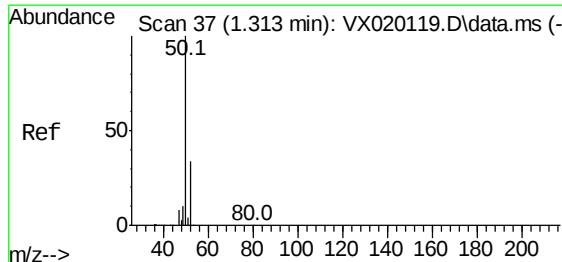

Chloromethane  
 Concen: 0.34 ug/l  
 RT: 1.312 min Scan# 37  
 Delta R.T. -0.001 min  
 Lab File: VX020122.D  
 Acq: 18 Dec 2020 13:07




Instrument :  
 MSVOA\_X  
 ClientSampled :  
 IBLK


Tgt Ion: 50 Resp: 1418  
 Ion Ratio Lower Upper  
 50 100  
 52 40.0 26.4 39.6#

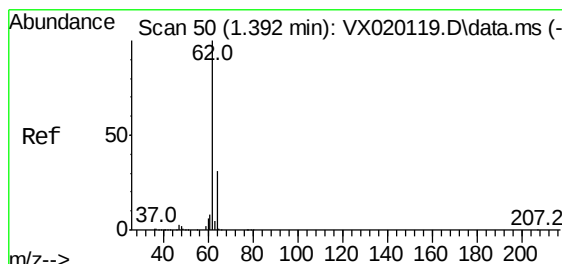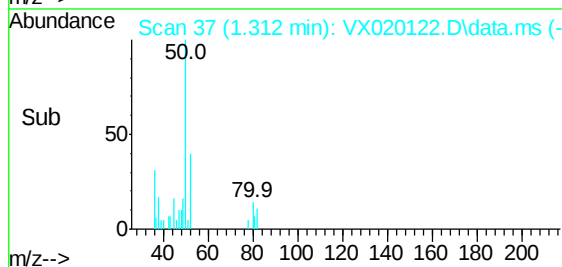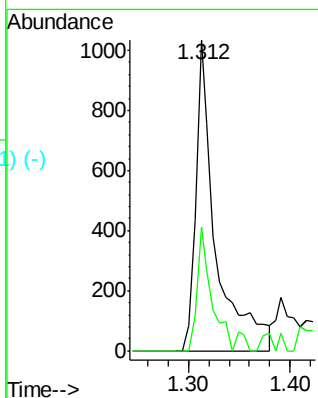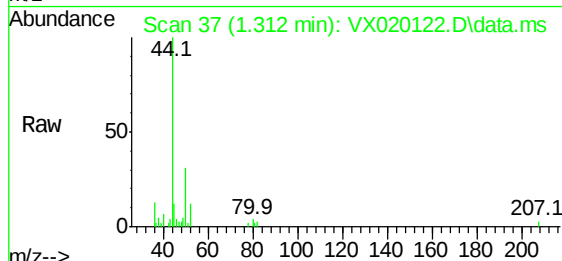

Vinyl Chloride  
 Concen: 0.21 ug/l  
 RT: 1.392 min Scan# 50  
 Delta R.T. -0.000 min  
 Lab File: VX020122.D  
 Acq: 18 Dec 2020 13:07

Tgt Ion: 62 Resp: 947  
 Ion Ratio Lower Upper  
 62 100  
 64 30.3 25.7 38.5


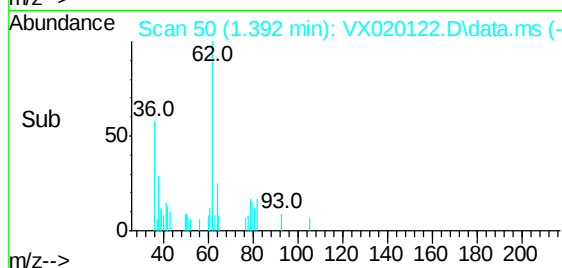
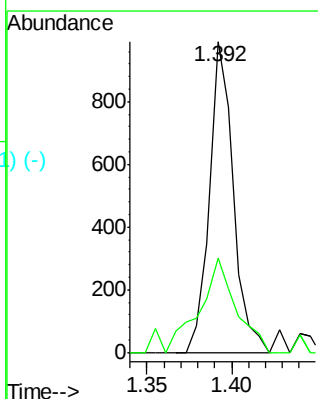
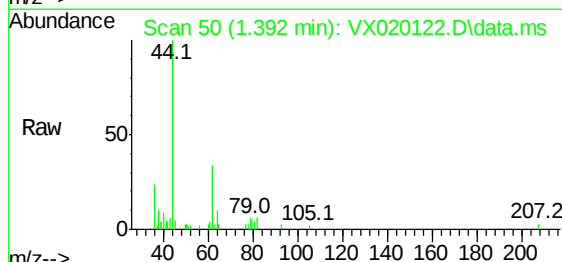


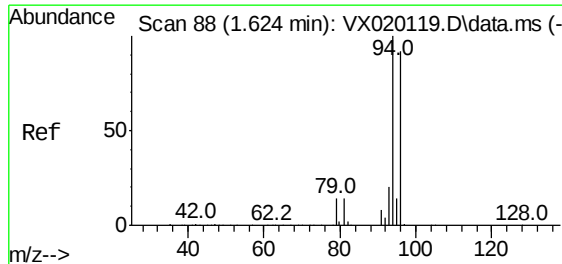

Bromomethane  
 Concen: 1.46 ug/l  
 RT: 1.629 min Scan# 89  
 Delta R.T. 0.005 min  
 Lab File: VX020122.D  
 Acq: 18 Dec 2020 13:07




Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 IBLK


Tgt Ion: 94 Resp: 2112  
 Ion Ratio Lower Upper  
 94 100  
 96 89.4 76.4 114.6

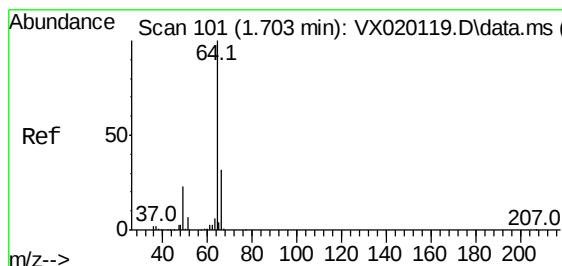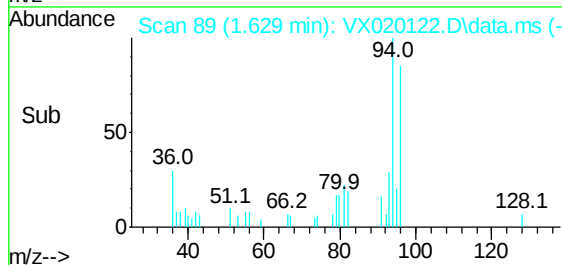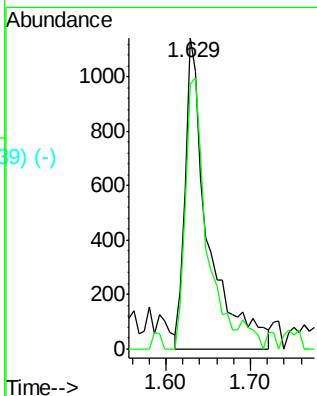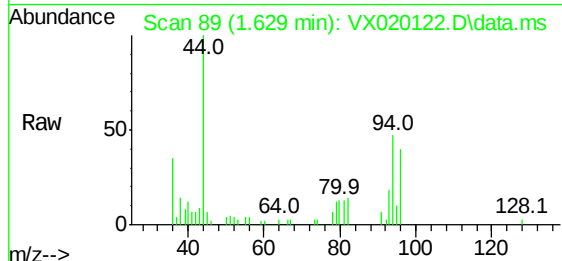

Chloroethane  
 Concen: 0.22 ug/l  
 RT: 1.715 min Scan# 103  
 Delta R.T. 0.012 min  
 Lab File: VX020122.D  
 Acq: 18 Dec 2020 13:07

Tgt Ion: 64 Resp: 620  
 Ion Ratio Lower Upper  
 64 100  
 66 6.3 25.4 38.0#


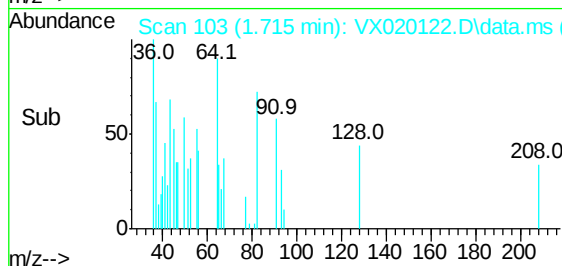
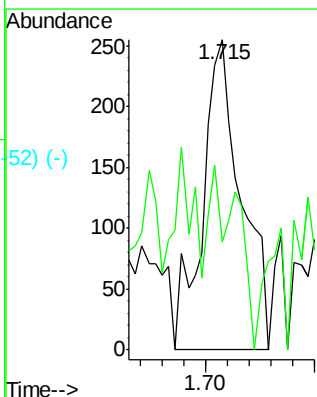
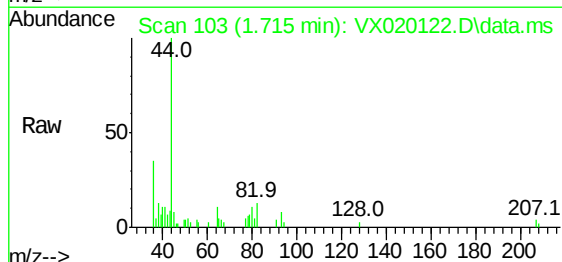




1,1,2-Trichlorotrifluoroethane  
Concen: 0.35 ug/l  
RT: 2.361 min Scan# 209  
Delta R.T. -0.000 min  
Lab File: VX020122.D  
Acq: 18 Dec 2020 13:07




Instrument :  
MSVOA\_X  
ClientSampleId :  
IBLK


|          |       |       |       |
|----------|-------|-------|-------|
| Tgt Ion: | 101   | Resp: | 1155  |
| Ion      | Ratio | Lower | Upper |
| 101      | 100   |       |       |
| 85       | 39.6  | 34.9  | 52.3  |
| 151      | 77.1  | 61.4  | 92.2  |

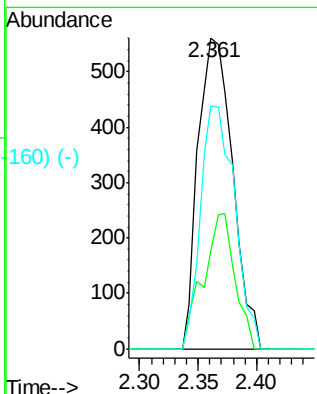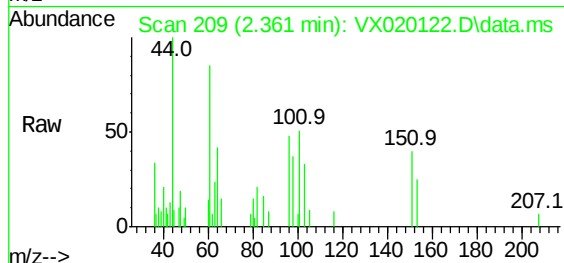

Methyl Iodide  
Concen: 3.92 ug/l  
RT: 2.495 min Scan# 231  
Delta R.T. 0.006 min  
Lab File: VX020122.D  
Acq: 18 Dec 2020 13:07

|          |       |       |       |
|----------|-------|-------|-------|
| Tgt Ion: | 142   | Resp: | 3018  |
| Ion      | Ratio | Lower | Upper |
| 142      | 100   |       |       |
| 127      | 43.4  | 33.3  | 49.9  |
| 141      | 14.3  | 11.4  | 17.0  |



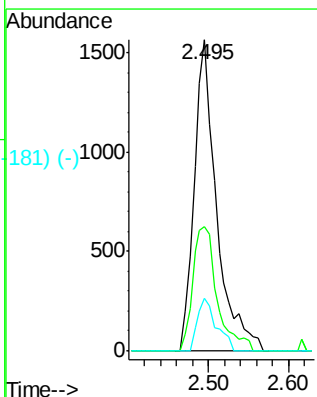





Tert butyl alcohol  
Concen: 3.58 ug/l  
RT: 2.995 min Scan# 313  
Delta R.T. -0.019 min  
Lab File: VX020122.D  
Acq: 18 Dec 2020 13:07




Instrument :  
MSVOA\_X  
ClientSampleId :  
IBLK


Tgt Ion: 59 Resp: 3526  
Ion Ratio Lower Upper  
59 100  
57 0.7 7.8 11.8#

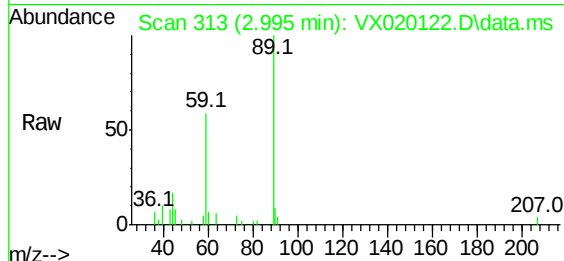

1,1-Dichloroethene  
Concen: 0.28 ug/l  
RT: 2.355 min Scan# 208  
Delta R.T. -0.000 min  
Lab File: VX020122.D  
Acq: 18 Dec 2020 13:07

Tgt Ion: 96 Resp: 926  
Ion Ratio Lower Upper  
96 100  
61 162.3 124.6 187.0  
98 64.8 50.6 76.0


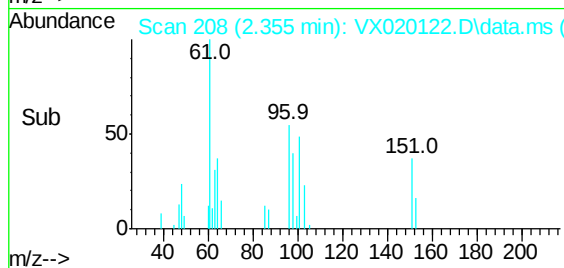




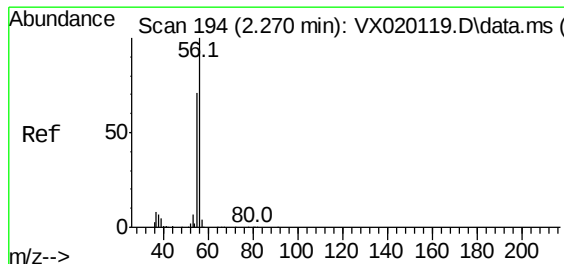

#18 (-)  
Acrolein  
Concen: 1.66 ug/l  
RT: 2.276 min Scan# 195  
Delta R.T. 0.006 min  
Lab File: VX020122.D  
Acq: 18 Dec 2020 13:07




Instrument :  
MSVOA\_X  
ClientSampleId :  
IBLK


Tgt Ion: 56 Resp: 1023  
Ion Ratio Lower Upper  
56 100  
55 90.2 56.4 84.6#

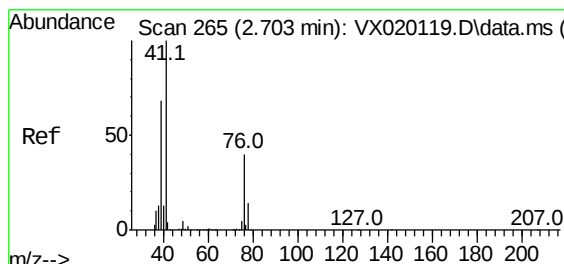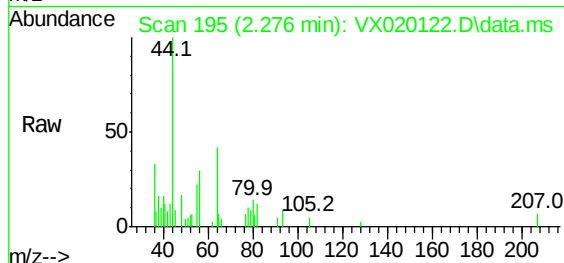

#19 (-)  
Allyl chloride  
Concen: 0.21 ug/l  
RT: 2.708 min Scan# 266  
Delta R.T. 0.005 min  
Lab File: VX020122.D  
Acq: 18 Dec 2020 13:07

Tgt Ion: 41 Resp: 1230  
Ion Ratio Lower Upper  
41 100  
39 61.3 51.6 77.4  
76 0.0 30.5 45.7#


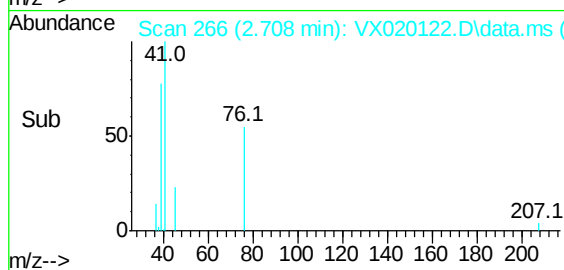




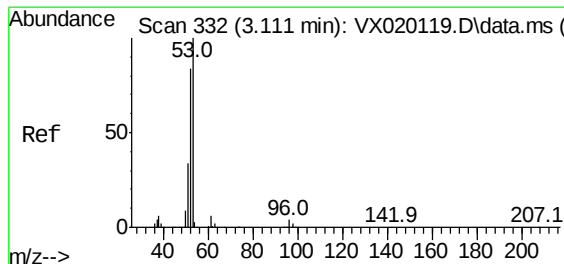

#15 (-)  
Acrylonitrile  
Concen: 1.14 ug/l  
RT: 3.117 min Scan# 333  
Delta R.T. 0.006 min  
Lab File: VX020122.D  
Acq: 18 Dec 2020 13:07




Instrument :  
MSVOA\_X  
ClientSampleId :  
IBLK


Tgt Ion: 53 Resp: 2576  
Ion Ratio Lower Upper  
53 100  
52 84.0 65.3 97.9  
51 35.1 28.2 42.2

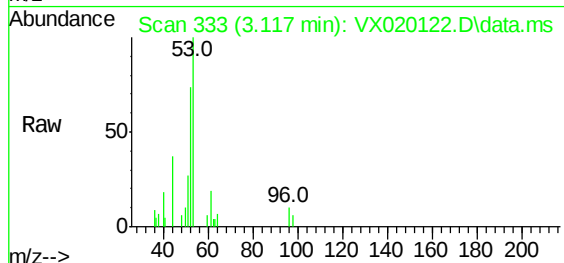

#16 (-)  
Acetone  
Concen: 1.00 ug/l  
RT: 2.416 min Scan# 218  
Delta R.T. -0.000 min  
Lab File: VX020122.D  
Acq: 18 Dec 2020 13:07

Tgt Ion: 43 Resp: 2000  
Ion Ratio Lower Upper  
43 100  
58 39.9 27.8 41.8


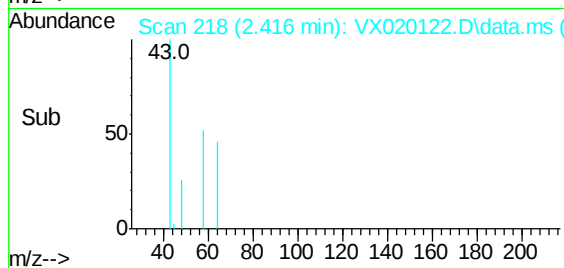




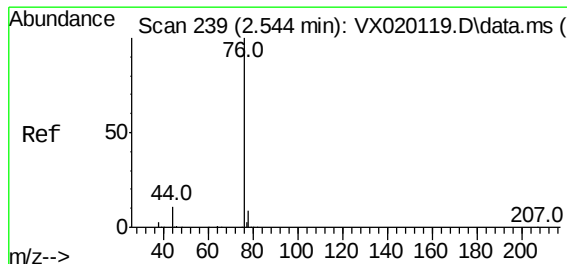

Carbon Disulfide  
Concen: 1.28 ug/l  
RT: 2.550 min Scan# 240  
Delta R.T. 0.006 min  
Lab File: VX020122.D  
Acq: 18 Dec 2020 13:07




Instrument :  
MSVOA\_X  
ClientSampleId :  
IBLK


Tgt Ion: 76 Resp: 12624  
Ion Ratio Lower Upper  
76 100  
78 9.1 7.2 10.8

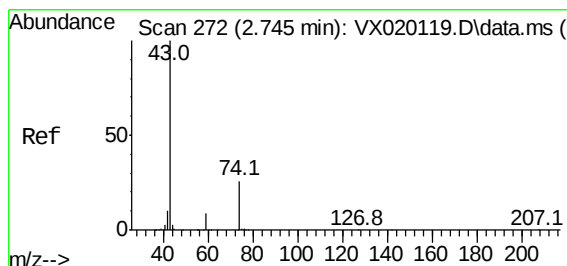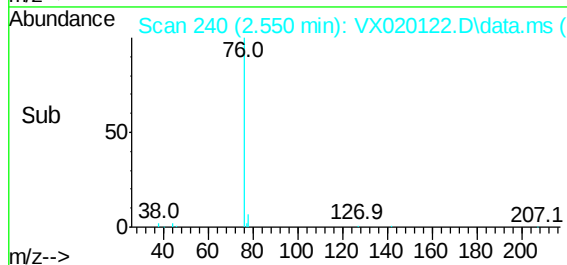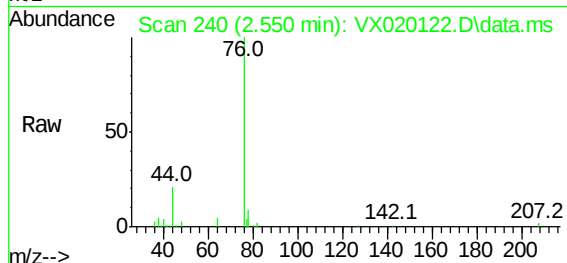

Methyl Acetate  
Concen: 0.29 ug/l  
RT: 2.745 min Scan# 272  
Delta R.T. 0.000 min  
Lab File: VX020122.D  
Acq: 18 Dec 2020 13:07

Tgt Ion: 43 Resp: 1297  
Ion Ratio Lower Upper  
43 100  
74 23.5 21.9 32.9

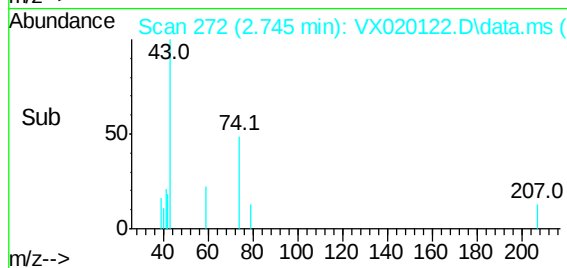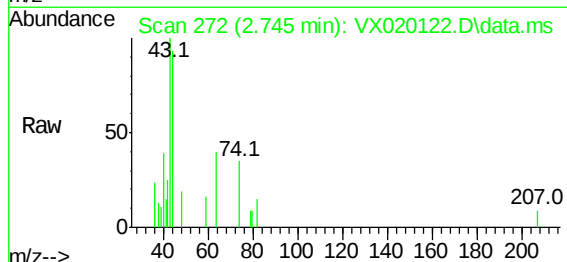




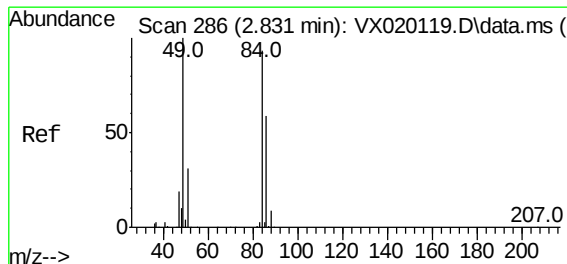


Methylene Chloride  
Concen: 0.30 ug/l  
RT: 2.830 min Scan# 286  
Delta R.T. -0.001 min  
Lab File: VX020122.D  
Acq: 18 Dec 2020 13:07

Instrument :  
MSVOA\_X  
ClientSampleId :  
IBLK

Tgt Ion: 84 Resp: 1341




| Ion | Ratio | Lower | Upper |
|-----|-------|-------|-------|
| 84  | 100   |       |       |
| 49  | 100.9 | 88.6  | 132.8 |
| 51  | 37.0  | 27.0  | 40.6  |
| 86  | 50.9  | 50.3  | 75.5  |

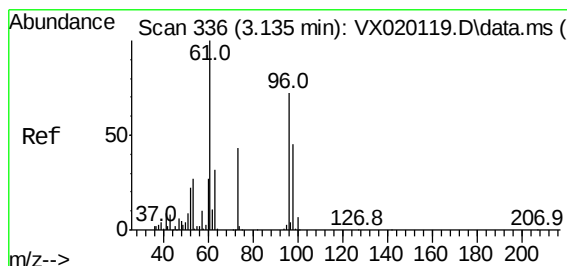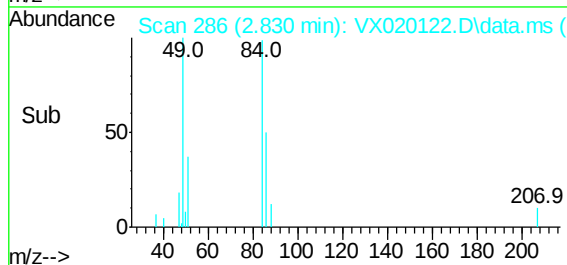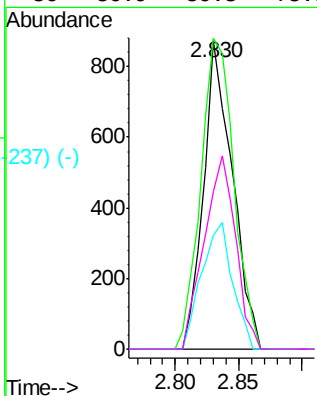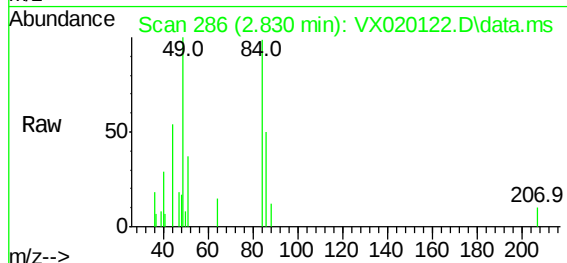


trans-1,2-Dichloroethene  
Concen: 0.51 ug/l  
RT: 3.141 min Scan# 337  
Delta R.T. 0.006 min  
Lab File: VX020122.D  
Acq: 18 Dec 2020 13:07

Tgt Ion: 96 Resp: 2060

| Ion | Ratio | Lower | Upper |
|-----|-------|-------|-------|
| 96  | 100   |       |       |
| 61  | 137.0 | 107.7 | 161.5 |
| 98  | 55.7  | 50.4  | 75.6  |


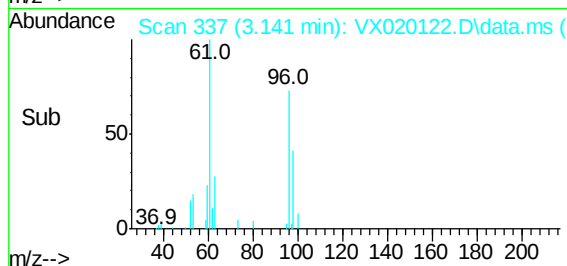
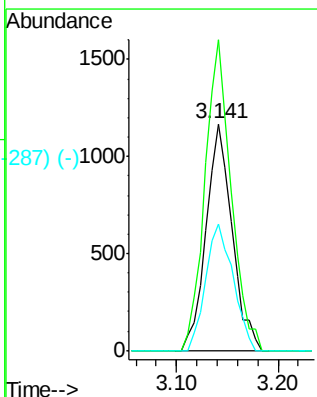
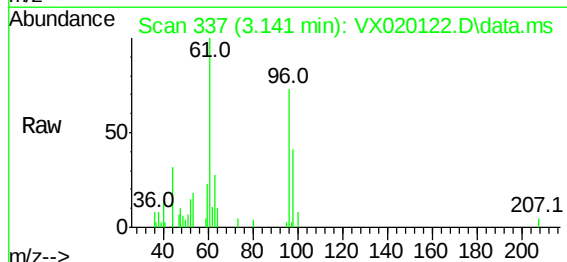


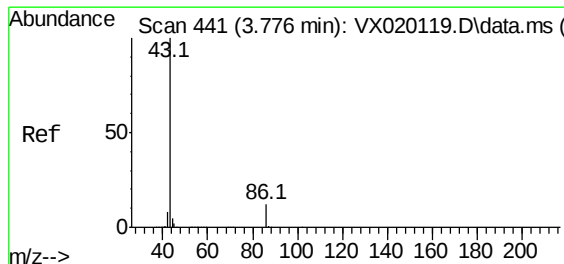

Vinyl Acetate  
Concen: 0.31 ug/l  
RT: 3.781 min Scan# 442  
Delta R.T. 0.005 min  
Lab File: VX020122.D  
Acq: 18 Dec 2020 13:07




Instrument :  
MSVOA\_X  
ClientSampleId :  
IBLK


Tgt Ion: 43 Resp: 3233  
Ion Ratio Lower Upper  
43 100  
86 10.0 9.9 14.9

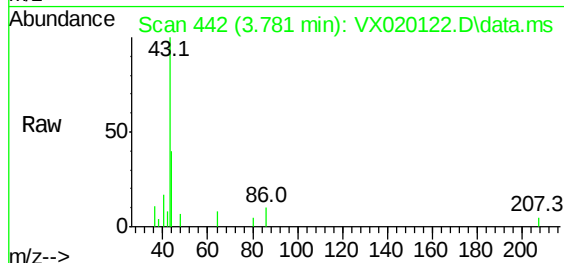

2-Butanone  
Concen: 0.47 ug/l  
RT: 4.647 min Scan# 584  
Delta R.T. 0.024 min  
Lab File: VX020122.D  
Acq: 18 Dec 2020 13:07

Tgt Ion: 43 Resp: 1366  
Ion Ratio Lower Upper  
43 100  
72 24.8 23.7 35.5


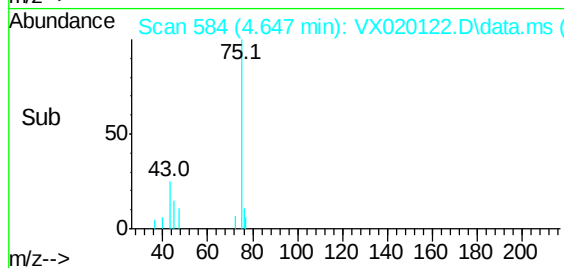




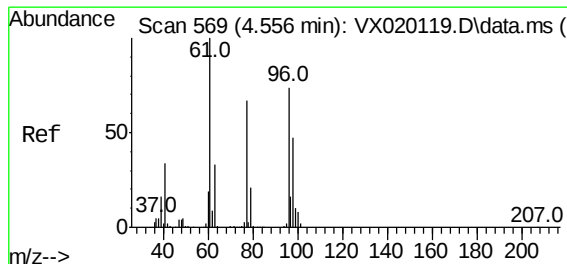

cis-1,2-Dichloroethene  
 Concen: 0.26 ug/l  
 RT: 4.562 min Scan# 570  
 Delta R.T. 0.006 min  
 Lab File: VX020122.D  
 Acq: 18 Dec 2020 13:07




Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 IBLK


|          |       |       |       |
|----------|-------|-------|-------|
| Tgt Ion: | 96    | Resp: | 1209  |
| Ion      | Ratio | Lower | Upper |
| 96       | 100   |       |       |
| 61       | 159.6 | 0.0   | 285.6 |
| 98       | 58.5  | 0.0   | 129.6 |

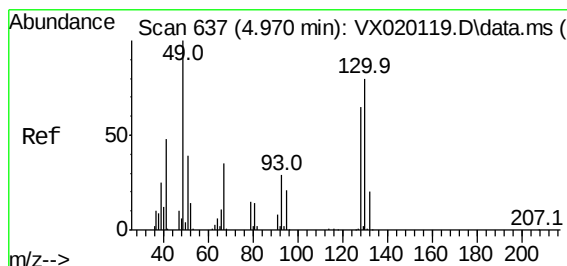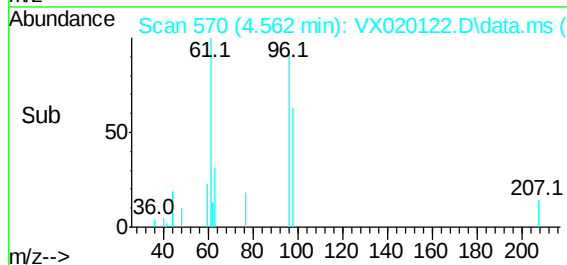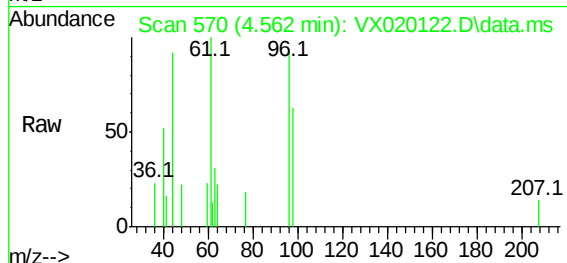

Bromochloromethane  
 Concen: 0.22 ug/l  
 RT: 4.982 min Scan# 639  
 Delta R.T. 0.012 min  
 Lab File: VX020122.D  
 Acq: 18 Dec 2020 13:07

|          |       |       |       |
|----------|-------|-------|-------|
| Tgt Ion: | 49    | Resp: | 700   |
| Ion      | Ratio | Lower | Upper |
| 49       | 100   |       |       |
| 129      | 0.0   | 0.0   | 4.0   |
| 130      | 74.0  | 68.2  | 102.2 |


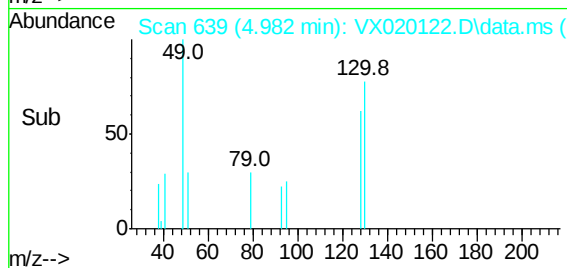

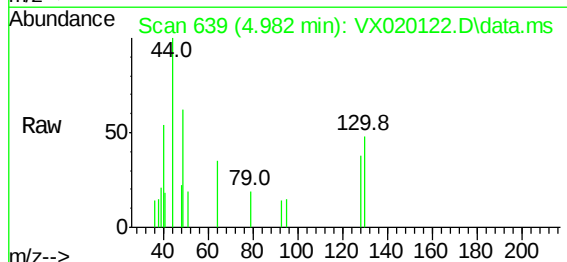


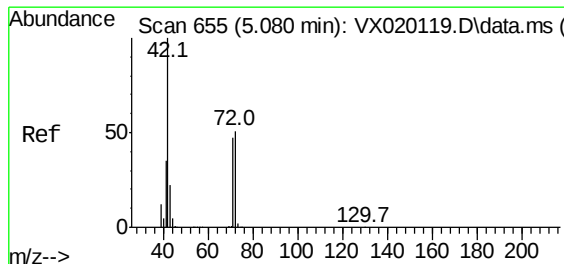

Tetrahydrofuran  
Concen: 0.67 ug/l  
RT: 5.117 min Scan# 661  
Delta R.T. 0.037 min  
Lab File: VX020122.D  
Acq: 18 Dec 2020 13:07




Instrument :  
MSVOA\_X  
ClientSampleId :  
IBLK


Tgt Ion: 42 Resp: 1223  
Ion Ratio Lower Upper  
42 100  
72 20.9 41.7 62.5#  
71 41.4 38.4 57.6

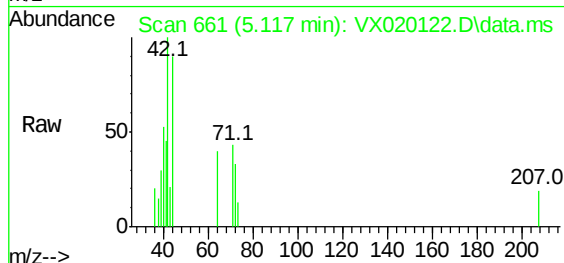

1,2-Dichloroethane-d4  
Concen: 45.76 ug/l  
RT: 6.031 min Scan# 811  
Delta R.T. 0.006 min  
Lab File: VX020122.D  
Acq: 18 Dec 2020 13:07

Tgt Ion: 65 Resp: 201228  
Ion Ratio Lower Upper  
65 100  
67 53.0 0.0 105.4


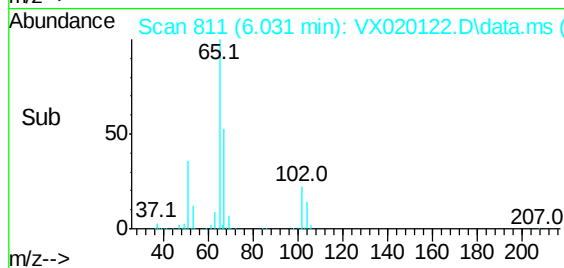




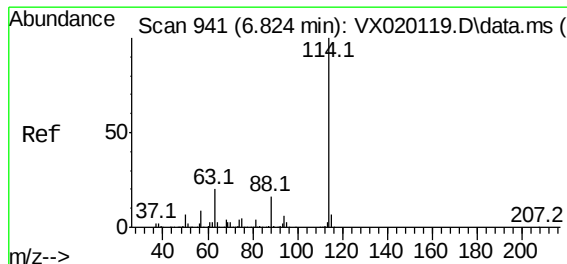

1,4-Difluorobenzene  
Concen: 50.00 ug/l  
RT: 6.830 min Scan# 942  
Delta R.T. 0.006 min  
Lab File: VX020122.D  
Acq: 18 Dec 2020 13:07




Instrument :  
MSVOA\_X  
ClientSampleId :  
IBLK


Tgt Ion:114 Resp: 536515  
Ion Ratio Lower Upper  
114 100  
63 20.7 0.0 40.8  
88 16.1 0.0 32.8

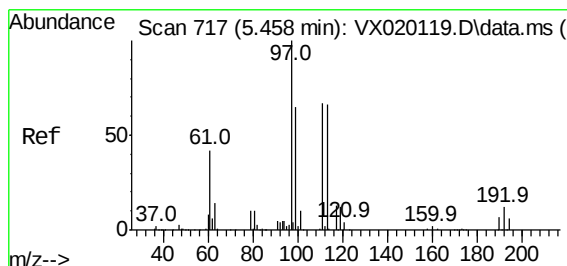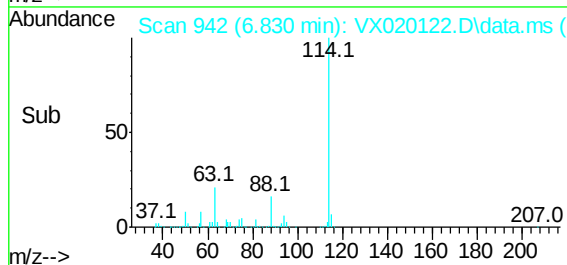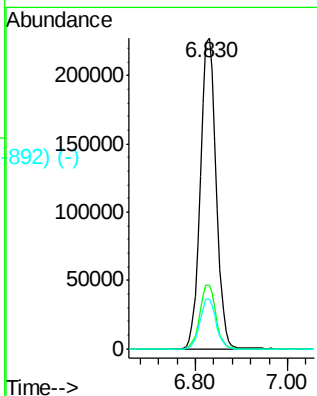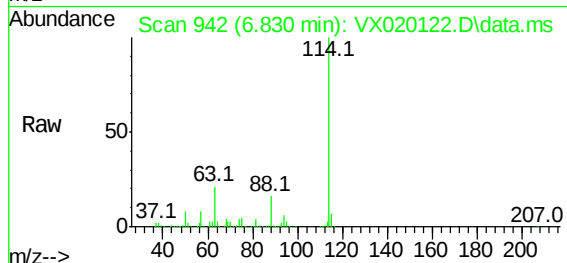

Dibromofluoromethane  
Concen: 47.21 ug/l  
RT: 5.458 min Scan# 717  
Delta R.T. -0.000 min  
Lab File: VX020122.D  
Acq: 18 Dec 2020 13:07

Tgt Ion:113 Resp: 162016  
Ion Ratio Lower Upper  
113 100  
111 103.4 81.9 122.9  
192 20.7 16.7 25.1


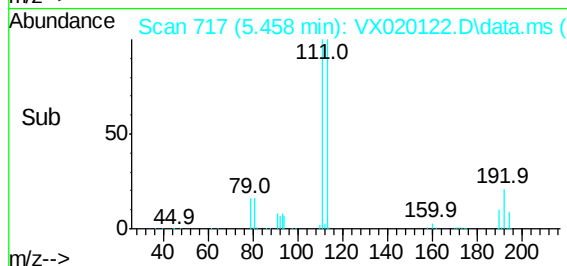
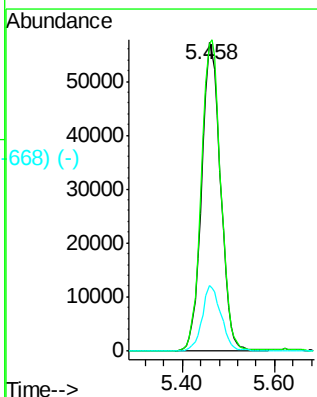
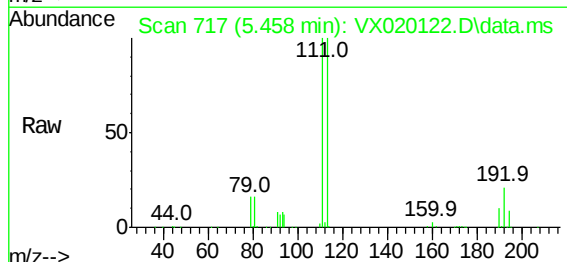


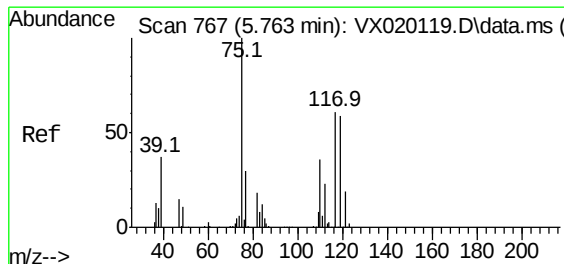

1,1-Dichloropropene  
Concen: 0.37 ug/l  
RT: 5.763 min Scan# 767  
Delta R.T. -0.000 min  
Lab File: VX020122.D  
Acq: 18 Dec 2020 13:07




Instrument :  
MSVOA\_X  
ClientSampleId :  
IBLK


|          |       |       |       |
|----------|-------|-------|-------|
| Tgt Ion: | 75    | Resp: | 1961  |
| Ion      | Ratio | Lower | Upper |
| 75       | 100   |       |       |
| 110      | 31.7  | 18.1  | 54.4  |
| 77       | 29.5  | 25.3  | 37.9  |

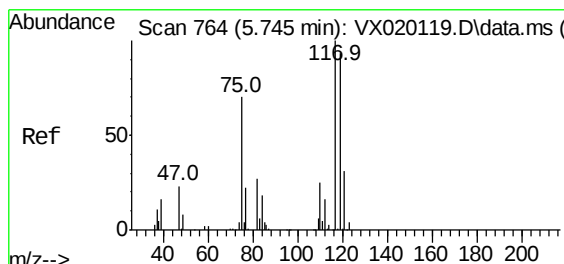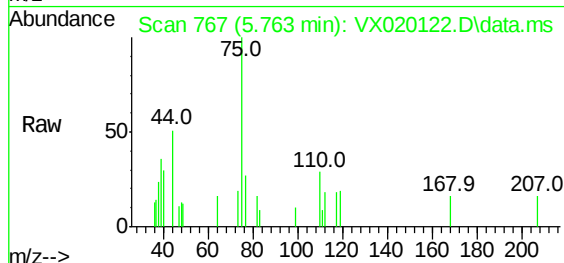

Carbon Tetrachloride  
Concen: 6.30 ug/l  
RT: 5.623 min Scan# 744  
Delta R.T. -0.122 min  
Lab File: VX020122.D  
Acq: 18 Dec 2020 13:07

|          |       |       |        |
|----------|-------|-------|--------|
| Tgt Ion: | 117   | Resp: | 31775  |
| Ion      | Ratio | Lower | Upper  |
| 117      | 100   |       |        |
| 119      | 5.6   | 76.2  | 114.2# |
| 121      | 0.0   | 24.8  | 37.2#  |


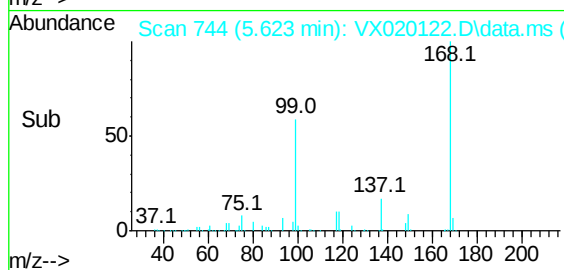




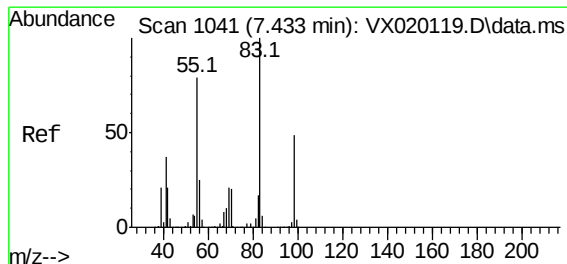

#829 (-)  
Methylcyclohexane  
Concen: 0.35 ug/l  
RT: 7.439 min Scan# 1042  
Delta R.T. 0.006 min  
Lab File: VX020122.D  
Acq: 18 Dec 2020 13:07




Instrument :  
MSVOA\_X  
ClientSampleId :  
IBLK


Tgt Ion: 83 Resp: 2139  
Ion Ratio Lower Upper  
83 100  
55 79.1 58.9 88.3  
98 44.1 38.1 57.1

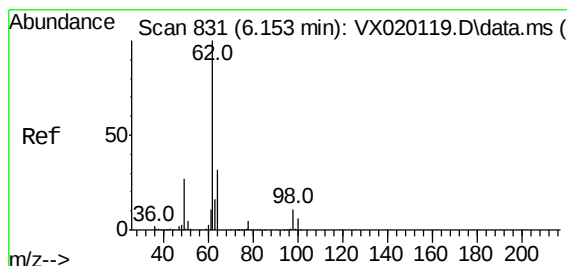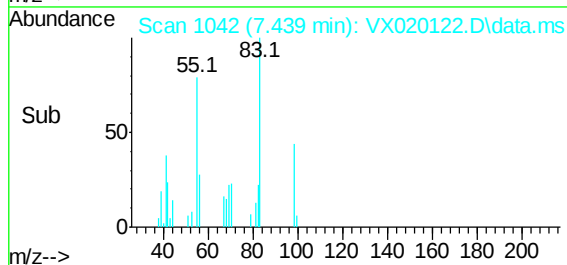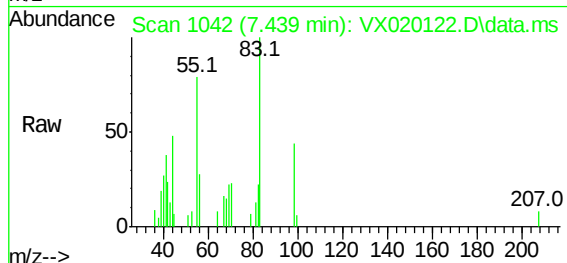

#832 (-)  
1,2-Dichloroethane  
Concen: 0.21 ug/l  
RT: 6.165 min Scan# 833  
Delta R.T. 0.012 min  
Lab File: VX020122.D  
Acq: 18 Dec 2020 13:07

Tgt Ion: 62 Resp: 1171  
Ion Ratio Lower Upper  
62 100  
98 4.1 0.0 20.2

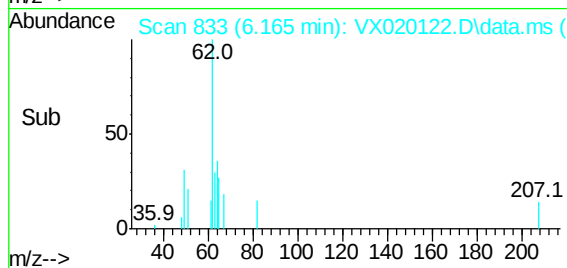

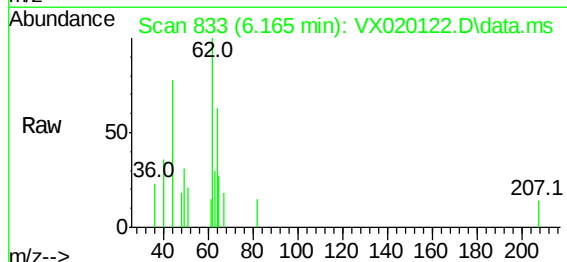





(-969) (-)  
 Trichloroethene  
 Concen: 0.34 ug/l  
 RT: 7.183 min Scan# 1000  
 Delta R.T. -0.001 min  
 Lab File: VX020122.D  
 Acq: 18 Dec 2020 13:07

Instrument :  
 MSVOA\_X  
 ClientSampled :  
 IBLK

Tgt Ion:130 Resp: 1467  
 Ion Ratio Lower Upper  
 130 100  
 95 96.3 0.0 198.0



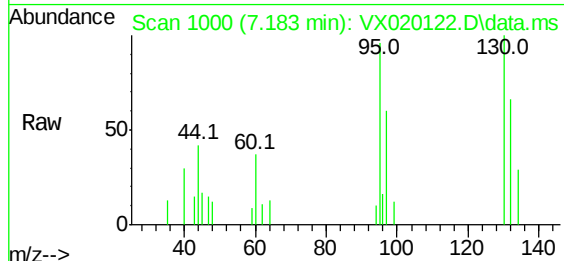


(-951) (-)




(-1064) (-)  
 Dibromomethane  
 Concen: 0.24 ug/l  
 RT: 7.634 min Scan# 1074  
 Delta R.T. -0.001 min  
 Lab File: VX020122.D  
 Acq: 18 Dec 2020 13:07

Tgt Ion: 93 Resp: 696  
 Ion Ratio Lower Upper  
 93 100  
 95 86.5 66.8 100.2  
 174 98.0 83.1 124.7

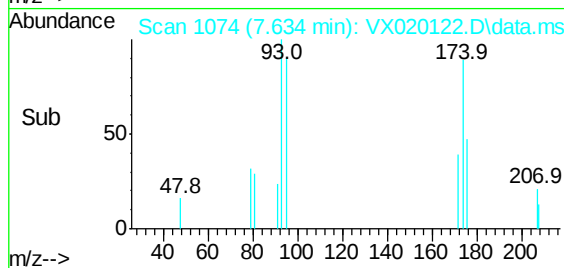

(-1025) (-)




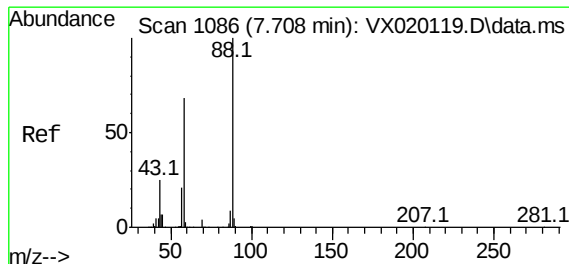


(-1099) (-)  
 1,4-Dioxane  
 Concen: 2.22 ug/l  
 RT: 7.720 min Scan# 1088  
 Delta R.T. 0.012 min  
 Lab File: VX020122.D  
 Acq: 18 Dec 2020 13:07

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 IBLK

Tgt Ion: 88 Resp: 222




| Ion | Ratio | Lower | Upper |
|-----|-------|-------|-------|
| 88  | 100   |       |       |
| 43  | 64.4  | 23.2  | 34.8  |
| 58  | 64.9  | 55.0  | 82.4  |

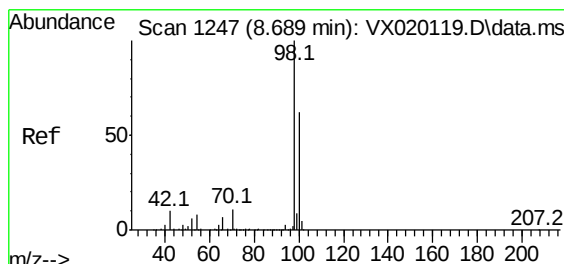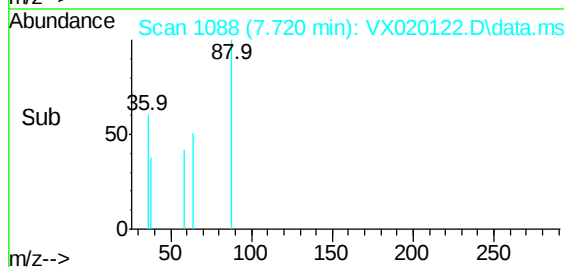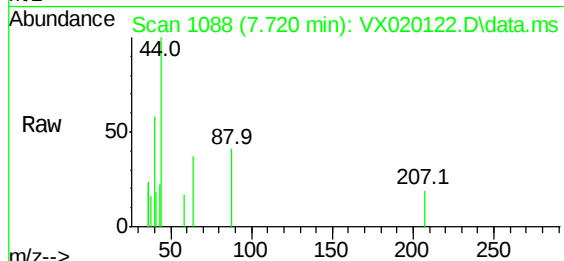


(-1299) (-)  
 Toluene-d8  
 Concen: 48.38 ug/l  
 RT: 8.695 min Scan# 1248  
 Delta R.T. 0.006 min  
 Lab File: VX020122.D  
 Acq: 18 Dec 2020 13:07

Tgt Ion: 98 Resp: 639137

| Ion | Ratio | Lower | Upper |
|-----|-------|-------|-------|
| 98  | 100   |       |       |
| 100 | 65.7  | 51.9  | 77.9  |


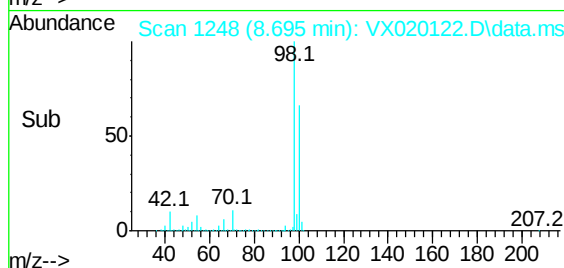




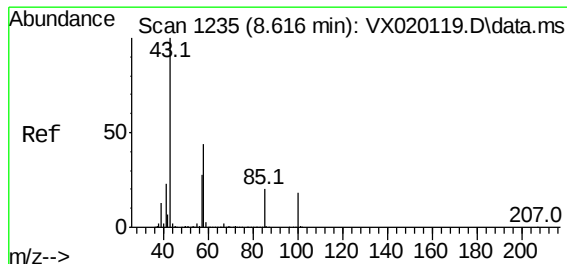

#516 (-)  
4-Methyl-2-Pentanone  
Concen: 0.22 ug/l  
RT: 8.622 min Scan# 1236  
Delta R.T. 0.006 min  
Lab File: VX020122.D  
Acq: 18 Dec 2020 13:07




Instrument :  
MSVOA\_X  
ClientSampled :  
IBLK


Tgt Ion: 43 Resp: 1198  
Ion Ratio Lower Upper  
43 100  
58 33.1 35.4 53.0#

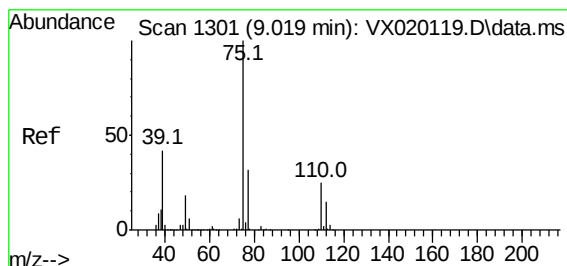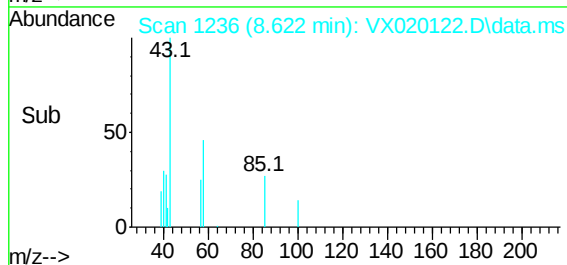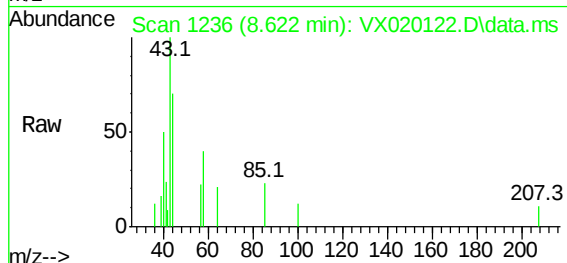

#518 (-)  
t-1,3-Dichloropropene  
Concen: 0.21 ug/l  
RT: 9.018 min Scan# 1301  
Delta R.T. -0.001 min  
Lab File: VX020122.D  
Acq: 18 Dec 2020 13:07

Tgt Ion: 75 Resp: 1286  
Ion Ratio Lower Upper  
75 100  
77 36.2 24.9 37.3


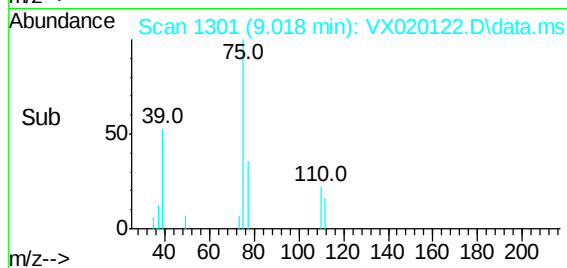

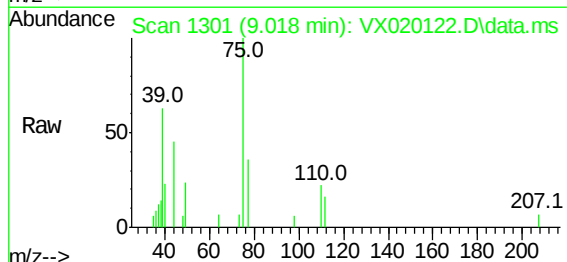


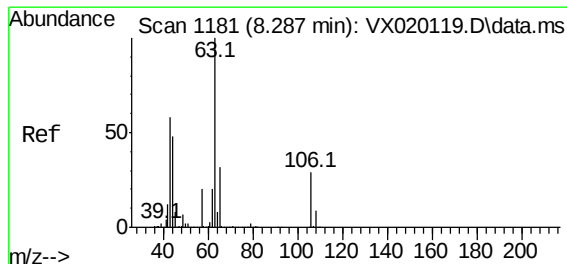

(-158) (-)  
2-Chloroethyl vinyl ether  
Concen: 0.34 ug/l  
RT: 8.287 min Scan# 1181  
Delta R.T. -0.000 min  
Lab File: VX020122.D  
Acq: 18 Dec 2020 13:07




Instrument :  
MSVOA\_X  
ClientSampled :  
IBLK


Tgt Ion: 63 Resp: 1079  
Ion Ratio Lower Upper  
63 100  
106 28.5 23.5 35.3

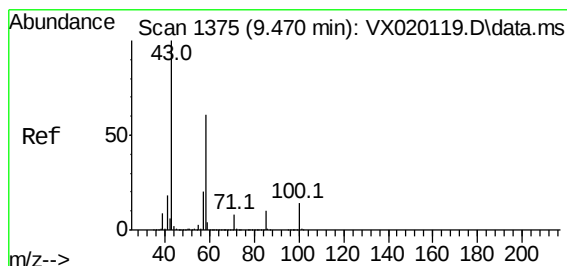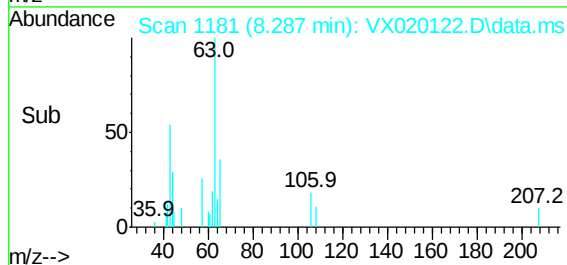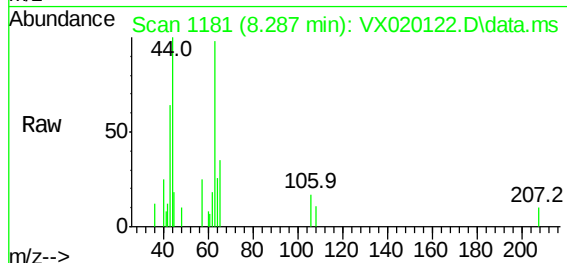

(-156) (-)  
2-Hexanone  
Concen: 0.30 ug/l  
RT: 9.469 min Scan# 1375  
Delta R.T. -0.001 min  
Lab File: VX020122.D  
Acq: 18 Dec 2020 13:07

Tgt Ion: 43 Resp: 1246  
Ion Ratio Lower Upper  
43 100  
58 44.1 30.9 92.8


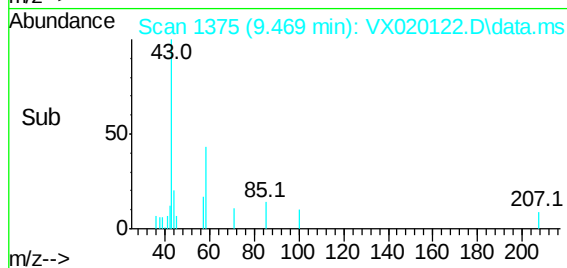

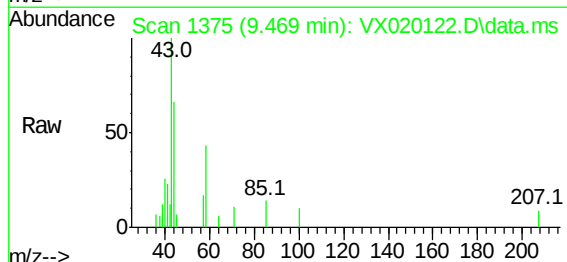




#639 (-)  
4-Bromofluorobenzene  
Concen: 45.15 ug/l  
RT: 11.122 min Scan# 1646  
Delta R.T. -0.000 min  
Lab File: VX020122.D  
Acq: 18 Dec 2020 13:07




Instrument :  
MSVOA\_X  
ClientSampleId :  
IBLK


|           |       |       |        |
|-----------|-------|-------|--------|
| Tgt Ion:  | 95    | Resp: | 228272 |
| Ion Ratio | Lower | Upper |        |
| 95        | 100   |       |        |
| 174       | 77.6  | 0.0   | 154.6  |
| 176       | 74.6  | 0.0   | 155.8  |

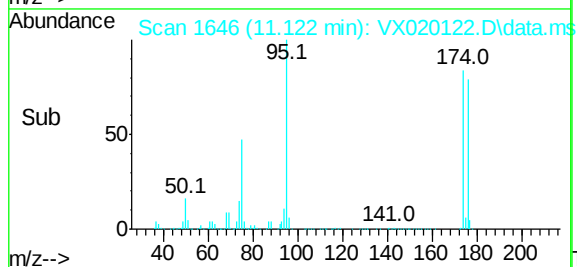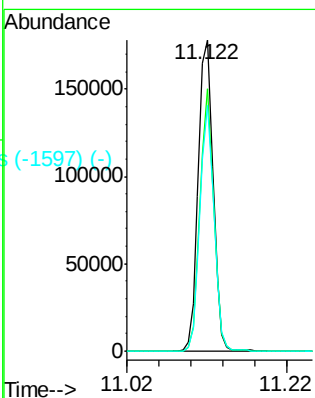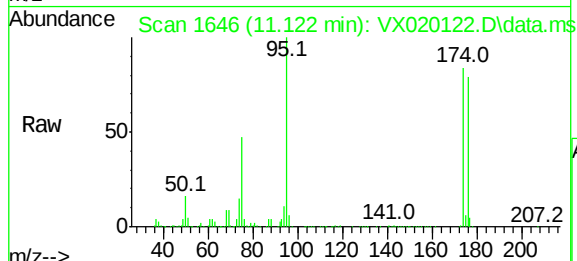

#640 (-)  
Chlorobenzene-d5  
Concen: 50.00 ug/l  
RT: 10.097 min Scan# 1478  
Delta R.T. 0.005 min  
Lab File: VX020122.D  
Acq: 18 Dec 2020 13:07

|           |       |       |        |
|-----------|-------|-------|--------|
| Tgt Ion:  | 117   | Resp: | 486388 |
| Ion Ratio | Lower | Upper |        |
| 117       | 100   |       |        |
| 82        | 54.1  | 47.4  | 71.2   |
| 119       | 31.8  | 26.6  | 39.8   |

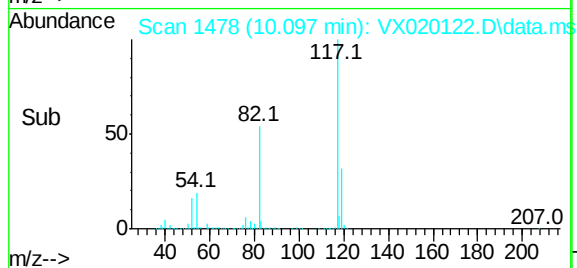
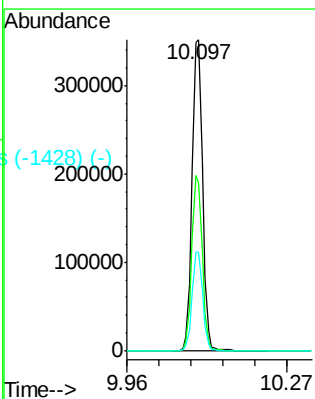



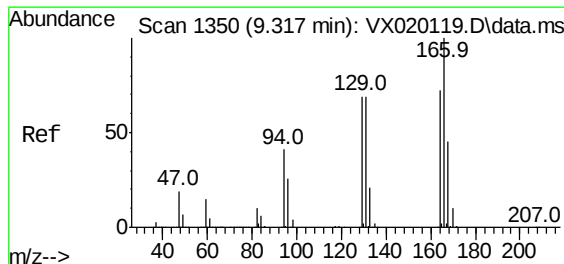


#642 (-)  
Tetrachloroethene  
Concen: 0.35 ug/l  
RT: 9.317 min Scan# 1350  
Delta R.T. 0.000 min  
Lab File: VX020122.D  
Acq: 18 Dec 2020 13:07

Instrument :  
MSVOA\_X  
ClientSampleId :  
IBLK

|           |       |       |       |
|-----------|-------|-------|-------|
| Tgt Ion:  | 164   | Resp: | 1281  |
| Ion Ratio | Lower | Upper |       |
| 164       | 100   |       |       |
| 166       | 126.8 | 103.4 | 155.2 |
| 129       | 99.4  | 70.8  | 106.2 |
| 131       | 91.0  | 72.5  | 108.7 |


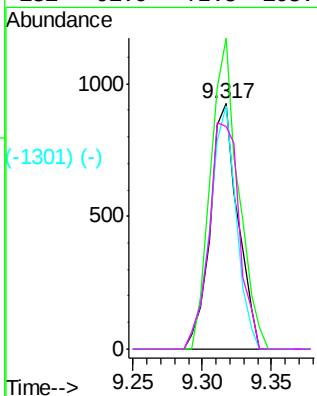
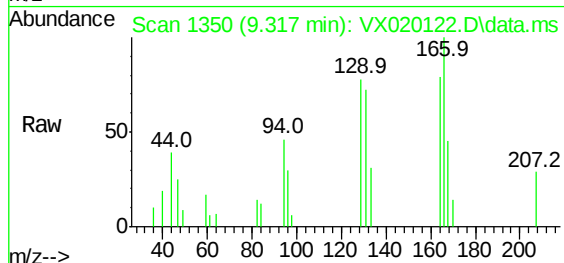


#1301 (-)




#654 (-)  
Chlorobenzene  
Concen: 0.21 ug/l  
RT: 10.122 min Scan# 1482  
Delta R.T. 0.006 min  
Lab File: VX020122.D  
Acq: 18 Dec 2020 13:07

|           |       |       |      |
|-----------|-------|-------|------|
| Tgt Ion:  | 112   | Resp: | 2156 |
| Ion Ratio | Lower | Upper |      |
| 112       | 100   |       |      |
| 114       | 31.0  | 25.8  | 38.6 |

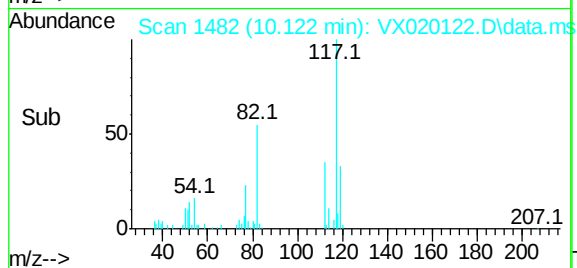





#1432 (-)



#6911 (-)  
m/p-Xylenes  
Concen: 0.37 ug/l  
RT: 10.341 min Scan# 1518  
Delta R.T. 0.000 min  
Lab File: VX020122.D  
Acq: 18 Dec 2020 13:07




Instrument :  
MSVOA\_X  
ClientSampleId :  
IBLK


Tgt Ion:106 Resp: 2529  
Ion Ratio Lower Upper  
106 100  
91 198.4 162.8 244.2

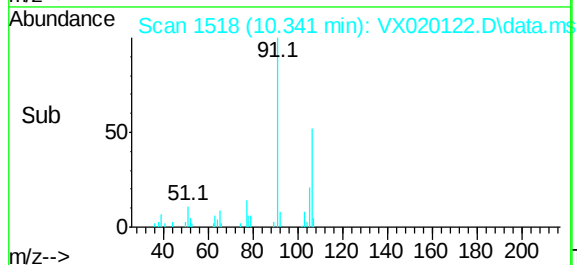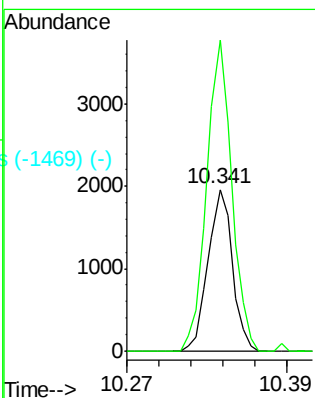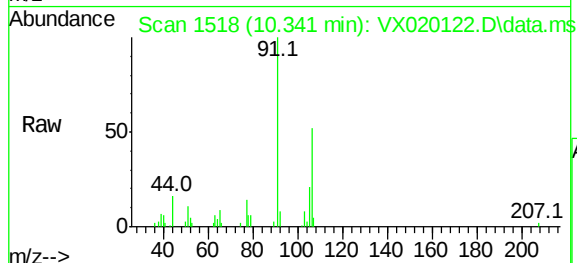

#7294 (-)  
1,4-Dichlorobenzene-d4  
Concen: 50.00 ug/l  
RT: 12.060 min Scan# 1800  
Delta R.T. -0.001 min  
Lab File: VX020122.D  
Acq: 18 Dec 2020 13:07


Tgt Ion:152 Resp: 212581  
Ion Ratio Lower Upper  
152 100  
115 60.4 41.1 123.3  
150 155.2 0.0 349.0

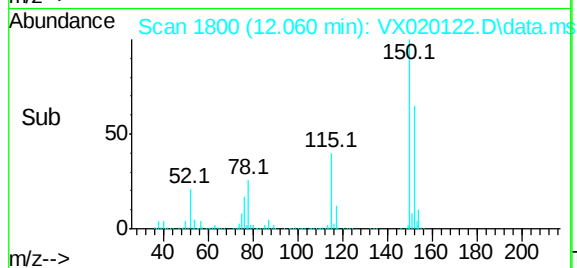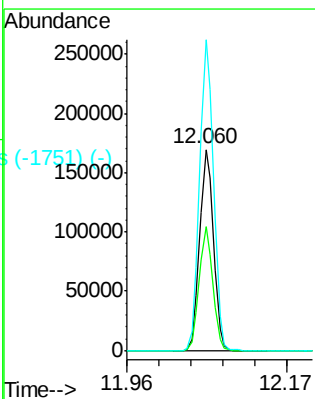






#1667 (-)  
 1,2,3-Trichloropropane  
 Concen: 21.08 ug/l  
 RT: 11.116 min Scan# 1645  
 Delta R.T. -0.164 min  
 Lab File: VX020122.D  
 Acq: 18 Dec 2020 13:07


Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 IBLK

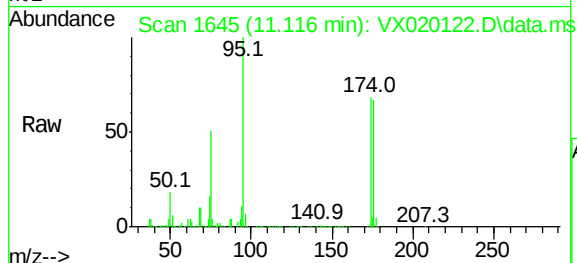



Tgt Ion: 75 Resp: 110370  
 Ion Ratio Lower Upper  
 75 100  
 77 1.2 19.1 57.5#

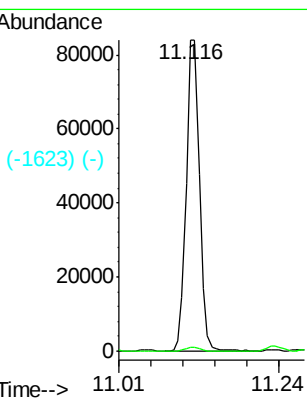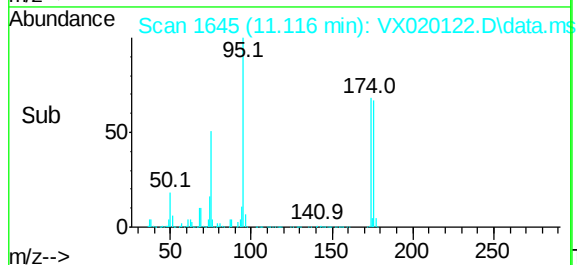


#1668 (-)  
 Bromobenzene  
 Concen: 0.27 ug/l  
 RT: 11.237 min Scan# 1665  
 Delta R.T. -0.001 min  
 Lab File: VX020122.D  
 Acq: 18 Dec 2020 13:07



Tgt Ion: 156 Resp: 1091  
 Ion Ratio Lower Upper  
 156 100  
 77 173.8 82.8 248.6  
 158 97.3 49.1 147.4



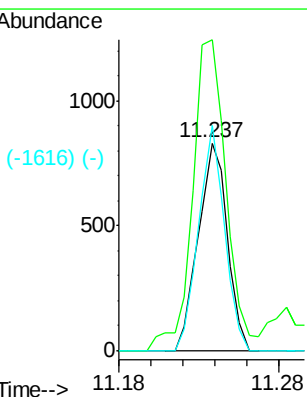





#1677 (-)  
n-propylbenzene  
Concen: 0.30 ug/l  
RT: 11.341 min Scan# 1682  
Delta R.T. 0.000 min  
Lab File: VX020122.D  
Acq: 18 Dec 2020 13:07




Instrument :  
MSVOA\_X  
ClientSampleId :  
IBLK


Tgt Ion: 91 Resp: 5305  
Ion Ratio Lower Upper  
91 100  
120 21.6 11.5 34.5

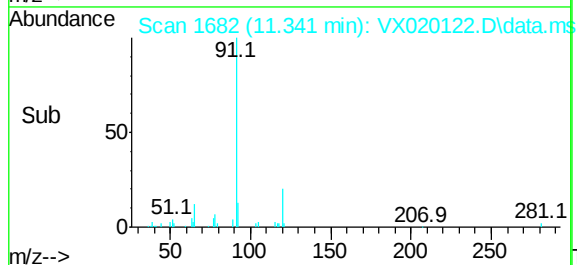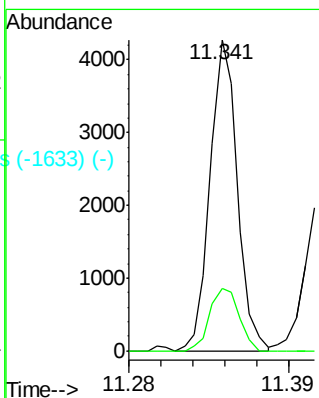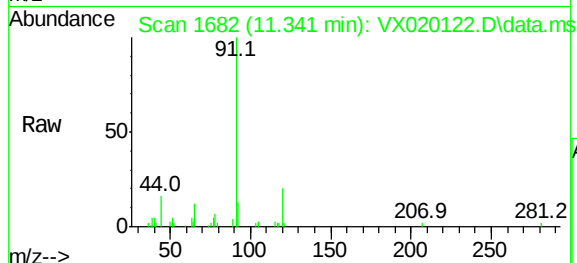

#1687 (-)  
2-Chlorotoluene  
Concen: 0.23 ug/l  
RT: 11.402 min Scan# 1692  
Delta R.T. 0.000 min  
Lab File: VX020122.D  
Acq: 18 Dec 2020 13:07

Tgt Ion: 91 Resp: 2517  
Ion Ratio Lower Upper  
91 100  
126 35.8 16.6 49.8


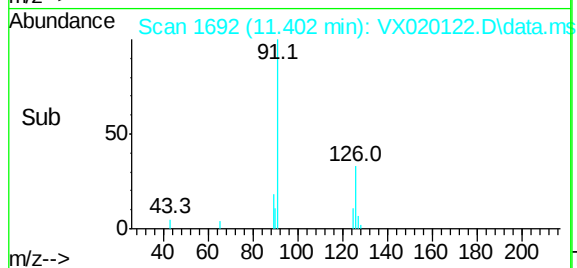
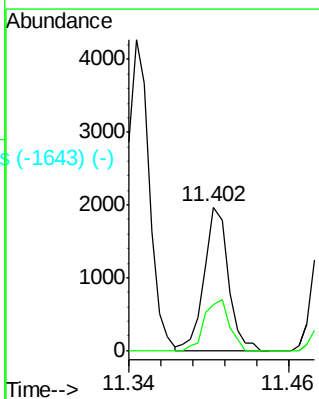





1,3,5-Trimethylbenzene  
 Concen: 0.21 ug/l  
 RT: 11.487 min Scan# 1706  
 Delta R.T. -0.001 min  
 Lab File: VX020122.D  
 Acq: 18 Dec 2020 13:07




Instrument :  
 MSVOA\_X  
 ClientSampleID :  
 IBLK


|           |       |       |      |
|-----------|-------|-------|------|
| Tgt Ion:  | 105   | Resp: | 2788 |
| Ion Ratio | Lower | Upper |      |
| 105       | 100   |       |      |
| 120       | 46.2  | 23.8  | 71.5 |

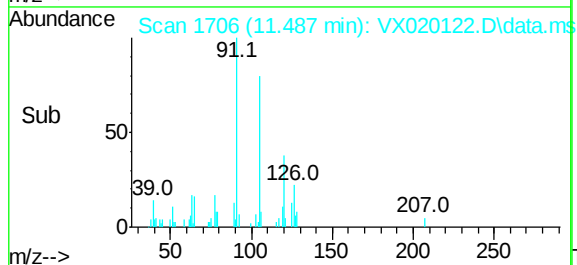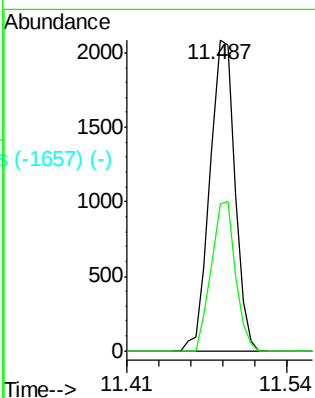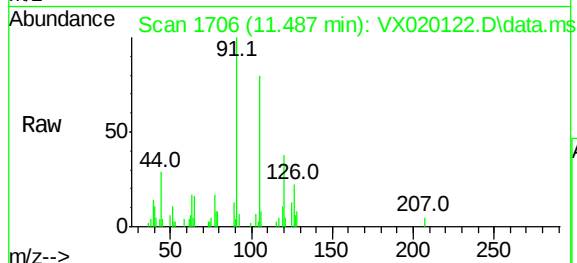

trans-1,4-Dichloro-2-butene  
 Concen: 62.53 ug/l  
 RT: 11.116 min Scan# 1645  
 Delta R.T. 0.061 min  
 Lab File: VX020122.D  
 Acq: 18 Dec 2020 13:07

|           |       |       |        |
|-----------|-------|-------|--------|
| Tgt Ion:  | 75    | Resp: | 110370 |
| Ion Ratio | Lower | Upper |        |
| 75        | 100   |       |        |
| 53        | 0.1   | 74.5  | 111.7# |
| 89        | 0.0   | 37.9  | 56.9#  |


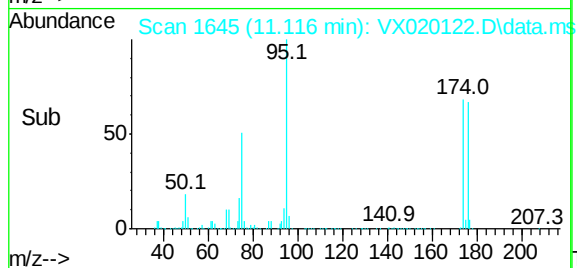
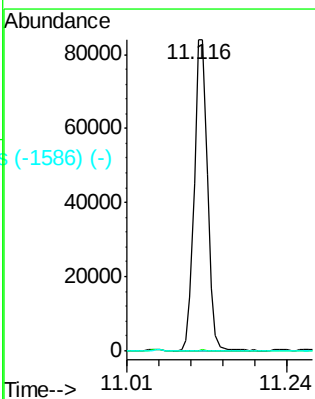





#889 (-)  
4-Chlorotoluene  
Concen: 0.35 ug/l  
RT: 11.493 min Scan# 1707  
Delta R.T. -0.001 min  
Lab File: VX020122.D  
Acq: 18 Dec 2020 13:07




Instrument :  
MSVOA\_X  
ClientSampleId :  
IBLK


|           |       |       |      |
|-----------|-------|-------|------|
| Tgt Ion:  | 91    | Resp: | 4562 |
| Ion Ratio | Lower | Upper |      |
| 91        | 100   |       |      |
| 126       | 29.2  | 14.9  | 44.5 |

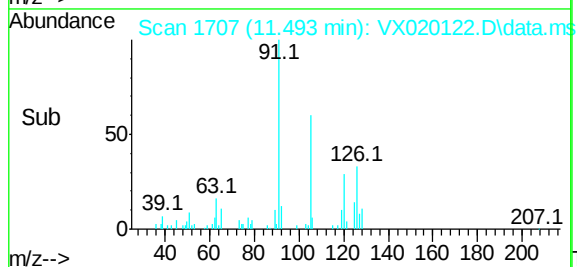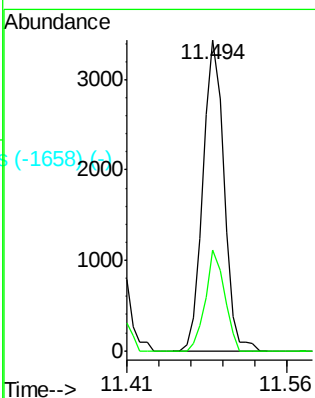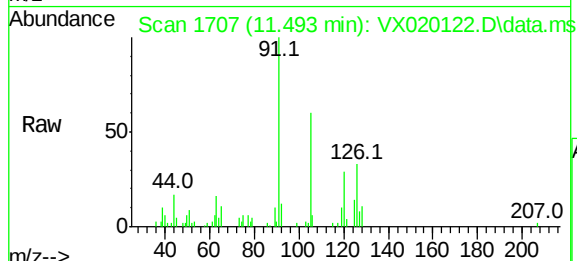

#8745 (-)  
1,2,4-Trimethylbenzene  
Concen: 0.23 ug/l  
RT: 11.792 min Scan# 1756  
Delta R.T. 0.000 min  
Lab File: VX020122.D  
Acq: 18 Dec 2020 13:07

|           |       |       |      |
|-----------|-------|-------|------|
| Tgt Ion:  | 105   | Resp: | 3014 |
| Ion Ratio | Lower | Upper |      |
| 105       | 100   |       |      |
| 120       | 43.4  | 22.4  | 67.3 |


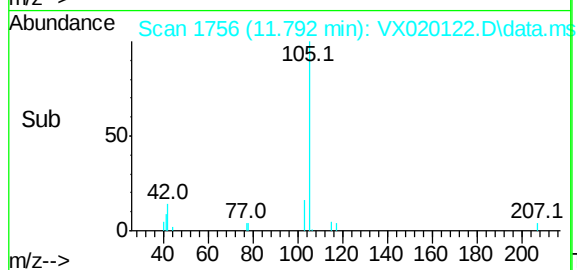
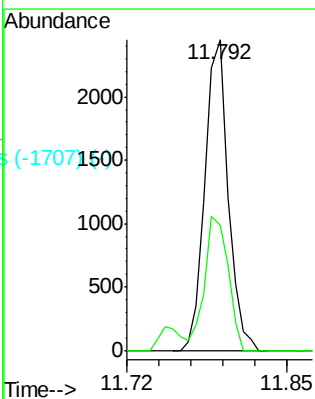





sec-Butylbenzene  
Concen: 0.31 ug/l  
RT: 11.932 min Scan# 1779  
Delta R.T. 0.005 min  
Lab File: VX020122.D  
Acq: 18 Dec 2020 13:07




Instrument :  
MSVOA\_X  
ClientSampleId :  
IBLK


Tgt Ion:105 Resp: 4402  
Ion Ratio Lower Upper  
105 100  
134 18.8 10.0 29.8

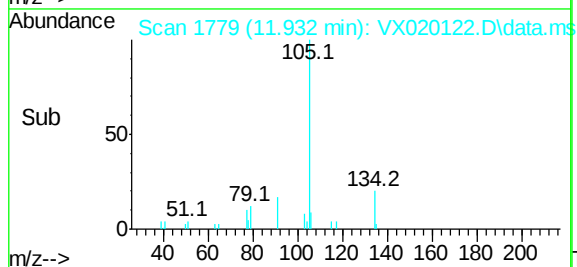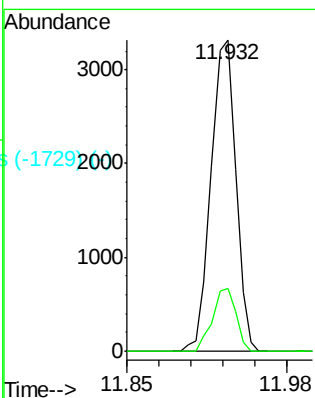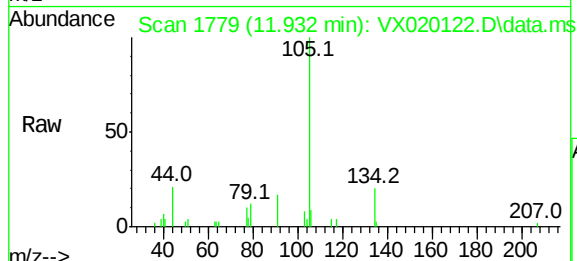

p-Isopropyltoluene  
Concen: 0.31 ug/l  
RT: 12.048 min Scan# 1798  
Delta R.T. 0.000 min  
Lab File: VX020122.D  
Acq: 18 Dec 2020 13:07

Tgt Ion:119 Resp: 4166  
Ion Ratio Lower Upper  
119 100  
134 29.5 12.9 38.7  
91 39.0 11.7 35.0#


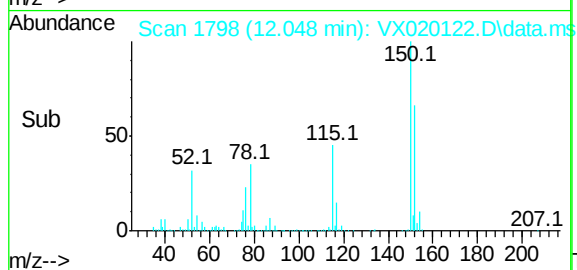
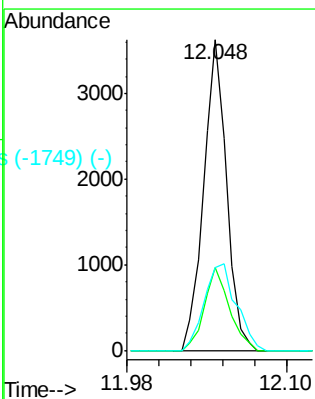





Scan 1791 (12.006 min): VX020119.D\data.ms (#8785) (-)  
 1,3-Dichlorobenzene  
 Concen: 0.45 ug/l  
 RT: 12.006 min Scan# 1791  
 Delta R.T. -0.000 min  
 Lab File: VX020122.D  
 Acq: 18 Dec 2020 13:07




Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 IBLK


|           |       |       |      |
|-----------|-------|-------|------|
| Tgt Ion:  | 146   | Resp: | 3267 |
| Ion Ratio | Lower | Upper |      |
| 146       | 100   |       |      |
| 111       | 46.9  | 20.2  | 60.5 |
| 148       | 66.7  | 31.9  | 95.7 |

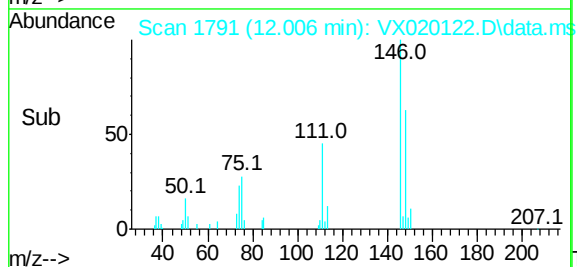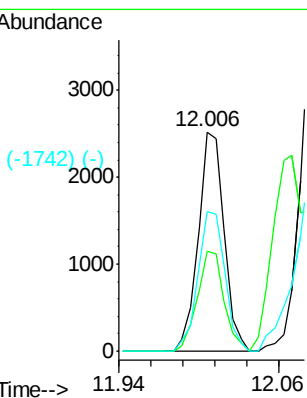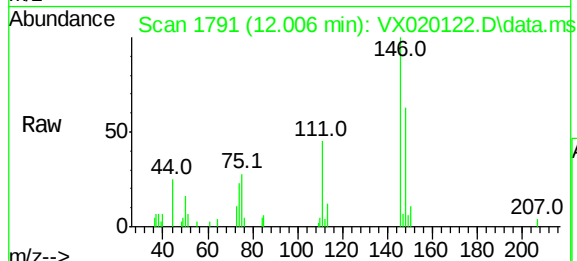

Scan 1803 (12.079 min): VX020119.D\data.ms (#8788) (-)  
 1,4-Dichlorobenzene  
 Concen: 0.43 ug/l  
 RT: 12.006 min Scan# 1791  
 Delta R.T. -0.073 min  
 Lab File: VX020122.D  
 Acq: 18 Dec 2020 13:07

|           |       |       |      |
|-----------|-------|-------|------|
| Tgt Ion:  | 146   | Resp: | 3267 |
| Ion Ratio | Lower | Upper |      |
| 146       | 100   |       |      |
| 111       | 46.9  | 19.6  | 58.8 |
| 148       | 66.7  | 31.6  | 95.0 |


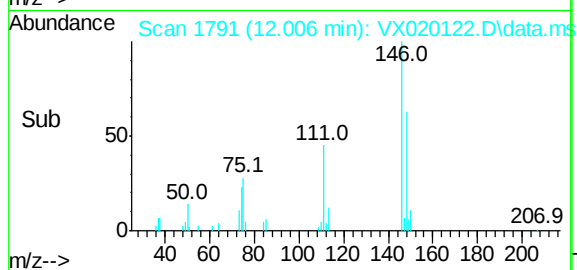
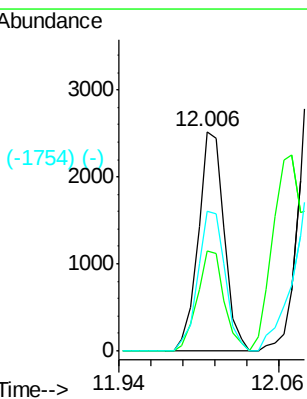





#913 (-)  
n-Butylbenzene  
Concen: 0.49 ug/l  
RT: 12.371 min Scan# 1851  
Delta R.T. -0.001 min  
Lab File: VX020122.D  
Acq: 18 Dec 2020 13:07




Instrument :  
MSVOA\_X  
ClientSampleId :  
IBLK


|          |       |       |       |
|----------|-------|-------|-------|
| Tgt Ion: | 91    | Resp: | 5660  |
| Ion      | Ratio | Lower | Upper |
| 91       | 100   |       |       |
| 92       | 57.1  | 27.4  | 82.0  |
| 134      | 24.9  | 13.2  | 39.5  |

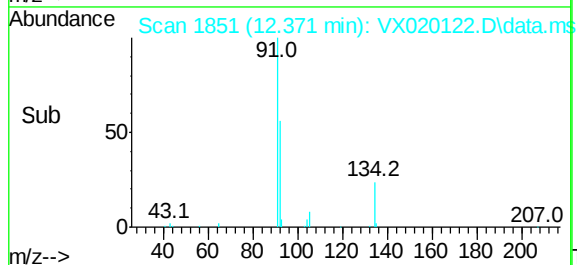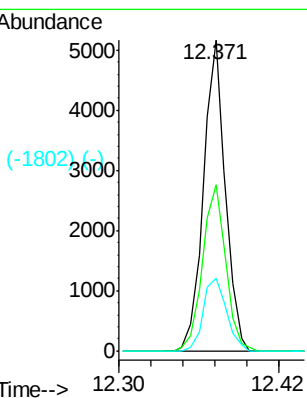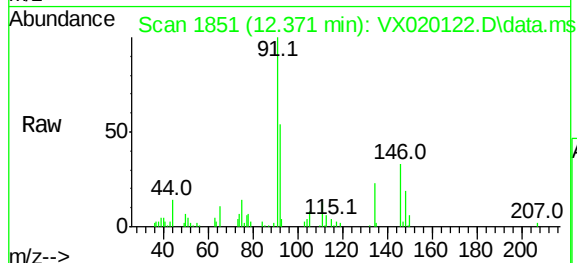

#914 (-)  
1,2-Dichlorobenzene  
Concen: 0.32 ug/l  
RT: 12.377 min Scan# 1852  
Delta R.T. 0.005 min  
Lab File: VX020122.D  
Acq: 18 Dec 2020 13:07

|          |       |       |       |
|----------|-------|-------|-------|
| Tgt Ion: | 146   | Resp: | 2281  |
| Ion      | Ratio | Lower | Upper |
| 146      | 100   |       |       |
| 111      | 39.8  | 20.8  | 62.2  |
| 148      | 63.8  | 31.9  | 95.5  |


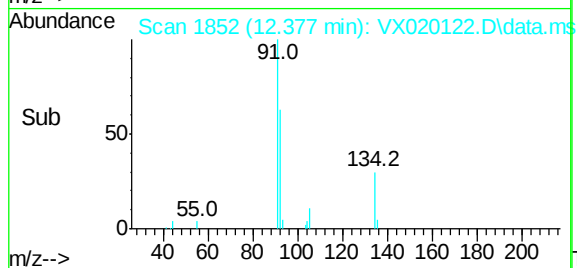
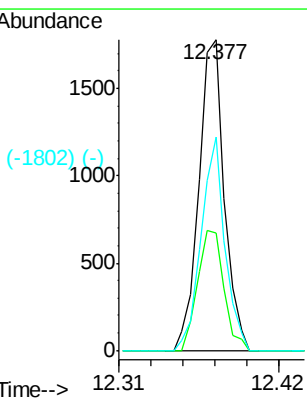





#9944 (-)  
 1,2-Dibromo-3-Chloropropane  
 Concen: 0.24 ug/l  
 RT: 12.981 min Scan# 1951  
 Delta R.T. 0.000 min  
 Lab File: VX020122.D  
 Acq: 18 Dec 2020 13:07




Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 IBLK


|          |       |       |        |
|----------|-------|-------|--------|
| Tgt Ion: | 75    | Resp: | 282    |
| Ion      | Ratio | Lower | Upper  |
| 75       | 100   |       |        |
| 155      | 42.9  | 45.3  | 135.9# |
| 157      | 76.2  | 57.7  | 173.1  |

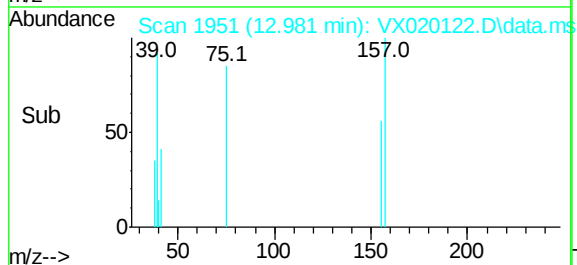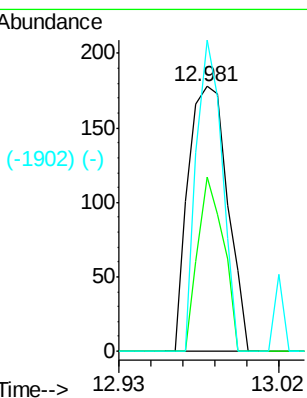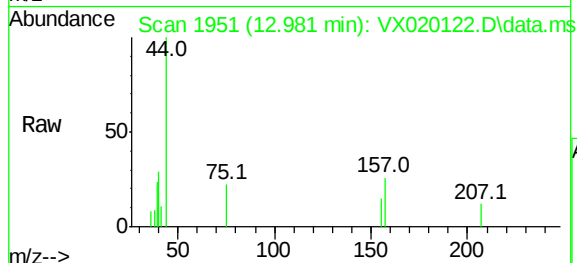

#9950 (-)  
 1,2,4-Trichlorobenzene  
 Concen: 0.96 ug/l  
 RT: 13.627 min Scan# 2057  
 Delta R.T. 0.000 min  
 Lab File: VX020122.D  
 Acq: 18 Dec 2020 13:07

|          |       |       |       |
|----------|-------|-------|-------|
| Tgt Ion: | 180   | Resp: | 4436  |
| Ion      | Ratio | Lower | Upper |
| 180      | 100   |       |       |
| 182      | 93.2  | 47.7  | 143.1 |
| 145      | 30.4  | 15.0  | 45.0  |


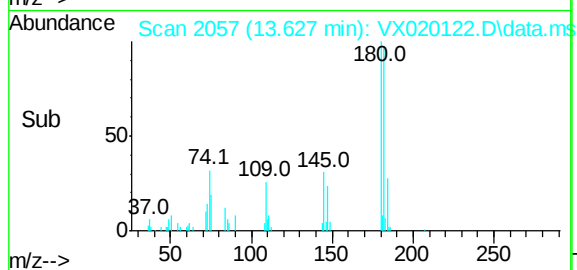
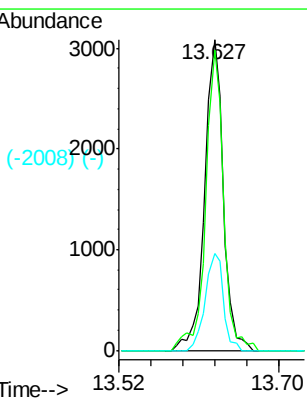





#94 (-)  
Hexachlorobutadiene  
Concen: 3.92 ug/l  
RT: 13.767 min Scan# 2080  
Delta R.T. -0.001 min  
Lab File: VX020122.D  
Acq: 18 Dec 2020 13:07




Instrument :  
MSVOA\_X  
ClientSampleId :  
IBLK


|           |       |       |      |
|-----------|-------|-------|------|
| Tgt Ion:  | 225   | Resp: | 2622 |
| Ion Ratio | Lower | Upper |      |
| 225       | 100   |       |      |
| 223       | 63.2  | 31.1  | 93.2 |
| 227       | 59.0  | 31.6  | 95.0 |

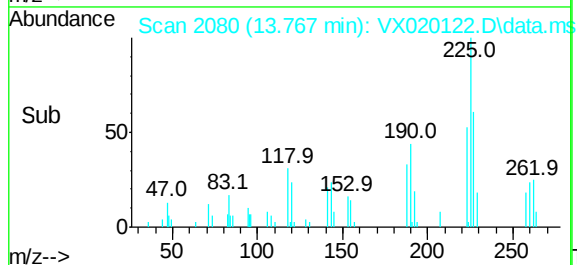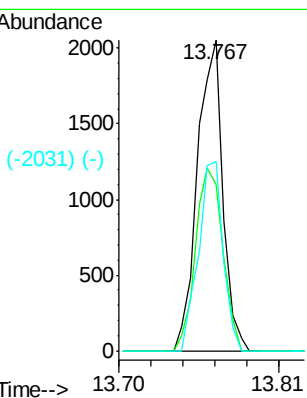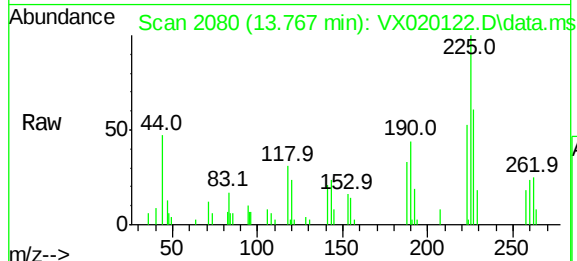

#95 (-)  
Naphthalene  
Concen: 0.67 ug/l  
RT: 13.816 min Scan# 2088  
Delta R.T. 0.000 min  
Lab File: VX020122.D  
Acq: 18 Dec 2020 13:07


|           |       |       |      |
|-----------|-------|-------|------|
| Tgt Ion:  | 128   | Resp: | 9870 |
| Ion Ratio | Lower | Upper |      |
| 128       | 100   |       |      |
| 127       | 12.2  | 10.3  | 15.5 |
| 129       | 11.3  | 8.8   | 13.2 |

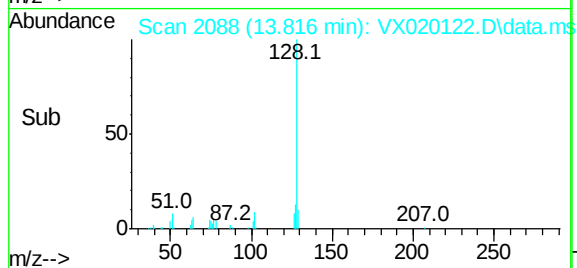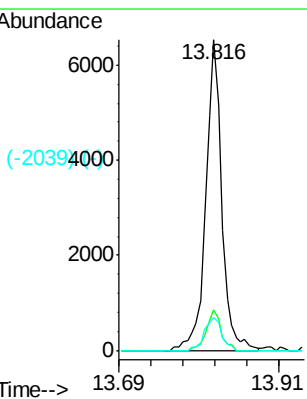



#9610 (-)  
 1,2,3-Trichlorobenzene  
 Concen: 0.89 ug/l  
 RT: 13.999 min Scan# 2118  
 Delta R.T. 0.000 min  
 Lab File: VX020122.D  
 Acq: 18 Dec 2020 13:07

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 IBLK



Tgt Ion:180 Resp: 4104

| Ion | Ratio | Lower | Upper |
|-----|-------|-------|-------|
| 180 | 100   |       |       |
| 182 | 92.3  | 47.6  | 142.9 |
| 145 | 31.1  | 16.1  | 48.3  |

