

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121821\
 Data File : VX025878.D
 Acq On : 17 Dec 2021 12:10
 Operator : JC/MD
 Sample : VX1218MBL01
 Misc : 5.0g/10mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX1218MBL01

Quant Time: Dec 19 02:33:13 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X121321W.M
 Quant Title : SW846 8260
 QLast Update : Tue Dec 14 07:02:11 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	145833	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	248394	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	221056	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	90989	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	93904	44.753	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	89.500%
35) Dibromofluoromethane	5.385	113	78665	45.410	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	90.820%
50) Toluene-d8	8.647	98	292002	46.263	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	92.520%
62) 4-Bromofluorobenzene	11.085	95	98759	41.191	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	82.380%#


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121821\
Data File : VX025878.D
Acq On : 17 Dec 2021 12:10
Operator : JC/MD
Sample : VX1218MBL01
Misc : 5.0g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX1218MBL01


Quant Time: Dec 19 02:33:13 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X121321W.M
Quant Title : SW846 8260
QLast Update : Tue Dec 14 07:02:11 2021
Response via : Initial Calibration

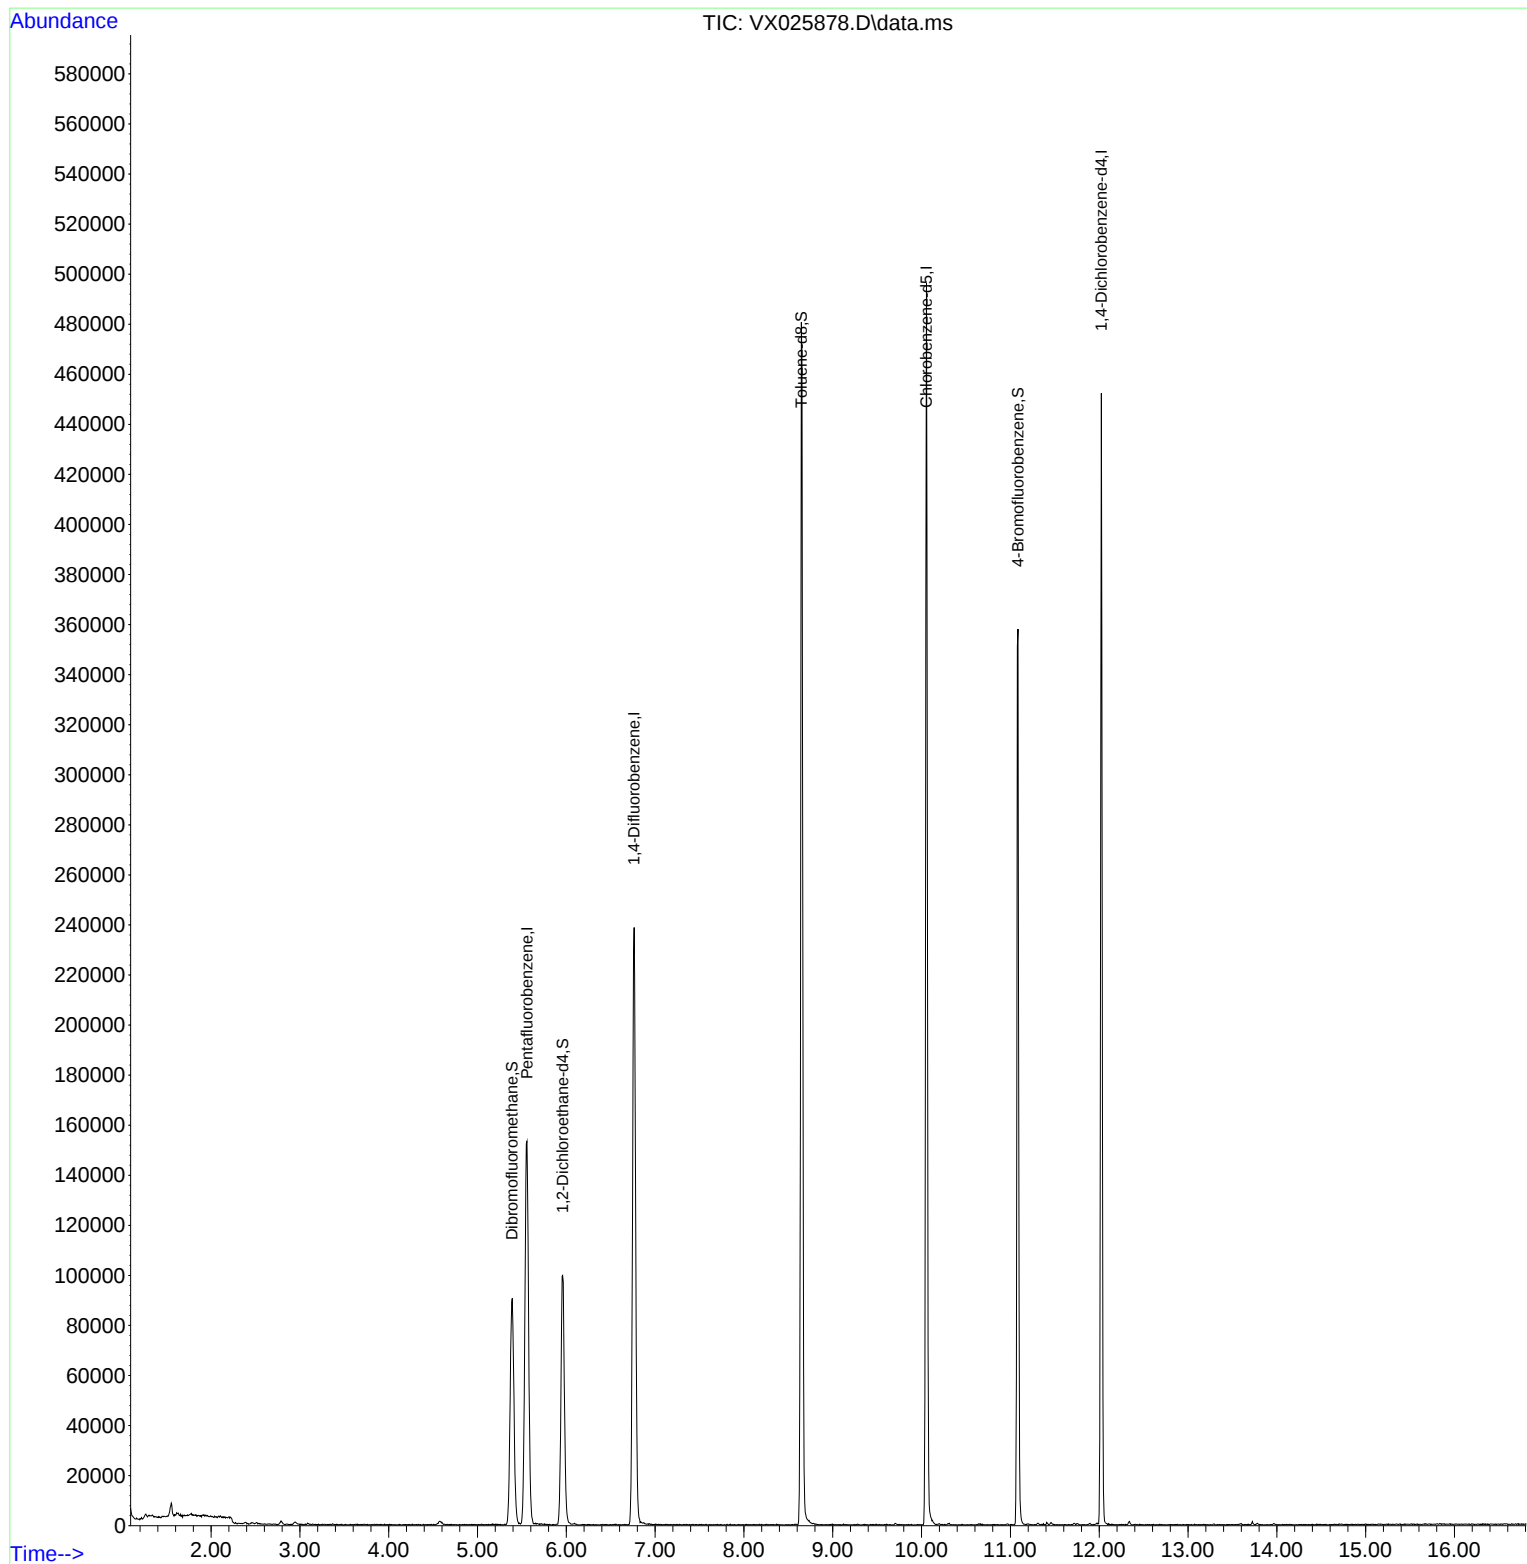



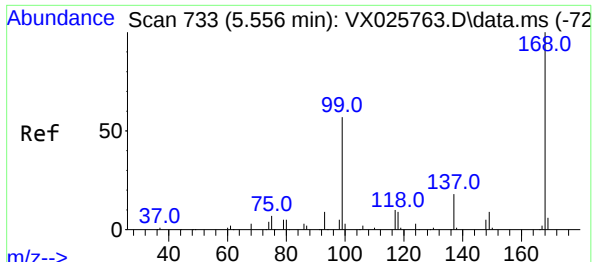


#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 713
Delta R.T. -0.000 min
Lab File: VX025878.D
Acq: 17 Dec 2021 12:10

Instrument :
MSVOA_X
ClientSampleId :
VX1218MBL01



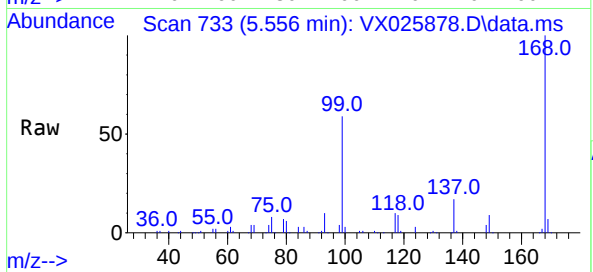



Tgt Ion:168 Resp: 145833
Ion Ratio Lower Upper
168 100
99 58.7 45.8 68.8

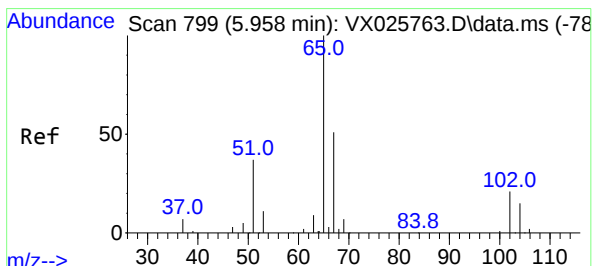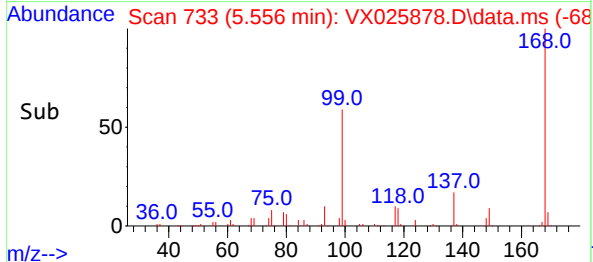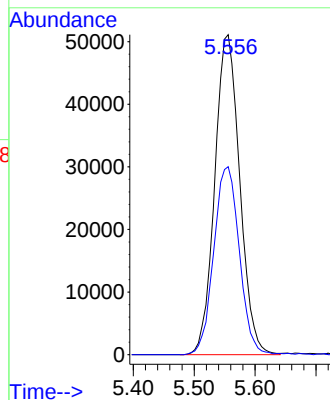

#33
1,2-Dichloroethane-d4
Concen: 44.753 ug/l
RT: 5.958 min Scan# 799
Delta R.T. -0.000 min
Lab File: VX025878.D
Acq: 17 Dec 2021 12:10

Tgt Ion: 65 Resp: 93904
Ion Ratio Lower Upper
65 100
67 52.1 0.0 103.4


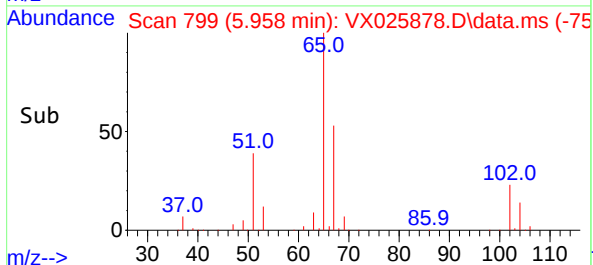
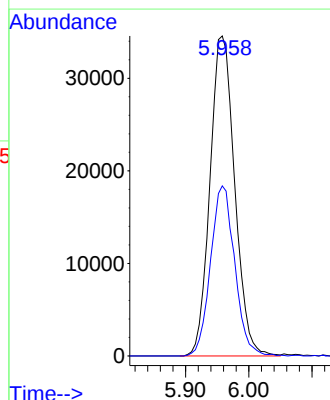
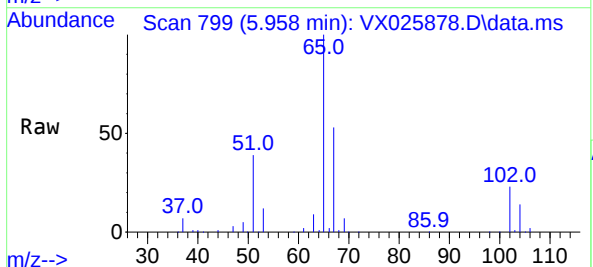


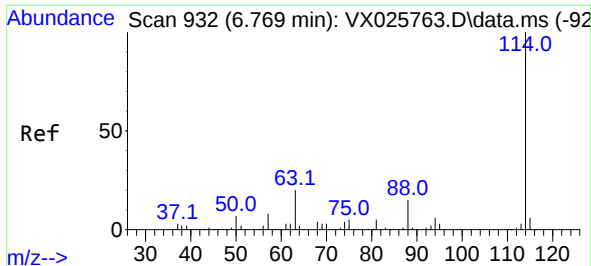

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. -0.006 min
Lab File: VX025878.D
Acq: 17 Dec 2021 12:10




Instrument :
MSVOA_X
ClientSampleId :
VX1218MBL01


Tgt Ion:114 Resp: 248394
Ion Ratio Lower Upper
114 100
63 18.9 0.0 40.0
88 14.8 0.0 30.6

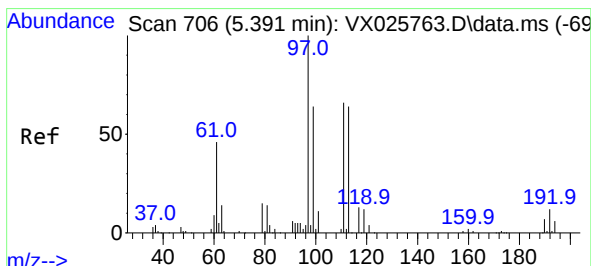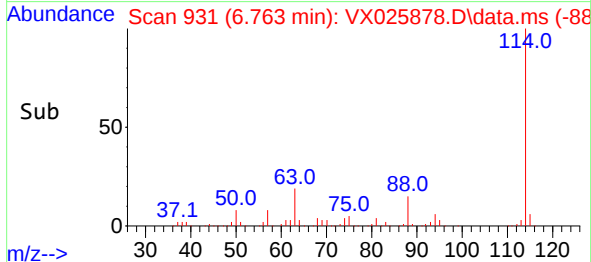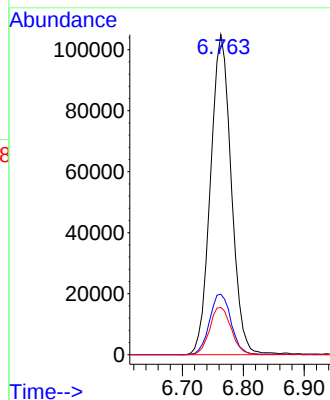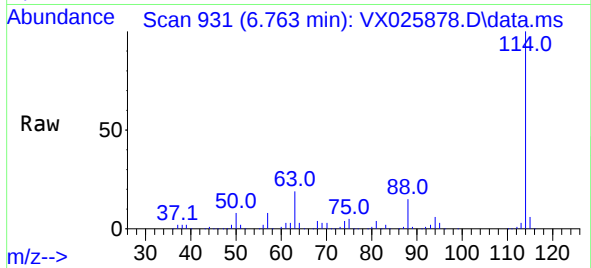

#35
Dibromofluoromethane
Concen: 45.410 ug/l
RT: 5.385 min Scan# 705
Delta R.T. -0.006 min
Lab File: VX025878.D
Acq: 17 Dec 2021 12:10

Tgt Ion:113 Resp: 78665
Ion Ratio Lower Upper
113 100
111 103.2 81.8 122.8
192 18.7 15.0 22.4


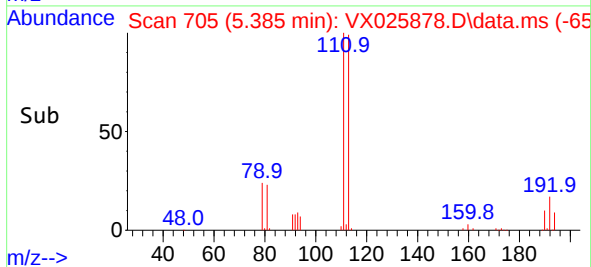
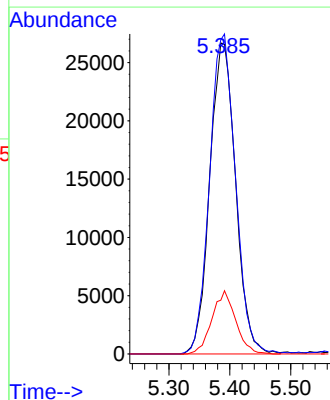
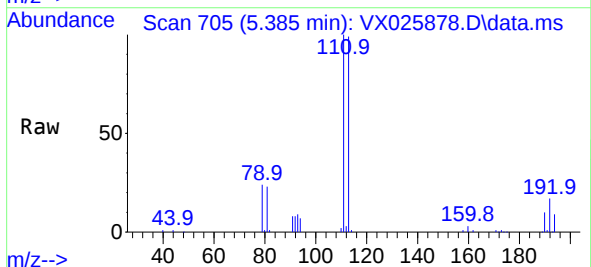


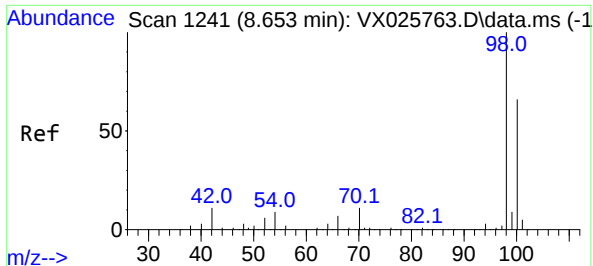

#50
Toluene-d8
Concen: 46.263 ug/l
RT: 8.647 min Scan# 11
Delta R.T. -0.006 min
Lab File: VX025878.D
Acq: 17 Dec 2021 12:10




Instrument :
MSVOA_X
ClientSampleId :
VX1218MBL01


Tgt Ion: 98 Resp: 292002
Ion Ratio Lower Upper
98 100
100 64.9 52.6 78.8

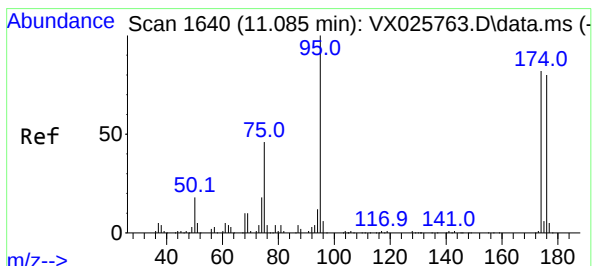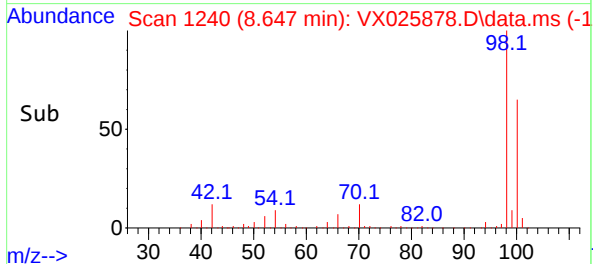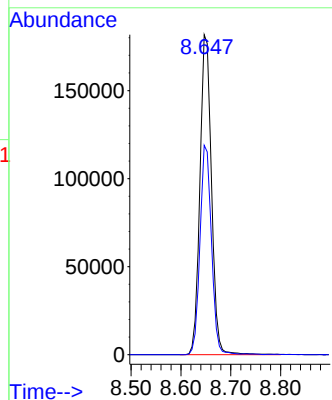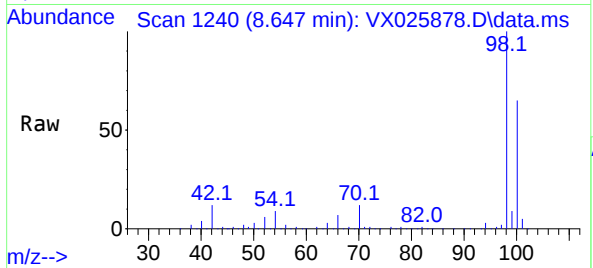

#62
4-Bromofluorobenzene
Concen: 41.191 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. -0.000 min
Lab File: VX025878.D
Acq: 17 Dec 2021 12:10

Tgt Ion: 95 Resp: 98759
Ion Ratio Lower Upper
95 100
174 76.7 0.0 157.4
176 74.6 0.0 154.6


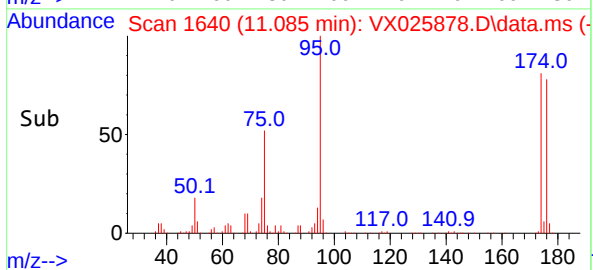
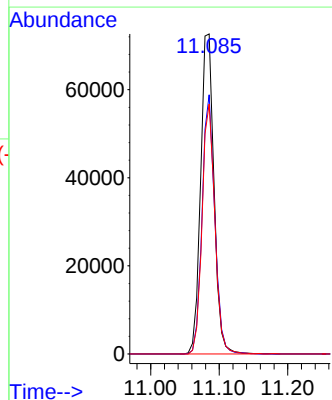
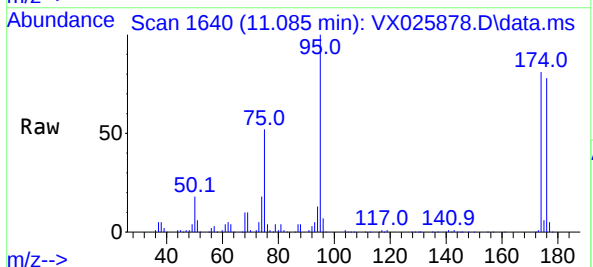


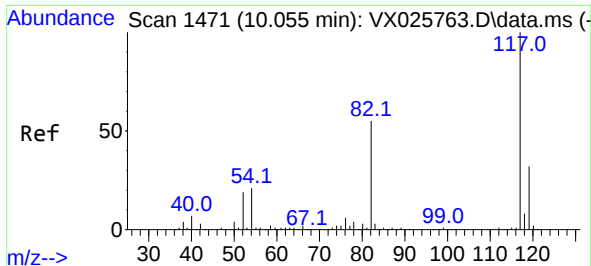

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX025878.D
Acq: 17 Dec 2021 12:10

Instrument :
MSVOA_X
ClientSampleId :
VX1218MBL01

Tgt Ion:117 Resp: 221056
Ion Ratio Lower Upper
117 100
82 55.0 43.8 65.6
119 32.3 25.2 37.8

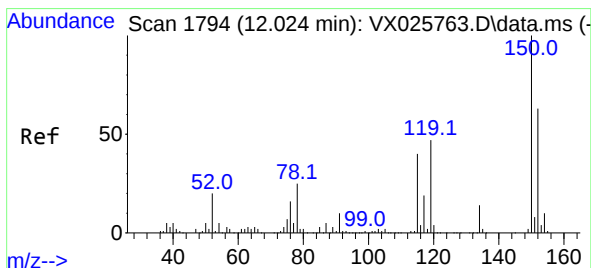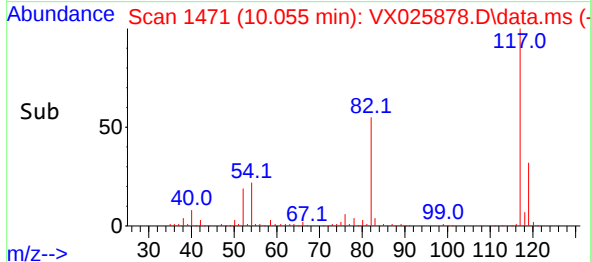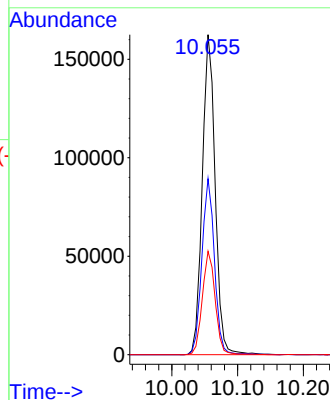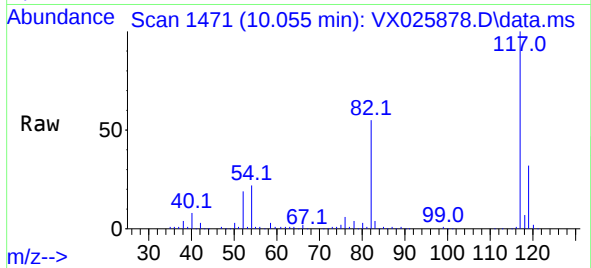

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. -0.000 min
Lab File: VX025878.D
Acq: 17 Dec 2021 12:10

Tgt Ion:152 Resp: 90989
Ion Ratio Lower Upper
152 100
115 61.2 41.3 123.9
150 155.2 0.0 351.8

