
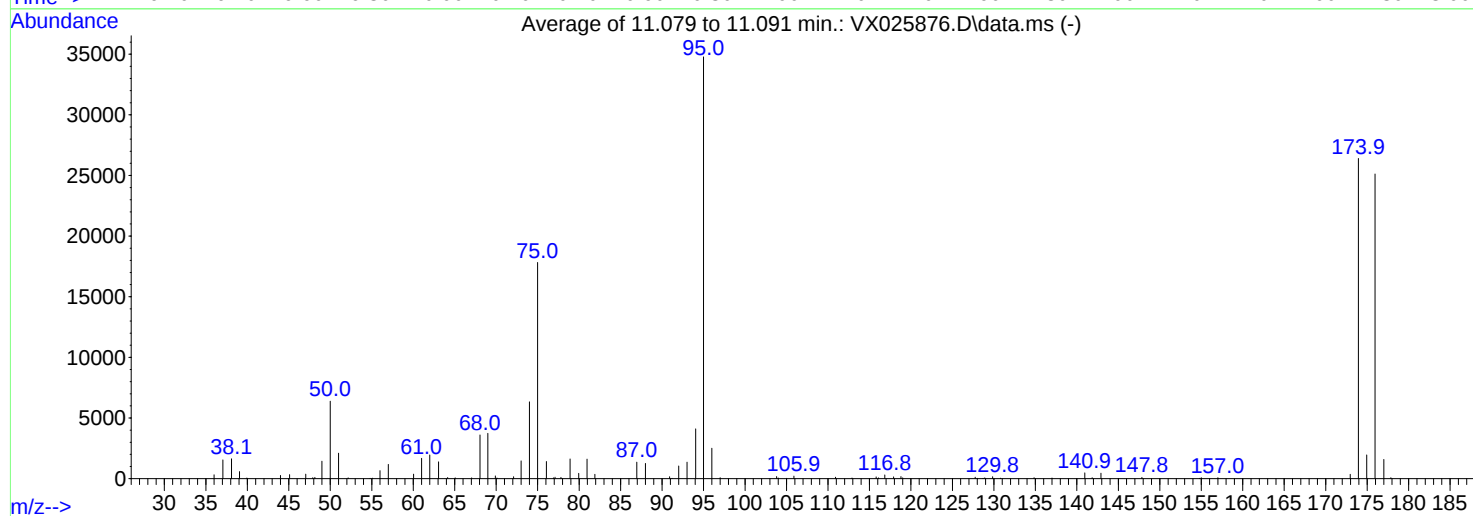


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121821\
 Data File : VX025876.D
 Acq On : 17 Dec 2021 09:18
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X121321W.M
 Title : SW846 8260
 Last Update : Tue Dec 14 07:02:11 2021

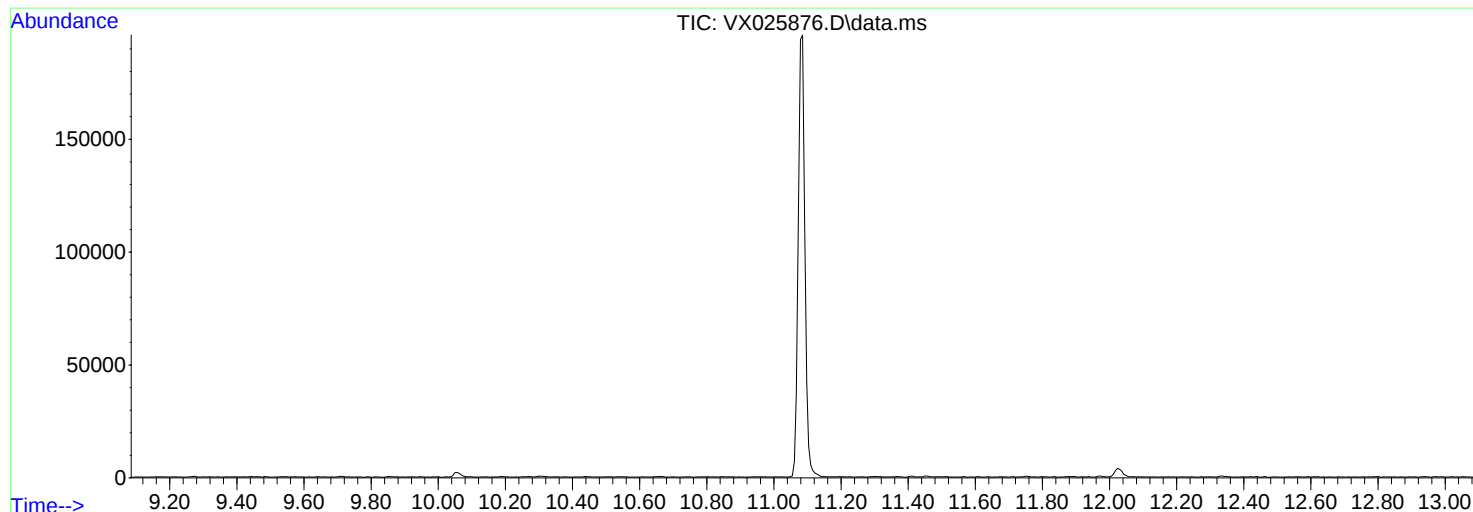

AutoFind: Scans 1639, 1640, 1641; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.4	6391	PASS
75	95	30	60	51.3	17833	PASS
95	95	100	100	100.0	34784	PASS
96	95	5	9	7.2	2503	PASS
173	174	0.00	2	1.3	352	PASS
174	95	50	100	75.9	26397	PASS
175	174	5	9	7.4	1954	PASS
176	174	95	101	95.2	25123	PASS
177	176	5	9	6.3	1588	PASS