

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121823\
 Data File : VX039300.D
 Acq On : 18 Dec 2023 10:51
 Operator : JC/MD
 Sample : VX1218WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK649

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

Signal : TIC: VX039300.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	43	46	58	rVB	104324	111637	12.24%	1.590%
2	1.666	91	95	105	rBV	66083	96072	10.53%	1.368%
3	2.306	194	200	209	rBV	195413	302105	33.11%	4.301%
4	2.508	230	233	236	rBV	1667	2544	0.28%	0.036%
5	2.794	274	280	287	rBV3	2095	4082	0.45%	0.058%
6	2.910	298	299	301	rBV	269	251	0.03%	0.004%
7	3.093	326	329	330	rBV2	499	522	0.06%	0.007%
8	3.129	333	335	337	rVV	350	298	0.03%	0.004%
9	3.276	357	359	362	rBV2	333	332	0.04%	0.005%
10	3.398	377	379	382	rBV2	236	283	0.03%	0.004%
11	3.453	386	388	390	rBV2	223	253	0.03%	0.004%
12	3.489	392	394	399	rBV2	287	406	0.04%	0.006%
13	3.599	411	412	414	rBV2	237	194	0.02%	0.003%
14	3.690	425	427	429	rBV	208	198	0.02%	0.003%
15	4.001	477	478	480	rBV	301	250	0.03%	0.004%
16	4.032	481	483	486	rVB	242	203	0.02%	0.003%
17	4.452	544	552	572	rBV	93950	263710	28.90%	3.755%
18	4.922	628	629	634	rVB3	278	342	0.04%	0.005%
19	5.056	639	651	668	rBV	115168	360840	39.55%	5.138%
20	5.391	700	706	708	rVV3	588	915	0.10%	0.013%
21	5.464	716	718	720	rVB	289	232	0.03%	0.003%
22	5.489	720	722	724	rVB2	339	229	0.03%	0.003%
23	5.538	727	730	731	rBV2	424	475	0.05%	0.007%
24	5.970	789	801	823	rBV2	304870	912358	100.00%	12.990%
25	6.257	846	848	850	rVB	317	203	0.02%	0.003%
26	6.373	866	867	870	rBV2	207	197	0.02%	0.003%
27	6.434	874	877	878	rVV2	236	225	0.02%	0.003%
28	6.476	882	884	888	rVB2	294	360	0.04%	0.005%
29	6.519	888	891	894	rBV	398	449	0.05%	0.006%
30	6.763	920	931	947	rBV	207316	508999	55.79%	7.247%
31	6.934	957	959	962	rBV3	265	223	0.02%	0.003%
32	7.001	968	970	971	rBV	215	216	0.02%	0.003%
33	7.123	988	990	992	rBV2	686	704	0.08%	0.010%
34	7.196	999	1002	1006	rBV2	187	278	0.03%	0.004%
35	7.306	1012	1020	1032	rBV	186119	413585	45.33%	5.889%
36	7.482	1047	1049	1051	rBV2	312	283	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121823\
 Data File : VX039300.D
 Acq On : 18 Dec 2023 10:51
 Operator : JC/MD
 Sample : VX1218WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK649

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

37	7.531	1055	1057	1059	rBV2	226	211	0.02%	0.003%
38	7.683	1081	1082	1085	rVB	259	205	0.02%	0.003%
39	7.720	1085	1088	1089	rBV2	229	235	0.03%	0.003%
40	7.830	1104	1106	1109	rVB2	311	304	0.03%	0.004%
41	7.964	1125	1128	1130	rVV2	336	375	0.04%	0.005%
42	8.275	1178	1179	1181	rBV	266	201	0.02%	0.003%
43	8.324	1181	1187	1202	rVV	132627	220480	24.17%	3.139%
44	8.574	1225	1228	1229	rBV2	356	318	0.03%	0.005%
45	8.647	1233	1240	1263	rBV	458709	718091	78.71%	10.224%
46	8.891	1279	1280	1284	rVB2	331	231	0.03%	0.003%
47	8.952	1284	1290	1302	rBV	94393	146921	16.10%	2.092%
48	9.080	1309	1311	1314	rVB3	320	285	0.03%	0.004%
49	9.165	1322	1325	1328	rBV	388	425	0.05%	0.006%
50	9.275	1337	1343	1352	rBV2	2655	4254	0.47%	0.061%
51	9.384	1355	1361	1381	rBV	417852	602820	66.07%	8.583%
52	9.610	1396	1398	1402	rVB3	444	367	0.04%	0.005%
53	9.659	1404	1406	1408	rVB	281	221	0.02%	0.003%
54	9.811	1428	1431	1433	rBV2	249	367	0.04%	0.005%
55	9.915	1445	1448	1451	rBV2	259	293	0.03%	0.004%
56	9.994	1459	1461	1463	rBV2	304	269	0.03%	0.004%
57	10.055	1465	1471	1489	rBV	439977	627933	68.83%	8.941%
58	10.201	1492	1495	1497	rVB2	942	1118	0.12%	0.016%
59	10.311	1509	1513	1518	rVB2	973	1426	0.16%	0.020%
60	10.646	1564	1568	1569	rBV2	826	840	0.09%	0.012%
61	10.799	1590	1593	1595	rBV2	186	219	0.02%	0.003%
62	10.860	1601	1603	1606	rVB2	192	203	0.02%	0.003%
63	10.963	1617	1620	1624	rVB2	863	1011	0.11%	0.014%
64	11.043	1628	1633	1637	rVB2	242	433	0.05%	0.006%
65	11.189	1652	1657	1670	rBV	352627	456113	49.99%	6.494%
66	11.311	1672	1677	1683	rVB2	3132	4044	0.44%	0.058%
67	11.451	1697	1700	1706	rVB2	924	1448	0.16%	0.021%
68	11.756	1746	1750	1754	rBV3	1044	1332	0.15%	0.019%
69	11.969	1781	1785	1788	rBV4	1372	1810	0.20%	0.026%
70	12.024	1788	1794	1804	rVV	475612	617878	67.72%	8.798%
71	12.317	1837	1842	1853	rBV	462479	609432	66.80%	8.677%
72	12.573	1879	1884	1886	rVB2	189	330	0.04%	0.005%
73	12.762	1911	1915	1919	rVB3	812	1085	0.12%	0.015%
74	13.054	1960	1963	1965	rBV2	235	283	0.03%	0.004%
75	13.115	1971	1973	1977	rVB2	1177	1414	0.15%	0.020%
76	13.341	2008	2010	2013	rVB2	279	218	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121823\
 Data File : VX039300.D
 Acq On : 18 Dec 2023 10:51
 Operator : JC/MD
 Sample : VX1218WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK649

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

77	13.378	2013	2016	2018	rBV	260	290	0.03%	0.004%
78	13.536	2040	2042	2045	rVB	299	246	0.03%	0.004%
79	13.591	2045	2051	2055	rBV2	1741	2414	0.26%	0.034%
80	13.786	2078	2083	2086	rBV	1588	2038	0.22%	0.029%
81	13.914	2100	2104	2108	rBV2	201	303	0.03%	0.004%
82	13.963	2108	2112	2116	rVV3	1345	1921	0.21%	0.027%
83	14.024	2121	2122	2126	rBV	234	265	0.03%	0.004%
84	14.079	2129	2131	2133	rBV2	185	201	0.02%	0.003%
85	14.127	2136	2139	2147	rVB2	704	1156	0.13%	0.016%
86	14.377	2176	2180	2182	rBV2	193	258	0.03%	0.004%
87	14.554	2208	2209	2212	rVV	348	298	0.03%	0.004%
88	14.621	2218	2220	2223	rVV3	295	360	0.04%	0.005%
89	14.670	2225	2228	2231	rBV2	314	427	0.05%	0.006%
90	14.737	2237	2239	2240	rBV2	272	230	0.03%	0.003%
91	14.847	2254	2257	2259	rBV2	320	425	0.05%	0.006%
92	15.079	2293	2295	2299	rBV2	247	424	0.05%	0.006%
93	15.383	2342	2345	2346	rBV3	447	478	0.05%	0.007%
94	15.566	2373	2375	2376	rBV2	290	199	0.02%	0.003%
95	15.853	2421	2422	2424	rBV	261	221	0.02%	0.003%
96	15.950	2437	2438	2440	rBV	334	227	0.02%	0.003%
97	16.066	2455	2457	2460	rBV2	305	257	0.03%	0.004%
98	16.243	2484	2486	2487	rBV2	252	258	0.03%	0.004%
99	16.316	2496	2498	2499	rBV	326	264	0.03%	0.004%
100	16.731	2564	2566	2569	rBV2	266	255	0.03%	0.004%




Sum of corrected areas: 7023311

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121823\
Data File : VX039300.D
Acq On : 18 Dec 2023 10:51
Operator : JC/MD
Sample : VX1218WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK649

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

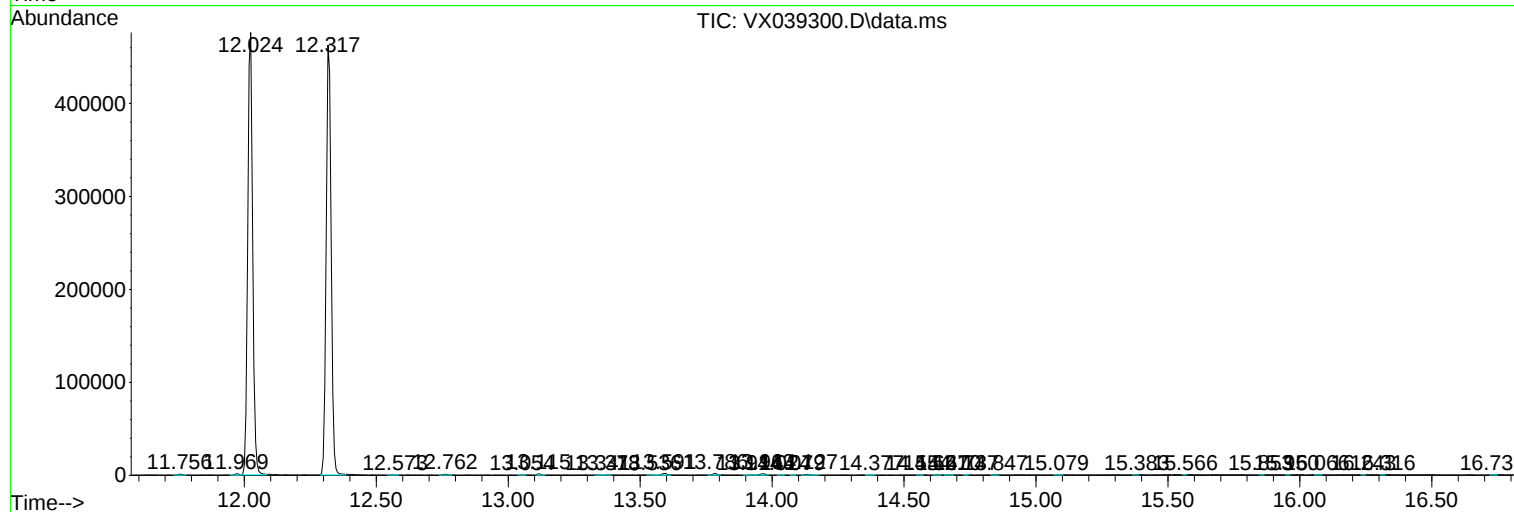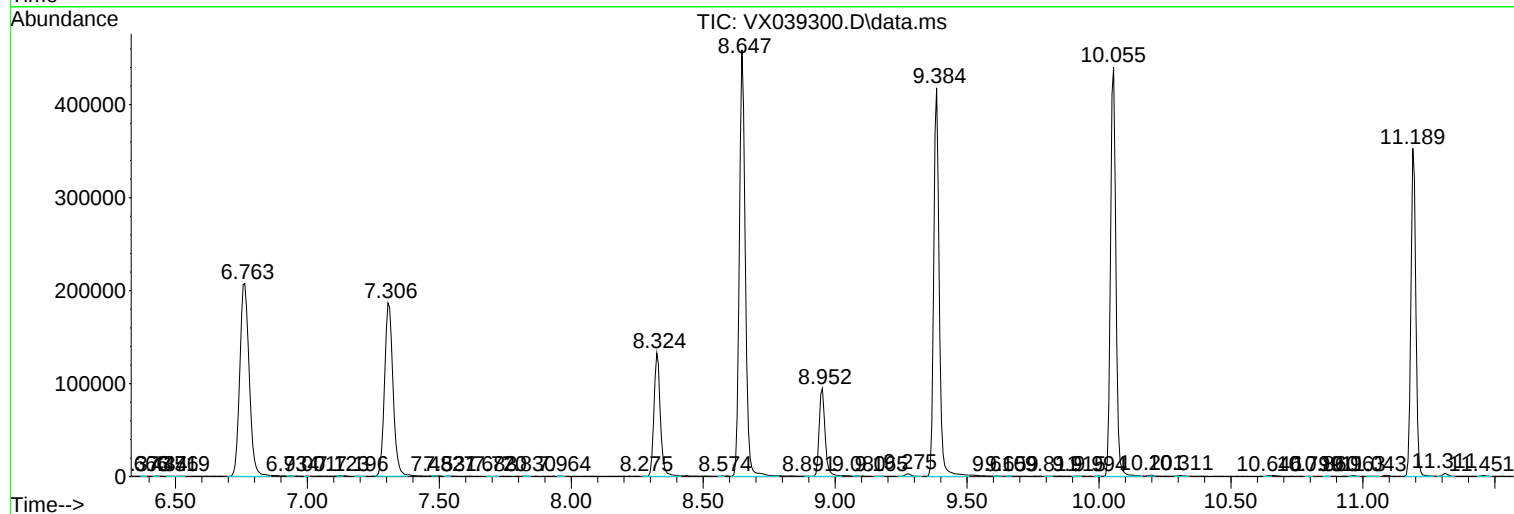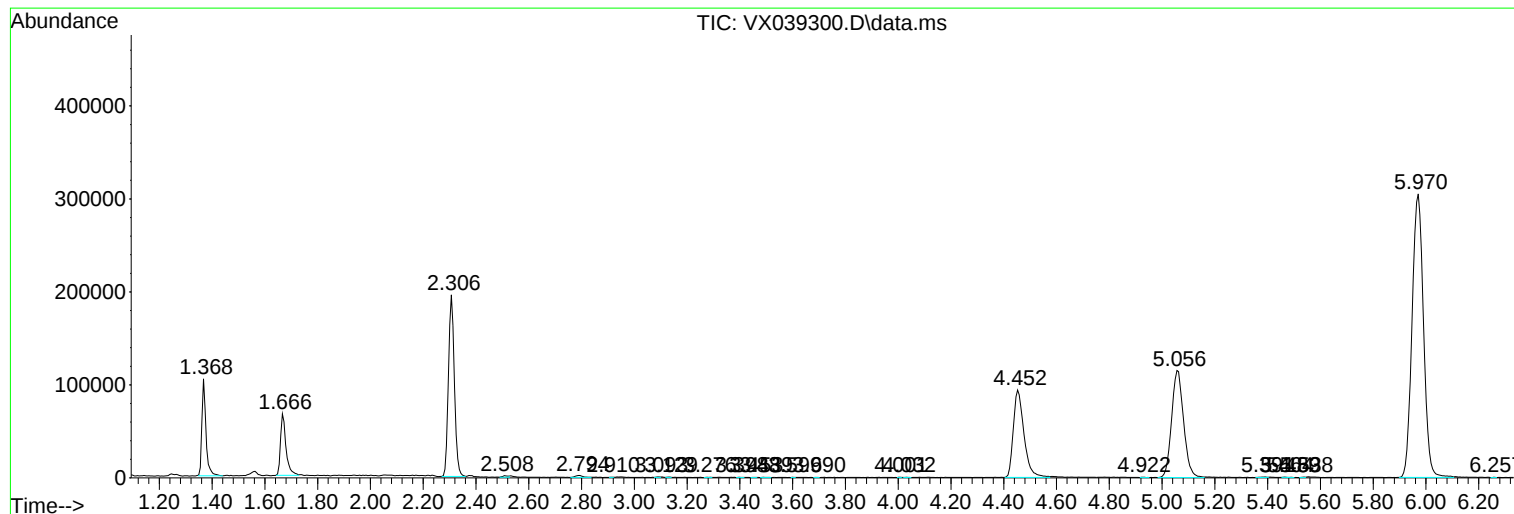

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121823\
Data File : VX039300.D
Acq On : 18 Dec 2023 10:51
Operator : JC/MD
Sample : VX1218WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK649

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121823\
Data File : VX039300.D
Acq On : 18 Dec 2023 10:51
Operator : JC/MD
Sample : VX1218WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK649

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------