

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121823\
 Data File : VX039302.D
 Acq On : 18 Dec 2023 11:38
 Operator : JC/MD
 Sample : 05823-01 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0AW7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

Signal : TIC: VX039302.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	22	26	33	rBV2	5278	11927	1.41%	0.172%
2	1.368	42	46	56	rVB	82631	86436	10.24%	1.247%
3	1.666	91	95	106	rBV	60037	84225	9.98%	1.215%
4	2.307	194	200	208	rBV	165901	255999	30.33%	3.694%
5	2.380	208	212	219	rVB	8736	14832	1.76%	0.214%
6	2.532	231	237	249	rVB3	3311	7447	0.88%	0.107%
7	2.794	274	280	285	rBV4	4020	8320	0.99%	0.120%
8	2.947	299	305	311	rVB2	3446	7993	0.95%	0.115%
9	3.117	331	333	337	rBV2	302	341	0.04%	0.005%
10	3.319	365	366	368	rBV	321	258	0.03%	0.004%
11	3.380	374	376	382	rVV2	195	349	0.04%	0.005%
12	3.861	452	455	456	rBV2	607	610	0.07%	0.009%
13	4.306	524	528	530	rBV2	187	289	0.03%	0.004%
14	4.459	541	553	566	rBV2	86671	254244	30.12%	3.669%
15	4.818	610	612	614	rBV3	236	207	0.02%	0.003%
16	4.916	626	628	631	rBV	203	204	0.02%	0.003%
17	5.062	639	652	673	rBV	108486	337721	40.01%	4.873%
18	5.379	702	704	706	rBV2	567	489	0.06%	0.007%
19	5.739	761	763	764	rBV	287	233	0.03%	0.003%
20	5.971	789	801	817	rBV3	279684	843993	100.00%	12.178%
21	6.470	882	883	885	rVB	472	197	0.02%	0.003%
22	6.489	885	886	890	rVB2	313	270	0.03%	0.004%
23	6.537	890	894	895	rBV2	219	306	0.04%	0.004%
24	6.666	912	915	916	rBV2	275	253	0.03%	0.004%
25	6.763	922	931	944	rBV	237999	575386	68.17%	8.302%
26	7.007	969	971	973	rBV2	288	282	0.03%	0.004%
27	7.111	984	988	995	rVB6	1344	2937	0.35%	0.042%
28	7.306	1011	1020	1038	rBV	176662	390871	46.31%	5.640%
29	7.489	1047	1050	1058	rVB2	1080	1730	0.20%	0.025%
30	7.574	1062	1064	1066	rVB	250	210	0.02%	0.003%
31	7.653	1072	1077	1090	rBV2	3668	8402	1.00%	0.121%
32	7.830	1105	1106	1109	rVB	342	270	0.03%	0.004%
33	7.873	1109	1113	1114	rBV	398	412	0.05%	0.006%
34	7.940	1122	1124	1125	rBV2	323	225	0.03%	0.003%
35	8.141	1156	1157	1160	rVV	317	259	0.03%	0.004%
36	8.324	1181	1187	1198	rBV	125544	205233	24.32%	2.961%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121823\
 Data File : VX039302.D
 Acq On : 18 Dec 2023 11:38
 Operator : JC/MD
 Sample : 05823-01 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0AW7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
 Title : VOC Analysis

37	8.501	1214	1216	1219	rBV2	351	324	0.04%	0.005%
38	8.647	1234	1240	1257	rBV	409102	656112	77.74%	9.467%
39	8.909	1280	1283	1284	rBV	250	272	0.03%	0.004%
40	8.952	1284	1290	1304	rVV	90086	138672	16.43%	2.001%
41	9.244	1336	1338	1342	rBV2	578	616	0.07%	0.009%
42	9.287	1342	1345	1346	rBV3	249	237	0.03%	0.003%
43	9.317	1346	1350	1355	rVV3	2412	4113	0.49%	0.059%
44	9.385	1355	1361	1385	rVV	413395	595635	70.57%	8.595%
45	9.665	1405	1407	1409	rBV3	175	217	0.03%	0.003%
46	9.695	1409	1412	1415	rVB3	472	616	0.07%	0.009%
47	9.848	1433	1437	1442	rVB3	326	604	0.07%	0.009%
48	10.055	1465	1471	1484	rBV	509980	707962	83.88%	10.215%
49	10.244	1500	1502	1504	rBV2	293	237	0.03%	0.003%
50	10.305	1510	1512	1517	rVB3	440	736	0.09%	0.011%
51	10.384	1523	1525	1529	rVB2	172	211	0.03%	0.003%
52	10.512	1541	1546	1549	rBV3	751	1061	0.13%	0.015%
53	10.714	1575	1579	1580	rBV2	192	266	0.03%	0.004%
54	10.964	1617	1620	1623	rVB2	426	359	0.04%	0.005%
55	11.092	1636	1641	1644	rBV3	1060	1446	0.17%	0.021%
56	11.189	1652	1657	1667	rBV	337634	442986	52.49%	6.392%
57	11.317	1676	1678	1680	rVB	346	213	0.03%	0.003%
58	11.366	1684	1686	1688	rVB	323	196	0.02%	0.003%
59	11.762	1747	1751	1754	rVV3	496	579	0.07%	0.008%
60	11.860	1764	1767	1771	rBV2	168	269	0.03%	0.004%
61	11.976	1782	1786	1788	rBV2	797	864	0.10%	0.012%
62	12.024	1788	1794	1804	rVV	512372	672470	79.68%	9.703%
63	12.213	1824	1825	1827	rBV2	302	214	0.03%	0.003%
64	12.317	1837	1842	1856	rBV	455316	587657	69.63%	8.480%
65	12.549	1878	1880	1883	rVB2	219	240	0.03%	0.003%
66	12.762	1913	1915	1918	rVB	369	442	0.05%	0.006%
67	12.872	1932	1933	1935	rBV	284	200	0.02%	0.003%
68	12.994	1951	1953	1956	rVB2	171	213	0.03%	0.003%
69	13.061	1960	1964	1966	rBV	343	316	0.04%	0.005%
70	13.384	2015	2017	2019	rBV2	244	215	0.03%	0.003%
71	13.512	2035	2038	2040	rBV	200	195	0.02%	0.003%
72	13.542	2040	2043	2047	rVV2	226	254	0.03%	0.004%
73	13.591	2048	2051	2057	rVB4	817	998	0.12%	0.014%
74	13.652	2059	2061	2064	rVB2	244	250	0.03%	0.004%
75	13.786	2080	2083	2085	rBV2	352	441	0.05%	0.006%
76	13.975	2110	2114	2115	rVB2	492	576	0.07%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121823\
 Data File : VX039302.D
 Acq On : 18 Dec 2023 11:38
 Operator : JC/MD
 Sample : 05823-01 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0AW7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

77	13.993	2115	2117	2120	rBV2	244	224	0.03%	0.003%
78	14.067	2125	2129	2132	rBV2	230	241	0.03%	0.003%
79	14.128	2135	2139	2142	rBV3	640	1049	0.12%	0.015%
80	14.189	2147	2149	2153	rBV2	150	199	0.02%	0.003%
81	14.548	2207	2208	2211	rBV2	241	208	0.02%	0.003%
82	14.591	2214	2215	2217	rBV2	294	219	0.03%	0.003%
83	14.823	2250	2253	2255	rBV3	271	328	0.04%	0.005%
84	14.938	2268	2272	2274	rBV2	320	440	0.05%	0.006%
85	15.030	2284	2287	2288	rBV2	191	222	0.03%	0.003%
86	15.073	2292	2294	2298	rVV	363	373	0.04%	0.005%
87	15.109	2298	2300	2303	rVB3	324	258	0.03%	0.004%
88	15.347	2337	2339	2342	rVB2	310	285	0.03%	0.004%
89	15.377	2342	2344	2345	rBV2	407	376	0.04%	0.005%
90	15.524	2367	2368	2370	rBV2	406	277	0.03%	0.004%
91	15.664	2388	2391	2392	rBV2	379	305	0.04%	0.004%
92	15.682	2392	2394	2395	rBV	329	234	0.03%	0.003%
93	15.902	2428	2430	2433	rVB	351	234	0.03%	0.003%
94	16.072	2456	2458	2460	rBV	335	332	0.04%	0.005%
95	16.152	2470	2471	2473	rBV	372	263	0.03%	0.004%
96	16.316	2497	2498	2502	rVB2	389	347	0.04%	0.005%
97	16.353	2502	2504	2505	rBV2	371	234	0.03%	0.003%
98	16.402	2511	2512	2514	rBV2	336	259	0.03%	0.004%
99	16.542	2533	2535	2536	rVB	425	236	0.03%	0.003%
100	16.560	2536	2538	2539	rBV	429	339	0.04%	0.005%


Sum of corrected areas: 6930326

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121823\
Data File : VX039302.D
Acq On : 18 Dec 2023 11:38
Operator : JC/MD
Sample : 05823-01 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0AW7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

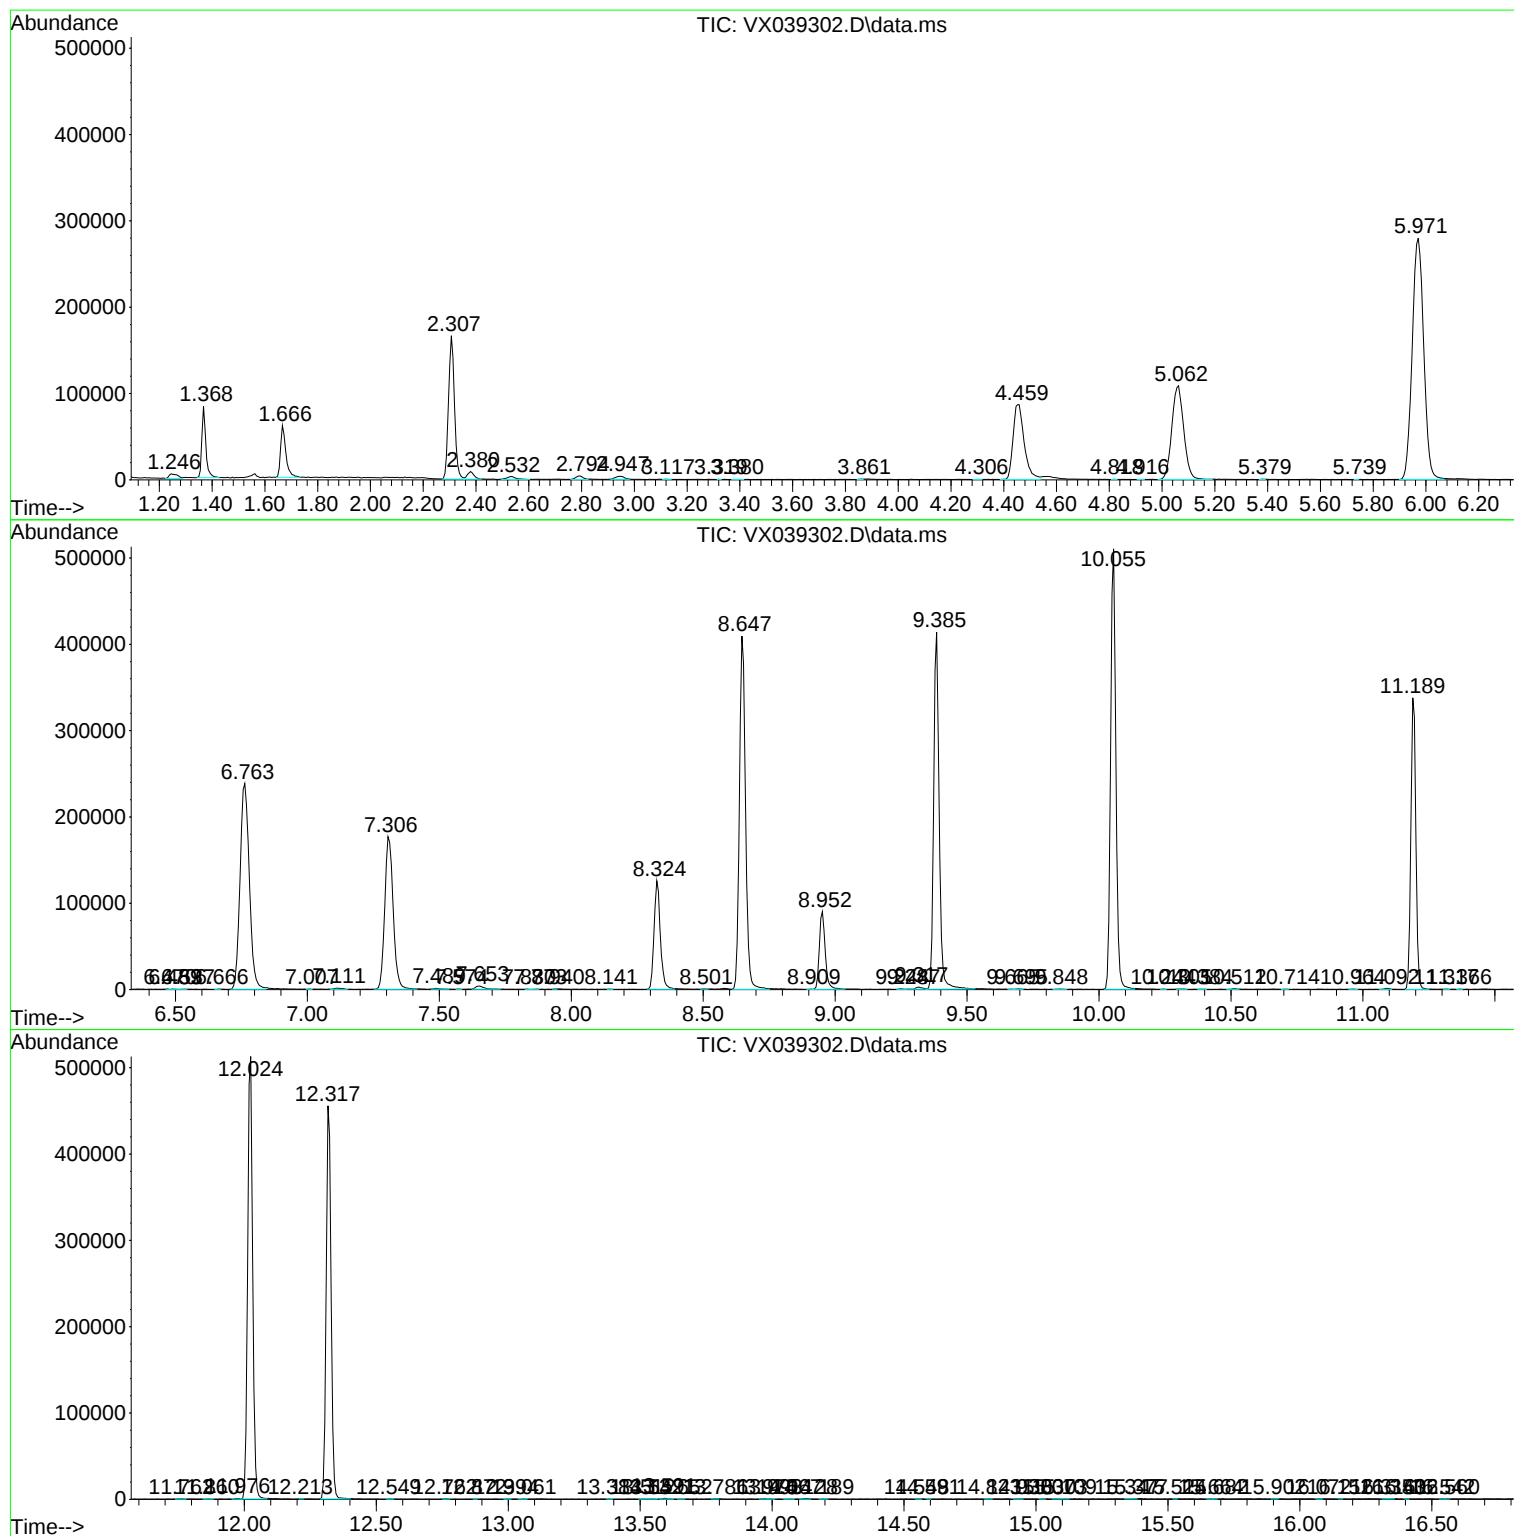

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121823\
Data File : VX039302.D
Acq On : 18 Dec 2023 11:38
Operator : JC/MD
Sample : 05823-01 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0AW7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121823\
Data File : VX039302.D
Acq On : 18 Dec 2023 11:38
Operator : JC/MD
Sample : 05823-01 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0AW7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------