

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121823\
 Data File : VX039303.D
 Acq On : 18 Dec 2023 11:59
 Operator : JC/MD
 Sample : 05823-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

Signal : TIC: VX039303.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	23	26	36	rBV4	4710	11293	1.58%	0.202%
2	1.368	42	46	54	rVB	74850	77830	10.87%	1.390%
3	1.666	91	95	107	rBV	48752	70844	9.89%	1.266%
4	2.307	194	200	209	rBV	139929	217801	30.42%	3.891%
5	2.508	230	233	234	rBV2	504	574	0.08%	0.010%
6	2.672	257	260	262	rBV2	320	342	0.05%	0.006%
7	2.794	273	280	287	rBV4	2182	4547	0.63%	0.081%
8	3.014	314	316	317	rBV2	270	204	0.03%	0.004%
9	3.105	328	331	335	rBV2	319	440	0.06%	0.008%
10	3.276	356	359	361	rBV2	215	299	0.04%	0.005%
11	3.312	363	365	368	rBV2	249	251	0.04%	0.004%
12	3.739	434	435	438	rBV2	197	255	0.04%	0.005%
13	3.794	443	444	449	rVV2	169	272	0.04%	0.005%
14	3.916	462	464	468	rVB2	164	214	0.03%	0.004%
15	4.154	501	503	508	rVB	277	298	0.04%	0.005%
16	4.459	543	553	570	rBV	86814	250278	34.95%	4.471%
17	4.654	583	585	587	rBV	372	481	0.07%	0.009%
18	4.770	602	604	606	rBV	376	272	0.04%	0.005%
19	5.062	635	652	666	rBV	91881	279289	39.00%	4.989%
20	5.257	682	684	686	rBV2	284	294	0.04%	0.005%
21	5.276	686	687	690	rVB2	273	245	0.03%	0.004%
22	5.556	728	733	734	rBV3	367	529	0.07%	0.009%
23	5.635	745	746	750	rBV2	276	381	0.05%	0.007%
24	5.702	755	757	760	rVB	300	269	0.04%	0.005%
25	5.727	760	761	764	rBV	243	254	0.04%	0.005%
26	5.971	789	801	822	rBV2	237572	716072	100.00%	12.792%
27	6.245	844	846	848	rBV	362	307	0.04%	0.005%
28	6.312	855	857	858	rBV	318	277	0.04%	0.005%
29	6.763	923	931	944	rVV	161305	380497	53.14%	6.797%
30	7.044	975	977	978	rBV2	224	206	0.03%	0.004%
31	7.220	1004	1006	1011	rBV2	206	234	0.03%	0.004%
32	7.312	1011	1021	1042	rBV	151739	332019	46.37%	5.931%
33	7.452	1042	1044	1046	rBV2	270	231	0.03%	0.004%
34	7.476	1046	1048	1050	rBV3	279	290	0.04%	0.005%
35	7.550	1058	1060	1063	rVB2	185	187	0.03%	0.003%
36	7.611	1066	1070	1072	rBV2	239	379	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121823\
 Data File : VX039303.D
 Acq On : 18 Dec 2023 11:59
 Operator : JC/MD
 Sample : 05823-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
 Title : VOC Analysis

37	7.818	1101	1104	1106	rBV2	194	235	0.03%	0.004%
38	7.854	1108	1110	1113	rBV2	336	302	0.04%	0.005%
39	7.988	1129	1132	1135	rVB2	226	255	0.04%	0.005%
40	8.013	1135	1136	1140	rBV2	213	273	0.04%	0.005%
41	8.098	1145	1150	1152	rBV2	284	317	0.04%	0.006%
42	8.324	1181	1187	1196	rBV	104918	172170	24.04%	3.076%
43	8.488	1212	1214	1215	rBV	202	199	0.03%	0.004%
44	8.580	1226	1229	1231	rBV2	376	499	0.07%	0.009%
45	8.647	1234	1240	1257	rBV	328225	544177	75.99%	9.721%
46	8.860	1274	1275	1281	rVB2	243	270	0.04%	0.005%
47	8.952	1285	1290	1302	rBV	77139	117652	16.43%	2.102%
48	9.171	1324	1326	1328	rBV2	292	242	0.03%	0.004%
49	9.275	1339	1343	1348	rVB2	978	1454	0.20%	0.026%
50	9.385	1356	1361	1376	rBV	387255	557008	77.79%	9.950%
51	9.653	1403	1405	1406	rBV2	242	201	0.03%	0.004%
52	9.738	1418	1419	1422	rVB	354	248	0.03%	0.004%
53	10.055	1465	1471	1482	rBV	358052	484248	67.63%	8.651%
54	10.238	1499	1501	1503	rBV2	254	234	0.03%	0.004%
55	10.305	1509	1512	1513	rBV	301	338	0.05%	0.006%
56	10.372	1521	1523	1525	rBV	246	244	0.03%	0.004%
57	10.616	1560	1563	1565	rBV2	202	239	0.03%	0.004%
58	10.677	1572	1573	1579	rVB2	358	424	0.06%	0.008%
59	10.970	1618	1621	1625	rVB2	453	533	0.07%	0.010%
60	11.006	1625	1627	1631	rBV	251	321	0.04%	0.006%
61	11.092	1637	1641	1646	rBV4	776	1097	0.15%	0.020%
62	11.189	1652	1657	1669	rBV	304606	393096	54.90%	7.022%
63	11.311	1674	1677	1681	rVB3	1178	1559	0.22%	0.028%
64	11.457	1696	1701	1706	rVB3	467	759	0.11%	0.014%
65	11.701	1737	1741	1744	rBV2	286	450	0.06%	0.008%
66	11.756	1747	1750	1752	rBV2	358	342	0.05%	0.006%
67	11.976	1784	1786	1788	rVV2	807	743	0.10%	0.013%
68	12.024	1788	1794	1809	rVV	363739	478614	66.84%	8.550%
69	12.140	1811	1813	1818	rVB2	438	480	0.07%	0.009%
70	12.219	1824	1826	1829	rBV3	195	248	0.03%	0.004%
71	12.317	1837	1842	1851	rBV	355886	478446	66.82%	8.547%
72	12.640	1893	1895	1898	rVB2	337	288	0.04%	0.005%
73	12.762	1911	1915	1920	rVB3	397	702	0.10%	0.013%
74	12.896	1936	1937	1941	rBV	246	243	0.03%	0.004%
75	13.024	1956	1958	1963	rBV2	213	283	0.04%	0.005%
76	13.170	1979	1982	1985	rBV	231	323	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121823\
 Data File : VX039303.D
 Acq On : 18 Dec 2023 11:59
 Operator : JC/MD
 Sample : 05823-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

77	13.219	1988	1990	1993	rVV2	243	225	0.03%	0.004%
78	13.286	1999	2001	2004	rVB	282	250	0.03%	0.004%
79	13.591	2049	2051	2056	rVB4	816	930	0.13%	0.017%
80	13.780	2079	2082	2085	rVV	676	846	0.12%	0.015%
81	13.963	2109	2112	2115	rBV2	492	596	0.08%	0.011%
82	14.073	2128	2130	2132	rBV	288	262	0.04%	0.005%
83	14.128	2134	2139	2148	rVB3	622	989	0.14%	0.018%
84	14.219	2151	2154	2155	rBV	227	261	0.04%	0.005%
85	14.384	2180	2181	2184	rVB	276	213	0.03%	0.004%
86	14.445	2187	2191	2192	rBV	346	271	0.04%	0.005%
87	14.493	2198	2199	2202	rBV3	256	286	0.04%	0.005%
88	14.591	2212	2215	2218	rBV2	193	211	0.03%	0.004%
89	14.756	2240	2242	2244	rBV2	327	285	0.04%	0.005%
90	14.798	2247	2249	2250	rVB	305	195	0.03%	0.003%
91	14.823	2250	2253	2254	rBV2	283	248	0.03%	0.004%
92	14.865	2254	2260	2262	rBV3	304	444	0.06%	0.008%
93	15.341	2336	2338	2344	rVB2	247	399	0.06%	0.007%
94	15.390	2344	2346	2351	rBV3	641	900	0.13%	0.016%
95	15.560	2372	2374	2377	rVB2	454	324	0.05%	0.006%
96	16.054	2453	2455	2460	rBV3	292	406	0.06%	0.007%
97	16.176	2473	2475	2478	rBV2	305	191	0.03%	0.003%
98	16.207	2478	2480	2484	rBV	221	309	0.04%	0.006%
99	16.255	2486	2488	2492	rBV2	315	335	0.05%	0.006%
100	16.731	2565	2566	2568	rBV	397	227	0.03%	0.004%




Sum of corrected areas: 5597814

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121823\
Data File : VX039303.D
Acq On : 18 Dec 2023 11:59
Operator : JC/MD
Sample : 05823-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

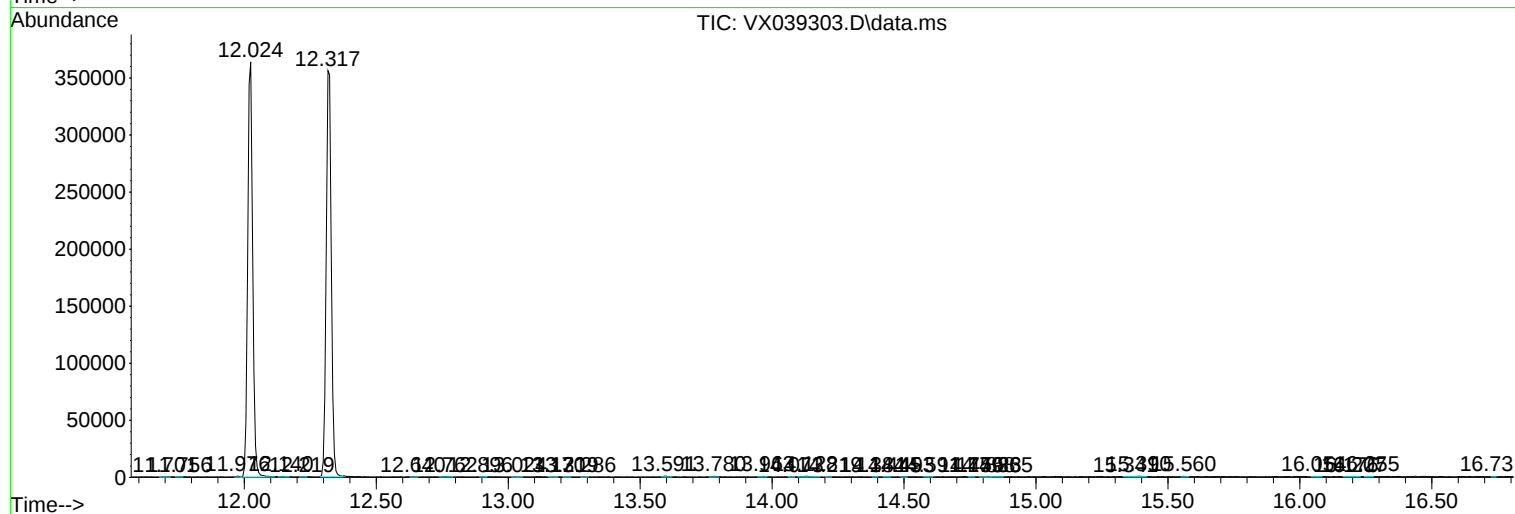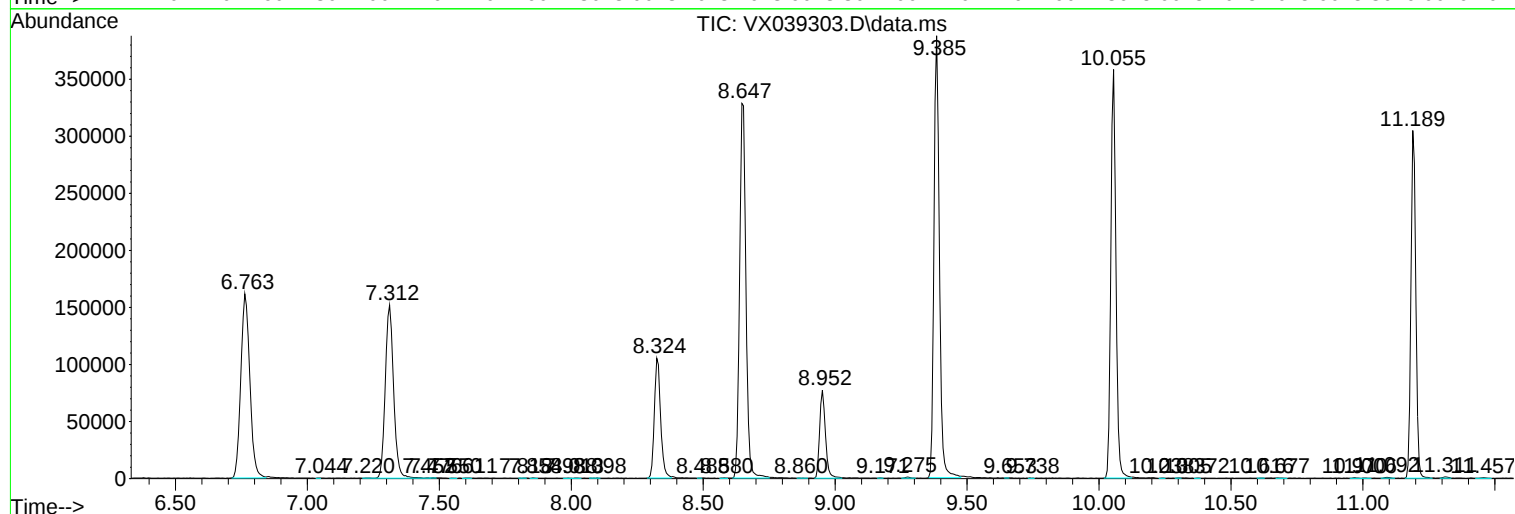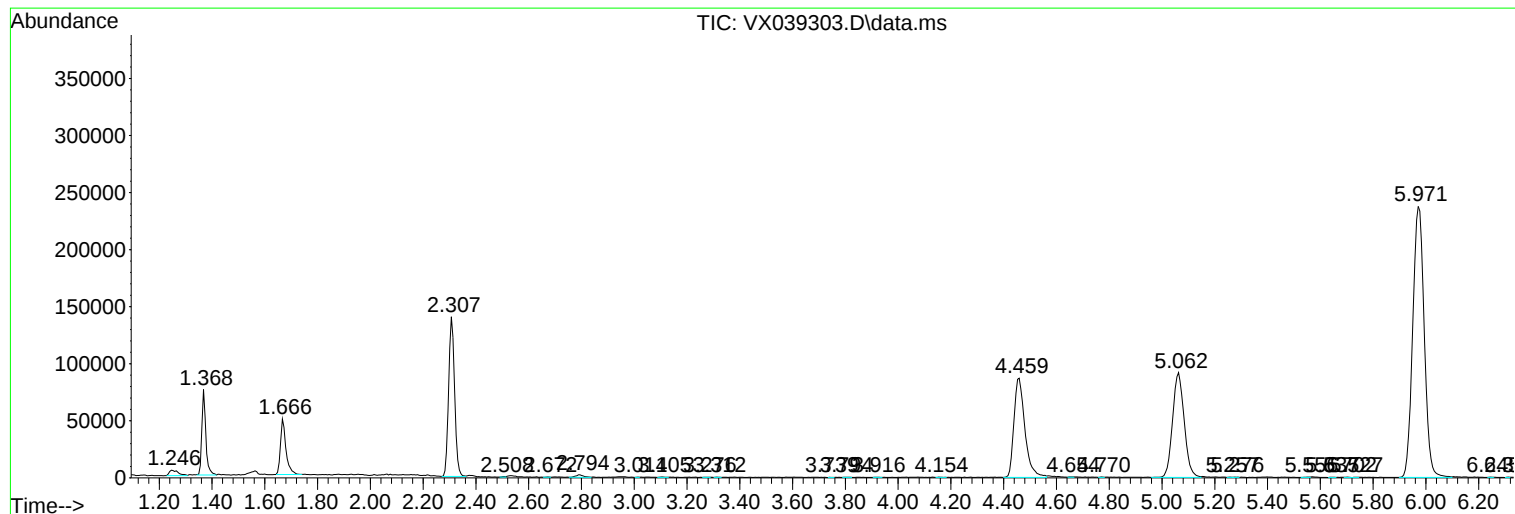

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121823\
Data File : VX039303.D
Acq On : 18 Dec 2023 11:59
Operator : JC/MD
Sample : 05823-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121823\
Data File : VX039303.D
Acq On : 18 Dec 2023 11:59
Operator : JC/MD
Sample : 05823-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc