

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121823\
 Data File : VX039312.D
 Acq On : 18 Dec 2023 15:27
 Operator : JC/MD
 Sample : 05807-15 50X
 Misc : 1.92g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0B00

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

Signal : TIC: VX039312.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	57	rBV	110816	115356	11.55%	1.476%
2	1.666	91	95	110	rVB	75242	106120	10.62%	1.358%
3	2.307	193	200	210	rBV	205993	317284	31.76%	4.059%
4	2.691	259	263	264	rBV	310	459	0.05%	0.006%
5	2.794	274	280	287	rBV4	1623	3141	0.31%	0.040%
6	2.947	297	305	314	rBV	7004	16182	1.62%	0.207%
7	3.184	342	344	348	rVB2	282	293	0.03%	0.004%
8	3.270	355	358	361	rBV2	204	322	0.03%	0.004%
9	3.380	375	376	379	rBV	233	217	0.02%	0.003%
10	3.422	381	383	386	rBV2	286	286	0.03%	0.004%
11	3.562	401	406	409	rBV2	329	664	0.07%	0.008%
12	3.825	447	449	451	rBV2	199	229	0.02%	0.003%
13	4.135	498	500	501	rBV2	207	159	0.02%	0.002%
14	4.392	538	542	543	rBV	285	241	0.02%	0.003%
15	4.453	544	552	565	rBV	96963	269943	27.03%	3.453%
16	4.794	606	608	610	rVB	360	229	0.02%	0.003%
17	4.824	611	613	616	rVB	565	519	0.05%	0.007%
18	4.849	616	617	620	rBV2	354	337	0.03%	0.004%
19	5.056	640	651	667	rBV	123593	381285	38.17%	4.877%
20	5.300	687	691	693	rBV2	165	257	0.03%	0.003%
21	5.385	700	705	706	rBV3	520	682	0.07%	0.009%
22	5.465	715	718	719	rBV2	215	153	0.02%	0.002%
23	5.483	719	721	725	rVB2	172	184	0.02%	0.002%
24	5.568	733	735	737	rBV3	368	422	0.04%	0.005%
25	5.971	789	801	823	rBV2	328496	998849	100.00%	12.778%
26	6.178	833	835	836	rVB	436	259	0.03%	0.003%
27	6.227	840	843	845	rBV3	251	349	0.03%	0.004%
28	6.300	852	855	856	rVB3	236	224	0.02%	0.003%
29	6.367	864	866	867	rVB	229	147	0.01%	0.002%
30	6.416	872	874	877	rBV2	212	191	0.02%	0.002%
31	6.446	877	879	881	rBV	198	194	0.02%	0.002%
32	6.556	895	897	899	rVB	261	193	0.02%	0.002%
33	6.598	902	904	909	rBV2	250	248	0.02%	0.003%
34	6.641	909	911	913	rBV2	276	230	0.02%	0.003%
35	6.763	921	931	951	rBV	246689	592385	59.31%	7.578%
36	7.117	984	989	1000	rVB4	1745	4118	0.41%	0.053%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121823\
 Data File : VX039312.D
 Acq On : 18 Dec 2023 15:27
 Operator : JC/MD
 Sample : 05807-15 50X
 Misc : 1.92g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0B00

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
 Title : VOC Analysis

37	7.202	1000	1003	1006	rBV2	207	226	0.02%	0.003%
38	7.306	1012	1020	1036	rBV	202252	449397	44.99%	5.749%
39	7.934	1121	1123	1124	rBV	331	181	0.02%	0.002%
40	8.324	1181	1187	1200	rBV	139128	230893	23.12%	2.954%
41	8.580	1226	1229	1234	rBV4	471	893	0.09%	0.011%
42	8.647	1234	1240	1261	rBV	492566	780044	78.09%	9.979%
43	8.952	1284	1290	1300	rBV	102848	152194	15.24%	1.947%
44	9.202	1329	1331	1332	rBV	213	187	0.02%	0.002%
45	9.269	1340	1342	1348	rVB2	573	782	0.08%	0.010%
46	9.385	1355	1361	1374	rBV	447907	629233	63.00%	8.049%
47	9.702	1408	1413	1416	rBV3	1064	1567	0.16%	0.020%
48	9.836	1433	1435	1436	rBV2	247	215	0.02%	0.003%
49	9.970	1455	1457	1462	rBV	293	267	0.03%	0.003%
50	10.055	1465	1471	1488	rBV2	525964	865828	86.68%	11.076%
51	10.397	1524	1527	1529	rVB2	257	205	0.02%	0.003%
52	10.476	1539	1540	1543	rVB	361	190	0.02%	0.002%
53	10.579	1555	1557	1562	rVB2	211	300	0.03%	0.004%
54	10.647	1562	1568	1574	rBV3	592	1196	0.12%	0.015%
55	10.909	1609	1611	1612	rBV	282	158	0.02%	0.002%
56	10.927	1612	1614	1616	rVV2	225	148	0.01%	0.002%
57	10.970	1616	1621	1625	rVV3	467	767	0.08%	0.010%
58	11.085	1638	1640	1644	rVV3	844	1138	0.11%	0.015%
59	11.189	1652	1657	1668	rBV	367842	485884	48.64%	6.216%
60	11.415	1691	1694	1696	rBV	196	241	0.02%	0.003%
61	11.457	1699	1701	1703	rVB	579	427	0.04%	0.005%
62	11.634	1727	1730	1732	rBV2	241	310	0.03%	0.004%
63	11.671	1732	1736	1737	rVV	183	203	0.02%	0.003%
64	11.719	1742	1744	1746	rVB2	280	188	0.02%	0.002%
65	11.750	1746	1749	1756	rBV2	568	921	0.09%	0.012%
66	11.799	1756	1757	1759	rBV	177	158	0.02%	0.002%
67	11.976	1783	1786	1788	rBV2	465	579	0.06%	0.007%
68	12.024	1788	1794	1804	rBV	541040	717583	71.84%	9.180%
69	12.317	1837	1842	1858	rBV	520777	671209	67.20%	8.586%
70	12.421	1858	1859	1862	rVB	585	323	0.03%	0.004%
71	12.445	1862	1863	1865	rBV	312	178	0.02%	0.002%
72	12.518	1873	1875	1876	rBV	370	257	0.03%	0.003%
73	12.616	1888	1891	1892	rBV2	219	227	0.02%	0.003%
74	12.719	1905	1908	1909	rVB	205	148	0.01%	0.002%
75	12.738	1909	1911	1912	rBV	303	219	0.02%	0.003%
76	12.963	1945	1948	1949	rBV2	203	181	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121823\
 Data File : VX039312.D
 Acq On : 18 Dec 2023 15:27
 Operator : JC/MD
 Sample : 05807-15 50X
 Misc : 1.92g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0B00

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

77	13.055	1962	1963	1967	rVB2	232	243	0.02%	0.003%
78	13.268	1995	1998	1999	rBV	371	251	0.03%	0.003%
79	13.323	2006	2007	2009	rBV	322	155	0.02%	0.002%
80	13.487	2031	2034	2036	rVB2	243	237	0.02%	0.003%
81	13.591	2047	2051	2056	rBV4	1093	1438	0.14%	0.018%
82	13.628	2056	2057	2060	rBV	294	220	0.02%	0.003%
83	13.731	2072	2074	2077	rVB2	209	236	0.02%	0.003%
84	13.847	2091	2093	2094	rBV2	234	169	0.02%	0.002%
85	13.963	2110	2112	2113	rVV2	365	306	0.03%	0.004%
86	14.006	2116	2119	2120	rBV2	141	154	0.02%	0.002%
87	14.109	2133	2136	2137	rVV2	263	342	0.03%	0.004%
88	14.128	2137	2139	2144	rVV	1268	1592	0.16%	0.020%
89	14.201	2148	2151	2153	rVB	260	230	0.02%	0.003%
90	14.335	2171	2173	2175	rBV2	211	208	0.02%	0.003%
91	14.420	2184	2187	2188	rBV2	240	252	0.03%	0.003%
92	14.756	2236	2242	2247	rBV5	546	1442	0.14%	0.018%
93	15.152	2305	2307	2310	rBV2	248	256	0.03%	0.003%
94	15.255	2322	2324	2325	rBV	285	220	0.02%	0.003%
95	15.469	2357	2359	2361	rBV2	321	240	0.02%	0.003%
96	15.560	2372	2374	2375	rBV	373	159	0.02%	0.002%
97	16.213	2478	2481	2484	rBV2	272	375	0.04%	0.005%
98	16.359	2504	2505	2507	rVB	552	306	0.03%	0.004%
99	16.475	2523	2524	2528	rBV2	326	285	0.03%	0.004%
100	16.773	2571	2573	2575	rBV2	396	316	0.03%	0.004%

Sum of corrected areas: 7817228




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121823\
Data File : VX039312.D
Acq On : 18 Dec 2023 15:27
Operator : JC/MD
Sample : 05807-15 50X
Misc : 1.92g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0B00

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

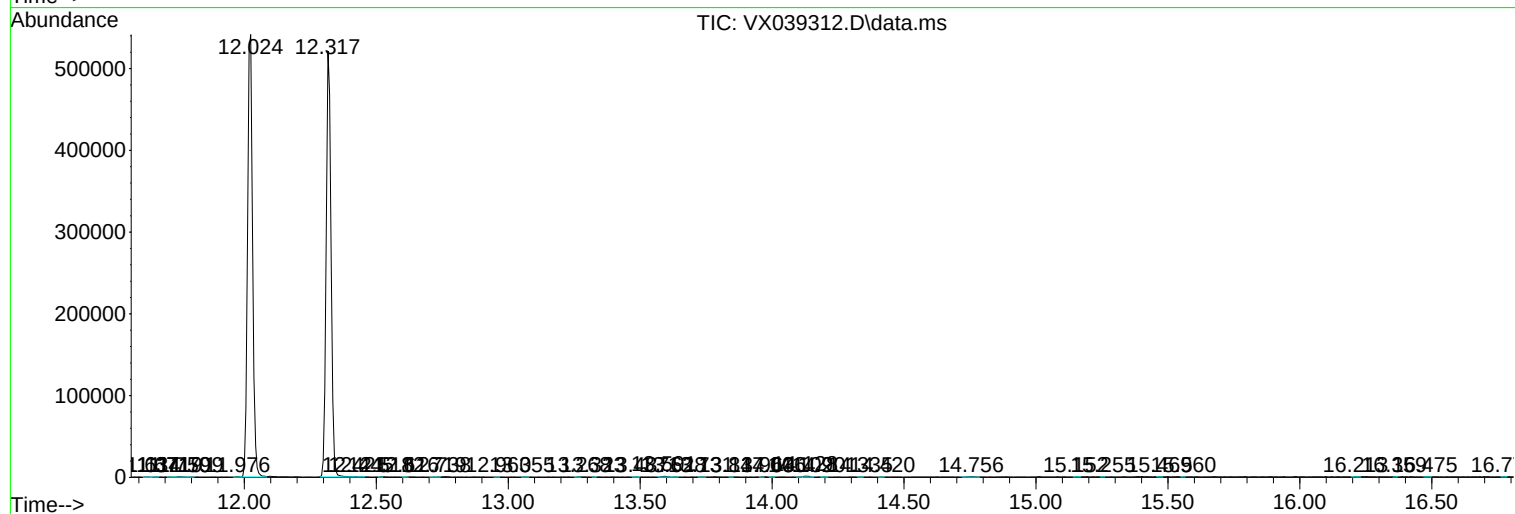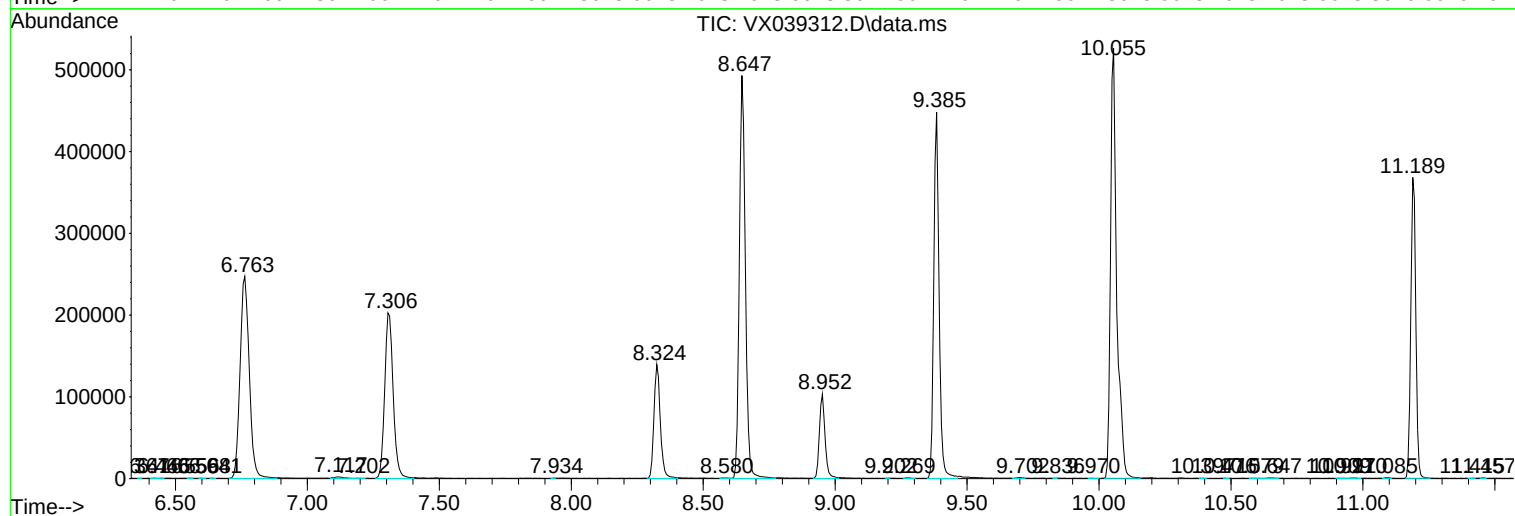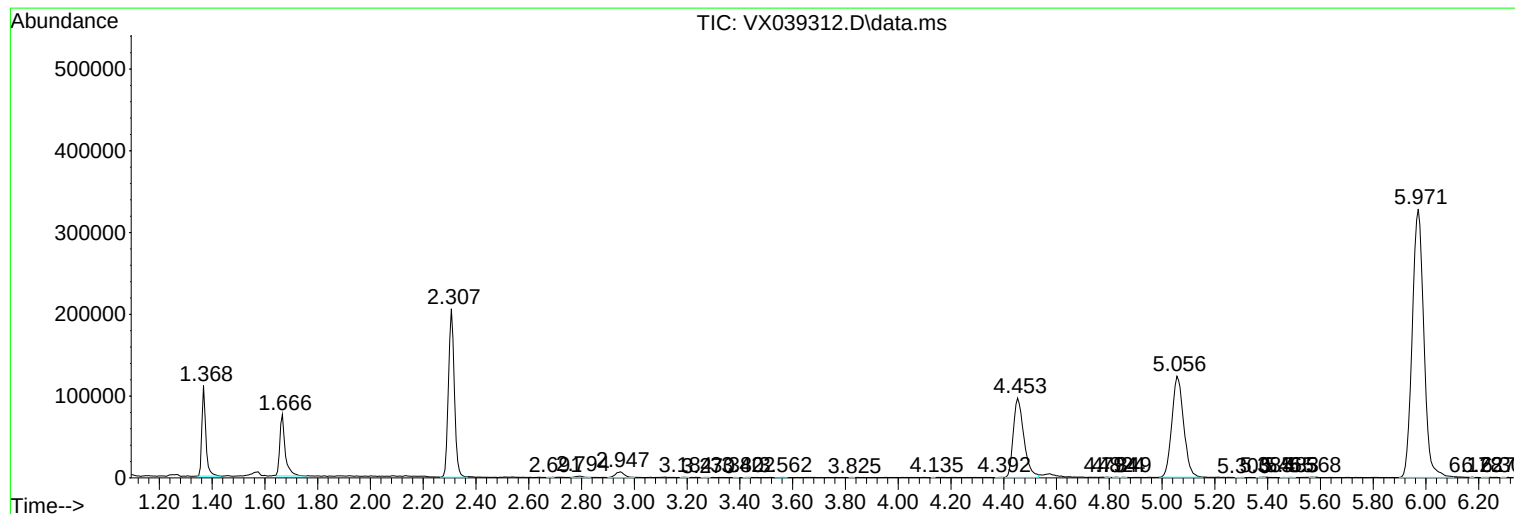

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121823\
Data File : VX039312.D
Acq On : 18 Dec 2023 15:27
Operator : JC/MD
Sample : 05807-15 50X
Misc : 1.92g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0B00

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121823\
Data File : VX039312.D
Acq On : 18 Dec 2023 15:27
Operator : JC/MD
Sample : 05807-15 50X
Misc : 1.92g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0B00

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc