

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121823\
 Data File : VX039313.D
 Acq On : 18 Dec 2023 15:50
 Operator : JC/MD
 Sample : 05807-16 50X
 Misc : 4.97g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0B01

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M

Title : VOC Analysis

Signal : TIC: VX039313.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.367	43	46	61	rVB	105351	111725	11.80%	1.500%
2	1.666	90	95	106	rBV	70888	103183	10.90%	1.386%
3	2.306	194	200	212	rVB	195819	306324	32.34%	4.113%
4	2.605	247	249	252	rBV2	191	206	0.02%	0.003%
5	2.794	275	280	285	rBV4	1758	3223	0.34%	0.043%
6	2.861	285	291	299	rVV2	8420	17000	1.80%	0.228%
7	2.946	299	305	314	rVB2	4878	10816	1.14%	0.145%
8	3.099	329	330	332	rBV2	300	253	0.03%	0.003%
9	3.123	332	334	338	rVB2	419	341	0.04%	0.005%
10	3.251	353	355	358	rVB	259	294	0.03%	0.004%
11	3.373	372	375	377	rVV2	232	269	0.03%	0.004%
12	3.623	411	416	417	rBV	196	251	0.03%	0.003%
13	3.702	426	429	431	rVV	190	178	0.02%	0.002%
14	4.068	487	489	490	rBV	223	169	0.02%	0.002%
15	4.208	510	512	514	rBV	234	200	0.02%	0.003%
16	4.355	532	536	537	rBV	251	323	0.03%	0.004%
17	4.452	544	552	567	rBV	94764	268726	28.37%	3.609%
18	4.781	604	606	607	rBV	239	203	0.02%	0.003%
19	5.062	639	652	671	rVV	117787	368953	38.96%	4.954%
20	5.214	673	677	680	rVB2	346	627	0.07%	0.008%
21	5.312	690	693	695	rBV	325	312	0.03%	0.004%
22	5.556	731	733	736	rVB	357	270	0.03%	0.004%
23	5.696	754	756	757	rVB2	264	167	0.02%	0.002%
24	5.708	757	758	761	rBV	194	189	0.02%	0.003%
25	5.970	789	801	818	rBV2	317337	947067	100.00%	12.718%
26	6.220	840	842	844	rVB	303	200	0.02%	0.003%
27	6.244	844	846	847	rVB2	323	194	0.02%	0.003%
28	6.305	853	856	859	rBV2	241	393	0.04%	0.005%
29	6.549	894	896	898	rVB	211	198	0.02%	0.003%
30	6.580	898	901	903	rBV	199	200	0.02%	0.003%
31	6.763	921	931	944	rBV	235139	565402	59.70%	7.592%
32	6.994	967	969	971	rBV2	302	214	0.02%	0.003%
33	7.074	980	982	984	rVB2	231	192	0.02%	0.003%
34	7.110	984	988	989	rBV2	1442	1847	0.20%	0.025%
35	7.311	1012	1021	1037	rBV	193136	433444	45.77%	5.820%
36	7.598	1064	1068	1069	rBV2	299	354	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121823\
 Data File : VX039313.D
 Acq On : 18 Dec 2023 15:50
 Operator : JC/MD
 Sample : 05807-16 50X
 Misc : 4.97g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0B01

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
 Title : VOC Analysis

37	7.775	1095	1097	1100	rBV	332	258	0.03%	0.003%
38	7.921	1118	1121	1123	rBV2	110	160	0.02%	0.002%
39	8.000	1132	1134	1137	rBV	210	176	0.02%	0.002%
40	8.110	1150	1152	1157	rBV	268	400	0.04%	0.005%
41	8.323	1180	1187	1206	rBV	137469	226837	23.95%	3.046%
42	8.646	1234	1240	1256	rBV	460290	746934	78.87%	10.030%
43	8.872	1275	1277	1280	rVB2	294	177	0.02%	0.002%
44	8.896	1280	1281	1284	rVB	200	175	0.02%	0.002%
45	8.951	1284	1290	1305	rBV	98481	148851	15.72%	1.999%
46	9.250	1335	1339	1340	rBV2	146	175	0.02%	0.002%
47	9.281	1340	1344	1347	rVB2	740	779	0.08%	0.010%
48	9.384	1356	1361	1373	rBV	435777	618990	65.36%	8.312%
49	9.646	1401	1404	1406	rBV	233	322	0.03%	0.004%
50	9.701	1409	1413	1418	rVB3	875	1266	0.13%	0.017%
51	9.823	1430	1433	1434	rBV2	265	275	0.03%	0.004%
52	9.854	1437	1438	1441	rVV	250	261	0.03%	0.004%
53	10.055	1465	1471	1484	rVV	500636	698956	73.80%	9.386%
54	10.256	1501	1504	1506	rBV	316	357	0.04%	0.005%
55	10.494	1539	1543	1546	rVV2	184	262	0.03%	0.004%
56	10.561	1553	1554	1557	rVB	272	195	0.02%	0.003%
57	10.719	1578	1580	1583	rBV2	168	199	0.02%	0.003%
58	10.805	1592	1594	1596	rBV	236	189	0.02%	0.003%
59	10.963	1617	1620	1622	rBV3	246	302	0.03%	0.004%
60	11.091	1638	1641	1647	rVB4	631	980	0.10%	0.013%
61	11.189	1652	1657	1672	rVB	370065	477294	50.40%	6.409%
62	11.372	1686	1687	1688	rBV	321	163	0.02%	0.002%
63	11.622	1725	1728	1729	rBV2	295	292	0.03%	0.004%
64	11.646	1730	1732	1734	rVB	188	160	0.02%	0.002%
65	11.707	1739	1742	1745	rVV2	267	303	0.03%	0.004%
66	11.762	1747	1751	1755	rVB3	652	877	0.09%	0.012%
67	11.847	1761	1765	1766	rBV	185	237	0.03%	0.003%
68	11.975	1784	1786	1788	rBV	643	609	0.06%	0.008%
69	12.024	1788	1794	1807	rVV	541367	702193	74.14%	9.429%
70	12.323	1837	1843	1853	rBV	487208	650585	68.69%	8.736%
71	12.585	1883	1886	1888	rBV	166	214	0.02%	0.003%
72	12.762	1913	1915	1920	rVB3	569	744	0.08%	0.010%
73	12.823	1923	1925	1926	rVB	255	167	0.02%	0.002%
74	12.841	1926	1928	1929	rBV	260	205	0.02%	0.003%
75	12.932	1941	1943	1944	rBV	215	170	0.02%	0.002%
76	12.951	1944	1946	1949	rVB2	193	232	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121823\
 Data File : VX039313.D
 Acq On : 18 Dec 2023 15:50
 Operator : JC/MD
 Sample : 05807-16 50X
 Misc : 4.97g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0B01

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M

Title : VOC Analysis

77	13.085	1966	1968	1969	rBV2	230	203	0.02%	0.003%
78	13.170	1979	1982	1983	rVB	205	163	0.02%	0.002%
79	13.255	1994	1996	1998	rVV2	176	215	0.02%	0.003%
80	13.304	2002	2004	2005	rBV	274	167	0.02%	0.002%
81	13.390	2016	2018	2022	rBV2	171	258	0.03%	0.003%
82	13.591	2047	2051	2056	rBV2	8093	11131	1.18%	0.149%
83	13.755	2076	2078	2079	rBV2	184	175	0.02%	0.002%
84	13.883	2096	2099	2103	rBV2	224	315	0.03%	0.004%
85	13.963	2107	2112	2120	rVB4	1971	2623	0.28%	0.035%
86	14.097	2132	2134	2136	rBV2	188	177	0.02%	0.002%
87	14.127	2136	2139	2143	rVV	1374	1899	0.20%	0.026%
88	14.225	2151	2155	2158	rBV2	190	289	0.03%	0.004%
89	14.438	2186	2190	2193	rBV2	292	480	0.05%	0.006%
90	14.517	2202	2203	2205	rBV	290	209	0.02%	0.003%
91	14.700	2231	2233	2234	rVB2	332	160	0.02%	0.002%
92	14.749	2239	2241	2242	rBV	341	251	0.03%	0.003%
93	15.395	2344	2347	2350	rVB4	568	784	0.08%	0.011%
94	15.462	2356	2358	2359	rBV	229	181	0.02%	0.002%
95	15.481	2359	2361	2363	rVB2	391	305	0.03%	0.004%
96	15.664	2389	2391	2394	rBV3	329	286	0.03%	0.004%
97	15.816	2414	2416	2417	rVB	357	188	0.02%	0.003%
98	16.072	2456	2458	2460	rBV2	268	232	0.02%	0.003%
99	16.230	2482	2484	2485	rVV	331	185	0.02%	0.002%
100	16.755	2568	2570	2571	rBV	392	249	0.03%	0.003%

Sum of corrected areas: 7446953


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121823\
Data File : VX039313.D
Acq On : 18 Dec 2023 15:50
Operator : JC/MD
Sample : 05807-16 50X
Misc : 4.97g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0B01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

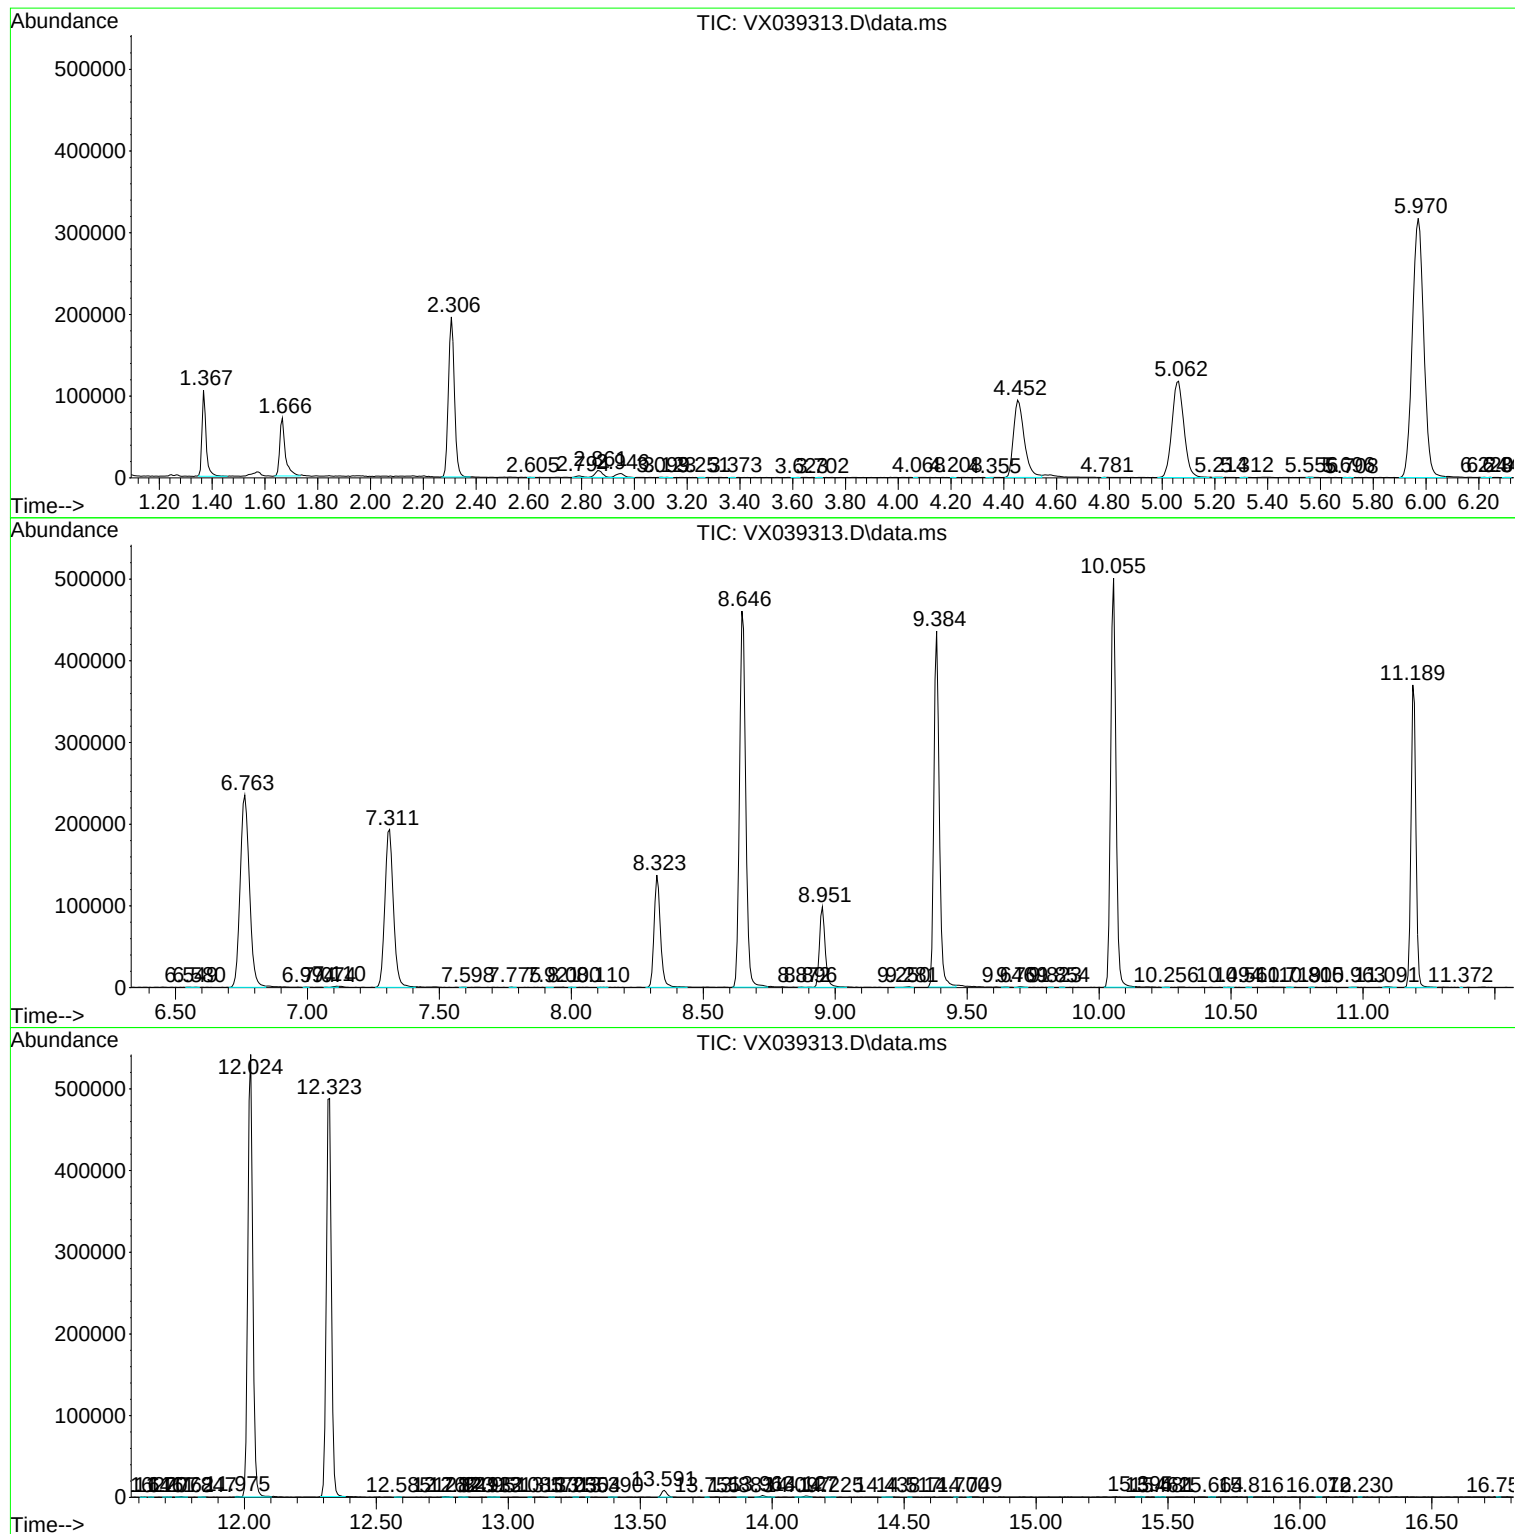

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121823\
Data File : VX039313.D
Acq On : 18 Dec 2023 15:50
Operator : JC/MD
Sample : 05807-16 50X
Misc : 4.97g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0B01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121823\
Data File : VX039313.D
Acq On : 18 Dec 2023 15:50
Operator : JC/MD
Sample : 05807-16 50X
Misc : 4.97g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0B01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
