

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121823\
 Data File : VX039317.D
 Acq On : 18 Dec 2023 17:23
 Operator : JC/MD
 Sample : 05807-18 50X
 Misc : 2.36g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0B19

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

Signal : TIC: VX039317.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	55	rBV	101360	106207	6.65%	1.275%
2	1.666	90	95	105	rBV	65723	96362	6.04%	1.157%
3	2.307	193	200	210	rBV	189970	298687	18.71%	3.586%
4	2.514	230	234	237	rVB2	1154	1650	0.10%	0.020%
5	2.666	256	259	262	rBV2	344	542	0.03%	0.007%
6	2.794	275	280	288	rVB3	1696	4003	0.25%	0.048%
7	2.947	298	305	314	rVB	5645	12495	0.78%	0.150%
8	3.520	396	399	401	rBV2	229	265	0.02%	0.003%
9	3.636	415	418	421	rBV2	317	377	0.02%	0.005%
10	3.745	434	436	437	rVV	367	230	0.01%	0.003%
11	3.776	439	441	443	rVV2	306	255	0.02%	0.003%
12	3.800	443	445	449	rVV2	161	249	0.02%	0.003%
13	3.849	451	453	456	rBV	367	261	0.02%	0.003%
14	3.892	456	460	461	rBV2	169	185	0.01%	0.002%
15	4.154	502	503	505	rBV	189	170	0.01%	0.002%
16	4.453	543	552	567	rBV	94626	268707	16.83%	3.226%
17	4.715	593	595	600	rVB2	432	570	0.04%	0.007%
18	4.885	621	623	625	rVB	317	201	0.01%	0.002%
19	5.056	639	651	668	rBV	116078	364771	22.85%	4.379%
20	5.233	679	680	682	rVB2	356	166	0.01%	0.002%
21	5.257	682	684	686	rVB2	435	420	0.03%	0.005%
22	5.282	686	688	689	rBV2	288	288	0.02%	0.003%
23	5.379	701	704	705	rBV3	316	376	0.02%	0.005%
24	5.471	714	719	721	rBV3	545	896	0.06%	0.011%
25	5.599	738	740	744	rVB2	184	170	0.01%	0.002%
26	5.739	761	763	766	rVB2	191	167	0.01%	0.002%
27	5.800	772	773	775	rBV2	272	183	0.01%	0.002%
28	5.873	781	785	788	rBV2	154	270	0.02%	0.003%
29	5.971	788	801	809	rBV2	309002	935743	58.61%	11.234%
30	6.239	843	845	847	rVB2	292	238	0.01%	0.003%
31	6.263	847	849	850	rBV	242	178	0.01%	0.002%
32	6.300	853	855	858	rVV2	218	255	0.02%	0.003%
33	6.531	890	893	894	rBV	176	176	0.01%	0.002%
34	6.550	894	896	899	rVV2	253	309	0.02%	0.004%
35	6.763	921	931	950	rBV	237307	571423	35.79%	6.860%
36	7.123	983	990	996	rBV7	1606	3939	0.25%	0.047%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121823\
 Data File : VX039317.D
 Acq On : 18 Dec 2023 17:23
 Operator : JC/MD
 Sample : 05807-18 50X
 Misc : 2.36g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0B19

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
 Title : VOC Analysis

37	7.312	1011	1021	1040	rBV	189370	430231	26.95%	5.165%
38	7.489	1046	1050	1051	rBV3	631	910	0.06%	0.011%
39	7.751	1091	1093	1098	rVB2	190	184	0.01%	0.002%
40	7.818	1103	1104	1109	rBV	236	206	0.01%	0.002%
41	7.891	1113	1116	1117	rBV2	214	236	0.01%	0.003%
42	7.958	1124	1127	1131	rVB3	269	420	0.03%	0.005%
43	8.025	1136	1138	1140	rBV2	230	236	0.01%	0.003%
44	8.062	1142	1144	1148	rVB	225	243	0.02%	0.003%
45	8.110	1148	1152	1155	rVB2	206	329	0.02%	0.004%
46	8.324	1181	1187	1199	rBV	131446	220580	13.82%	2.648%
47	8.574	1226	1228	1234	rBV2	523	522	0.03%	0.006%
48	8.647	1234	1240	1249	rBV	455833	721408	45.19%	8.661%
49	8.891	1278	1280	1283	rVB2	285	307	0.02%	0.004%
50	8.952	1284	1290	1302	rBV	94690	145118	9.09%	1.742%
51	9.275	1340	1343	1347	rVB4	1020	1407	0.09%	0.017%
52	9.385	1355	1361	1375	rBV	430341	620895	38.89%	7.454%
53	9.604	1395	1397	1402	rVB2	430	482	0.03%	0.006%
54	9.696	1409	1412	1419	rVB4	620	1151	0.07%	0.014%
55	9.854	1434	1438	1439	rBV	273	310	0.02%	0.004%
56	9.885	1441	1443	1446	rBV2	264	262	0.02%	0.003%
57	10.055	1465	1471	1488	rBV	512277	779960	48.85%	9.364%
58	10.195	1492	1494	1499	rVB2	997	1298	0.08%	0.016%
59	10.269	1504	1506	1509	rBV2	180	170	0.01%	0.002%
60	10.317	1509	1514	1517	rVV2	853	1332	0.08%	0.016%
61	10.372	1521	1523	1524	rVB	332	172	0.01%	0.002%
62	10.488	1540	1542	1545	rBV	206	217	0.01%	0.003%
63	10.653	1565	1569	1575	rBV3	865	1703	0.11%	0.020%
64	10.927	1612	1614	1615	rBV	245	186	0.01%	0.002%
65	10.964	1616	1620	1625	rVB3	1060	1525	0.10%	0.018%
66	11.092	1639	1641	1646	rVB3	719	924	0.06%	0.011%
67	11.189	1652	1657	1666	rBV	363577	466714	29.23%	5.603%
68	11.366	1683	1686	1690	rBV2	998	1232	0.08%	0.015%
69	11.457	1697	1701	1705	rVV2	1349	1573	0.10%	0.019%
70	11.756	1747	1750	1755	rBV2	1263	1704	0.11%	0.020%
71	11.969	1780	1785	1788	rBV2	1523	2065	0.13%	0.025%
72	12.037	1788	1796	1806	rBV2	749210	1596559	100.00%	19.168%
73	12.317	1837	1842	1850	rBV	499230	637323	39.92%	7.651%
74	12.768	1911	1916	1921	rBV	670	918	0.06%	0.011%
75	12.811	1921	1923	1926	rVV	268	234	0.01%	0.003%
76	12.878	1932	1934	1936	rVV2	232	199	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121823\
 Data File : VX039317.D
 Acq On : 18 Dec 2023 17:23
 Operator : JC/MD
 Sample : 05807-18 50X
 Misc : 2.36g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0B19

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

77	13.116	1969	1973	1979	rBV3	1266	1717	0.11%	0.021%
78	13.225	1989	1991	1994	rVB2	271	175	0.01%	0.002%
79	13.402	2017	2020	2022	rBV2	263	304	0.02%	0.004%
80	13.512	2035	2038	2039	rBV2	186	226	0.01%	0.003%
81	13.591	2048	2051	2054	rBV2	2470	2630	0.16%	0.032%
82	13.689	2065	2067	2070	rVB2	279	242	0.02%	0.003%
83	13.780	2078	2082	2088	rVB2	1882	2516	0.16%	0.030%
84	13.872	2095	2097	2099	rBV	379	324	0.02%	0.004%
85	13.969	2106	2113	2120	rBV4	1467	2403	0.15%	0.029%
86	14.134	2136	2140	2143	rVB	1403	1826	0.11%	0.022%
87	14.201	2150	2151	2154	rBV	167	190	0.01%	0.002%
88	14.359	2176	2177	2180	rVB2	372	245	0.02%	0.003%
89	14.390	2180	2182	2185	rBV	186	208	0.01%	0.002%
90	14.445	2190	2191	2193	rBV2	272	189	0.01%	0.002%
91	14.500	2199	2200	2203	rBV2	283	201	0.01%	0.002%
92	14.945	2269	2273	2275	rBV3	242	349	0.02%	0.004%
93	14.975	2275	2278	2279	rVV2	369	314	0.02%	0.004%
94	15.518	2363	2367	2369	rBV3	413	434	0.03%	0.005%
95	15.566	2373	2375	2376	rBV	318	275	0.02%	0.003%
96	15.987	2441	2444	2446	rBV2	297	348	0.02%	0.004%
97	16.072	2456	2458	2460	rVB2	490	334	0.02%	0.004%
98	16.298	2493	2495	2499	rVB	826	591	0.04%	0.007%
99	16.389	2508	2510	2513	rBV3	403	364	0.02%	0.004%
100	16.524	2530	2532	2533	rBV2	344	263	0.02%	0.003%




Sum of corrected areas: 8329497

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121823\
Data File : VX039317.D
Acq On : 18 Dec 2023 17:23
Operator : JC/MD
Sample : 05807-18 50X
Misc : 2.36g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0B19

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

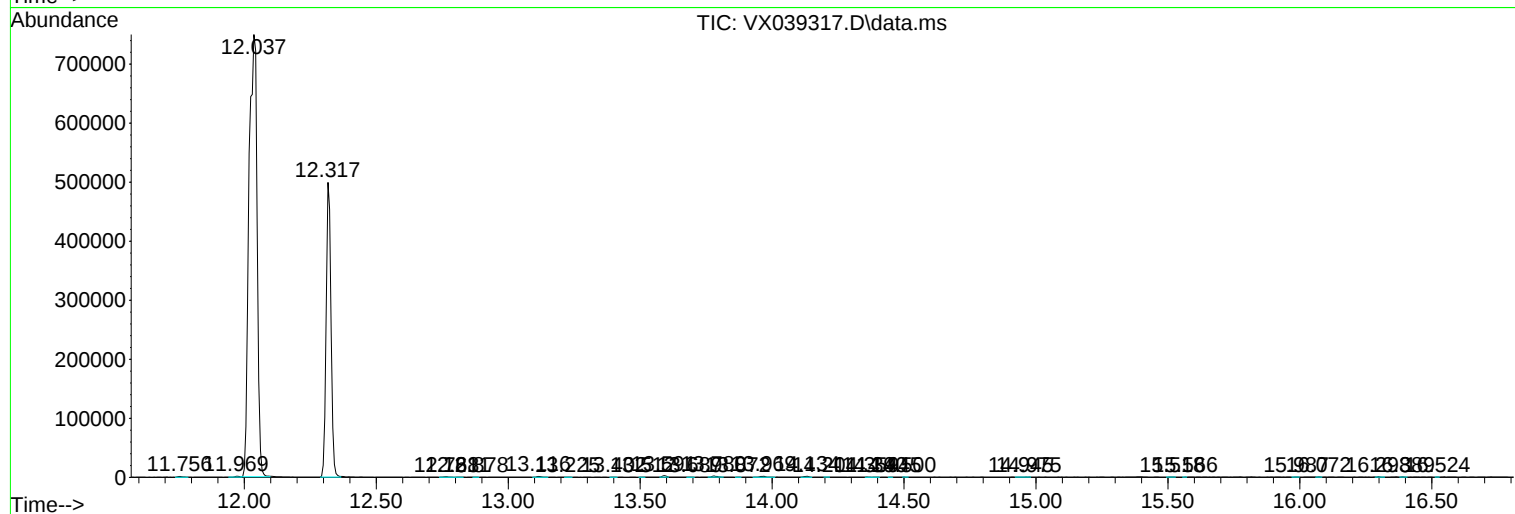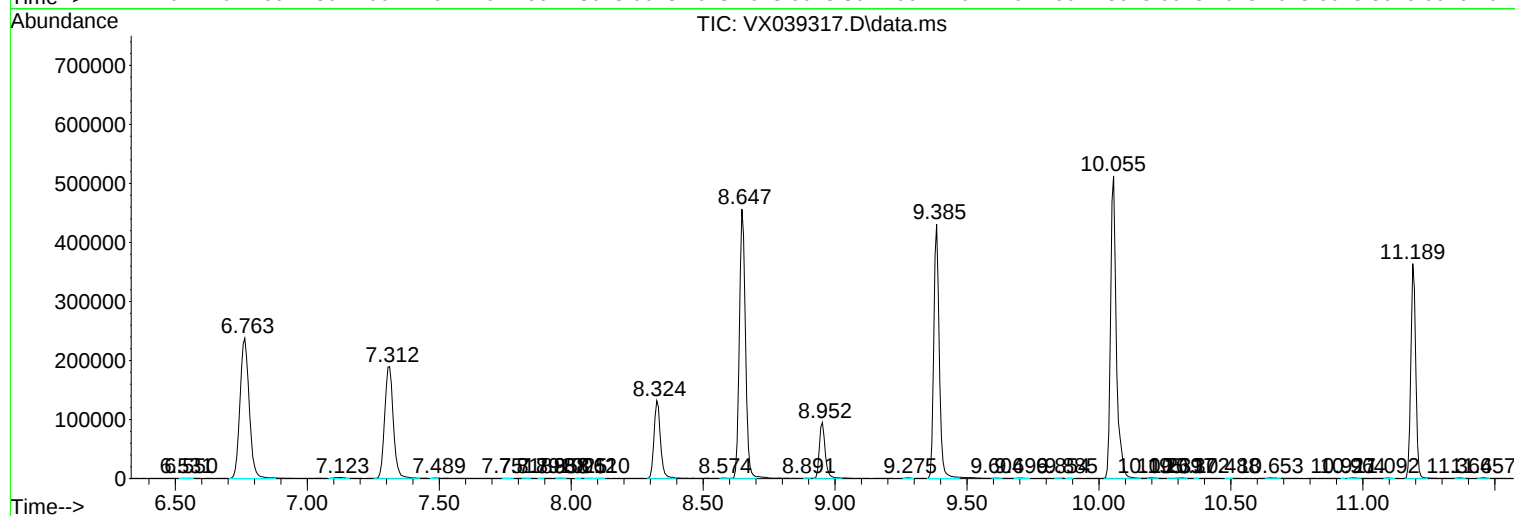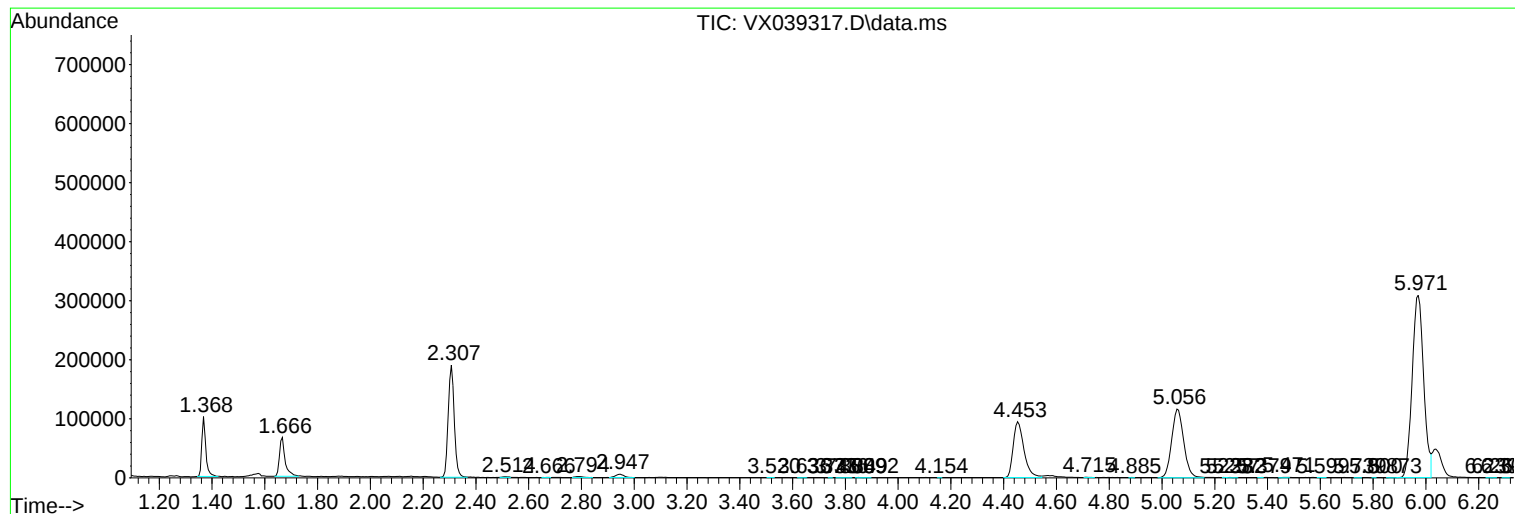

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121823\
Data File : VX039317.D
Acq On : 18 Dec 2023 17:23
Operator : JC/MD
Sample : 05807-18 50X
Misc : 2.36g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0B19

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121823\
Data File : VX039317.D
Acq On : 18 Dec 2023 17:23
Operator : JC/MD
Sample : 05807-18 50X
Misc : 2.36g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0B19

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc