

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121823\
 Data File : VX039318.D
 Acq On : 18 Dec 2023 17:46
 Operator : JC/MD
 Sample : 05807-19 50X
 Misc : 1.82g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0B20

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

Signal : TIC: VX039318.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	56	rBV	99202	106324	11.85%	1.474%
2	1.666	90	95	109	rVB	63085	96802	10.79%	1.342%
3	2.306	194	200	210	rBV	182002	288021	32.10%	3.992%
4	2.508	231	233	234	rBV	578	319	0.04%	0.004%
5	2.788	274	279	286	rBV5	1978	3616	0.40%	0.050%
6	2.947	298	305	314	rVB	5271	12471	1.39%	0.173%
7	3.038	318	320	323	rBV	262	228	0.03%	0.003%
8	3.093	327	329	330	rBV2	458	345	0.04%	0.005%
9	3.453	384	388	391	rBV2	309	401	0.04%	0.006%
10	3.514	396	398	400	rVV	233	244	0.03%	0.003%
11	3.550	402	404	407	rVB2	307	365	0.04%	0.005%
12	3.587	407	410	411	rBV	187	237	0.03%	0.003%
13	3.611	413	414	417	rVB2	285	199	0.02%	0.003%
14	3.776	440	441	444	rBV2	305	229	0.03%	0.003%
15	3.977	471	474	475	rBV2	174	212	0.02%	0.003%
16	4.019	477	481	482	rBV2	183	277	0.03%	0.004%
17	4.141	498	501	504	rBV2	196	255	0.03%	0.004%
18	4.361	536	537	539	rBV	311	208	0.02%	0.003%
19	4.452	543	552	565	rBV	89923	257144	28.66%	3.564%
20	4.885	621	623	625	rVB	365	214	0.02%	0.003%
21	4.916	625	628	629	rBV2	304	256	0.03%	0.004%
22	4.977	636	638	639	rBV	306	182	0.02%	0.003%
23	5.056	639	651	671	rVV	111450	352449	39.28%	4.885%
24	5.397	702	707	710	rVB3	508	891	0.10%	0.012%
25	5.440	710	714	715	rBV	236	334	0.04%	0.005%
26	5.470	715	719	724	rVB3	479	734	0.08%	0.010%
27	5.531	726	729	730	rBV	207	210	0.02%	0.003%
28	5.623	741	744	746	rBV	149	197	0.02%	0.003%
29	5.830	776	778	780	rVB2	256	212	0.02%	0.003%
30	5.861	780	783	785	rBV	261	198	0.02%	0.003%
31	5.970	789	801	808	rBV2	304204	897273	100.00%	12.436%
32	6.348	862	863	867	rVV	196	235	0.03%	0.003%
33	6.482	884	885	889	rVB	322	207	0.02%	0.003%
34	6.763	921	931	953	rBV	231362	556500	62.02%	7.713%
35	7.123	984	990	998	rVB3	1463	3547	0.40%	0.049%
36	7.312	1012	1021	1040	rBV	181885	409830	45.68%	5.680%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121823\
 Data File : VX039318.D
 Acq On : 18 Dec 2023 17:46
 Operator : JC/MD
 Sample : 05807-19 50X
 Misc : 1.82g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0B20

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
 Title : VOC Analysis

37	7.690	1081	1083	1087	rVB	180	196	0.02%	0.003%
38	7.757	1092	1094	1097	rVV2	238	205	0.02%	0.003%
39	7.958	1125	1127	1130	rVV3	377	397	0.04%	0.006%
40	8.025	1137	1138	1141	rBV	211	218	0.02%	0.003%
41	8.104	1149	1151	1154	rBV2	200	210	0.02%	0.003%
42	8.171	1160	1162	1164	rBV	207	225	0.03%	0.003%
43	8.275	1176	1179	1181	rVB2	305	382	0.04%	0.005%
44	8.324	1181	1187	1195	rBV	125138	209703	23.37%	2.906%
45	8.647	1234	1240	1264	rBV	444830	708523	78.96%	9.820%
46	8.952	1284	1290	1301	rBV	91749	140823	15.69%	1.952%
47	9.061	1307	1308	1312	rVB3	365	327	0.04%	0.005%
48	9.110	1312	1316	1318	rVB2	257	252	0.03%	0.003%
49	9.177	1323	1327	1330	rVB2	296	437	0.05%	0.006%
50	9.208	1330	1332	1334	rBV	292	291	0.03%	0.004%
51	9.275	1340	1343	1348	rVB3	684	1038	0.12%	0.014%
52	9.323	1348	1351	1354	rBV	304	334	0.04%	0.005%
53	9.384	1356	1361	1376	rBV	427547	595731	66.39%	8.257%
54	9.665	1405	1407	1410	rBV2	311	406	0.05%	0.006%
55	9.701	1410	1413	1417	rVV3	1048	1419	0.16%	0.020%
56	9.756	1420	1422	1425	rBV3	293	328	0.04%	0.005%
57	9.866	1438	1440	1441	rVB	485	285	0.03%	0.004%
58	9.988	1456	1460	1461	rVB2	162	189	0.02%	0.003%
59	10.055	1465	1471	1473	rBV	505286	735055	81.92%	10.188%
60	10.268	1502	1506	1508	rVB	349	251	0.03%	0.003%
61	10.299	1509	1511	1512	rBV	453	315	0.04%	0.004%
62	10.537	1549	1550	1554	rVB	346	243	0.03%	0.003%
63	10.579	1554	1557	1558	rBV	301	296	0.03%	0.004%
64	10.659	1565	1570	1574	rVB4	690	1396	0.16%	0.019%
65	10.841	1598	1600	1602	rBV	283	263	0.03%	0.004%
66	10.969	1615	1621	1622	rBV3	894	1276	0.14%	0.018%
67	11.091	1639	1641	1645	rVB3	591	616	0.07%	0.009%
68	11.146	1648	1650	1652	rBV2	219	248	0.03%	0.003%
69	11.189	1652	1657	1668	rBV	352503	459109	51.17%	6.363%
70	11.354	1682	1684	1686	rBV2	196	208	0.02%	0.003%
71	11.396	1690	1691	1695	rVV2	149	193	0.02%	0.003%
72	11.457	1698	1701	1705	rVB2	681	1002	0.11%	0.014%
73	11.567	1717	1719	1721	rBV2	220	215	0.02%	0.003%
74	11.640	1729	1731	1733	rBV2	201	185	0.02%	0.003%
75	11.756	1746	1750	1754	rBV	927	1188	0.13%	0.016%
76	11.969	1781	1785	1788	rBV2	3187	3926	0.44%	0.054%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121823\
 Data File : VX039318.D
 Acq On : 18 Dec 2023 17:46
 Operator : JC/MD
 Sample : 05807-19 50X
 Misc : 1.82g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0B20

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

77	12.024	1788	1794	1804	rVB	530690	716503	79.85%	9.931%
78	12.244	1828	1830	1833	rVB2	246	210	0.02%	0.003%
79	12.317	1837	1842	1850	rBV	472668	626746	69.85%	8.687%
80	12.548	1876	1880	1883	rVB2	288	431	0.05%	0.006%
81	12.676	1899	1901	1903	rBV	262	188	0.02%	0.003%
82	12.805	1918	1922	1925	rVB2	237	203	0.02%	0.003%
83	12.987	1950	1952	1954	rBV2	184	215	0.02%	0.003%
84	13.122	1970	1974	1979	rVB3	721	913	0.10%	0.013%
85	13.189	1983	1985	1988	rVB2	190	207	0.02%	0.003%
86	13.591	2049	2051	2057	rVV3	1493	1646	0.18%	0.023%
87	13.780	2079	2082	2088	rBV2	874	1613	0.18%	0.022%
88	13.969	2109	2113	2116	rBV	886	1010	0.11%	0.014%
89	14.127	2136	2139	2145	rVB	1471	1868	0.21%	0.026%
90	14.219	2153	2154	2157	rBV	354	349	0.04%	0.005%
91	14.347	2172	2175	2176	rBV2	326	241	0.03%	0.003%
92	14.518	2201	2203	2205	rBV	284	207	0.02%	0.003%
93	14.670	2226	2228	2230	rVV2	222	211	0.02%	0.003%
94	14.737	2234	2239	2240	rBV2	363	547	0.06%	0.008%
95	15.072	2292	2294	2297	rVB2	268	191	0.02%	0.003%
96	15.359	2336	2341	2342	rBV2	317	416	0.05%	0.006%
97	15.389	2343	2346	2353	rVB4	875	1310	0.15%	0.018%
98	15.456	2355	2357	2358	rVB2	348	210	0.02%	0.003%
99	15.822	2416	2417	2419	rBV	255	186	0.02%	0.003%
100	16.371	2506	2507	2510	rBV2	319	187	0.02%	0.003%


Sum of corrected areas: 7215078

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121823\
Data File : VX039318.D
Acq On : 18 Dec 2023 17:46
Operator : JC/MD
Sample : 05807-19 50X
Misc : 1.82g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0B20

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

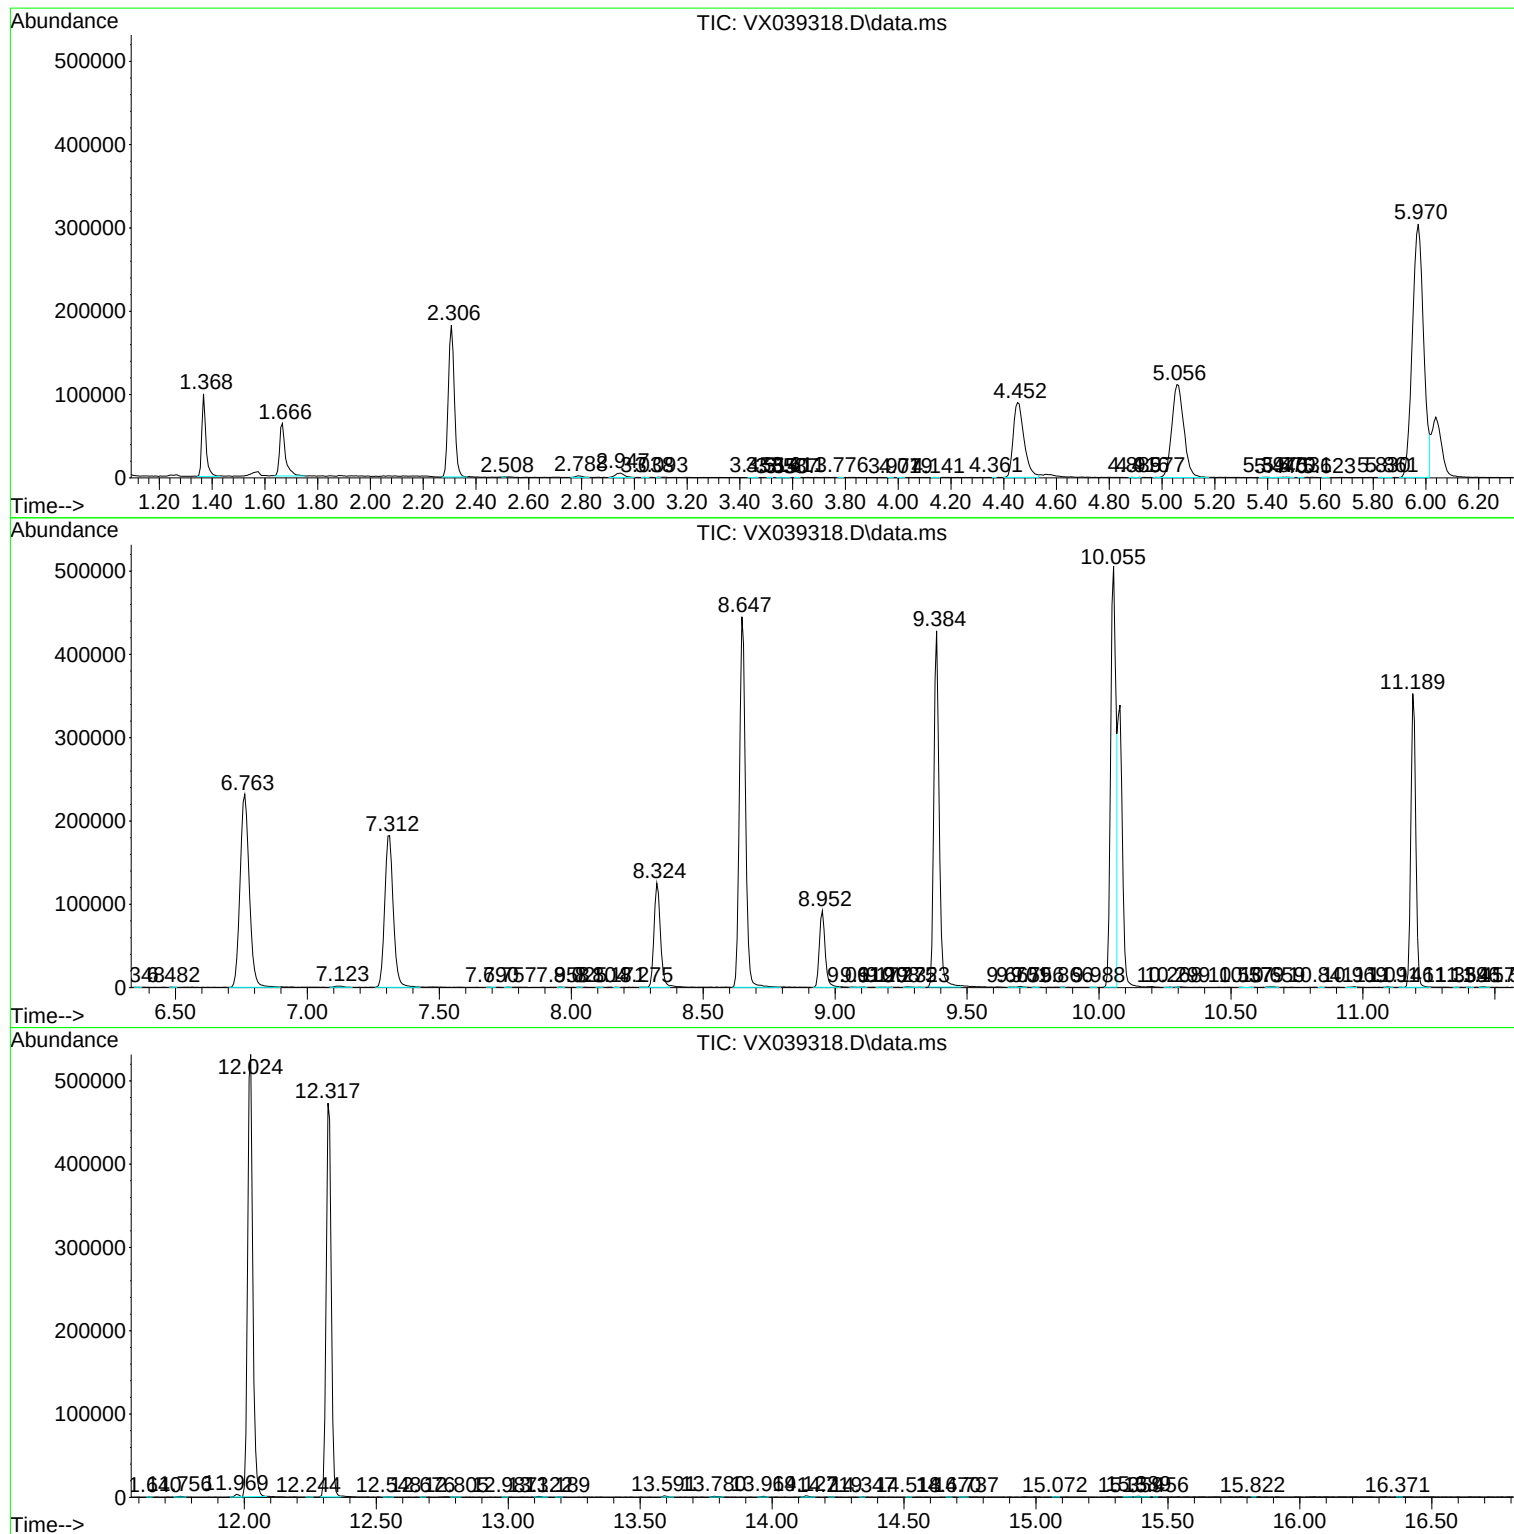

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121823\
Data File : VX039318.D
Acq On : 18 Dec 2023 17:46
Operator : JC/MD
Sample : 05807-19 50X
Misc : 1.82g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0B20

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121823\
Data File : VX039318.D
Acq On : 18 Dec 2023 17:46
Operator : JC/MD
Sample : 05807-19 50X
Misc : 1.82g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0B20

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc