

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121823\
 Data File : VX039319.D
 Acq On : 18 Dec 2023 18:09
 Operator : JC/MD
 Sample : 05823-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

Signal : TIC: VX039319.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	57	rVB	101302	106942	11.69%	1.461%
2	1.666	91	95	107	rVB	65334	95826	10.48%	1.309%
3	2.306	194	200	211	rBV	185578	289811	31.69%	3.960%
4	2.502	230	232	233	rBV2	506	481	0.05%	0.007%
5	2.745	270	272	274	rBV2	255	224	0.02%	0.003%
6	2.788	274	279	286	rVV3	2662	4529	0.50%	0.062%
7	2.880	291	294	296	rVB	266	270	0.03%	0.004%
8	2.898	296	297	299	rBV	279	213	0.02%	0.003%
9	2.940	299	304	309	rBV3	600	1328	0.15%	0.018%
10	3.343	368	370	372	rBV	254	244	0.03%	0.003%
11	3.483	391	393	395	rVB	402	285	0.03%	0.004%
12	3.910	461	463	465	rBV	208	206	0.02%	0.003%
13	3.928	465	466	469	rVB	345	217	0.02%	0.003%
14	3.965	469	472	475	rBV	402	506	0.06%	0.007%
15	4.209	510	512	517	rBV2	158	263	0.03%	0.004%
16	4.452	542	552	568	rBV	94603	272733	29.83%	3.726%
17	4.672	587	588	591	rBV2	360	272	0.03%	0.004%
18	4.739	597	599	602	rBV2	205	197	0.02%	0.003%
19	5.056	640	651	669	rBV	112981	359609	39.33%	4.913%
20	5.294	688	690	693	rBV2	281	242	0.03%	0.003%
21	5.318	693	694	697	rVB	293	208	0.02%	0.003%
22	5.391	704	706	711	rVB2	370	478	0.05%	0.007%
23	5.452	712	716	718	rBV2	279	346	0.04%	0.005%
24	5.550	729	732	733	rBV3	333	303	0.03%	0.004%
25	5.641	745	747	750	rBV2	247	301	0.03%	0.004%
26	5.672	750	752	756	rVB	309	299	0.03%	0.004%
27	5.970	789	801	819	rBV2	303695	914428	100.00%	12.494%
28	6.220	840	842	846	rBV2	345	541	0.06%	0.007%
29	6.440	876	878	880	rVB	408	262	0.03%	0.004%
30	6.629	906	909	912	rBV2	229	347	0.04%	0.005%
31	6.763	922	931	946	rBV	239842	570618	62.40%	7.797%
32	7.117	984	989	997	rVB7	1485	3679	0.40%	0.050%
33	7.306	1012	1020	1037	rBV	190430	421978	46.15%	5.766%
34	7.684	1079	1082	1084	rVV	200	236	0.03%	0.003%
35	7.799	1100	1101	1103	rBV	384	268	0.03%	0.004%
36	7.946	1123	1125	1127	rBV	218	203	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121823\
 Data File : VX039319.D
 Acq On : 18 Dec 2023 18:09
 Operator : JC/MD
 Sample : 05823-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

37	8.141	1155	1157	1159	rBV2	226	176	0.02%	0.002%
38	8.324	1181	1187	1202	rBV	131159	217888	23.83%	2.977%
39	8.580	1226	1229	1234	rBV3	527	789	0.09%	0.011%
40	8.647	1234	1240	1250	rBV	443279	711967	77.86%	9.728%
41	8.854	1272	1274	1280	rBB2	263	356	0.04%	0.005%
42	8.952	1284	1290	1303	rBV	98469	146614	16.03%	2.003%
43	9.092	1311	1313	1314	rBV	207	184	0.02%	0.003%
44	9.171	1323	1326	1327	rBV2	291	344	0.04%	0.005%
45	9.202	1329	1331	1332	rVV	238	181	0.02%	0.002%
46	9.275	1340	1343	1347	rBV3	744	738	0.08%	0.010%
47	9.384	1355	1361	1382	rBV	430009	632244	69.14%	8.639%
48	9.640	1401	1403	1407	rVB3	396	454	0.05%	0.006%
49	9.701	1411	1413	1416	rVV	351	339	0.04%	0.005%
50	9.738	1417	1419	1421	rVB2	312	183	0.02%	0.003%
51	9.860	1435	1439	1441	rVB	296	378	0.04%	0.005%
52	9.909	1443	1447	1448	rBV	211	243	0.03%	0.003%
53	10.055	1465	1471	1489	rBV	512802	711726	77.83%	9.724%
54	10.195	1492	1494	1498	rVV3	815	961	0.11%	0.013%
55	10.305	1510	1512	1513	rBV2	457	362	0.04%	0.005%
56	10.500	1541	1544	1545	rVB2	290	241	0.03%	0.003%
57	10.646	1563	1568	1569	rBV3	689	854	0.09%	0.012%
58	10.841	1598	1600	1601	rBV2	215	199	0.02%	0.003%
59	10.878	1605	1606	1609	rVV2	258	183	0.02%	0.003%
60	10.970	1617	1621	1626	rBV3	710	1051	0.11%	0.014%
61	11.091	1638	1641	1645	rVB3	576	839	0.09%	0.011%
62	11.189	1652	1657	1670	rBV	365967	472025	51.62%	6.449%
63	11.396	1689	1691	1693	rVB2	203	194	0.02%	0.003%
64	11.457	1696	1701	1704	rBV3	796	1158	0.13%	0.016%
65	11.713	1740	1743	1746	rVB2	188	273	0.03%	0.004%
66	11.750	1746	1749	1755	rBV3	653	1177	0.13%	0.016%
67	11.847	1763	1765	1767	rBV	166	188	0.02%	0.003%
68	11.975	1782	1786	1788	rBV4	1003	1212	0.13%	0.017%
69	12.024	1788	1794	1805	rVV	547316	709129	77.55%	9.689%
70	12.317	1837	1842	1854	rBV	499594	640991	70.10%	8.758%
71	12.591	1885	1887	1889	rBV2	270	231	0.03%	0.003%
72	12.658	1897	1898	1902	rBV2	202	188	0.02%	0.003%
73	12.756	1912	1914	1919	rVB	634	737	0.08%	0.010%
74	12.945	1944	1945	1948	rBV2	219	221	0.02%	0.003%
75	13.115	1970	1973	1980	rBV3	570	942	0.10%	0.013%
76	13.378	2014	2016	2017	rBV	341	196	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121823\
 Data File : VX039319.D
 Acq On : 18 Dec 2023 18:09
 Operator : JC/MD
 Sample : 05823-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
 Title : VOC Analysis

77	13.408	2020	2021	2024	rVV	331	213	0.02%	0.003%
78	13.457	2027	2029	2034	rVB2	175	209	0.02%	0.003%
79	13.597	2046	2052	2057	rBV4	1021	1644	0.18%	0.022%
80	13.707	2067	2070	2072	rBV	255	256	0.03%	0.003%
81	13.780	2080	2082	2088	rVB3	597	934	0.10%	0.013%
82	13.963	2110	2112	2116	rVB	799	746	0.08%	0.010%
83	14.134	2136	2140	2144	rVB	1093	1758	0.19%	0.024%
84	14.188	2147	2149	2152	rBV2	176	205	0.02%	0.003%
85	14.481	2195	2197	2199	rVB	207	174	0.02%	0.002%
86	14.566	2208	2211	2214	rBV2	258	419	0.05%	0.006%
87	14.676	2228	2229	2230	rBV	399	198	0.02%	0.003%
88	14.694	2230	2232	2233	rVV	332	197	0.02%	0.003%
89	14.725	2235	2237	2239	rBV	303	217	0.02%	0.003%
90	14.804	2248	2250	2252	rVB	309	230	0.03%	0.003%
91	14.847	2255	2257	2259	rBV2	263	208	0.02%	0.003%
92	15.060	2290	2292	2294	rBV	218	216	0.02%	0.003%
93	15.200	2313	2315	2316	rBV2	293	201	0.02%	0.003%
94	15.389	2342	2346	2352	rBV5	853	1522	0.17%	0.021%
95	15.511	2363	2366	2367	rBV2	280	282	0.03%	0.004%
96	15.633	2384	2386	2388	rVB2	339	236	0.03%	0.003%
97	15.810	2413	2415	2417	rBV2	446	320	0.03%	0.004%
98	15.828	2417	2418	2421	rVV2	356	257	0.03%	0.004%
99	16.395	2507	2511	2513	rBV2	334	543	0.06%	0.007%
100	16.682	2555	2558	2560	rBV3	324	462	0.05%	0.006%




Sum of corrected areas: 7318896

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121823\
Data File : VX039319.D
Acq On : 18 Dec 2023 18:09
Operator : JC/MD
Sample : 05823-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

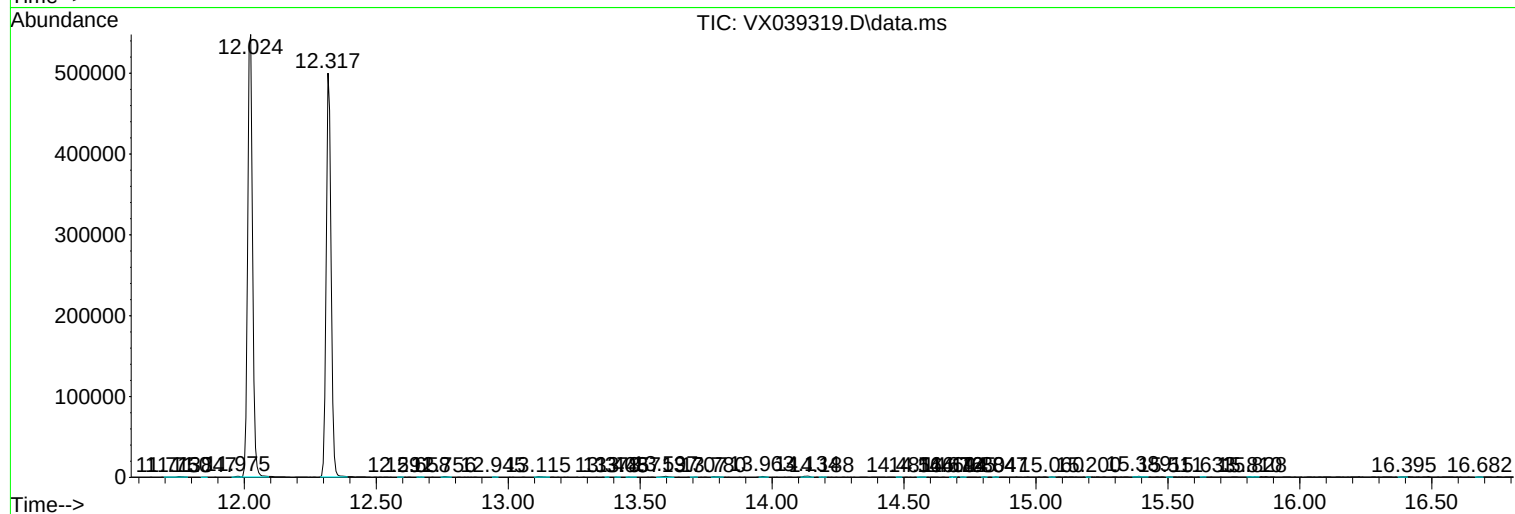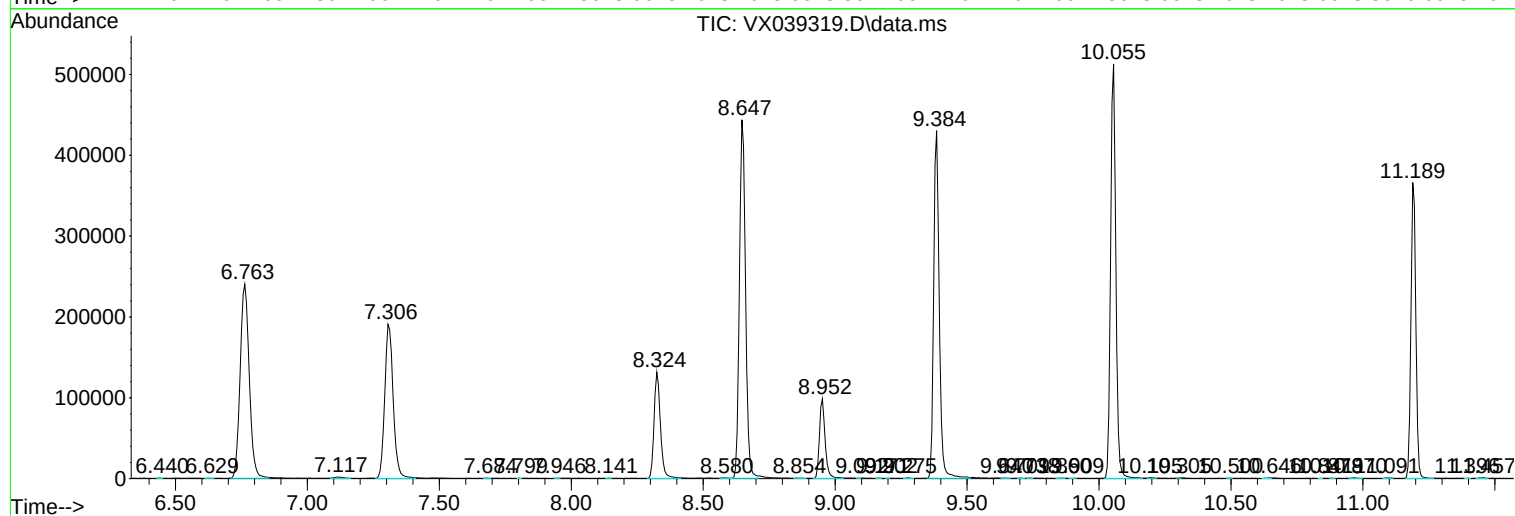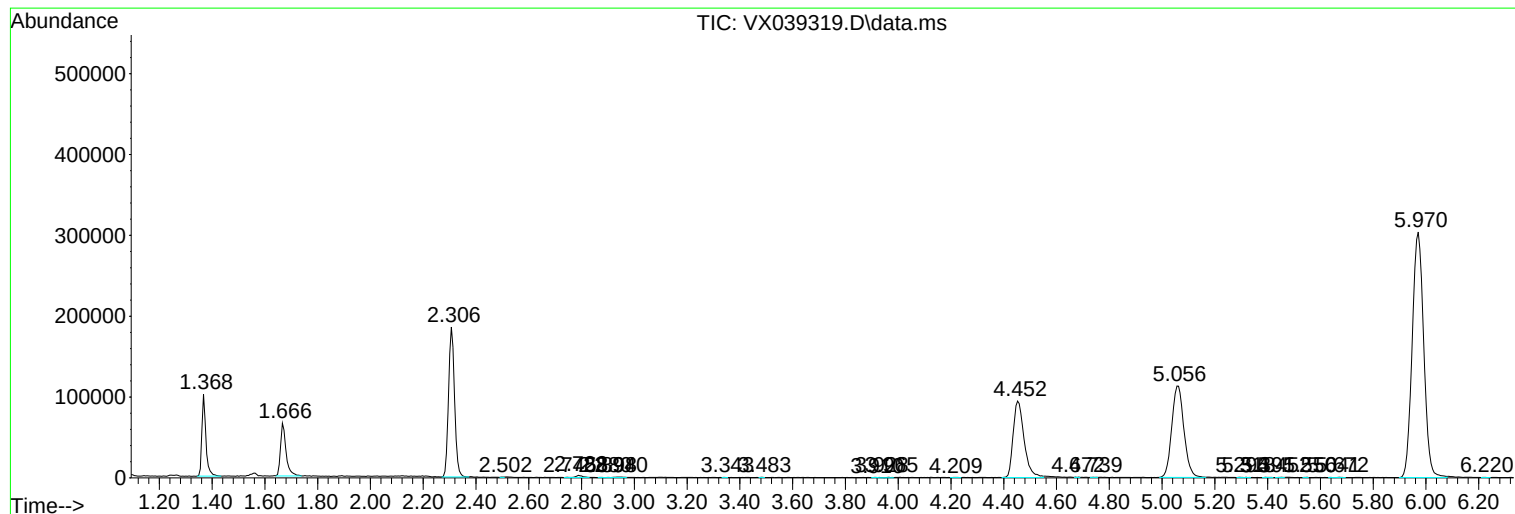

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121823\
Data File : VX039319.D
Acq On : 18 Dec 2023 18:09
Operator : JC/MD
Sample : 05823-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121823\
Data File : VX039319.D
Acq On : 18 Dec 2023 18:09
Operator : JC/MD
Sample : 05823-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc