

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121823\
 Data File : VX039321.D
 Acq On : 18 Dec 2023 18:55
 Operator : JC/MD
 Sample : 05835-04 100X
 Misc : 4.22g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0B34

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M

Title : VOC Analysis

Signal : TIC: VX039321.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	58	rVB	104119	109523	11.40%	1.457%
2	1.666	90	95	107	rBV	72340	100716	10.48%	1.340%
3	2.307	194	200	210	rBV	192632	302641	31.50%	4.026%
4	2.672	259	260	262	rBV	228	178	0.02%	0.002%
5	2.703	262	265	267	rVV	263	327	0.03%	0.004%
6	2.727	267	269	270	rVV2	410	250	0.03%	0.003%
7	2.752	270	273	274	rVV	264	242	0.03%	0.003%
8	2.788	274	279	284	rVV2	1945	3580	0.37%	0.048%
9	2.947	298	305	314	rVB2	5376	12916	1.34%	0.172%
10	3.184	342	344	347	rVB	220	217	0.02%	0.003%
11	3.373	373	375	376	rBV	226	190	0.02%	0.003%
12	3.514	396	398	399	rBV	216	192	0.02%	0.003%
13	3.904	459	462	464	rBV2	297	266	0.03%	0.004%
14	4.099	491	494	495	rBV2	228	176	0.02%	0.002%
15	4.160	502	504	506	rVB	257	207	0.02%	0.003%
16	4.178	506	507	509	rBV	300	199	0.02%	0.003%
17	4.215	511	513	516	rVB	374	295	0.03%	0.004%
18	4.257	516	520	521	rBV	328	337	0.04%	0.004%
19	4.453	543	552	565	rBV2	102345	291109	30.30%	3.872%
20	5.062	639	652	669	rBV	121697	381460	39.70%	5.074%
21	5.452	714	716	718	rBV2	180	231	0.02%	0.003%
22	5.532	727	729	730	rBV2	266	179	0.02%	0.002%
23	5.971	786	801	822	rBV2	323355	960873	100.00%	12.782%
24	6.446	877	879	882	rVB	474	335	0.03%	0.004%
25	6.489	882	886	888	rBV2	234	343	0.04%	0.005%
26	6.611	905	906	909	rBV	167	217	0.02%	0.003%
27	6.763	922	931	944	rBV	228474	553066	57.56%	7.357%
28	7.111	984	988	989	rBV2	1418	1708	0.18%	0.023%
29	7.306	1011	1020	1037	rBV	194201	441136	45.91%	5.868%
30	7.470	1045	1047	1050	rBV3	205	266	0.03%	0.004%
31	7.586	1061	1066	1069	rBV2	242	481	0.05%	0.006%
32	7.610	1069	1070	1076	rVB2	227	270	0.03%	0.004%
33	7.952	1124	1126	1128	rBV2	306	269	0.03%	0.004%
34	7.995	1131	1133	1136	rVB3	227	226	0.02%	0.003%
35	8.110	1149	1152	1155	rVB2	181	263	0.03%	0.003%
36	8.324	1180	1187	1203	rVV	137424	226897	23.61%	3.018%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121823\
 Data File : VX039321.D
 Acq On : 18 Dec 2023 18:55
 Operator : JC/MD
 Sample : 05835-04 100X
 Misc : 4.22g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0B34

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
 Title : VOC Analysis

37	8.580	1226	1229	1232	rVB	376	339	0.04%	0.005%
38	8.647	1234	1240	1258	rVV	459828	738345	76.84%	9.821%
39	8.897	1279	1281	1284	rBV	213	262	0.03%	0.003%
40	8.952	1284	1290	1301	rBV	102073	153420	15.97%	2.041%
41	9.074	1309	1310	1314	rBV3	352	395	0.04%	0.005%
42	9.281	1339	1344	1348	rBV3	599	927	0.10%	0.012%
43	9.385	1355	1361	1372	rBV	458927	663569	69.06%	8.827%
44	9.695	1408	1412	1416	rBV2	762	1080	0.11%	0.014%
45	9.756	1419	1422	1427	rBV2	287	469	0.05%	0.006%
46	9.830	1433	1434	1436	rBV	278	231	0.02%	0.003%
47	9.927	1449	1450	1455	rVB2	205	243	0.03%	0.003%
48	10.055	1465	1471	1487	rBV	486983	688476	71.65%	9.158%
49	10.195	1492	1494	1498	rVB3	904	767	0.08%	0.010%
50	10.470	1536	1539	1543	rBV2	236	366	0.04%	0.005%
51	10.506	1543	1545	1548	rVV	183	172	0.02%	0.002%
52	10.555	1548	1553	1554	rVB2	219	288	0.03%	0.004%
53	10.640	1563	1567	1568	rBV2	514	472	0.05%	0.006%
54	10.970	1617	1621	1627	rBV3	511	1084	0.11%	0.014%
55	11.085	1638	1640	1644	rBV3	332	468	0.05%	0.006%
56	11.189	1652	1657	1672	rVV	392993	504326	52.49%	6.709%
57	11.311	1675	1677	1680	rBV	250	193	0.02%	0.003%
58	11.451	1697	1700	1708	rVB3	621	1097	0.11%	0.015%
59	11.756	1747	1750	1757	rBV2	697	889	0.09%	0.012%
60	11.872	1767	1769	1772	rBV	249	358	0.04%	0.005%
61	11.902	1772	1774	1777	rVB	204	182	0.02%	0.002%
62	11.976	1783	1786	1788	rBV3	736	838	0.09%	0.011%
63	12.024	1788	1794	1804	rBV	505362	689386	71.75%	9.170%
64	12.317	1837	1842	1852	rBV	508415	663167	69.02%	8.821%
65	12.482	1867	1869	1872	rBV3	200	195	0.02%	0.003%
66	12.555	1878	1881	1883	rVB2	214	236	0.02%	0.003%
67	12.585	1883	1886	1887	rBV	237	177	0.02%	0.002%
68	12.603	1887	1889	1891	rBV	169	176	0.02%	0.002%
69	12.628	1891	1893	1896	rVB	275	244	0.03%	0.003%
70	12.664	1896	1899	1900	rBV2	194	223	0.02%	0.003%
71	12.756	1911	1914	1920	rVB3	581	951	0.10%	0.013%
72	12.853	1927	1930	1931	rBV	242	191	0.02%	0.003%
73	13.030	1957	1959	1962	rVB2	295	329	0.03%	0.004%
74	13.116	1969	1973	1977	rBV3	490	709	0.07%	0.009%
75	13.353	2011	2012	2015	rBV	398	240	0.02%	0.003%
76	13.439	2024	2026	2029	rVB2	218	186	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121823\
 Data File : VX039321.D
 Acq On : 18 Dec 2023 18:55
 Operator : JC/MD
 Sample : 05835-04 100X
 Misc : 4.22g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0B34

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

77	13.597	2048	2052	2057	rBV4	743	1069	0.11%	0.014%
78	13.683	2062	2066	2067	rVB2	222	286	0.03%	0.004%
79	13.780	2079	2082	2089	rVV2	557	871	0.09%	0.012%
80	13.957	2109	2111	2113	rBV3	572	518	0.05%	0.007%
81	14.054	2122	2127	2129	rBV2	146	303	0.03%	0.004%
82	14.128	2135	2139	2145	rVB2	1508	2096	0.22%	0.028%
83	14.262	2158	2161	2163	rBV	279	271	0.03%	0.004%
84	14.408	2181	2185	2189	rVB2	319	420	0.04%	0.006%
85	14.621	2218	2220	2223	rVB2	273	208	0.02%	0.003%
86	14.688	2229	2231	2234	rBV2	263	208	0.02%	0.003%
87	14.816	2250	2252	2254	rBV2	236	204	0.02%	0.003%
88	14.932	2269	2271	2273	rBV2	241	179	0.02%	0.002%
89	14.957	2273	2275	2279	rVB3	339	365	0.04%	0.005%
90	14.993	2279	2281	2283	rBV2	244	190	0.02%	0.003%
91	15.030	2285	2287	2289	rBV2	469	325	0.03%	0.004%
92	15.231	2316	2320	2321	rBV2	289	382	0.04%	0.005%
93	15.365	2340	2342	2343	rBV2	240	242	0.03%	0.003%
94	15.383	2343	2345	2346	rBV2	470	388	0.04%	0.005%
95	15.926	2432	2434	2435	rBV	272	183	0.02%	0.002%
96	16.005	2445	2447	2448	rVB	406	224	0.02%	0.003%
97	16.060	2453	2456	2457	rVB	317	238	0.02%	0.003%
98	16.127	2465	2467	2470	rBV2	276	299	0.03%	0.004%
99	16.304	2493	2496	2497	rBV2	317	350	0.04%	0.005%
100	16.335	2500	2501	2504	rBV2	401	399	0.04%	0.005%


Sum of corrected areas: 7517665

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121823\
Data File : VX039321.D
Acq On : 18 Dec 2023 18:55
Operator : JC/MD
Sample : 05835-04 100X
Misc : 4.22g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0B34

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

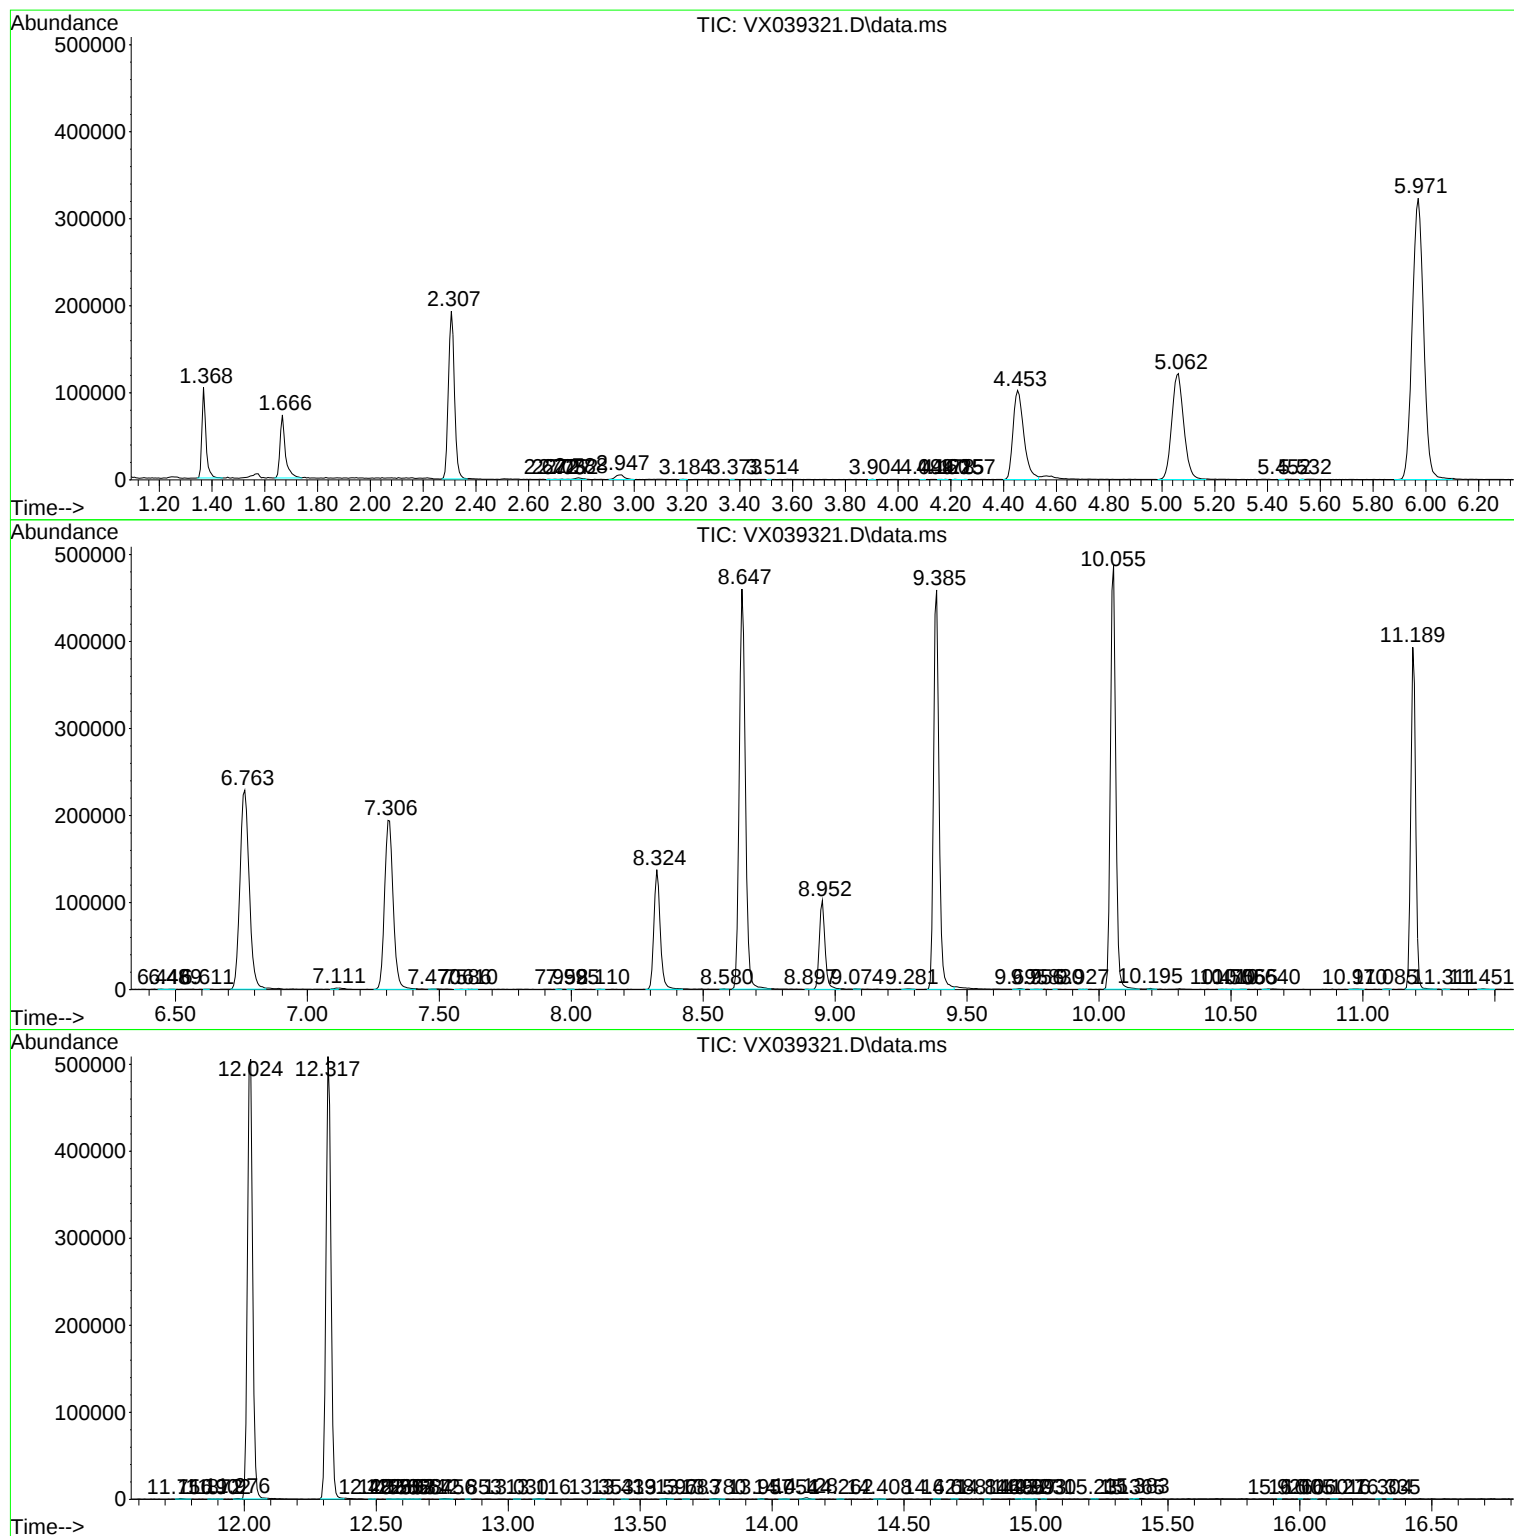

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121823\
Data File : VX039321.D
Acq On : 18 Dec 2023 18:55
Operator : JC/MD
Sample : 05835-04 100X
Misc : 4.22g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0B34

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121823\
Data File : VX039321.D
Acq On : 18 Dec 2023 18:55
Operator : JC/MD
Sample : 05835-04 100X
Misc : 4.22g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0B34

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------