

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121823\
 Data File : VX039323.D
 Acq On : 18 Dec 2023 20:04
 Operator : JC/MD
 Sample : VX1218MBL02
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK650

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
 Title : VOC Analysis

Signal : TIC: VX039323.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	57	rBV	111419	117629	12.01%	1.552%
2	1.666	91	95	111	rVB	71886	109672	11.19%	1.447%
3	2.306	193	200	209	rBV	211448	327988	33.48%	4.329%
4	2.434	219	221	224	rVB2	292	267	0.03%	0.004%
5	2.514	231	234	241	rVB4	1132	1999	0.20%	0.026%
6	2.703	263	265	267	rBV2	371	389	0.04%	0.005%
7	2.788	274	279	287	rVB2	3411	6052	0.62%	0.080%
8	2.867	287	292	294	rBV3	250	438	0.04%	0.006%
9	2.947	298	305	312	rVB	2870	5806	0.59%	0.077%
10	3.093	326	329	332	rBV2	526	700	0.07%	0.009%
11	3.471	390	391	393	rBV	263	192	0.02%	0.003%
12	3.556	403	405	407	rBV2	219	234	0.02%	0.003%
13	3.715	429	431	434	rBV2	275	226	0.02%	0.003%
14	4.062	486	488	490	rBV	222	237	0.02%	0.003%
15	4.452	543	552	566	rBV	95397	275506	28.12%	3.636%
16	4.702	592	593	594	rBV	360	184	0.02%	0.002%
17	4.745	598	600	603	rVB	344	274	0.03%	0.004%
18	5.056	639	651	671	rBV	121261	386984	39.50%	5.107%
19	5.294	688	690	693	rBV2	171	211	0.02%	0.003%
20	5.367	700	702	703	rBV	267	253	0.03%	0.003%
21	5.458	712	717	718	rBV2	498	541	0.06%	0.007%
22	5.556	729	733	737	rBV3	349	689	0.07%	0.009%
23	5.666	747	751	753	rBV2	284	343	0.04%	0.005%
24	5.751	763	765	769	rBV2	178	247	0.03%	0.003%
25	5.970	789	801	823	rBV2	326117	979770	100.00%	12.930%
26	6.324	857	859	862	rVB	238	183	0.02%	0.002%
27	6.513	889	890	893	rVB2	248	200	0.02%	0.003%
28	6.763	920	931	953	rBV	227766	559142	57.07%	7.379%
29	6.958	961	963	966	rBV3	217	241	0.02%	0.003%
30	7.019	971	973	975	rVV2	283	231	0.02%	0.003%
31	7.062	978	980	981	rVB2	309	191	0.02%	0.003%
32	7.123	981	990	996	rBV7	1777	4422	0.45%	0.058%
33	7.220	1004	1006	1011	rBV2	239	322	0.03%	0.004%
34	7.306	1011	1020	1036	rBV	199321	449010	45.83%	5.926%
35	8.007	1131	1135	1136	rBV2	193	247	0.03%	0.003%
36	8.062	1140	1144	1147	rBV2	207	271	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121823\
 Data File : VX039323.D
 Acq On : 18 Dec 2023 20:04
 Operator : JC/MD
 Sample : VX1218MBL02
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK650

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
 Title : VOC Analysis

37	8.269	1175	1178	1181	rBV	238	206	0.02%	0.003%
38	8.324	1181	1187	1203	rBV	140496	232916	23.77%	3.074%
39	8.586	1227	1230	1231	rBV2	301	304	0.03%	0.004%
40	8.647	1234	1240	1261	rBV	482956	772923	78.89%	10.201%
41	8.836	1269	1271	1274	rBV	235	186	0.02%	0.002%
42	8.952	1284	1290	1308	rBV	103014	154069	15.73%	2.033%
43	9.074	1308	1310	1315	rVB2	424	425	0.04%	0.006%
44	9.147	1318	1322	1324	rBV	195	278	0.03%	0.004%
45	9.275	1340	1343	1347	rVB2	780	731	0.07%	0.010%
46	9.384	1355	1361	1376	rBV	435850	634649	64.78%	8.376%
47	9.604	1395	1397	1399	rBV2	392	471	0.05%	0.006%
48	9.695	1410	1412	1416	rBV4	872	1185	0.12%	0.016%
49	9.817	1429	1432	1434	rBV2	259	346	0.04%	0.005%
50	9.848	1434	1437	1438	rBV2	203	214	0.02%	0.003%
51	10.000	1460	1462	1465	rVV	182	189	0.02%	0.002%
52	10.055	1465	1471	1489	rVV	493462	686372	70.05%	9.058%
53	10.171	1489	1490	1491	rVV	565	299	0.03%	0.004%
54	10.195	1491	1494	1500	rVV3	1194	1762	0.18%	0.023%
55	10.268	1503	1506	1507	rBV2	218	193	0.02%	0.003%
56	10.311	1507	1513	1516	rBV3	676	1201	0.12%	0.016%
57	10.439	1531	1534	1535	rBV2	218	183	0.02%	0.002%
58	10.488	1540	1542	1544	rBV2	187	193	0.02%	0.003%
59	10.579	1554	1557	1559	rVV2	235	240	0.02%	0.003%
60	10.622	1563	1564	1566	rVV	228	198	0.02%	0.003%
61	10.646	1566	1568	1570	rVV3	644	757	0.08%	0.010%
62	10.970	1617	1621	1625	rVV3	936	1178	0.12%	0.016%
63	11.085	1636	1640	1648	rVB5	1014	1645	0.17%	0.022%
64	11.189	1651	1657	1667	rBV	376113	483838	49.38%	6.385%
65	11.287	1670	1673	1674	rVB2	218	231	0.02%	0.003%
66	11.457	1697	1701	1705	rVB2	902	1098	0.11%	0.014%
67	11.610	1724	1726	1727	rBV	244	181	0.02%	0.002%
68	11.713	1739	1743	1745	rBV	328	329	0.03%	0.004%
69	11.756	1746	1750	1755	rBV3	994	1338	0.14%	0.018%
70	11.878	1765	1770	1772	rBV	156	237	0.02%	0.003%
71	11.975	1783	1786	1788	rBV2	1326	1393	0.14%	0.018%
72	12.024	1788	1794	1805	rVV	518883	680565	69.46%	8.982%
73	12.177	1817	1819	1821	rVB	315	181	0.02%	0.002%
74	12.317	1837	1842	1859	rVV	512185	668828	68.26%	8.827%
75	12.512	1872	1874	1876	rVB	355	241	0.02%	0.003%
76	12.878	1930	1934	1935	rBV2	227	309	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121823\
 Data File : VX039323.D
 Acq On : 18 Dec 2023 20:04
 Operator : JC/MD
 Sample : VX1218MBL02
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK650

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

77	12.957	1946	1947	1951	rBV2	265	285	0.03%	0.004%
78	13.115	1970	1973	1980	rVB3	1201	1512	0.15%	0.020%
79	13.329	2005	2008	2011	rVV	270	318	0.03%	0.004%
80	13.591	2048	2051	2055	rBV4	1386	1846	0.19%	0.024%
81	13.786	2079	2083	2087	rVB2	1106	1439	0.15%	0.019%
82	13.963	2109	2112	2119	rBV4	1147	1763	0.18%	0.023%
83	14.134	2136	2140	2144	rVB2	1200	1429	0.15%	0.019%
84	14.225	2153	2155	2156	rBV2	199	201	0.02%	0.003%
85	14.323	2167	2171	2174	rBV2	273	336	0.03%	0.004%
86	14.451	2190	2192	2193	rVB	367	186	0.02%	0.002%
87	14.621	2218	2220	2221	rBV	297	242	0.02%	0.003%
88	14.658	2223	2226	2228	rVV2	213	257	0.03%	0.003%
89	14.847	2256	2257	2261	rBV2	372	547	0.06%	0.007%
90	14.951	2271	2274	2278	rBV2	253	397	0.04%	0.005%
91	15.243	2320	2322	2325	rVV3	301	277	0.03%	0.004%
92	15.475	2358	2360	2362	rBV3	285	224	0.02%	0.003%
93	15.548	2370	2372	2375	rVB3	269	199	0.02%	0.003%
94	15.993	2442	2445	2446	rBV2	220	216	0.02%	0.003%
95	16.103	2460	2463	2464	rBV2	347	284	0.03%	0.004%
96	16.164	2470	2473	2474	rVB	401	319	0.03%	0.004%
97	16.273	2489	2491	2492	rBV2	223	197	0.02%	0.003%
98	16.322	2498	2499	2501	rBV	321	234	0.02%	0.003%
99	16.359	2503	2505	2507	rBV	297	319	0.03%	0.004%
100	16.658	2549	2554	2557	rBV4	424	830	0.08%	0.011%


Sum of corrected areas: 7577230

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121823\
Data File : VX039323.D
Acq On : 18 Dec 2023 20:04
Operator : JC/MD
Sample : VX1218MBL02
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK650

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

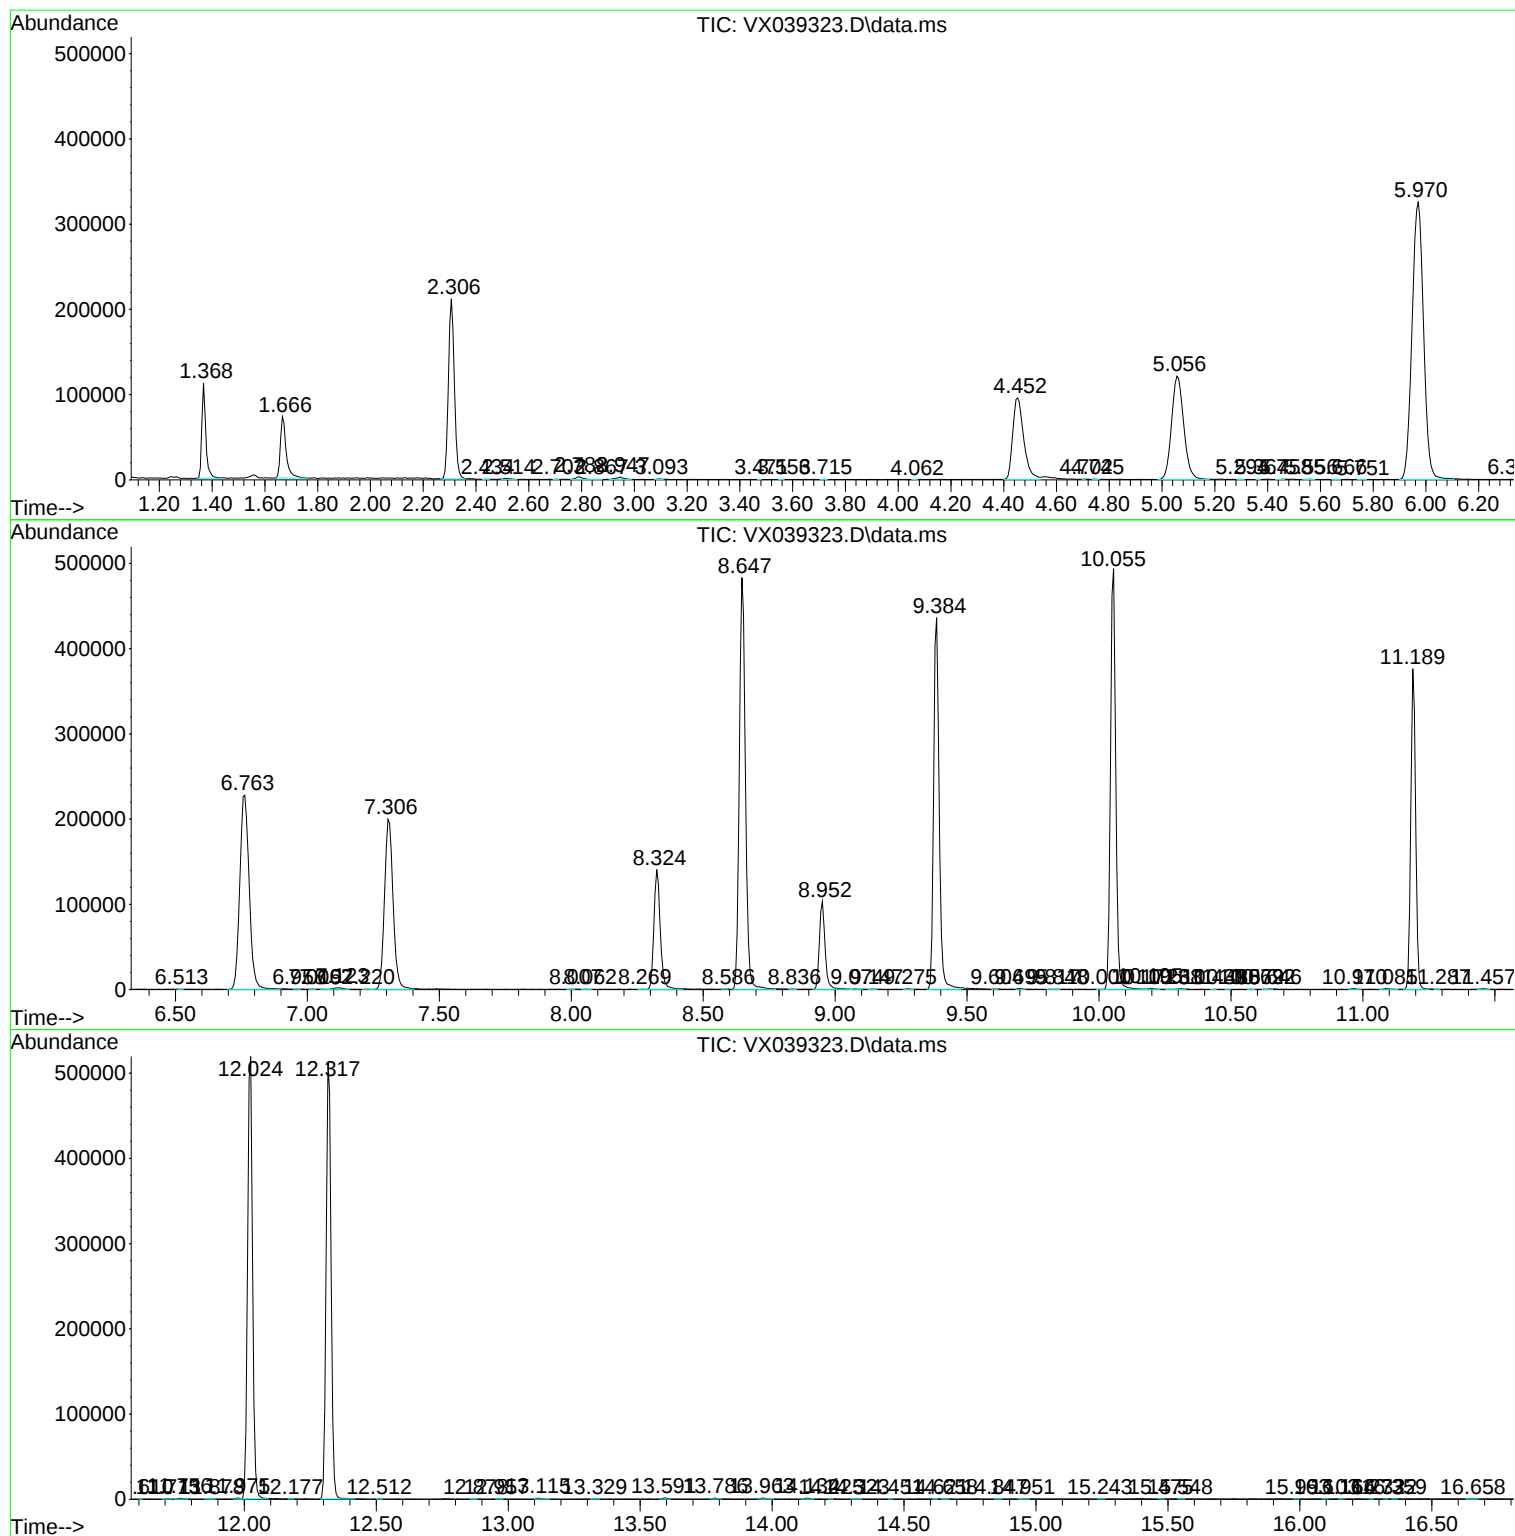

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121823\
Data File : VX039323.D
Acq On : 18 Dec 2023 20:04
Operator : JC/MD
Sample : VX1218MBL02
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK650

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121823\
Data File : VX039323.D
Acq On : 18 Dec 2023 20:04
Operator : JC/MD
Sample : VX1218MBL02
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK650

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc