

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121823\
 Data File : VX039324.D
 Acq On : 18 Dec 2023 20:27
 Operator : JC/MD
 Sample : 05835-05 100X
 Misc : 4.03g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0B37

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

Signal : TIC: VX039324.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	57	rVB	96287	99703	11.75%	1.457%
2	1.666	90	95	111	rVB	62270	90131	10.62%	1.317%
3	2.307	194	200	210	rVB	173095	269794	31.80%	3.943%
4	2.514	230	234	241	rVB3	597	1244	0.15%	0.018%
5	2.788	275	279	286	rVB3	1630	3505	0.41%	0.051%
6	3.105	326	331	332	rBV2	452	548	0.06%	0.008%
7	3.197	342	346	349	rVV	276	337	0.04%	0.005%
8	3.386	374	377	379	rVV2	205	204	0.02%	0.003%
9	3.556	403	405	407	rVB	276	191	0.02%	0.003%
10	3.587	407	410	411	rBV2	230	235	0.03%	0.003%
11	3.629	413	417	418	rBV2	211	244	0.03%	0.004%
12	3.971	471	473	477	rVB2	182	245	0.03%	0.004%
13	4.452	543	552	566	rBV	89048	254946	30.05%	3.726%
14	4.733	595	598	599	rBV3	250	280	0.03%	0.004%
15	4.940	630	632	634	rBV	360	209	0.02%	0.003%
16	5.056	639	651	668	rBV2	106005	339103	39.96%	4.956%
17	5.367	698	702	704	rBV2	299	457	0.05%	0.007%
18	5.440	713	714	716	rBV	224	200	0.02%	0.003%
19	5.824	773	777	778	rVB2	206	235	0.03%	0.003%
20	5.842	778	780	781	rBV	176	185	0.02%	0.003%
21	5.970	789	801	823	rBV2	284053	848539	100.00%	12.402%
22	6.300	851	855	858	rBV2	257	397	0.05%	0.006%
23	6.324	858	859	861	rVV	252	209	0.02%	0.003%
24	6.763	920	931	945	rBV	227523	544984	64.23%	7.965%
25	7.050	976	978	981	rBV3	197	234	0.03%	0.003%
26	7.123	984	990	994	rVV4	1320	2989	0.35%	0.044%
27	7.220	1004	1006	1008	rVB2	304	248	0.03%	0.004%
28	7.251	1008	1011	1012	rBV	374	360	0.04%	0.005%
29	7.306	1012	1020	1040	rBV	175277	393209	46.34%	5.747%
30	7.714	1084	1087	1091	rBV2	238	417	0.05%	0.006%
31	7.934	1122	1123	1125	rBV	271	180	0.02%	0.003%
32	7.952	1125	1126	1128	rVV2	374	225	0.03%	0.003%
33	8.098	1149	1150	1154	rBV2	167	224	0.03%	0.003%
34	8.208	1167	1168	1170	rBV	256	195	0.02%	0.003%
35	8.324	1181	1187	1199	rBV	119665	199220	23.48%	2.912%
36	8.519	1217	1219	1221	rBV2	450	429	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121823\
 Data File : VX039324.D
 Acq On : 18 Dec 2023 20:27
 Operator : JC/MD
 Sample : 05835-05 100X
 Misc : 4.03g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0B37

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
 Title : VOC Analysis

37	8.568	1224	1227	1228	rBV2	235	221	0.03%	0.003%
38	8.647	1234	1240	1251	rBV	419569	658986	77.66%	9.631%
39	8.952	1284	1290	1302	rBV	84920	132013	15.56%	1.929%
40	9.141	1318	1321	1326	rBV3	241	379	0.04%	0.006%
41	9.202	1329	1331	1332	rBV2	247	207	0.02%	0.003%
42	9.281	1340	1344	1349	rBV3	641	832	0.10%	0.012%
43	9.385	1355	1361	1373	rBV	408321	585234	68.97%	8.553%
44	9.695	1408	1412	1418	rVB2	1023	1221	0.14%	0.018%
45	9.805	1427	1430	1433	rBV2	221	231	0.03%	0.003%
46	10.055	1465	1471	1484	rBV	480394	676231	79.69%	9.883%
47	10.201	1492	1495	1500	rVB3	796	1316	0.16%	0.019%
48	10.250	1500	1503	1506	rBV	164	237	0.03%	0.003%
49	10.397	1522	1527	1528	rBV2	172	265	0.03%	0.004%
50	10.445	1532	1535	1538	rVV2	150	241	0.03%	0.004%
51	10.640	1563	1567	1570	rBV3	465	762	0.09%	0.011%
52	10.744	1582	1584	1585	rBV2	215	193	0.02%	0.003%
53	10.878	1602	1606	1609	rBV2	149	240	0.03%	0.004%
54	10.963	1617	1620	1624	rVV2	933	1070	0.13%	0.016%
55	11.024	1626	1630	1631	rVB3	177	232	0.03%	0.003%
56	11.043	1631	1633	1635	rBV	167	189	0.02%	0.003%
57	11.092	1638	1641	1644	rVB2	743	662	0.08%	0.010%
58	11.189	1652	1657	1665	rBV	350449	444220	52.35%	6.492%
59	11.274	1670	1671	1675	rVB3	347	359	0.04%	0.005%
60	11.451	1696	1700	1703	rBV2	827	1091	0.13%	0.016%
61	11.732	1745	1746	1748	rBV	239	214	0.03%	0.003%
62	11.756	1748	1750	1755	rVB3	609	796	0.09%	0.012%
63	11.835	1760	1763	1766	rBV2	248	342	0.04%	0.005%
64	11.902	1772	1774	1776	rBV	314	212	0.02%	0.003%
65	11.976	1782	1786	1788	rBV	839	969	0.11%	0.014%
66	12.024	1788	1794	1808	rBV	514259	672384	79.24%	9.827%
67	12.244	1829	1830	1834	rBV2	330	296	0.03%	0.004%
68	12.317	1837	1842	1856	rVV	455640	593286	69.92%	8.671%
69	12.500	1869	1872	1873	rBV2	207	190	0.02%	0.003%
70	12.536	1876	1878	1882	rVB2	279	328	0.04%	0.005%
71	12.579	1882	1885	1889	rBV2	217	384	0.05%	0.006%
72	12.713	1904	1907	1908	rBV	228	227	0.03%	0.003%
73	12.762	1912	1915	1918	rVB2	667	836	0.10%	0.012%
74	12.853	1927	1930	1932	rBV2	265	269	0.03%	0.004%
75	12.939	1943	1944	1946	rBV	261	217	0.03%	0.003%
76	13.122	1970	1974	1979	rVB4	610	920	0.11%	0.013%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121823\
 Data File : VX039324.D
 Acq On : 18 Dec 2023 20:27
 Operator : JC/MD
 Sample : 05835-05 100X
 Misc : 4.03g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0B37

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

77	13.396	2017	2019	2023	rBV2	246	272	0.03%	0.004%
78	13.506	2036	2037	2040	rBV	222	184	0.02%	0.003%
79	13.548	2042	2044	2047	rVB	341	227	0.03%	0.003%
80	13.597	2047	2052	2055	rBV3	1077	1386	0.16%	0.020%
81	13.676	2062	2065	2067	rBV2	282	356	0.04%	0.005%
82	13.780	2077	2082	2084	rVV2	740	885	0.10%	0.013%
83	13.817	2086	2088	2090	rVB	309	182	0.02%	0.003%
84	13.841	2090	2092	2096	rBV	234	278	0.03%	0.004%
85	13.963	2110	2112	2117	rVV2	691	859	0.10%	0.013%
86	14.024	2119	2122	2126	rBV	184	270	0.03%	0.004%
87	14.134	2135	2140	2144	rVV2	1244	1649	0.19%	0.024%
88	14.201	2148	2151	2152	rBV	292	214	0.03%	0.003%
89	14.286	2164	2165	2168	rBV2	233	189	0.02%	0.003%
90	14.402	2181	2184	2185	rBV	302	260	0.03%	0.004%
91	14.542	2205	2207	2208	rVB	320	180	0.02%	0.003%
92	14.579	2211	2213	2214	rBV	200	182	0.02%	0.003%
93	14.682	2228	2230	2231	rBV2	242	192	0.02%	0.003%
94	14.768	2243	2244	2247	rVB2	285	178	0.02%	0.003%
95	14.798	2247	2249	2252	rVB3	295	342	0.04%	0.005%
96	14.823	2252	2253	2255	rBV2	284	246	0.03%	0.004%
97	15.341	2336	2338	2340	rBV2	222	208	0.02%	0.003%
98	15.365	2340	2342	2343	rBV	307	224	0.03%	0.003%
99	15.383	2343	2345	2348	rBV	450	435	0.05%	0.006%
100	16.542	2533	2535	2537	rBV2	281	225	0.03%	0.003%

Sum of corrected areas: 6842180




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121823\
Data File : VX039324.D
Acq On : 18 Dec 2023 20:27
Operator : JC/MD
Sample : 05835-05 100X
Misc : 4.03g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0B37

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

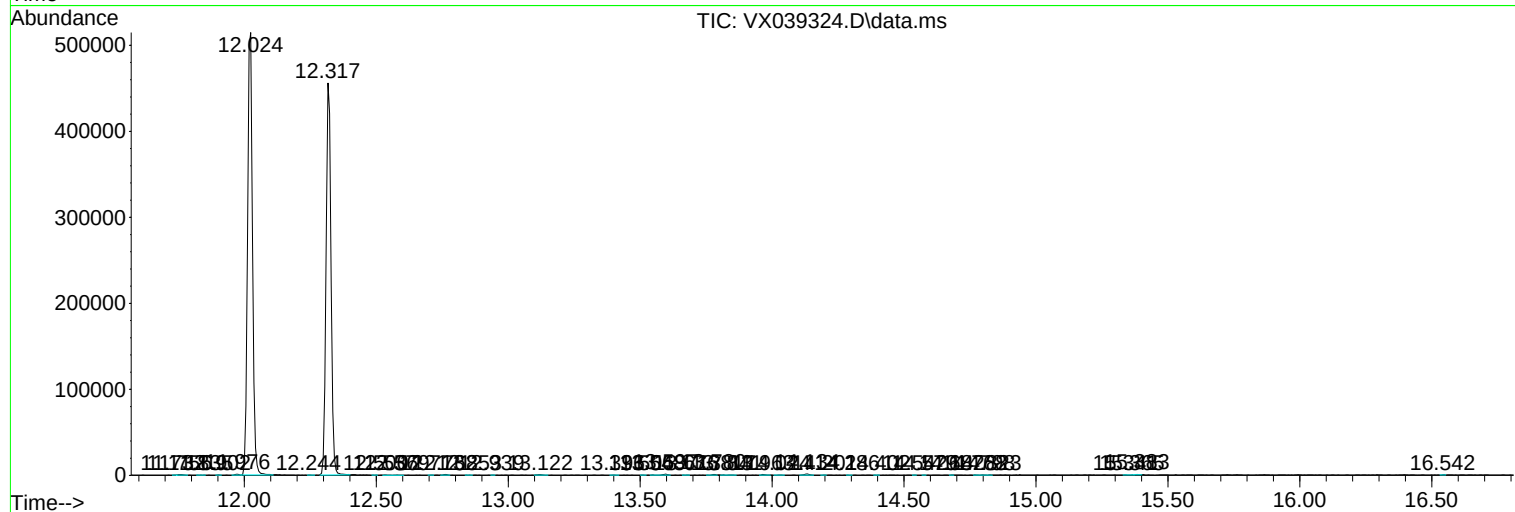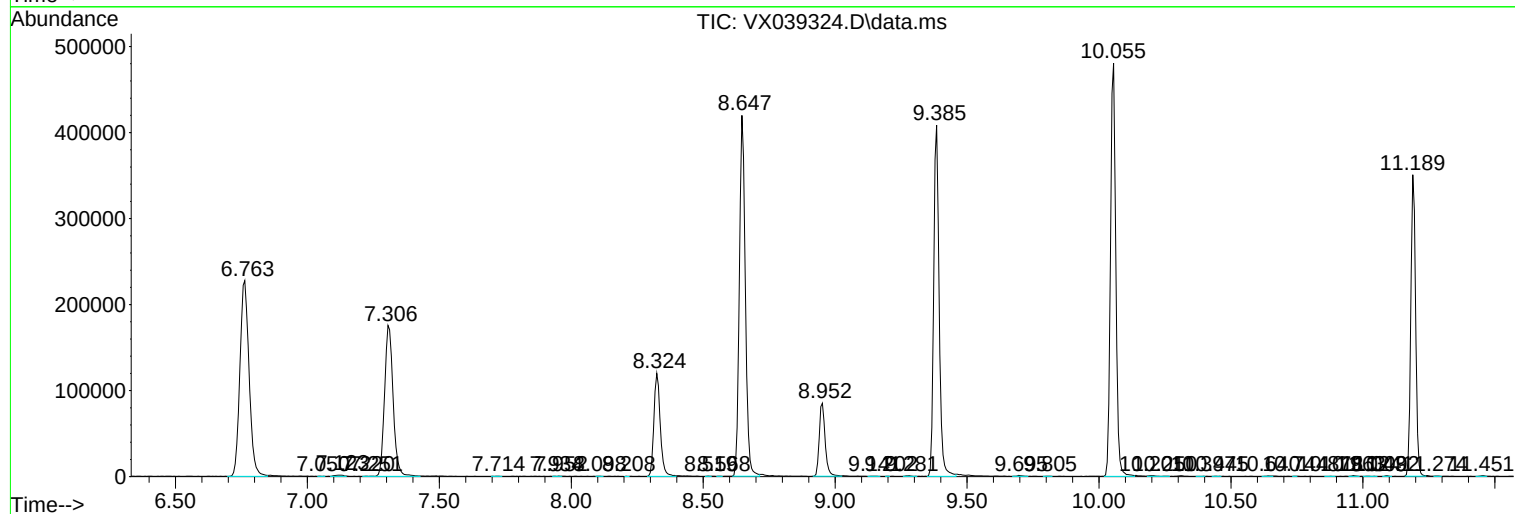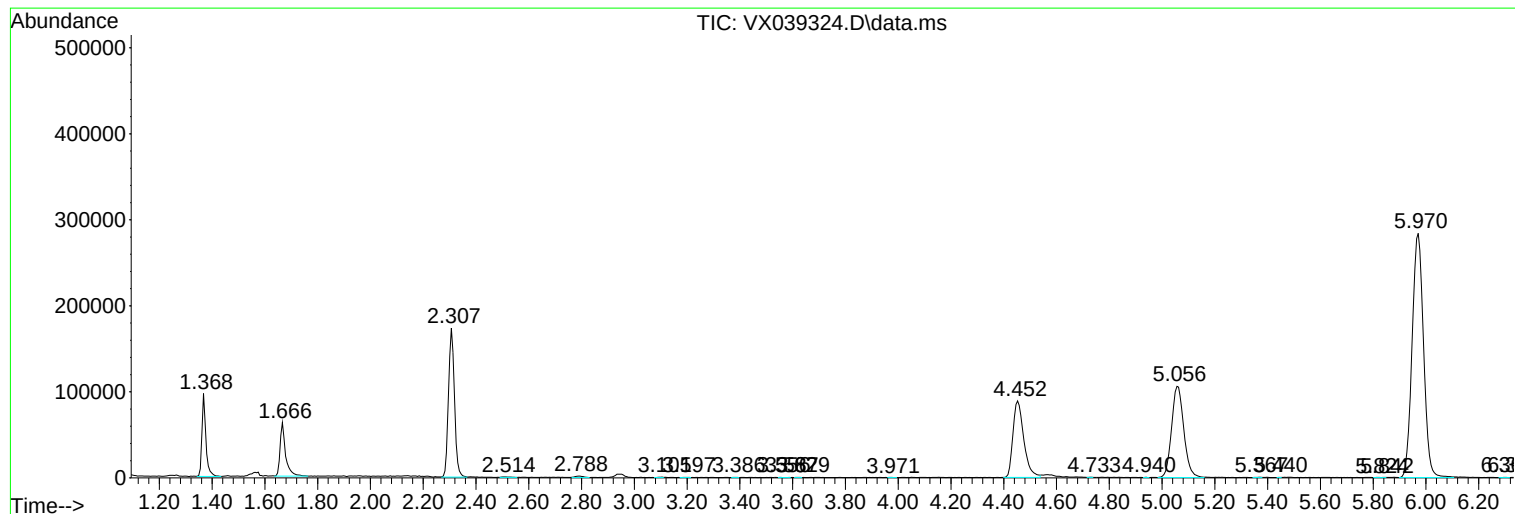

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121823\
Data File : VX039324.D
Acq On : 18 Dec 2023 20:27
Operator : JC/MD
Sample : 05835-05 100X
Misc : 4.03g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0B37

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121823\
Data File : VX039324.D
Acq On : 18 Dec 2023 20:27
Operator : JC/MD
Sample : 05835-05 100X
Misc : 4.03g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0B37

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc