

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121823\
 Data File : VX039331.D
 Acq On : 18 Dec 2023 23:08
 Operator : JC/MD
 Sample : 05835-13 100X
 Misc : 2.05g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0AR0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

Signal : TIC: VX039331.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	55	rBV	84928	91235	11.17%	1.393%
2	1.666	91	95	109	rVB	57292	85480	10.46%	1.305%
3	2.307	194	200	213	rBV	156867	246012	30.11%	3.756%
4	2.459	223	225	226	rBV	324	275	0.03%	0.004%
5	2.788	275	279	286	rVB3	1642	3046	0.37%	0.047%
6	2.855	288	290	293	rVV2	208	218	0.03%	0.003%
7	2.941	296	304	314	rVV	4527	10002	1.22%	0.153%
8	3.111	327	332	333	rBV3	363	488	0.06%	0.007%
9	3.465	388	390	393	rVB2	211	195	0.02%	0.003%
10	3.562	404	406	410	rVB	231	242	0.03%	0.004%
11	3.617	412	415	417	rBV2	305	357	0.04%	0.005%
12	3.709	428	430	431	rVB	294	182	0.02%	0.003%
13	3.733	431	434	438	rBV2	331	407	0.05%	0.006%
14	3.782	441	442	447	rBV2	157	203	0.02%	0.003%
15	3.879	457	458	464	rVB2	185	223	0.03%	0.003%
16	3.928	464	466	469	rVB2	202	187	0.02%	0.003%
17	3.965	469	472	474	rVB	373	318	0.04%	0.005%
18	4.154	500	503	504	rVB	225	181	0.02%	0.003%
19	4.446	543	551	566	rBV	85714	249474	30.54%	3.809%
20	4.830	611	614	615	rBV	259	204	0.02%	0.003%
21	4.940	630	632	636	rBV2	212	345	0.04%	0.005%
22	5.056	639	651	671	rVV	102703	334154	40.90%	5.102%
23	5.288	686	689	691	rBV2	148	187	0.02%	0.003%
24	5.391	704	706	707	rBV2	223	209	0.03%	0.003%
25	5.428	710	712	714	rVB	216	185	0.02%	0.003%
26	5.465	716	718	721	rVV2	359	349	0.04%	0.005%
27	5.647	744	748	754	rVB2	326	682	0.08%	0.010%
28	5.971	788	801	818	rBV2	267612	816920	100.00%	12.473%
29	6.324	856	859	860	rBV	238	241	0.03%	0.004%
30	6.556	895	897	901	rBV	343	290	0.04%	0.004%
31	6.763	921	931	946	rBV	211954	514993	63.04%	7.863%
32	7.111	984	988	996	rBV5	1371	3065	0.38%	0.047%
33	7.306	1012	1020	1035	rBV	173111	382976	46.88%	5.848%
34	7.623	1069	1072	1073	rBV	232	193	0.02%	0.003%
35	7.830	1103	1106	1109	rVB2	159	176	0.02%	0.003%
36	7.867	1109	1112	1115	rBV	225	202	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121823\
 Data File : VX039331.D
 Acq On : 18 Dec 2023 23:08
 Operator : JC/MD
 Sample : 05835-13 100X
 Misc : 2.05g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0AR0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
 Title : VOC Analysis

37	7.928	1121	1122	1123	rBV	322	180	0.02%	0.003%
38	8.025	1136	1138	1141	rBV2	246	264	0.03%	0.004%
39	8.104	1148	1151	1154	rVB2	214	276	0.03%	0.004%
40	8.177	1161	1163	1166	rBV	202	222	0.03%	0.003%
41	8.324	1181	1187	1200	rBV	112683	189414	23.19%	2.892%
42	8.470	1210	1211	1215	rVB2	307	211	0.03%	0.003%
43	8.574	1225	1228	1234	rVB3	421	413	0.05%	0.006%
44	8.647	1234	1240	1256	rBV	389112	617037	75.53%	9.421%
45	8.824	1267	1269	1271	rBV3	351	320	0.04%	0.005%
46	8.872	1275	1277	1281	rVB2	356	338	0.04%	0.005%
47	8.952	1284	1290	1301	rBV	80469	125434	15.35%	1.915%
48	9.159	1322	1324	1326	rVV2	214	200	0.02%	0.003%
49	9.232	1333	1336	1337	rVB	327	277	0.03%	0.004%
50	9.275	1340	1343	1346	rBV3	377	519	0.06%	0.008%
51	9.385	1355	1361	1389	rBV	394885	575600	70.46%	8.789%
52	9.665	1406	1407	1409	rBV	429	257	0.03%	0.004%
53	9.702	1410	1413	1416	rVB2	885	973	0.12%	0.015%
54	9.872	1440	1441	1444	rVV	303	246	0.03%	0.004%
55	9.915	1447	1448	1451	rVB	345	264	0.03%	0.004%
56	10.055	1465	1471	1489	rBV	449786	662497	81.10%	10.115%
57	10.305	1509	1512	1513	rBV	560	586	0.07%	0.009%
58	10.372	1522	1523	1528	rVB	260	230	0.03%	0.004%
59	10.439	1532	1534	1536	rBV2	197	174	0.02%	0.003%
60	10.494	1540	1543	1546	rVB2	165	172	0.02%	0.003%
61	10.647	1565	1568	1569	rVV3	349	205	0.03%	0.003%
62	10.714	1575	1579	1580	rBV	220	279	0.03%	0.004%
63	10.732	1580	1582	1587	rVV2	253	248	0.03%	0.004%
64	10.836	1597	1599	1602	rVB	232	193	0.02%	0.003%
65	10.964	1617	1620	1623	rVB2	459	508	0.06%	0.008%
66	11.018	1628	1629	1632	rBV2	195	179	0.02%	0.003%
67	11.092	1639	1641	1643	rBV2	314	341	0.04%	0.005%
68	11.189	1652	1657	1665	rBV	338657	434083	53.14%	6.628%
69	11.366	1683	1686	1688	rBV2	201	194	0.02%	0.003%
70	11.451	1697	1700	1705	rVV2	284	468	0.06%	0.007%
71	11.488	1705	1706	1710	rVB	241	260	0.03%	0.004%
72	11.756	1747	1750	1754	rBV3	294	429	0.05%	0.007%
73	11.969	1784	1785	1788	rBV2	465	391	0.05%	0.006%
74	12.018	1788	1793	1802	rBV	468955	623191	76.29%	9.515%
75	12.219	1824	1826	1827	rBV	274	214	0.03%	0.003%
76	12.317	1837	1842	1857	rBV	439610	558667	68.39%	8.530%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121823\
 Data File : VX039331.D
 Acq On : 18 Dec 2023 23:08
 Operator : JC/MD
 Sample : 05835-13 100X
 Misc : 2.05g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0AR0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

77	12.512	1872	1874	1877	rBV2	217	218	0.03%	0.003%
78	12.573	1883	1884	1889	rVB	307	304	0.04%	0.005%
79	12.664	1898	1899	1903	rBV2	243	251	0.03%	0.004%
80	12.756	1912	1914	1919	rVB3	618	782	0.10%	0.012%
81	13.244	1991	1994	1996	rBV2	200	214	0.03%	0.003%
82	13.280	1997	2000	2003	rBV2	241	358	0.04%	0.005%
83	13.408	2020	2021	2025	rVB2	203	234	0.03%	0.004%
84	13.475	2030	2032	2035	rBV2	282	267	0.03%	0.004%
85	13.591	2048	2051	2056	rBV2	383	599	0.07%	0.009%
86	13.774	2076	2081	2083	rBV2	320	528	0.06%	0.008%
87	13.957	2109	2111	2115	rBV2	295	319	0.04%	0.005%
88	14.128	2135	2139	2146	rBV3	1246	1784	0.22%	0.027%
89	14.542	2205	2207	2211	rBV3	260	369	0.05%	0.006%
90	14.621	2217	2220	2221	rBV	274	215	0.03%	0.003%
91	15.292	2328	2330	2332	rBV2	270	218	0.03%	0.003%
92	15.371	2341	2343	2350	rBV4	421	841	0.10%	0.013%
93	15.444	2353	2355	2356	rBV2	209	175	0.02%	0.003%
94	15.487	2358	2362	2363	rBV2	277	340	0.04%	0.005%
95	15.536	2368	2370	2372	rVB2	433	230	0.03%	0.004%
96	15.591	2378	2379	2380	rBV	330	201	0.02%	0.003%
97	15.646	2386	2388	2390	rBV2	234	188	0.02%	0.003%
98	16.048	2450	2454	2455	rBV2	213	270	0.03%	0.004%
99	16.115	2463	2465	2467	rBV2	283	222	0.03%	0.003%
100	16.389	2509	2510	2512	rBV2	347	217	0.03%	0.003%


Sum of corrected areas: 6549394

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121823\
Data File : VX039331.D
Acq On : 18 Dec 2023 23:08
Operator : JC/MD
Sample : 05835-13 100X
Misc : 2.05g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COAR0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

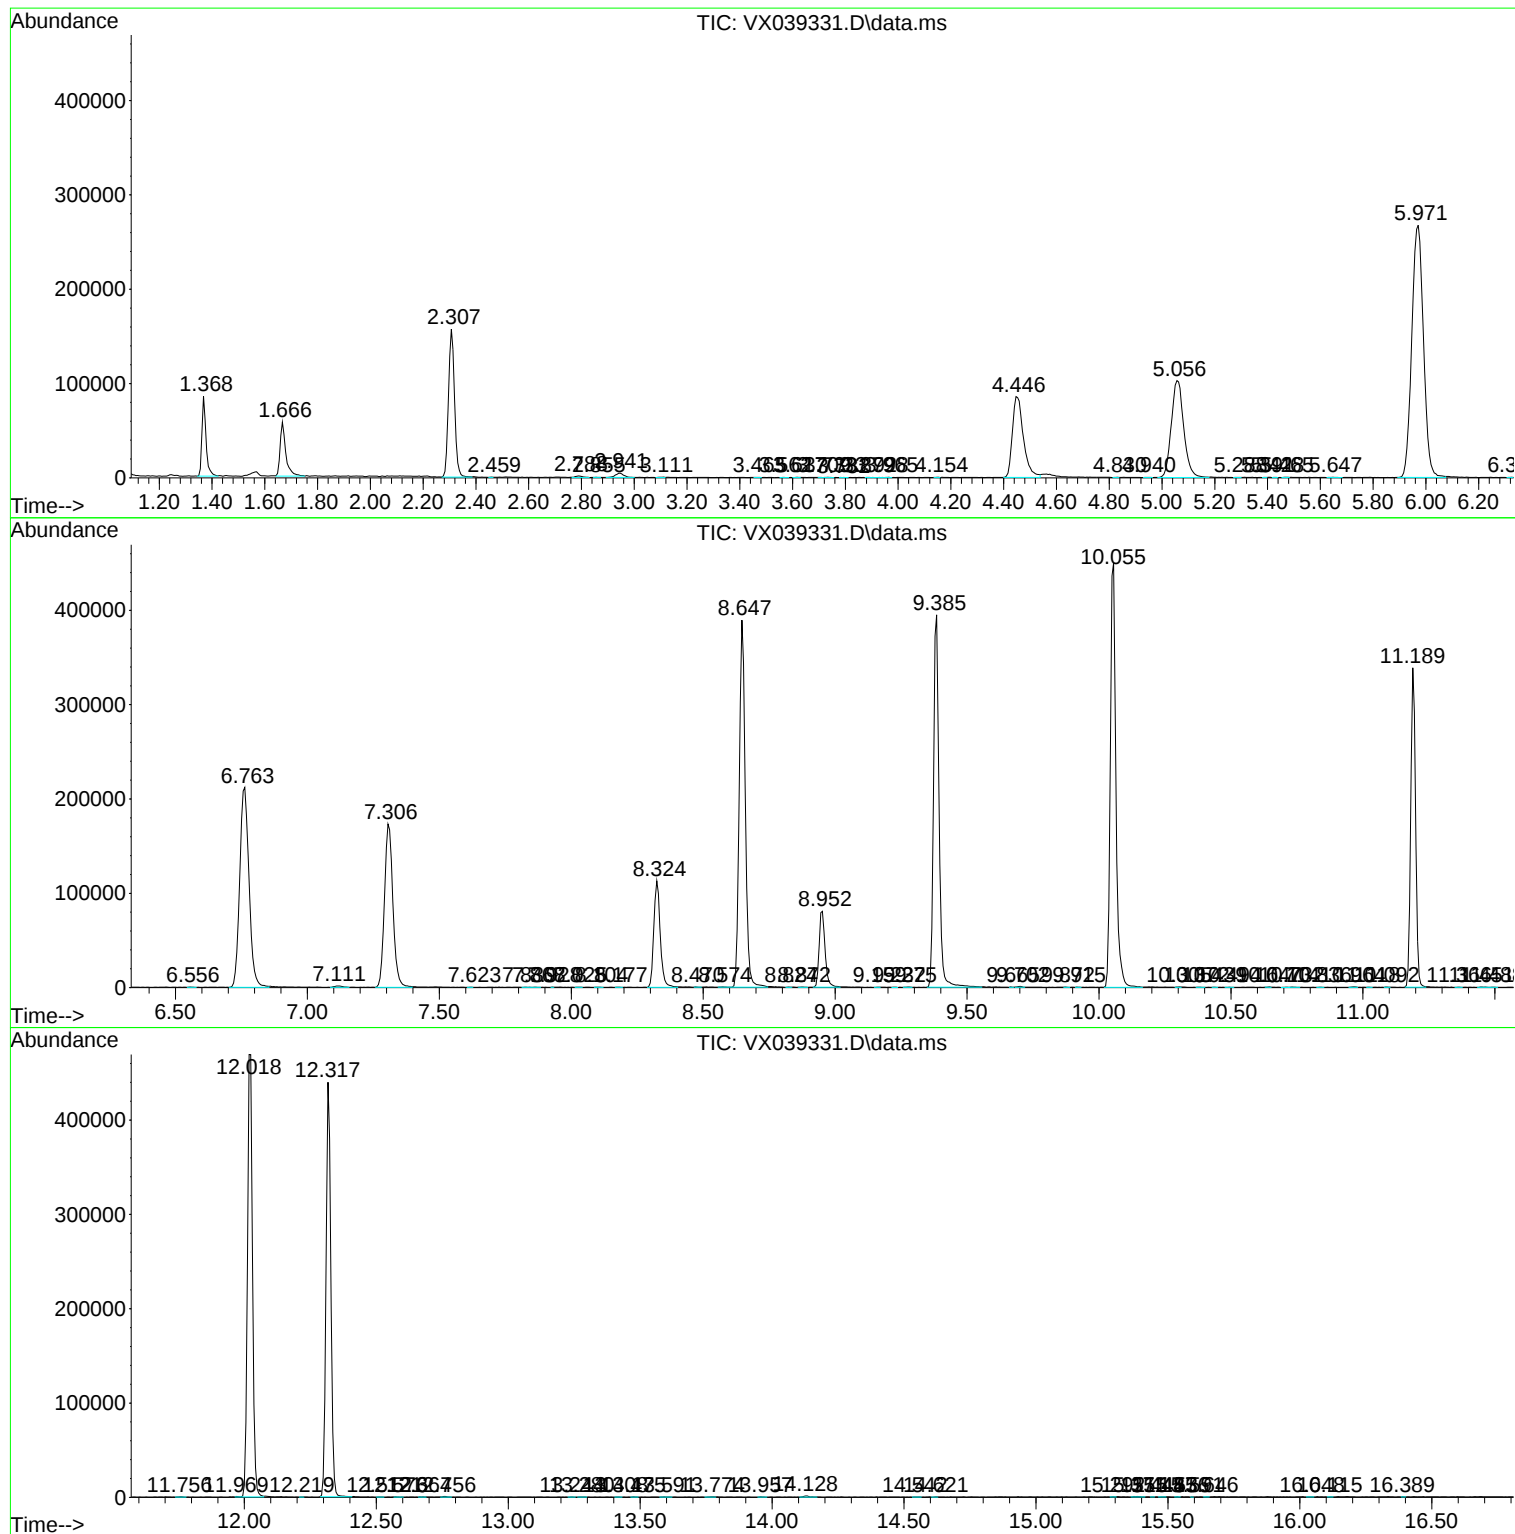

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121823\
Data File : VX039331.D
Acq On : 18 Dec 2023 23:08
Operator : JC/MD
Sample : 05835-13 100X
Misc : 2.05g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0AR0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121823\
Data File : VX039331.D
Acq On : 18 Dec 2023 23:08
Operator : JC/MD
Sample : 05835-13 100X
Misc : 2.05g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0AR0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc