

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121823\
 Data File : VX039332.D
 Acq On : 18 Dec 2023 23:31
 Operator : JC/MD
 Sample : 05835-14 100X
 Misc : 4.07g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0AR1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
 Title : VOC Analysis

Signal : TIC: VX039332.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.367	43	46	58	rVB	80746	86684	11.02%	1.348%
2	1.666	91	95	106	rBV	61183	84132	10.69%	1.308%
3	2.306	194	200	216	rVB	154980	244144	31.02%	3.796%
4	2.690	262	263	265	rBV2	330	298	0.04%	0.005%
5	2.788	275	279	286	rVB4	1694	2814	0.36%	0.044%
6	2.940	296	304	315	rBV3	4539	11053	1.40%	0.172%
7	3.440	384	386	387	rVB	289	182	0.02%	0.003%
8	3.550	402	404	406	rBV2	232	214	0.03%	0.003%
9	3.702	426	429	432	rBV2	291	341	0.04%	0.005%
10	3.782	438	442	445	rBV2	180	297	0.04%	0.005%
11	3.873	455	457	461	rBV2	203	312	0.04%	0.005%
12	4.190	508	509	513	rBV2	209	244	0.03%	0.004%
13	4.385	540	541	543	rBV	232	186	0.02%	0.003%
14	4.452	543	552	565	rBV	85010	240688	30.59%	3.742%
15	4.727	595	597	599	rVB	362	306	0.04%	0.005%
16	4.769	602	604	609	rVV3	303	434	0.06%	0.007%
17	4.855	616	618	620	rVV	318	284	0.04%	0.004%
18	4.879	620	622	623	rVB	286	200	0.03%	0.003%
19	5.056	640	651	668	rBV	101808	319743	40.63%	4.971%
20	5.604	738	741	744	rVB2	203	242	0.03%	0.004%
21	5.726	759	761	764	rVB	357	260	0.03%	0.004%
22	5.781	768	770	772	rBV2	219	246	0.03%	0.004%
23	5.970	787	801	815	rBV2	261048	786937	100.00%	12.235%
24	6.330	858	860	863	rVB2	269	232	0.03%	0.004%
25	6.525	890	892	894	rBV	300	217	0.03%	0.003%
26	6.555	894	897	899	rBV2	163	219	0.03%	0.003%
27	6.763	922	931	945	rBV	212975	513194	65.21%	7.979%
28	7.049	976	978	981	rBV2	184	267	0.03%	0.004%
29	7.110	984	988	995	rVV4	1376	2745	0.35%	0.043%
30	7.305	1012	1020	1037	rVV	165738	367591	46.71%	5.715%
31	7.702	1082	1085	1089	rVB2	206	331	0.04%	0.005%
32	7.744	1089	1092	1093	rBV	233	222	0.03%	0.003%
33	7.970	1127	1129	1132	rVV2	188	228	0.03%	0.004%
34	8.177	1160	1163	1164	rBV2	175	196	0.02%	0.003%
35	8.195	1164	1166	1170	rVB2	200	221	0.03%	0.003%
36	8.323	1181	1187	1204	rBV	109270	182857	23.24%	2.843%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121823\
 Data File : VX039332.D
 Acq On : 18 Dec 2023 23:31
 Operator : JC/MD
 Sample : 05835-14 100X
 Misc : 4.07g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0AR1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
 Title : VOC Analysis

37	8.531	1219	1221	1222	rVB	306	186	0.02%	0.003%
38	8.579	1226	1229	1231	rBV2	338	403	0.05%	0.006%
39	8.647	1233	1240	1259	rBV	371006	597689	75.95%	9.292%
40	8.848	1271	1273	1277	rBV3	216	275	0.03%	0.004%
41	8.951	1284	1290	1303	rBV	78958	122412	15.56%	1.903%
42	9.153	1320	1323	1326	rBV2	203	278	0.04%	0.004%
43	9.201	1326	1331	1334	rBV2	212	438	0.06%	0.007%
44	9.274	1340	1343	1348	rVB3	315	457	0.06%	0.007%
45	9.384	1355	1361	1380	rBV	375683	557459	70.84%	8.667%
46	9.695	1409	1412	1420	rBV4	891	1599	0.20%	0.025%
47	9.799	1426	1429	1431	rBV	168	193	0.02%	0.003%
48	9.915	1446	1448	1453	rVB2	304	327	0.04%	0.005%
49	10.055	1465	1471	1489	rBV	464485	703973	89.46%	10.945%
50	10.189	1491	1493	1494	rBV2	254	216	0.03%	0.003%
51	10.305	1510	1512	1517	rVB2	311	424	0.05%	0.007%
52	10.500	1540	1544	1546	rBV2	267	318	0.04%	0.005%
53	10.652	1564	1569	1573	rVV2	428	702	0.09%	0.011%
54	10.732	1576	1582	1585	rBV2	270	605	0.08%	0.009%
55	10.774	1585	1589	1590	rVV2	163	236	0.03%	0.004%
56	10.866	1602	1604	1608	rVB2	210	219	0.03%	0.003%
57	10.969	1618	1621	1625	rVB2	451	690	0.09%	0.011%
58	11.024	1625	1630	1631	rBV2	227	324	0.04%	0.005%
59	11.091	1638	1641	1643	rBV	464	500	0.06%	0.008%
60	11.189	1652	1657	1669	rBV	317660	417473	53.05%	6.491%
61	11.463	1695	1702	1705	rBV3	321	647	0.08%	0.010%
62	11.524	1711	1712	1715	rVV2	204	189	0.02%	0.003%
63	11.670	1735	1736	1739	rVB2	246	174	0.02%	0.003%
64	11.713	1739	1743	1744	rBV	182	200	0.03%	0.003%
65	11.756	1747	1750	1755	rBV3	479	651	0.08%	0.010%
66	11.829	1760	1762	1765	rVB2	274	226	0.03%	0.004%
67	11.859	1765	1767	1769	rBV	181	176	0.02%	0.003%
68	11.975	1783	1786	1788	rVB3	697	733	0.09%	0.011%
69	12.024	1788	1794	1807	rBV	465757	623923	79.28%	9.700%
70	12.195	1819	1822	1824	rVB2	220	202	0.03%	0.003%
71	12.317	1837	1842	1854	rVV	416700	537090	68.25%	8.350%
72	12.762	1911	1915	1918	rBV3	601	693	0.09%	0.011%
73	12.859	1929	1931	1934	rVB	272	199	0.03%	0.003%
74	12.896	1934	1937	1938	rBV2	254	188	0.02%	0.003%
75	13.042	1960	1961	1965	rBV2	197	249	0.03%	0.004%
76	13.188	1981	1985	1986	rVV	178	211	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121823\
 Data File : VX039332.D
 Acq On : 18 Dec 2023 23:31
 Operator : JC/MD
 Sample : 05835-14 100X
 Misc : 4.07g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0AR1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

77	13.432	2022	2025	2026	rBV2	193	211	0.03%	0.003%
78	13.524	2038	2040	2042	rBV	279	236	0.03%	0.004%
79	13.591	2049	2051	2055	rBV3	442	586	0.07%	0.009%
80	13.786	2080	2083	2088	rBV2	501	687	0.09%	0.011%
81	13.963	2109	2112	2114	rVB2	249	303	0.04%	0.005%
82	14.005	2117	2119	2121	rVB	352	186	0.02%	0.003%
83	14.097	2132	2134	2135	rBV	331	204	0.03%	0.003%
84	14.133	2135	2140	2142	rBV2	1145	1701	0.22%	0.026%
85	14.213	2151	2153	2154	rVB2	349	232	0.03%	0.004%
86	14.359	2175	2177	2179	rBV2	168	180	0.02%	0.003%
87	14.889	2259	2264	2265	rBV2	273	336	0.04%	0.005%
88	15.011	2281	2284	2285	rBV3	230	246	0.03%	0.004%
89	15.145	2304	2306	2310	rVB3	424	509	0.06%	0.008%
90	15.225	2315	2319	2320	rVV3	229	278	0.04%	0.004%
91	15.249	2322	2323	2325	rBV2	272	254	0.03%	0.004%
92	15.273	2325	2327	2330	rVV2	352	282	0.04%	0.004%
93	15.322	2333	2335	2342	rBV2	291	462	0.06%	0.007%
94	15.395	2342	2347	2350	rBV3	589	968	0.12%	0.015%
95	15.712	2397	2399	2402	rBV2	271	346	0.04%	0.005%
96	15.834	2417	2419	2422	rVB	229	195	0.02%	0.003%
97	15.859	2422	2423	2426	rBV3	479	411	0.05%	0.006%
98	16.139	2467	2469	2472	rBV2	396	500	0.06%	0.008%
99	16.298	2493	2495	2497	rVB3	438	351	0.04%	0.005%
100	16.322	2497	2499	2503	rBV2	309	383	0.05%	0.006%

Sum of corrected areas: 6431955




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121823\
Data File : VX039332.D
Acq On : 18 Dec 2023 23:31
Operator : JC/MD
Sample : 05835-14 100X
Misc : 4.07g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0AR1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

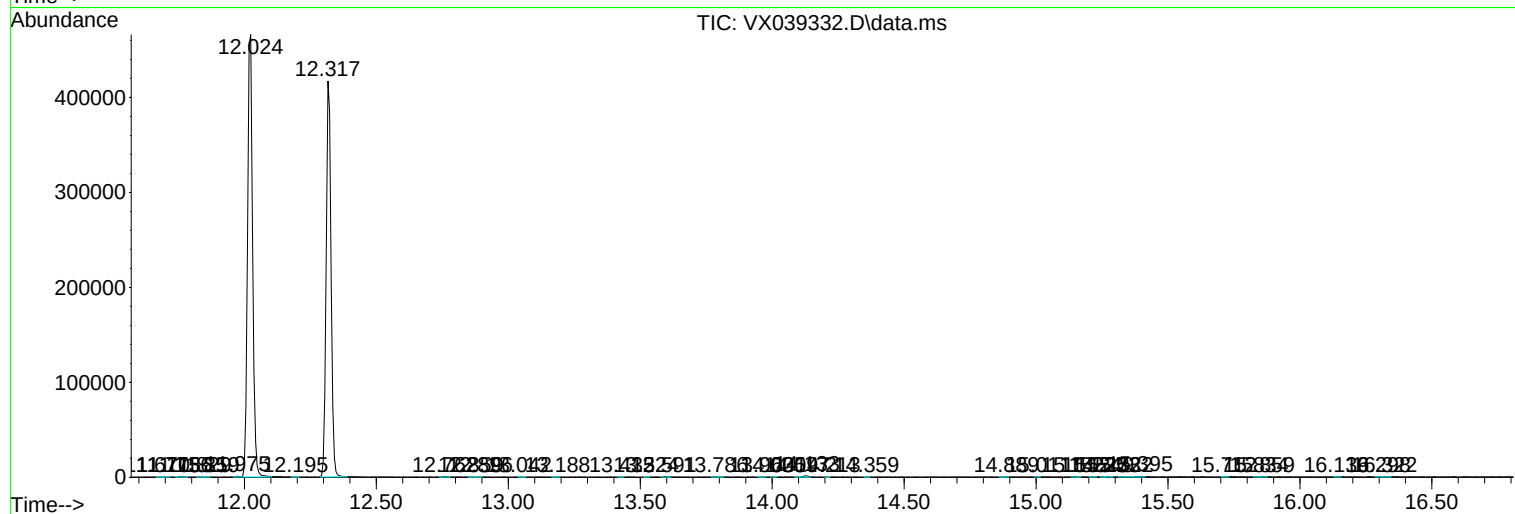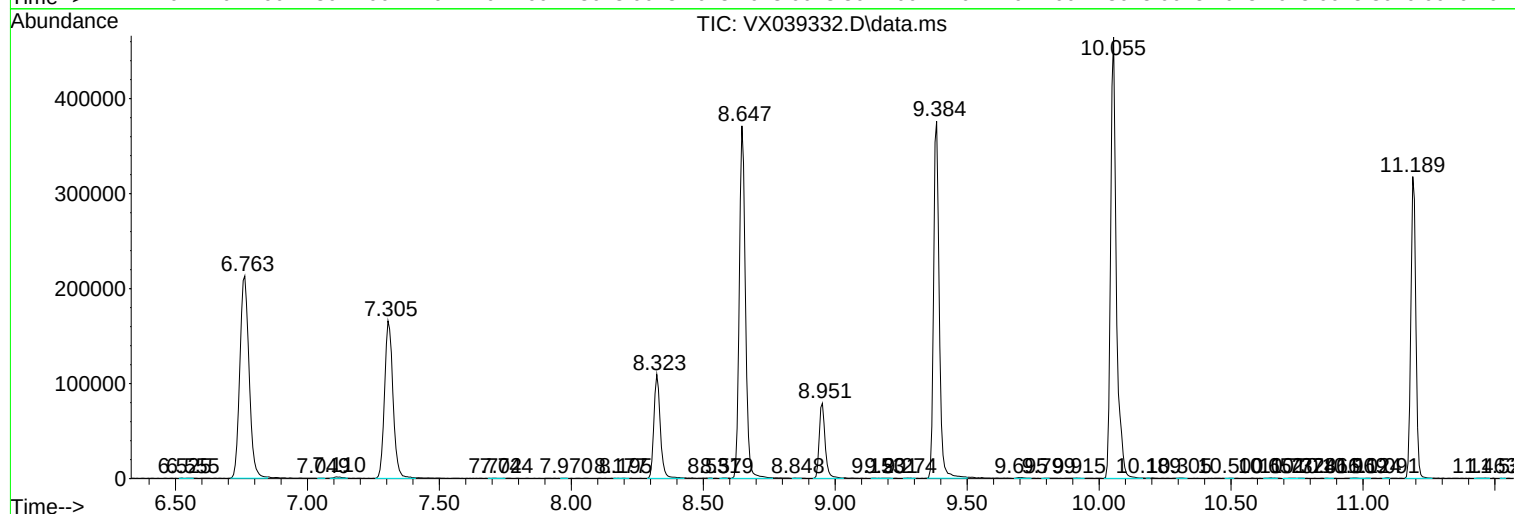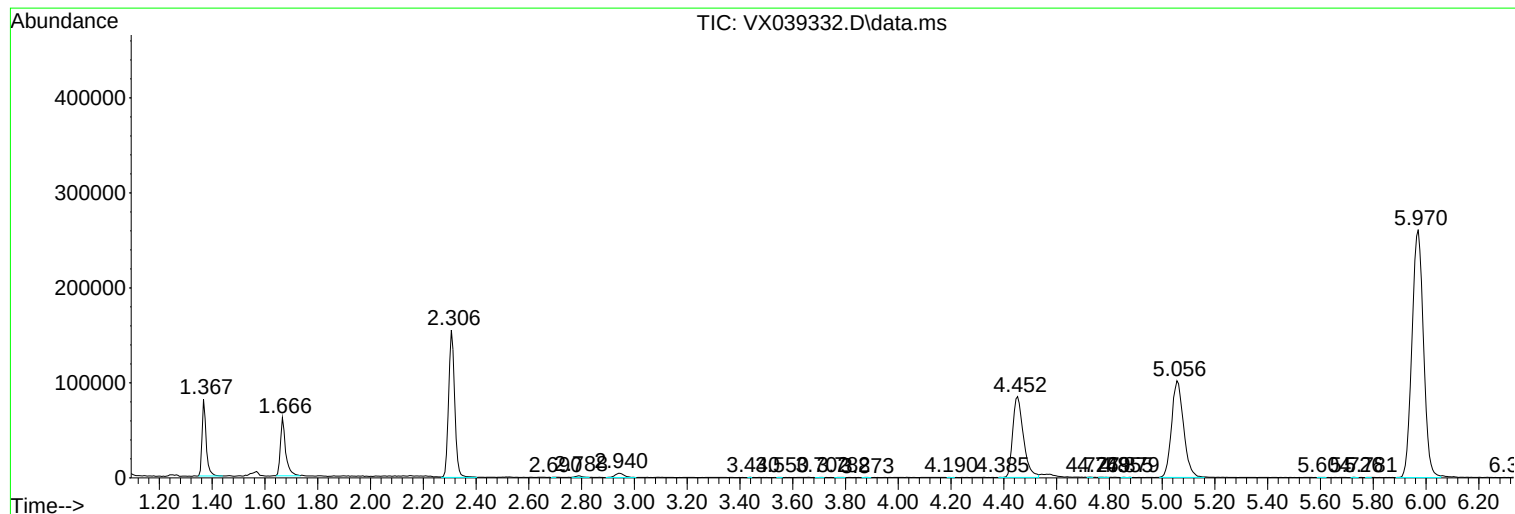

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121823\
Data File : VX039332.D
Acq On : 18 Dec 2023 23:31
Operator : JC/MD
Sample : 05835-14 100X
Misc : 4.07g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0AR1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121823\
Data File : VX039332.D
Acq On : 18 Dec 2023 23:31
Operator : JC/MD
Sample : 05835-14 100X
Misc : 4.07g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0AR1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc