

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121823\
 Data File : VX039336.D
 Acq On : 19 Dec 2023 01:03
 Operator : JC/MD
 Sample : 05835-18 100X
 Misc : 3.34g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0AR8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
 Title : VOC Analysis

Signal : TIC: VX039336.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	22	26	27	rBV2	1567	2033	0.03%	0.014%
2	1.368	43	46	58	rVB	80793	85068	1.39%	0.592%
3	1.666	91	95	108	rVB	55278	80894	1.33%	0.563%
4	2.306	194	200	210	rBV	143814	224921	3.68%	1.566%
5	2.514	232	234	237	rBV2	368	268	0.00%	0.002%
6	2.581	243	245	248	rBV2	225	261	0.00%	0.002%
7	2.605	248	249	256	rVV2	331	496	0.01%	0.003%
8	2.794	275	280	287	rVB2	1782	3325	0.05%	0.023%
9	2.946	297	305	316	rVB2	6259	14666	0.24%	0.102%
10	3.111	326	332	334	rBV2	247	495	0.01%	0.003%
11	3.196	341	346	351	rBV2	255	462	0.01%	0.003%
12	3.507	396	397	401	rVB	263	279	0.00%	0.002%
13	3.763	436	439	440	rBV	211	172	0.00%	0.001%
14	3.977	473	474	476	rBV	387	247	0.00%	0.002%
15	4.044	483	485	488	rBV2	270	332	0.01%	0.002%
16	4.227	513	515	516	rBV	276	277	0.00%	0.002%
17	4.452	543	552	565	rBV	83062	239406	3.92%	1.667%
18	5.056	638	651	669	rBV2	97374	313012	5.13%	2.179%
19	5.257	682	684	687	rVB	336	185	0.00%	0.001%
20	5.647	745	748	750	rVV2	194	220	0.00%	0.002%
21	5.690	753	755	758	rBV2	175	202	0.00%	0.001%
22	5.775	767	769	773	rVB2	271	286	0.00%	0.002%
23	5.970	788	801	811	rBV2	252442	781209	12.80%	5.439%
24	6.269	847	850	852	rBV2	194	241	0.00%	0.002%
25	6.489	885	886	889	rVB	281	185	0.00%	0.001%
26	6.568	893	899	902	rVB2	263	523	0.01%	0.004%
27	6.598	902	904	906	rBV	259	224	0.00%	0.002%
28	6.641	909	911	914	rBV2	159	210	0.00%	0.001%
29	6.763	920	931	946	rBV	204857	495111	8.11%	3.447%
30	7.116	983	989	995	rVB5	1471	3052	0.05%	0.021%
31	7.305	1012	1020	1037	rBV	162690	362673	5.94%	2.525%
32	7.470	1045	1047	1048	rBV2	410	262	0.00%	0.002%
33	7.659	1075	1078	1079	rVB	223	172	0.00%	0.001%
34	7.738	1090	1091	1094	rBV2	163	174	0.00%	0.001%
35	7.952	1121	1126	1127	rBV	385	326	0.01%	0.002%
36	7.970	1127	1129	1130	rVV	423	296	0.00%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121823\
 Data File : VX039336.D
 Acq On : 19 Dec 2023 01:03
 Operator : JC/MD
 Sample : 05835-18 100X
 Misc : 3.34g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0AR8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
 Title : VOC Analysis

37	8.013	1134	1136	1137	rVB2	313	179	0.00%	0.001%
38	8.031	1137	1139	1140	rBV	337	232	0.00%	0.002%
39	8.208	1166	1168	1170	rBV2	291	292	0.00%	0.002%
40	8.324	1181	1187	1203	rBV	109200	179470	2.94%	1.249%
41	8.647	1234	1240	1256	rBV	355690	562933	9.22%	3.919%
42	8.860	1273	1275	1278	rBV	168	194	0.00%	0.001%
43	8.952	1283	1290	1301	rBV	76860	119124	1.95%	0.829%
44	9.384	1355	1361	1376	rBV	374850	554034	9.08%	3.857%
45	9.628	1399	1401	1404	rVB2	361	287	0.00%	0.002%
46	9.701	1409	1413	1416	rBV2	861	1157	0.02%	0.008%
47	9.756	1420	1422	1425	rBV2	273	313	0.01%	0.002%
48	9.787	1425	1427	1429	rBV	305	196	0.00%	0.001%
49	10.006	1461	1463	1464	rVB	293	177	0.00%	0.001%
50	10.055	1465	1471	1472	rBV	471771	618740	10.14%	4.308%
51	10.079	1472	1475	1492	rVB	880994	1206454	19.77%	8.399%
52	10.311	1509	1513	1516	rVB3	501	696	0.01%	0.005%
53	10.366	1521	1522	1527	rBV2	266	273	0.00%	0.002%
54	10.640	1565	1567	1569	rBV3	274	265	0.00%	0.002%
55	10.726	1579	1581	1584	rVB2	206	185	0.00%	0.001%
56	10.768	1584	1588	1591	rVB2	198	327	0.01%	0.002%
57	11.030	1630	1631	1636	rVB2	131	209	0.00%	0.001%
58	11.091	1638	1641	1644	rVB2	418	492	0.01%	0.003%
59	11.189	1652	1657	1668	rVV	331257	414996	6.80%	2.889%
60	11.311	1675	1677	1680	rVB	172	171	0.00%	0.001%
61	11.366	1683	1686	1690	rBV3	607	806	0.01%	0.006%
62	11.457	1697	1701	1704	rBV2	621	919	0.02%	0.006%
63	11.756	1747	1750	1754	rVB3	339	447	0.01%	0.003%
64	11.866	1766	1768	1771	rBV2	251	177	0.00%	0.001%
65	11.969	1780	1785	1789	rBV	76392	94909	1.55%	0.661%
66	12.042	1789	1797	1812	rVB	4402248	6103772	100.00%	42.495%
67	12.323	1837	1843	1859	rVB2	483136	833576	13.66%	5.803%
68	12.481	1866	1869	1872	rBV	249	322	0.01%	0.002%
69	12.548	1878	1880	1883	rBV	270	248	0.00%	0.002%
70	12.701	1903	1905	1908	rVB2	427	421	0.01%	0.003%
71	12.762	1911	1915	1919	rVV2	742	1041	0.02%	0.007%
72	12.987	1951	1952	1956	rVB2	251	259	0.00%	0.002%
73	13.018	1956	1957	1959	rBV	241	217	0.00%	0.002%
74	13.061	1959	1964	1970	rVV3	15487	29403	0.48%	0.205%
75	13.109	1970	1972	1981	rVB3	2711	3792	0.06%	0.026%
76	13.201	1985	1987	1989	rBV2	184	198	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121823\
 Data File : VX039336.D
 Acq On : 19 Dec 2023 01:03
 Operator : JC/MD
 Sample : 05835-18 100X
 Misc : 3.34g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0AR8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

77	13.384	2013	2017	2022	rBV4	1707	2072	0.03%	0.014%
78	13.585	2045	2050	2062	rBV	395646	497432	8.15%	3.463%
79	13.707	2069	2070	2073	rBV2	215	187	0.00%	0.001%
80	13.780	2078	2082	2086	rBV2	666	894	0.01%	0.006%
81	13.871	2095	2097	2101	rVB2	308	275	0.00%	0.002%
82	13.957	2106	2111	2121	rVV	318354	412864	6.76%	2.874%
83	14.097	2131	2134	2136	rBV2	211	230	0.00%	0.002%
84	14.127	2136	2139	2142	rVV3	1246	1589	0.03%	0.011%
85	14.280	2160	2164	2166	rVB2	248	249	0.00%	0.002%
86	14.548	2204	2208	2210	rBV3	396	508	0.01%	0.004%
87	14.627	2218	2221	2224	rVB3	1413	1642	0.03%	0.011%
88	14.780	2239	2246	2251	rBV3	9828	18564	0.30%	0.129%
89	14.981	2278	2279	2281	rBV	362	240	0.00%	0.002%
90	15.030	2286	2287	2290	rVB2	383	287	0.00%	0.002%
91	15.249	2317	2323	2331	rVB	54157	78413	1.28%	0.546%
92	15.341	2337	2338	2340	rBV	325	234	0.00%	0.002%
93	15.737	2401	2403	2404	rVB	332	171	0.00%	0.001%
94	15.755	2404	2406	2409	rVB2	303	205	0.00%	0.001%
95	15.792	2411	2412	2414	rBV	497	356	0.01%	0.002%
96	15.871	2422	2425	2428	rVB3	367	418	0.01%	0.003%
97	16.170	2472	2474	2475	rBV	318	186	0.00%	0.001%
98	16.517	2526	2531	2535	rBV3	1230	2071	0.03%	0.014%
99	16.596	2542	2544	2546	rBV3	302	232	0.00%	0.002%
100	16.724	2563	2565	2566	rVB2	439	272	0.00%	0.002%




Sum of corrected areas: 14363659

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121823\
Data File : VX039336.D
Acq On : 19 Dec 2023 01:03
Operator : JC/MD
Sample : 05835-18 100X
Misc : 3.34g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0AR8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

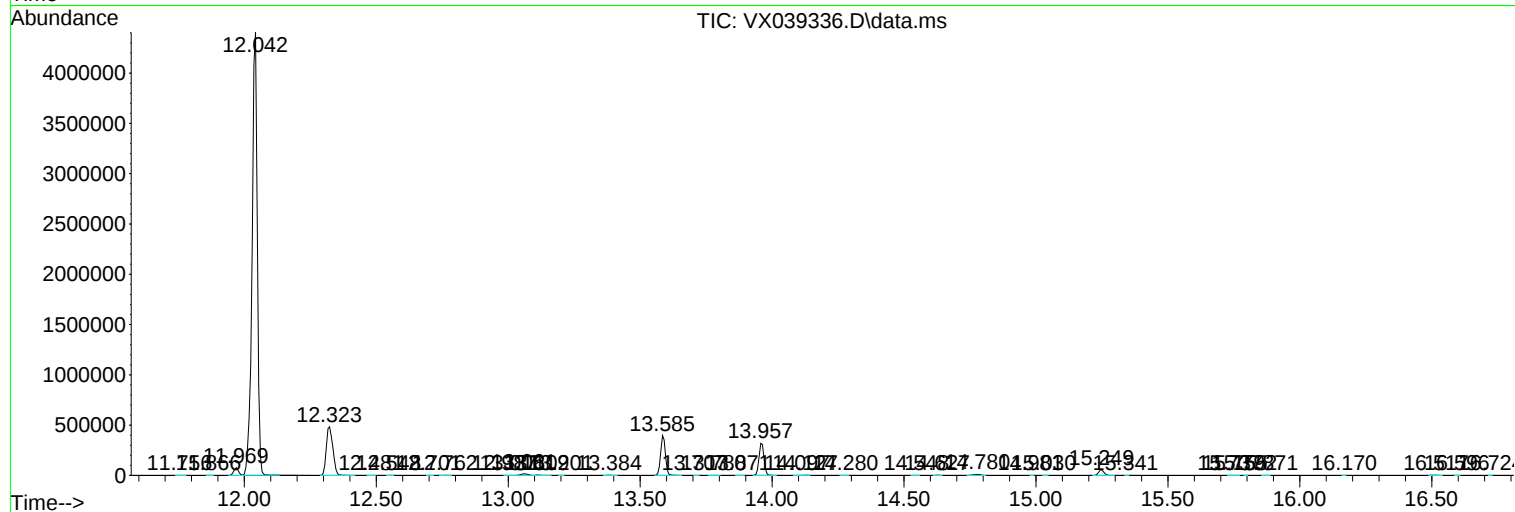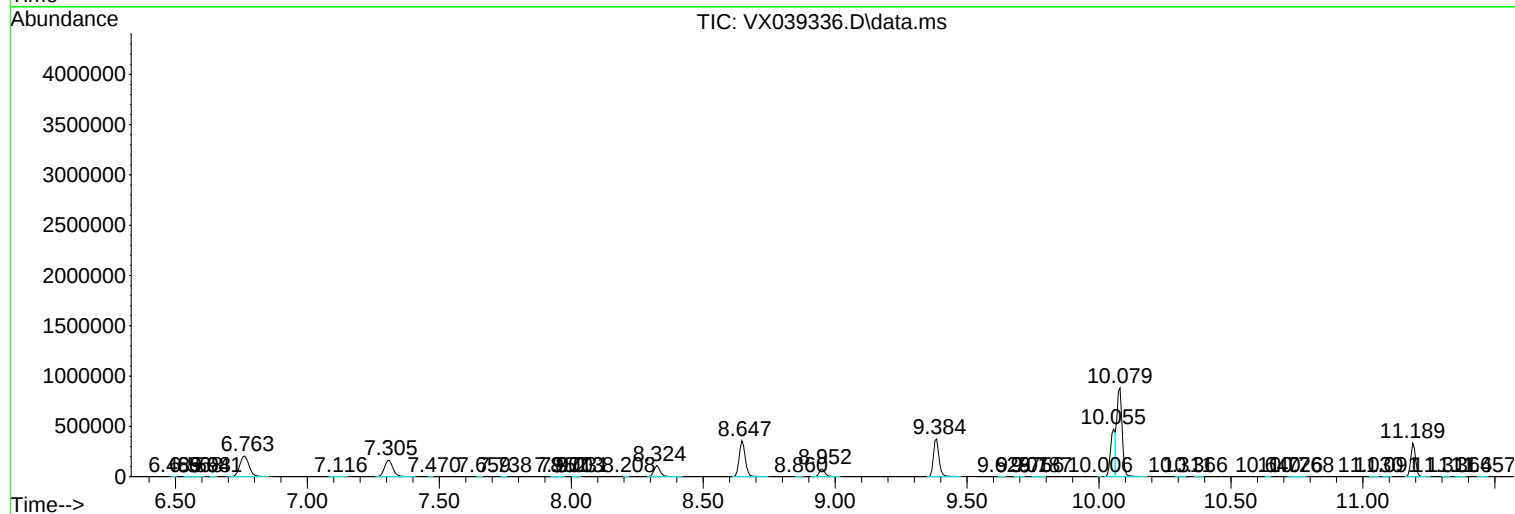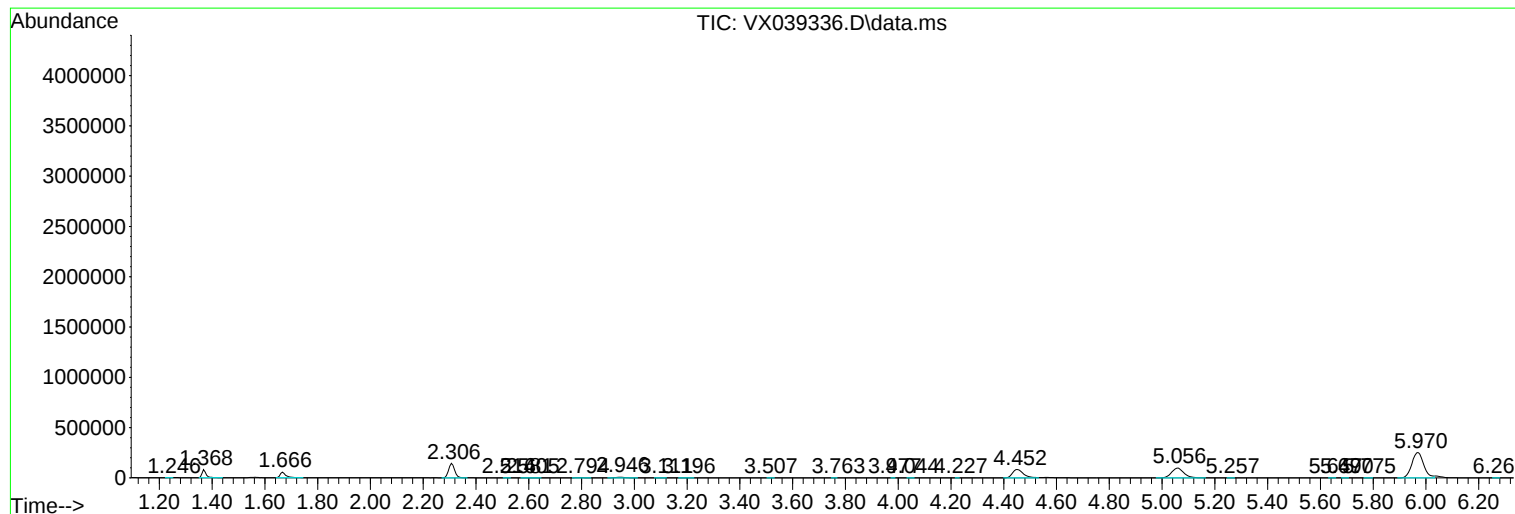

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121823\
Data File : VX039336.D
Acq On : 19 Dec 2023 01:03
Operator : JC/MD
Sample : 05835-18 100X
Misc : 3.34g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0AR8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121823\
Data File : VX039336.D
Acq On : 19 Dec 2023 01:03
Operator : JC/MD
Sample : 05835-18 100X
Misc : 3.34g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0AR8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
