

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121823\
 Data File : VX039338.D
 Acq On : 19 Dec 2023 01:48
 Operator : JC/MD
 Sample : 05835-20 100X
 Misc : 3.06g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0B24

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

Signal : TIC: VX039338.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.239	23	25	28	rBV3	1928	2899	0.37%	0.046%
2	1.368	42	46	59	rVB	82220	90844	11.54%	1.436%
3	1.666	91	95	106	rBV	56281	82024	10.42%	1.297%
4	2.306	194	200	212	rVB	150981	234387	29.77%	3.706%
5	2.703	264	265	267	rBV2	551	320	0.04%	0.005%
6	2.751	270	273	275	rBV	295	300	0.04%	0.005%
7	2.788	275	279	287	rVB3	1790	2970	0.38%	0.047%
8	2.940	298	304	315	rVB	5432	12121	1.54%	0.192%
9	3.111	328	332	334	rBV2	311	385	0.05%	0.006%
10	3.257	355	356	359	rVB2	210	171	0.02%	0.003%
11	3.392	377	378	380	rBV2	298	220	0.03%	0.003%
12	3.581	408	409	414	rVB2	254	271	0.03%	0.004%
13	3.678	424	425	428	rBV	167	196	0.02%	0.003%
14	3.855	452	454	455	rBV	268	197	0.03%	0.003%
15	3.879	455	458	462	rBV2	181	325	0.04%	0.005%
16	4.074	489	490	493	rVB2	213	180	0.02%	0.003%
17	4.135	497	500	503	rBV	244	289	0.04%	0.005%
18	4.227	513	515	517	rBV2	290	206	0.03%	0.003%
19	4.452	543	552	565	rBV	83394	238644	30.31%	3.773%
20	4.708	592	594	597	rBV3	308	328	0.04%	0.005%
21	4.739	597	599	601	rVV	327	287	0.04%	0.005%
22	4.775	603	605	606	rBV	245	181	0.02%	0.003%
23	5.056	639	651	670	rBV	105992	325589	41.36%	5.147%
24	5.330	693	696	699	rBV2	204	256	0.03%	0.004%
25	5.379	701	704	705	rBV	293	347	0.04%	0.005%
26	5.483	719	721	722	rVV	232	167	0.02%	0.003%
27	5.592	737	739	744	rVB2	214	342	0.04%	0.005%
28	5.635	744	746	749	rBV2	163	263	0.03%	0.004%
29	5.763	764	767	768	rBV	301	247	0.03%	0.004%
30	5.970	789	801	819	rBV2	261267	787239	100.00%	12.446%
31	6.397	868	871	875	rVB2	318	477	0.06%	0.008%
32	6.428	875	876	878	rBV	208	207	0.03%	0.003%
33	6.653	911	913	916	rVB	213	192	0.02%	0.003%
34	6.763	922	931	945	rBV	211458	509707	64.75%	8.058%
35	7.049	976	978	981	rBV2	313	289	0.04%	0.005%
36	7.116	983	989	994	rVB2	1463	3471	0.44%	0.055%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121823\
 Data File : VX039338.D
 Acq On : 19 Dec 2023 01:48
 Operator : JC/MD
 Sample : 05835-20 100X
 Misc : 3.06g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0B24

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
 Title : VOC Analysis

37	7.153	994	995	997	rBV	225	185	0.02%	0.003%
38	7.238	1005	1009	1012	rBV	217	260	0.03%	0.004%
39	7.305	1012	1020	1035	rBV	166608	367656	46.70%	5.812%
40	7.488	1045	1050	1054	rBV4	521	948	0.12%	0.015%
41	7.647	1075	1076	1080	rVB	263	188	0.02%	0.003%
42	8.092	1146	1149	1151	rBV2	245	281	0.04%	0.004%
43	8.135	1154	1156	1159	rVB	222	204	0.03%	0.003%
44	8.324	1181	1187	1198	rBV	105893	180428	22.92%	2.852%
45	8.580	1225	1229	1230	rBV	326	303	0.04%	0.005%
46	8.647	1234	1240	1260	rVV	374090	590966	75.07%	9.343%
47	8.952	1284	1290	1298	rBV	78255	119196	15.14%	1.884%
48	9.177	1325	1327	1330	rBV2	234	224	0.03%	0.004%
49	9.269	1339	1342	1344	rVV2	269	280	0.04%	0.004%
50	9.384	1355	1361	1380	rBV	373400	547343	69.53%	8.653%
51	9.665	1405	1407	1409	rVB	307	176	0.02%	0.003%
52	9.695	1409	1412	1418	rBV4	659	1183	0.15%	0.019%
53	9.884	1442	1443	1446	rBV	297	170	0.02%	0.003%
54	10.055	1465	1471	1482	rBV	443214	631555	80.22%	9.985%
55	10.317	1510	1514	1516	rVB2	409	453	0.06%	0.007%
56	10.683	1572	1574	1576	rBV2	282	210	0.03%	0.003%
57	10.854	1600	1602	1606	rVB2	183	239	0.03%	0.004%
58	10.933	1610	1615	1617	rVV2	176	232	0.03%	0.004%
59	10.976	1617	1622	1626	rVB2	360	653	0.08%	0.010%
60	11.049	1632	1634	1636	rBV2	170	171	0.02%	0.003%
61	11.189	1652	1657	1671	rVB	325154	414814	52.69%	6.558%
62	11.311	1674	1677	1679	rVV2	311	253	0.03%	0.004%
63	11.457	1697	1701	1702	rVV3	279	267	0.03%	0.004%
64	11.488	1704	1706	1711	rVB2	440	604	0.08%	0.010%
65	11.536	1711	1714	1718	rVB	328	416	0.05%	0.007%
66	11.567	1718	1719	1722	rBV2	164	198	0.03%	0.003%
67	11.756	1748	1750	1752	rVV2	399	331	0.04%	0.005%
68	11.774	1752	1753	1756	rVV2	325	259	0.03%	0.004%
69	11.945	1779	1781	1782	rBV	284	174	0.02%	0.003%
70	11.975	1782	1786	1788	rBV4	709	803	0.10%	0.013%
71	12.018	1788	1793	1804	rBV	460649	623045	79.14%	9.850%
72	12.164	1816	1817	1821	rVB3	355	352	0.04%	0.006%
73	12.201	1821	1823	1825	rBV2	202	213	0.03%	0.003%
74	12.317	1837	1842	1850	rBV	415253	532367	67.62%	8.416%
75	12.597	1886	1888	1892	rVV	227	233	0.03%	0.004%
76	12.670	1897	1900	1902	rBV	155	172	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121823\
 Data File : VX039338.D
 Acq On : 19 Dec 2023 01:48
 Operator : JC/MD
 Sample : 05835-20 100X
 Misc : 3.06g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0B24

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

77	12.768	1912	1916	1918	rVB3	562	699	0.09%	0.011%
78	13.128	1971	1975	1976	rBV2	207	198	0.03%	0.003%
79	13.359	2012	2013	2015	rBV	194	167	0.02%	0.003%
80	13.378	2015	2016	2020	rVV	294	249	0.03%	0.004%
81	13.463	2028	2030	2034	rBV	138	187	0.02%	0.003%
82	13.493	2034	2035	2039	rBV	220	204	0.03%	0.003%
83	13.597	2048	2052	2056	rBV3	1569	2077	0.26%	0.033%
84	13.719	2070	2072	2075	rVB2	258	245	0.03%	0.004%
85	13.774	2078	2081	2082	rBV2	265	313	0.04%	0.005%
86	13.884	2098	2099	2103	rVB	271	262	0.03%	0.004%
87	13.920	2103	2105	2108	rBV2	204	248	0.03%	0.004%
88	13.969	2108	2113	2117	rBV2	899	1242	0.16%	0.020%
89	14.127	2136	2139	2143	rVB2	1098	1423	0.18%	0.022%
90	14.420	2184	2187	2188	rBV	195	216	0.03%	0.003%
91	14.829	2252	2254	2258	rVB3	307	314	0.04%	0.005%
92	14.883	2261	2263	2266	rBV3	232	295	0.04%	0.005%
93	15.011	2283	2284	2285	rBV	365	231	0.03%	0.004%
94	15.176	2307	2311	2313	rBV2	370	543	0.07%	0.009%
95	15.389	2342	2346	2347	rBV2	438	523	0.07%	0.008%
96	15.420	2349	2351	2352	rVB2	422	246	0.03%	0.004%
97	15.554	2370	2373	2374	rBV2	273	223	0.03%	0.004%
98	16.151	2469	2471	2472	rBV	312	218	0.03%	0.003%
99	16.292	2492	2494	2497	rVB2	306	308	0.04%	0.005%
100	16.371	2506	2507	2510	rBV	258	170	0.02%	0.003%


Sum of corrected areas: 6325344

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121823\
Data File : VX039338.D
Acq On : 19 Dec 2023 01:48
Operator : JC/MD
Sample : 05835-20 100X
Misc : 3.06g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0B24

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

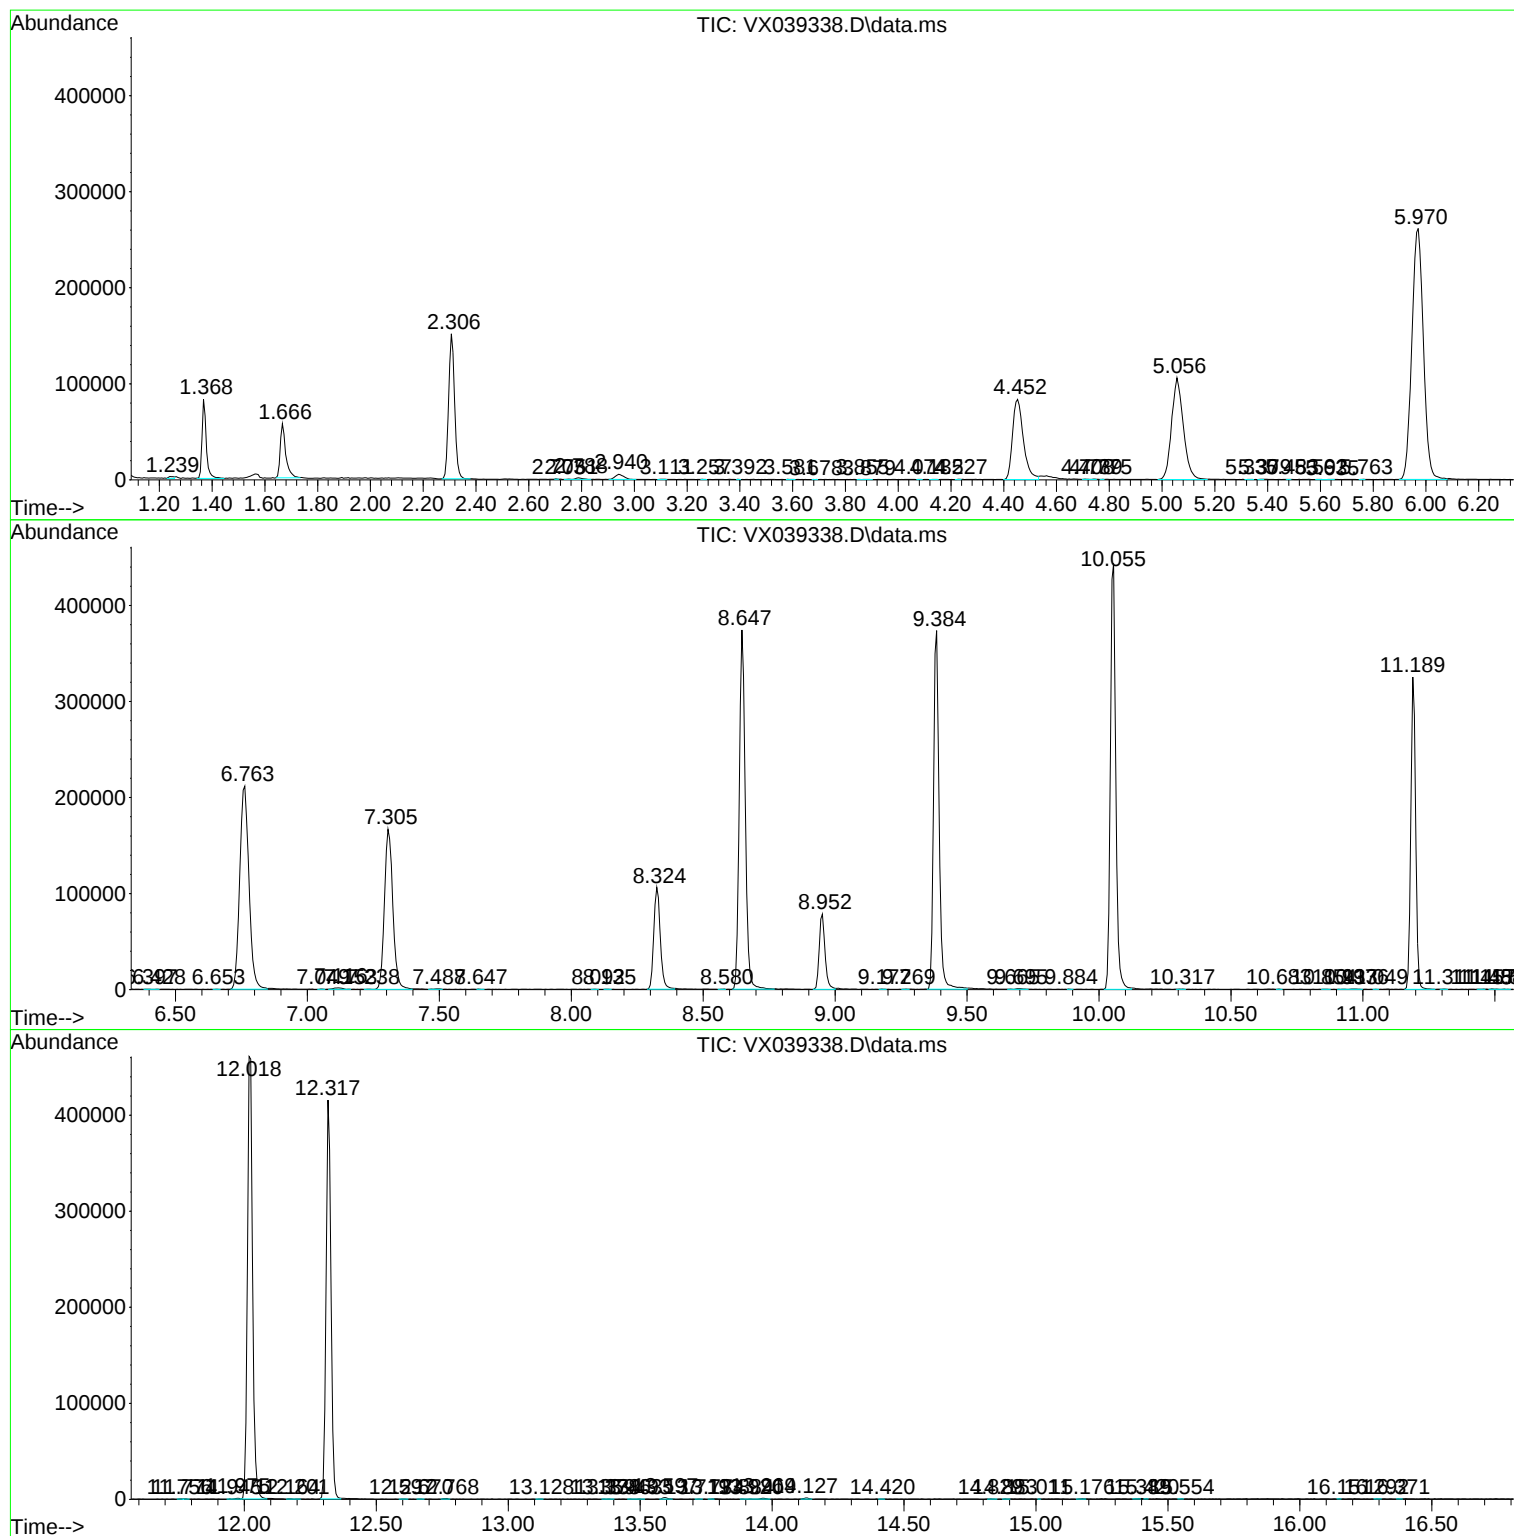

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121823\
Data File : VX039338.D
Acq On : 19 Dec 2023 01:48
Operator : JC/MD
Sample : 05835-20 100X
Misc : 3.06g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0B24

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121823\
Data File : VX039338.D
Acq On : 19 Dec 2023 01:48
Operator : JC/MD
Sample : 05835-20 100X
Misc : 3.06g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0B24

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
