
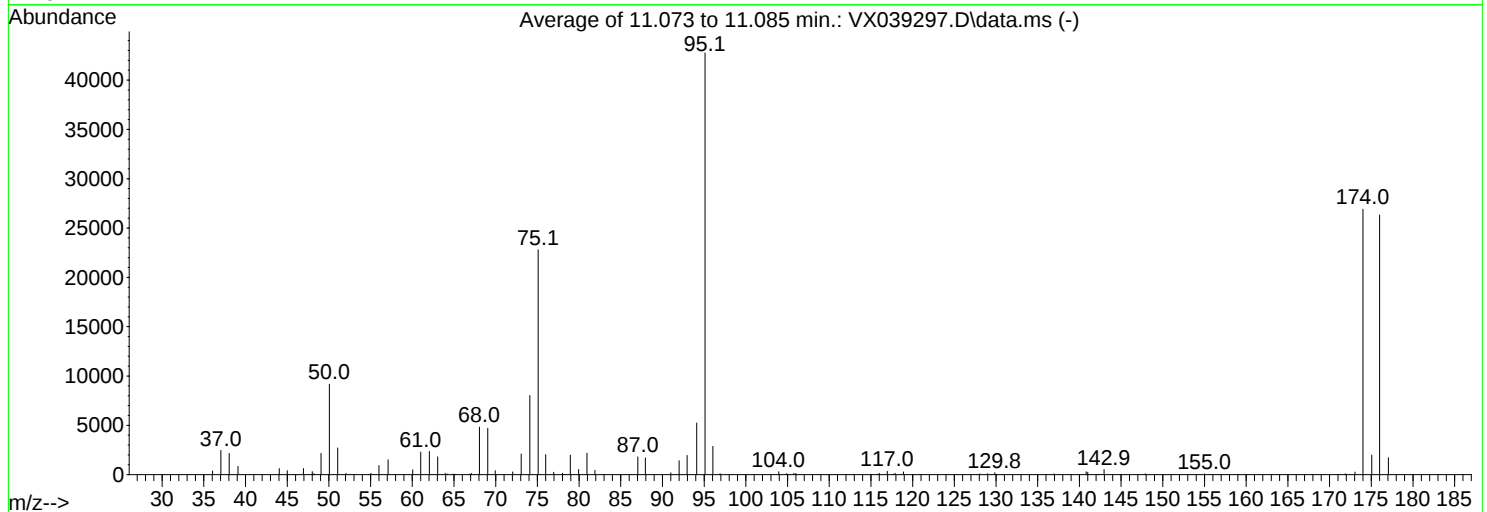


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121823\
Data File : VX039297.D
Acq On : 18 Dec 2023 08:17
Operator : JC/MD
Sample : BFB656
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB656

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
Title : VOC Analysis
Last Update : Mon Dec 18 22:55:37 2023

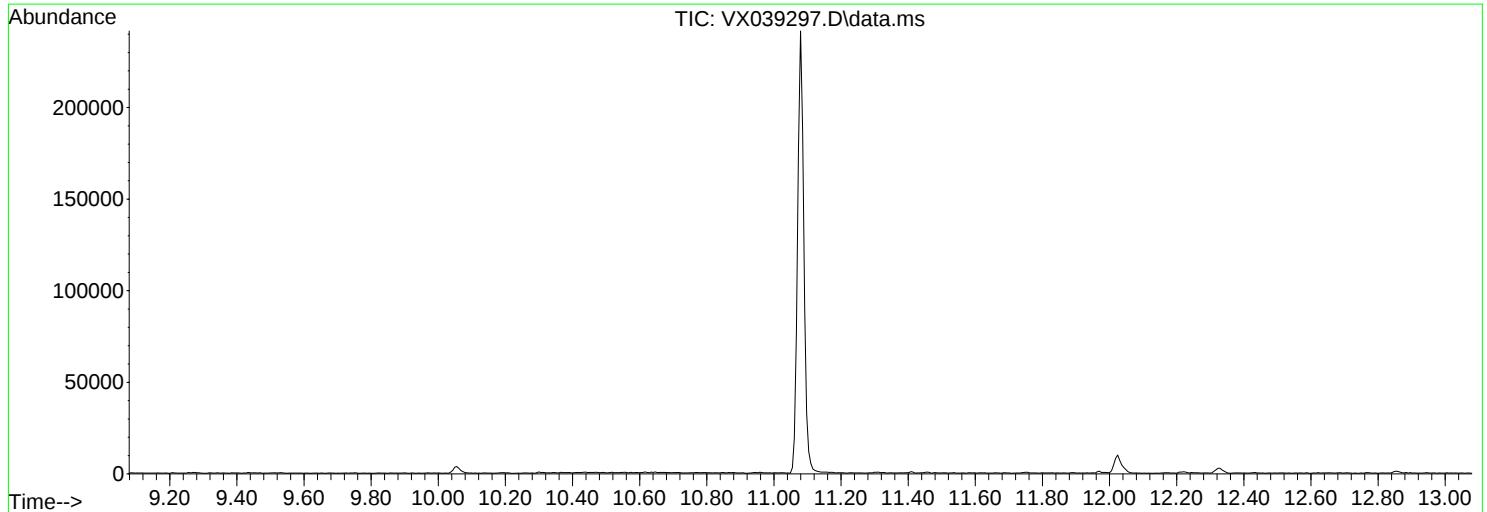

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.4	9165	PASS
75	95	30	80	53.3	22808	PASS
95	95	100	100	100.0	42760	PASS
96	95	5	9	6.7	2871	PASS
173	174	0.00	2	0.9	254	PASS
174	95	50	120	62.9	26917	PASS
175	174	5	9	7.3	1978	PASS
176	174	95	101	97.8	26328	PASS
177	176	5	9	6.6	1727	PASS

m/z	Abundance
36.10	128.0
39.90	213.0
43.80	221.0

Instrument :
MSVOA_X
ClientSampleId :
BFB656

m/z	Abundance
36.00	459.0
37.10	2462.0
38.10	2177.0
39.10	957.0
40.00	240.0
44.10	570.0
45.10	308.0
47.00	523.0
48.00	494.0
49.00	2133.0
50.00	8917.0
51.00	2900.0
52.00	181.0
55.00	167.0
56.00	797.0
57.10	1343.0
60.10	362.0
61.00	2250.0
62.10	2351.0
63.00	1620.0
64.00	176.0
64.90	98.0
66.90	176.0
68.00	4512.0
69.00	4411.0
70.00	482.0
72.10	203.0
73.10	2071.0
74.10	7235.0
75.10	21376.0
76.00	1876.0
77.00	206.0
78.10	192.0
78.90	1802.0
79.90	542.0
81.00	2018.0
81.80	430.0
87.10	1536.0
88.00	1683.0
91.10	218.0
92.00	1411.0
93.00	1837.0
94.10	4857.0
95.10	37232.0
96.10	2557.0
96.90	86.0
104.00	263.0
104.80	99.0
105.70	181.0
106.00	175.0
112.90	61.0
115.80	167.0
117.00	297.0
117.70	157.0
119.00	203.0
128.10	154.0
129.00	108.0
129.80	85.0
130.80	55.0
136.90	75.0
140.80	411.0
142.30	90.0
143.00	530.0
146.10	71.0
147.80	90.0
155.00	71.0
157.00	50.0
171.80	65.0
173.10	194.0
174.00	20168.0
175.00	1558.0
176.00	20064.0
177.00	1364.0

Instrument :
MSVOA_X
ClientSampleId :
BFB656

m/z	Abundance
36.10	587.0
37.00	2935.0
38.10	2333.0
39.10	971.0
40.10	176.0
44.00	637.0
45.00	457.0
45.80	59.0
46.20	53.0
46.90	716.0
48.00	443.0
49.10	2512.0
50.10	10587.0
51.00	3041.0
52.00	74.0
55.10	120.0
56.00	1155.0
57.10	1737.0
60.00	618.0
61.00	2783.0
62.00	2664.0
63.00	2338.0
64.20	210.0
65.20	117.0
67.10	154.0
68.10	5744.0
69.10	5617.0
69.90	411.0
72.10	343.0
73.00	2414.0
74.10	9635.0
75.10	27704.0
76.00	2622.0
76.90	294.0
77.90	192.0
79.00	2466.0
80.00	506.0
80.90	2704.0
81.90	471.0
82.90	51.0
87.00	2114.0
88.00	1903.0
90.90	262.0
92.00	1665.0
93.00	2202.0
94.10	6132.0
95.10	52136.0
96.10	3443.0
96.90	120.0
103.90	282.0
104.90	144.0
105.80	214.0
116.00	231.0
116.90	407.0
117.90	293.0
118.90	333.0
126.10	51.0
128.00	96.0
129.00	99.0
129.90	331.0
137.00	115.0
141.00	732.0
142.90	581.0
145.90	50.0
147.90	62.0
155.00	107.0
159.10	78.0
171.90	106.0
173.00	293.0
174.00	32256.0
175.10	2290.0
176.00	31752.0
177.10	2226.0

Instrument :
MSVOA_X
ClientSampleId :
BFB656

m/z	Abundance
36.10	443.0
37.10	1985.0
38.00	1956.0
39.00	613.0
40.10	187.0
44.00	646.0
44.90	472.0
47.00	595.0
48.20	269.0
49.10	1816.0
50.00	7992.0
51.10	2173.0
52.10	125.0
54.80	97.0
55.10	102.0
56.00	831.0
57.10	1453.0
57.90	87.0
60.00	505.0
61.00	1852.0
62.00	2048.0
63.10	1432.0
63.90	252.0
64.90	119.0
67.10	166.0
68.00	4198.0
69.00	4091.0
70.00	352.0
71.90	266.0
73.00	1782.0
74.10	7230.0
75.10	19344.0
76.00	1596.0
76.90	216.0
78.10	79.0
78.90	1652.0
79.90	517.0
81.00	1777.0
82.00	405.0
87.00	1771.0
87.90	1520.0
91.00	128.0
92.00	1158.0
92.90	1819.0
94.10	4719.0
95.10	38912.0
96.00	2612.0
97.00	68.0
103.90	359.0
105.00	82.0
106.00	217.0
112.90	51.0
116.00	156.0
116.90	333.0
117.90	150.0
118.80	301.0
127.70	96.0
128.90	88.0
129.70	164.0
130.10	107.0
136.90	66.0
140.80	460.0
142.90	466.0
148.00	93.0
155.00	76.0
161.00	78.0
172.00	95.0
173.10	274.0
174.00	28328.0
175.00	2087.0
176.00	27168.0
177.10	1592.0

Instrument :
MSVOA_X
ClientSampleId :
BFB656