

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121824\
 Data File : VX044416.D
 Acq On : 19 Dec 2024 06:04
 Operator : JC/MD
 Sample : P5317-18
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 RE132D5-20241217

Integration Parameters: RTEINT.P
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X121124W.M
 Title : SW846 8260

Signal : TIC: VX044416.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.587	68	82	83	rBV3	16891	50805	4.48%	1.126%
2	2.313	194	201	210	rBV4	37234	72848	6.43%	1.614%
3	5.385	693	705	721	rBV2	72077	217436	19.18%	4.819%
4	5.544	721	731	747	rVV	111560	325061	28.67%	7.204%
5	5.952	787	798	813	rBV2	84433	233006	20.55%	5.164%
6	6.757	919	930	948	rBV	186598	458408	40.44%	10.159%
7	7.123	979	990	1003	rBV	518950	1133625	100.00%	25.124%
8	8.647	1234	1240	1257	rBV	399401	628032	55.40%	13.919%
9	10.055	1465	1471	1484	rBV	387191	543693	47.96%	12.049%
10	11.079	1634	1639	1655	rBV	298005	387065	34.14%	8.578%
11	12.018	1788	1793	1807	rBV	354249	462195	40.77%	10.243%

Sum of corrected areas: 4512174




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121824\
Data File : VX044416.D
Acq On : 19 Dec 2024 06:04
Operator : JC/MD
Sample : P5317-18
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE132D5-20241217

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X121124W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

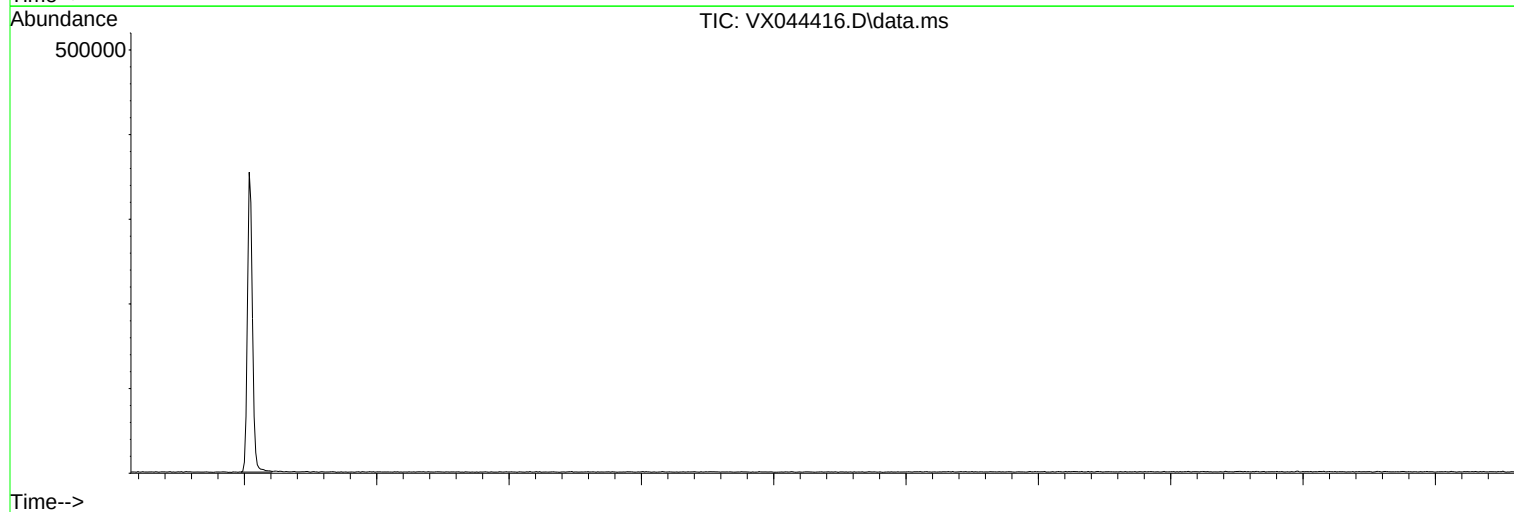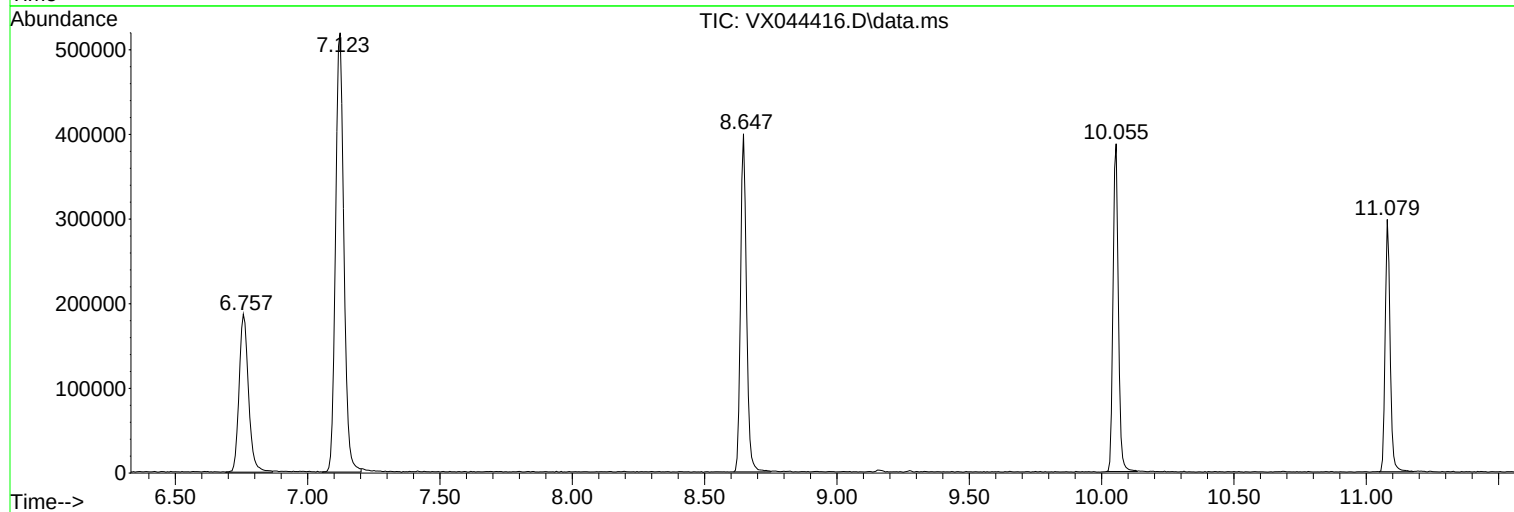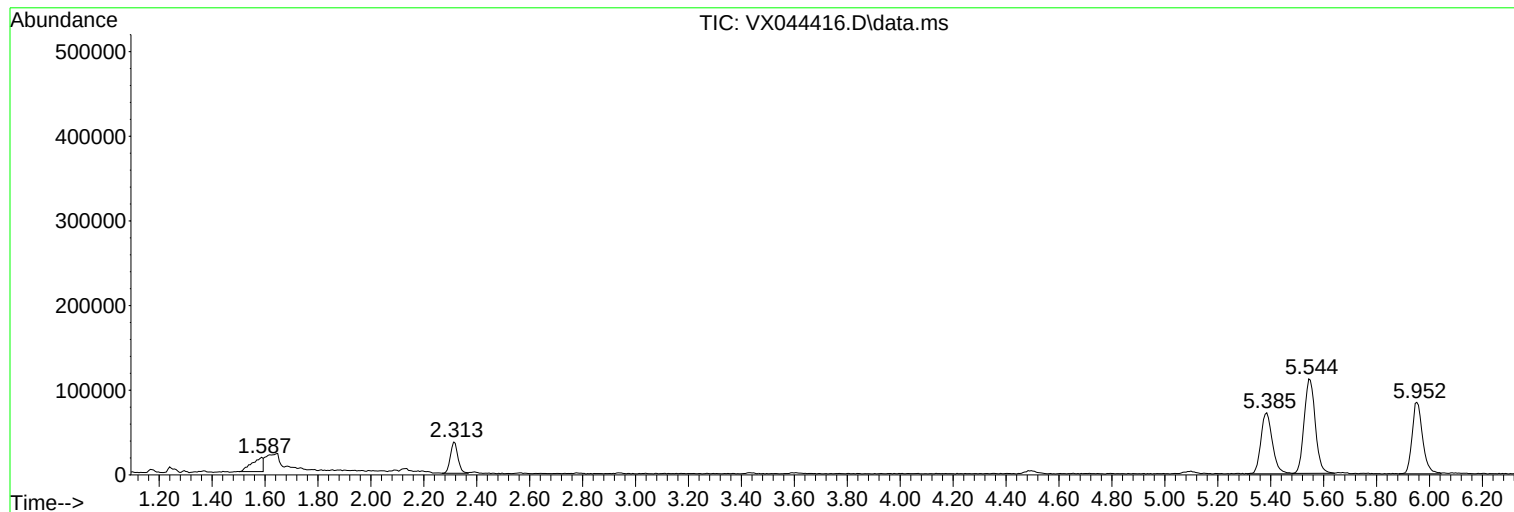

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121824\
Data File : VX044416.D
Acq On : 19 Dec 2024 06:04
Operator : JC/MD
Sample : P5317-18
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE132D5-20241217

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X121124W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121824\
Data File : VX044416.D
Acq On : 19 Dec 2024 06:04
Operator : JC/MD
Sample : P5317-18
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE132D5-20241217

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X121124W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--		
					#	RT	Resp Conc
