

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX121918\
 Data File : VX006638.D
 Acq On : 19 Dec 2018 15:51
 Operator : JC/MD
 Sample : J6479-06
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TRIP-BLANK

Quant Time: Dec 20 04:18:18 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X121818W.M
 Quant Title : SW846 8260
 QLast Update : Wed Dec 19 15:20:58 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.66	168	645006	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.86	114	1012714	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.11	117	923136	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.08	152	435250	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.07	65	348447	50.12	ug/l	0.00
Spiked Amount	50.000		Recovery	=	100.24%	
35) Dibromofluoromethane	5.50	113	308634	48.19	ug/l	0.00
Spiked Amount	50.000		Recovery	=	96.38%	
50) Toluene-d8	8.71	98	1199996	49.70	ug/l	0.00
Spiked Amount	50.000		Recovery	=	99.40%	
62) 4-Bromofluorobenzene	11.13	95	431690	48.82	ug/l	0.00
Spiked Amount	50.000		Recovery	=	97.64%	


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX121918\
Data File : VX006638.D
Acq On : 19 Dec 2018 15:51
Operator : JC/MD
Sample : J6479-06
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TRIP-BLANK

Quant Time: Dec 20 04:18:18 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X121818W.M
Quant Title : SW846 8260
QLast Update : Wed Dec 19 15:20:58 2018
Response via : Initial Calibration

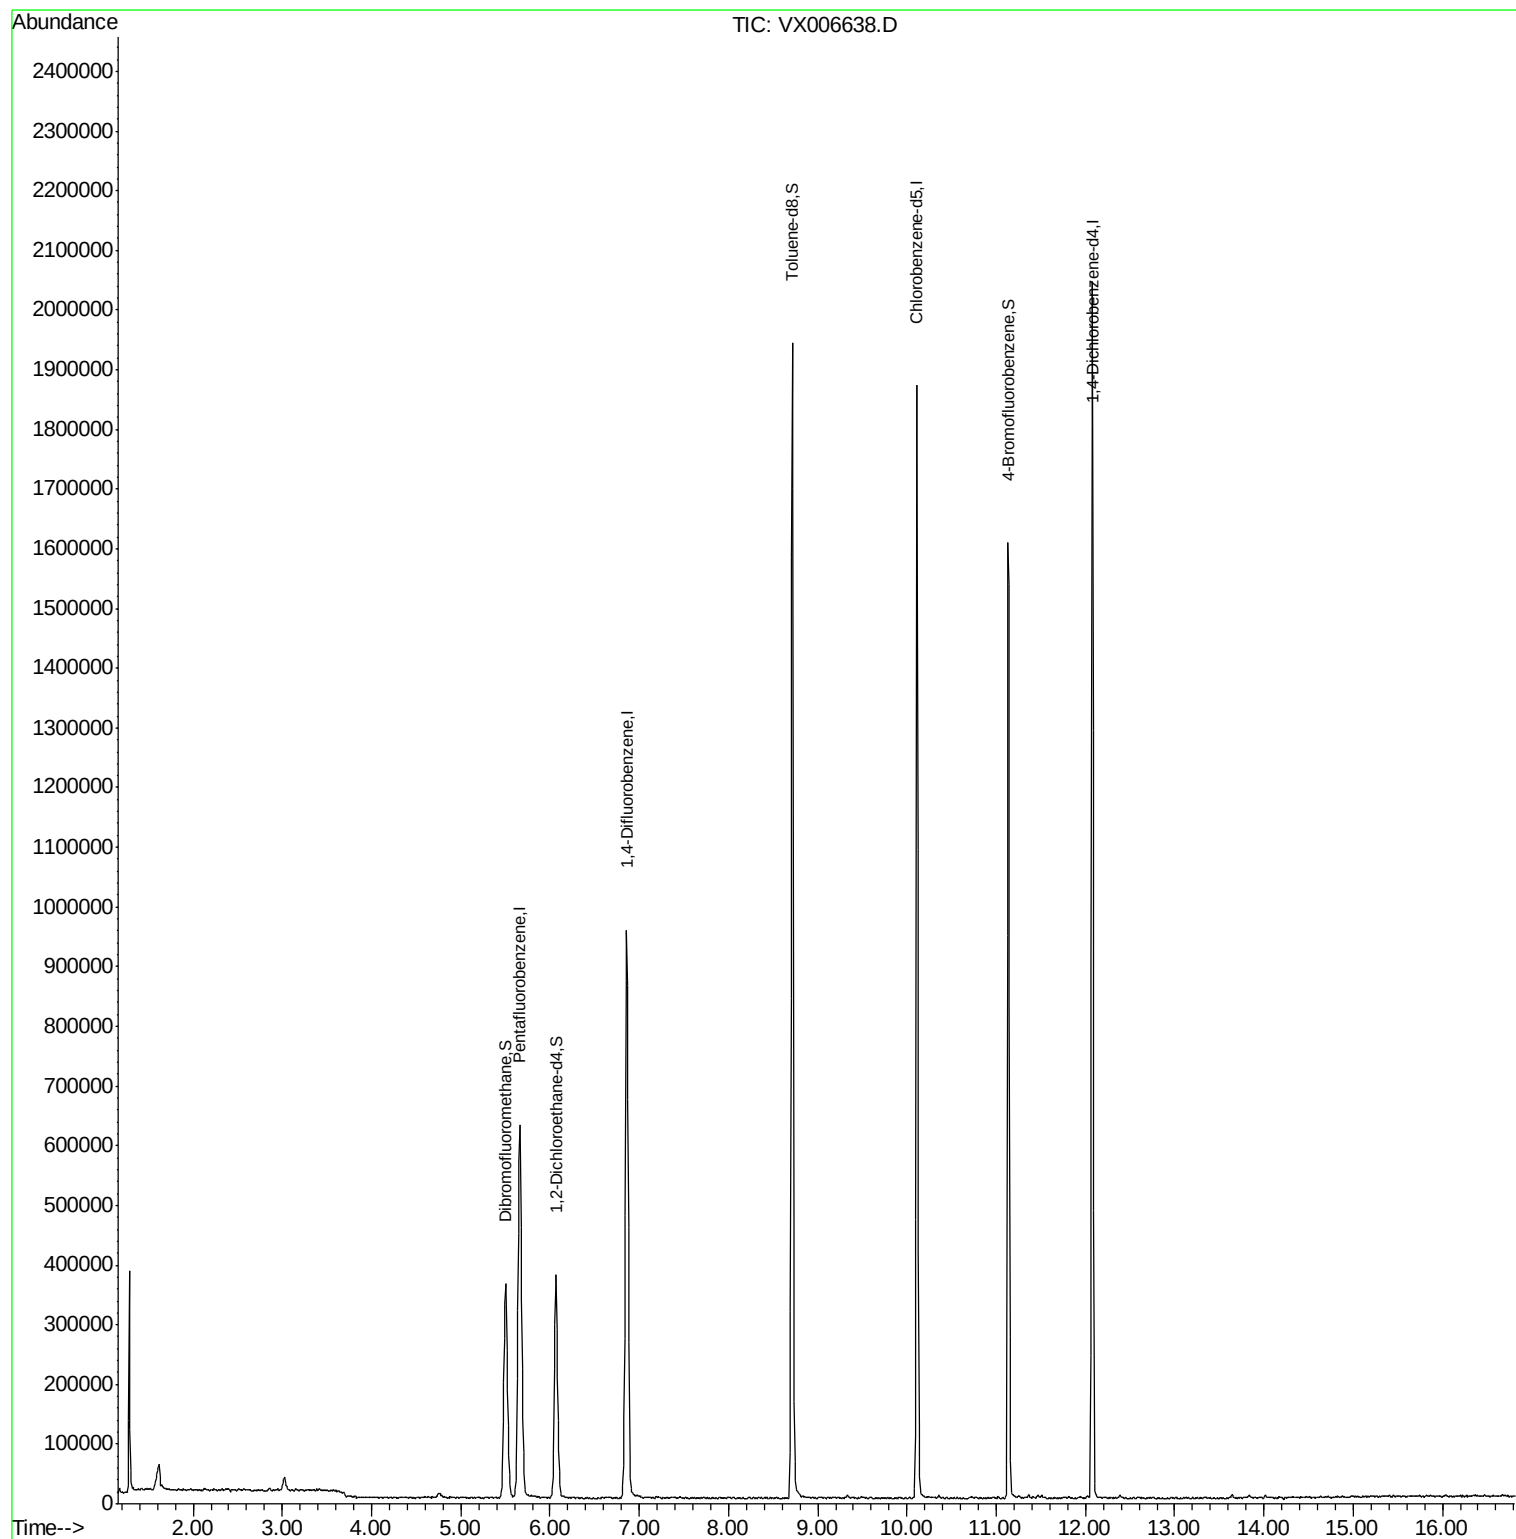

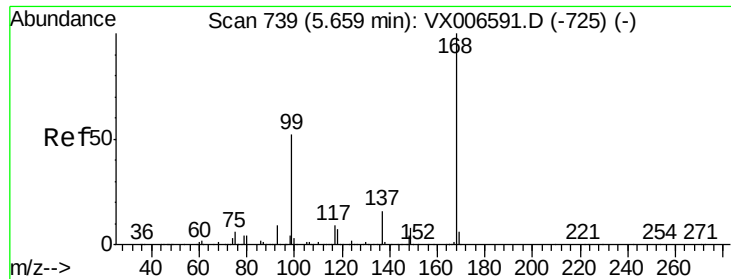

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.66 min Scan# 739

Delta R.T. -0.00 min

Lab File: VX006638.D

Acq: 19 Dec 2018 15:51

Instrument :

MSVOA_X

ClientSampleId :


TRIP-BLANK

Tot Ion:168 Resp: 645006

Ion Ratio Lower Upper

168 100

99 51.3 41.8 62.8

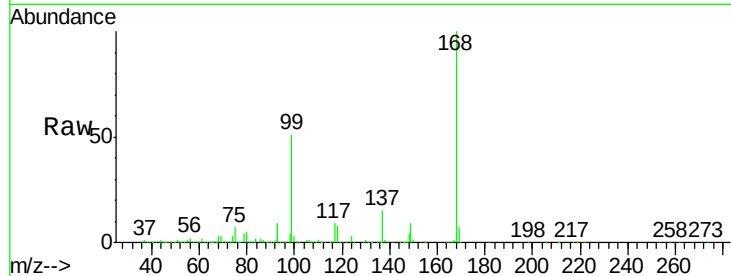

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.66

250000

200000



150000

100000

50000

0

Time-->

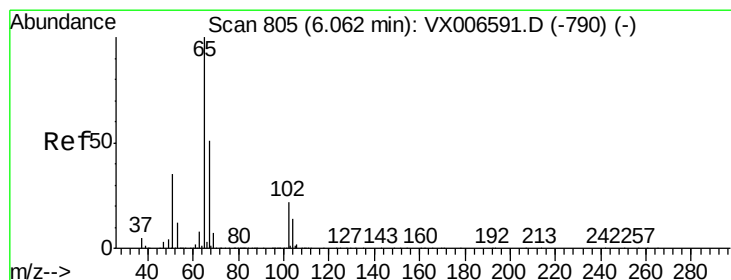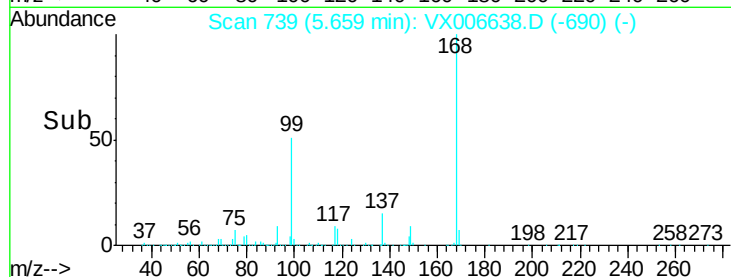

#33

1,2-Dichloroethane-d4

Concen: 50.125 ug/l

RT: 6.07 min Scan# 806

Delta R.T. 0.01 min

Lab File: VX006638.D


Acq: 19 Dec 2018 15:51

Tgt Ion: 65 Resp: 348447

Ion Ratio Lower Upper

65 100

67 53.9 0.0 105.0

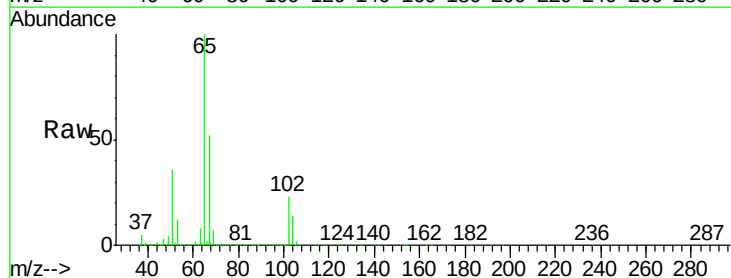

Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

6.07


150000


100000

50000

0

Time-->

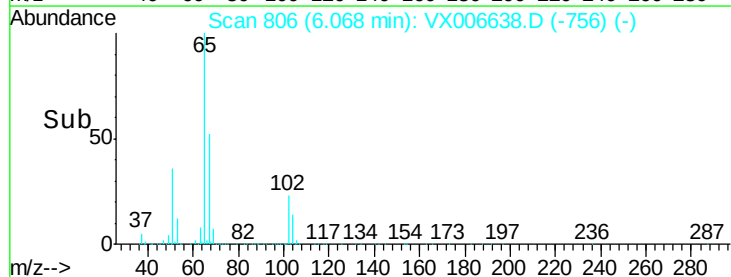

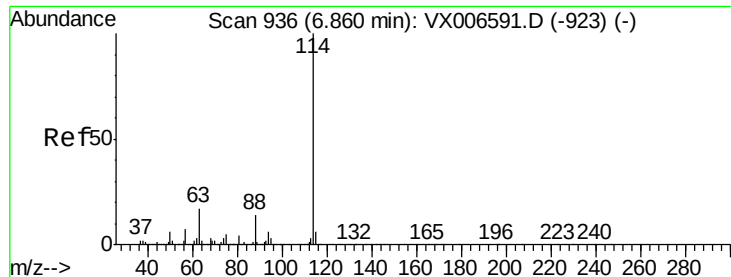

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.86 min Scan# 936

Delta R.T. -0.00 min

Lab File: VX006638.D

Acq: 19 Dec 2018 15:51

Instrument :

MSVOA_X

ClientSampleId :

TRIP-BLANK


Tot Ion:114 Resp: 1012714

Ion Ratio Lower Upper

114 100

63 18.1 0.0 34.8




88 14.9 0.0 28.8

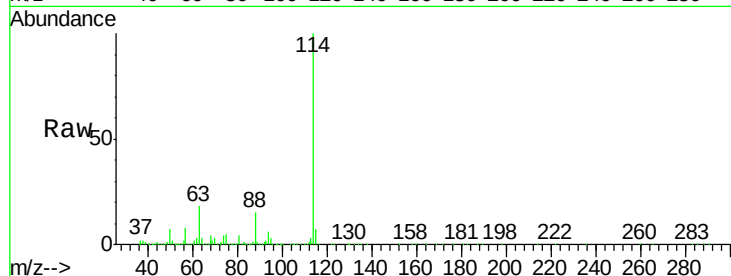

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

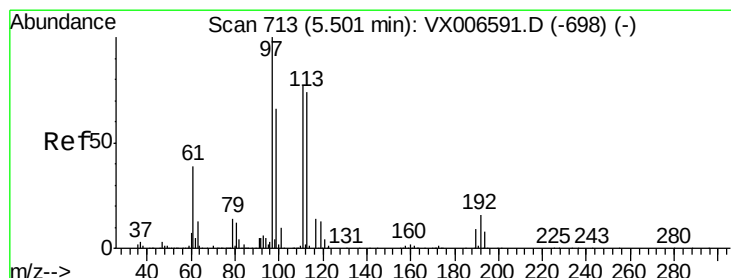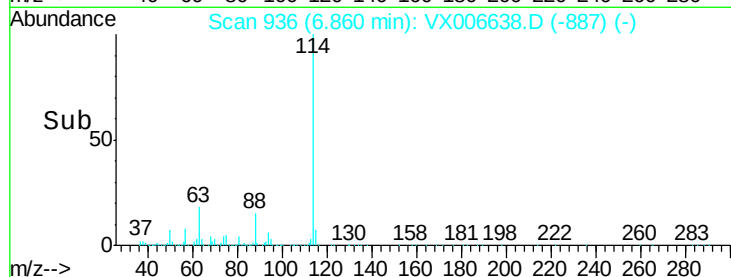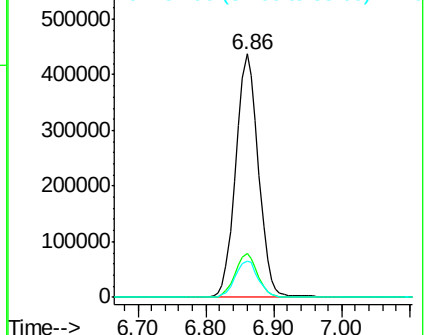

#35

Dibromofluoromethane

Concen: 48.192 ug/l

RT: 5.50 min Scan# 713

Delta R.T. -0.00 min

Lab File: VX006638.D

Acq: 19 Dec 2018 15:51


Tgt Ion:113 Resp: 308634

Ion Ratio Lower Upper

113 100

111 102.6 81.6 122.4



192 20.8 16.7 25.1

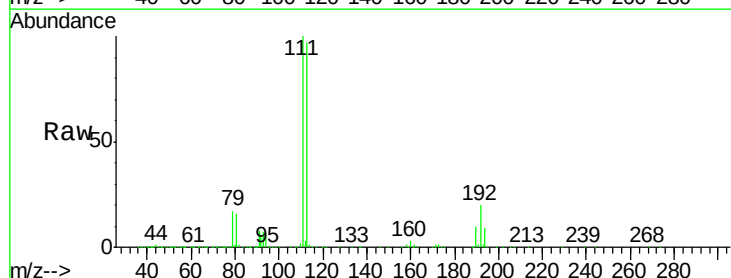


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V



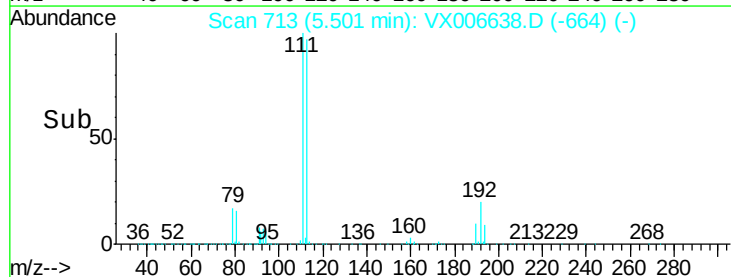
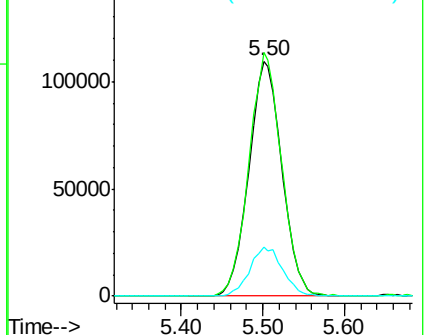


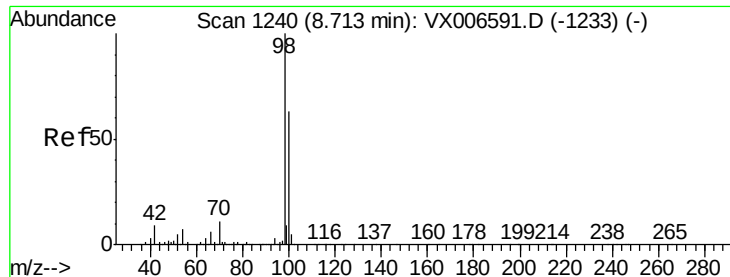

#50
Toluene-d8
Concen: 49.701 ug/l
RT: 8.71 min Scan# 1240
Delta R.T. -0.00 min
Lab File: VX006638.D
Acq: 19 Dec 2018 15:51




Instrument :
MSVOA_X
ClientSampleId :
TRIP-BLANK


Tot Ion: 98 Resp: 1199996
Ion Ratio Lower Upper
98 100
100 64.1 52.0 78.0

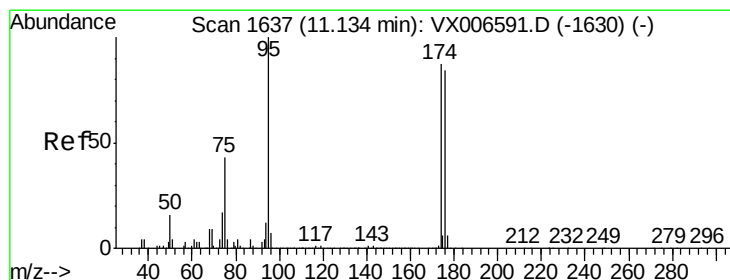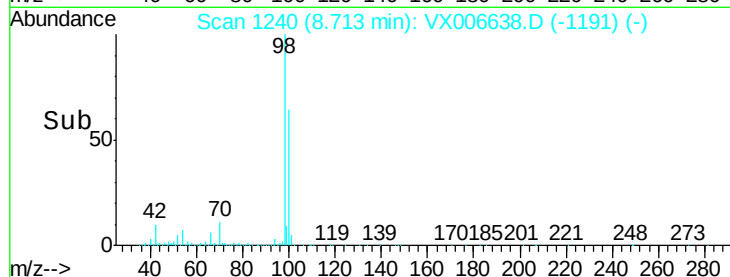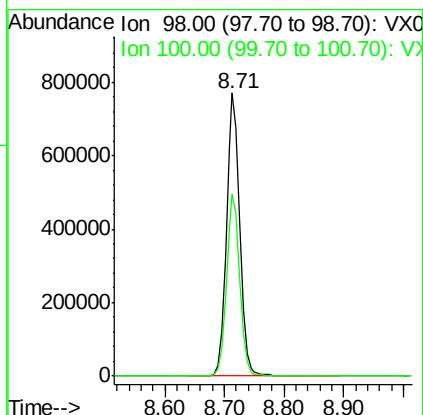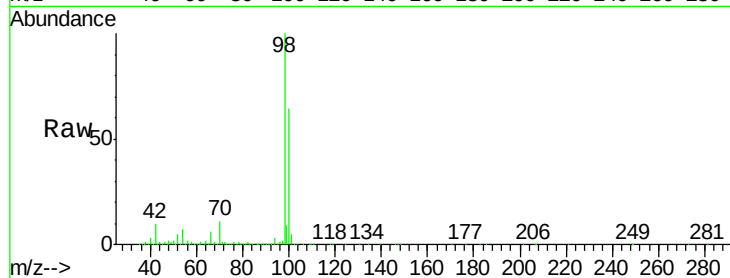

#62
4-Bromofluorobenzene
Concen: 48.819 ug/l
RT: 11.13 min Scan# 1637
Delta R.T. -0.00 min
Lab File: VX006638.D
Acq: 19 Dec 2018 15:51

Tgt Ion: 95 Resp: 431690
Ion Ratio Lower Upper
95 100
174 86.2 0.0 182.2
176 83.4 0.0 178.8


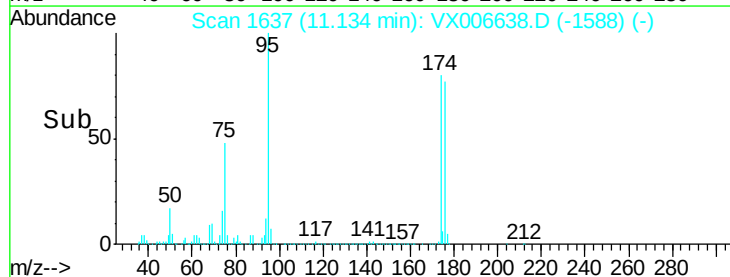
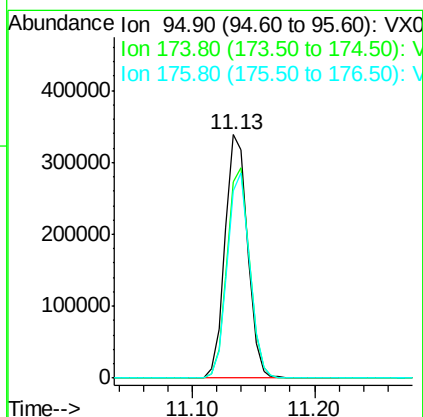
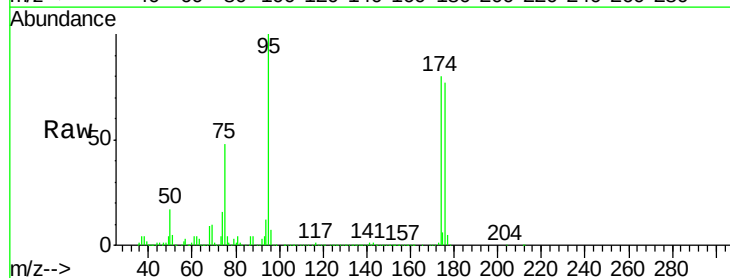


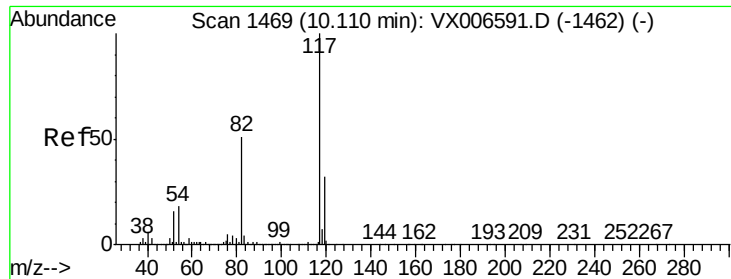

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.11 min Scan# 1469
Delta R.T. -0.00 min
Lab File: VX006638.D
Acq: 19 Dec 2018 15:51

Instrument :
MSVOA_X
ClientSampleId :
TRIP-BLANK

Tot Ion:117 Resp: 923136
Ion Ratio Lower Upper
117 100
82 52.4 41.0 61.6
119 32.1 25.4 38.0

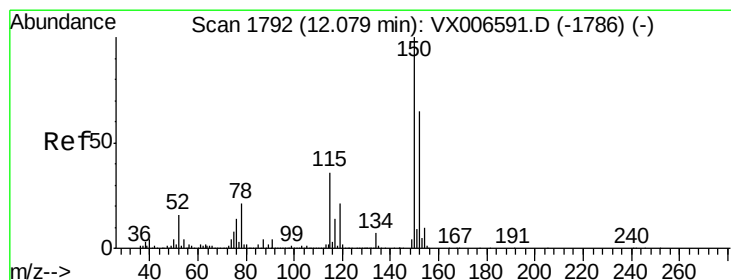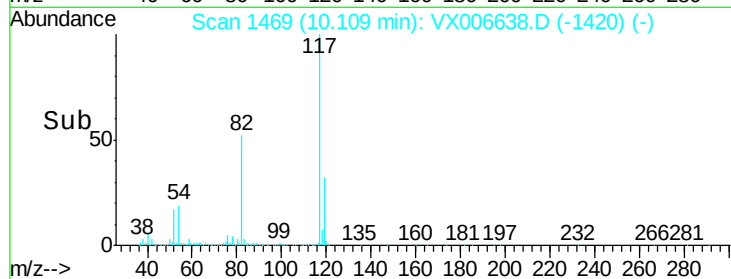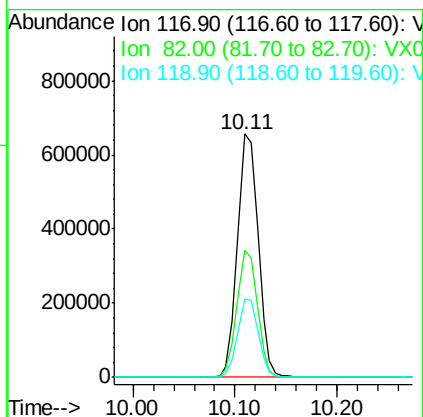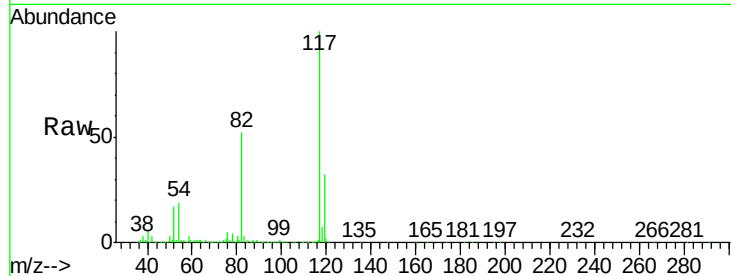

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.08 min Scan# 1792
Delta R.T. -0.00 min
Lab File: VX006638.D
Acq: 19 Dec 2018 15:51

Tgt Ion:152 Resp: 435250
Ion Ratio Lower Upper
152 100
115 56.8 39.1 117.2
150 158.0 0.0 344.8

