

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX121918\
 Data File : VX006640.D
 Acq On : 19 Dec 2018 16:44
 Operator : JC/MD
 Sample : J6488-01
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TB-01-181218

Quant Time: Dec 20 04:22:25 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X121818W.M
 Quant Title : SW846 8260
 QLast Update : Wed Dec 19 15:20:58 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.66	168	628122	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.86	114	1007989	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.12	117	918543	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.08	152	436658	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.07	65	347060	51.27	ug/l	0.00
Spiked Amount 50.000			Recovery	=	102.54%	
35) Dibromofluoromethane	5.51	113	300863	47.20	ug/l	0.00
Spiked Amount 50.000			Recovery	=	94.40%	
50) Toluene-d8	8.71	98	1189421	49.49	ug/l	0.00
Spiked Amount 50.000			Recovery	=	98.98%	
62) 4-Bromofluorobenzene	11.13	95	430297	48.89	ug/l	0.00
Spiked Amount 50.000			Recovery	=	97.78%	
Target Compounds						
16) Acetone	2.45	43	22707	7.301	ug/l	Qvalue 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX121918\
Data File : VX006640.D
Acq On : 19 Dec 2018 16:44
Operator : JC/MD
Sample : J6488-01
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TB-01-181218

Quant Time: Dec 20 04:22:25 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X121818W.M
Quant Title : SW846 8260
QLast Update : Wed Dec 19 15:20:58 2018
Response via : Initial Calibration

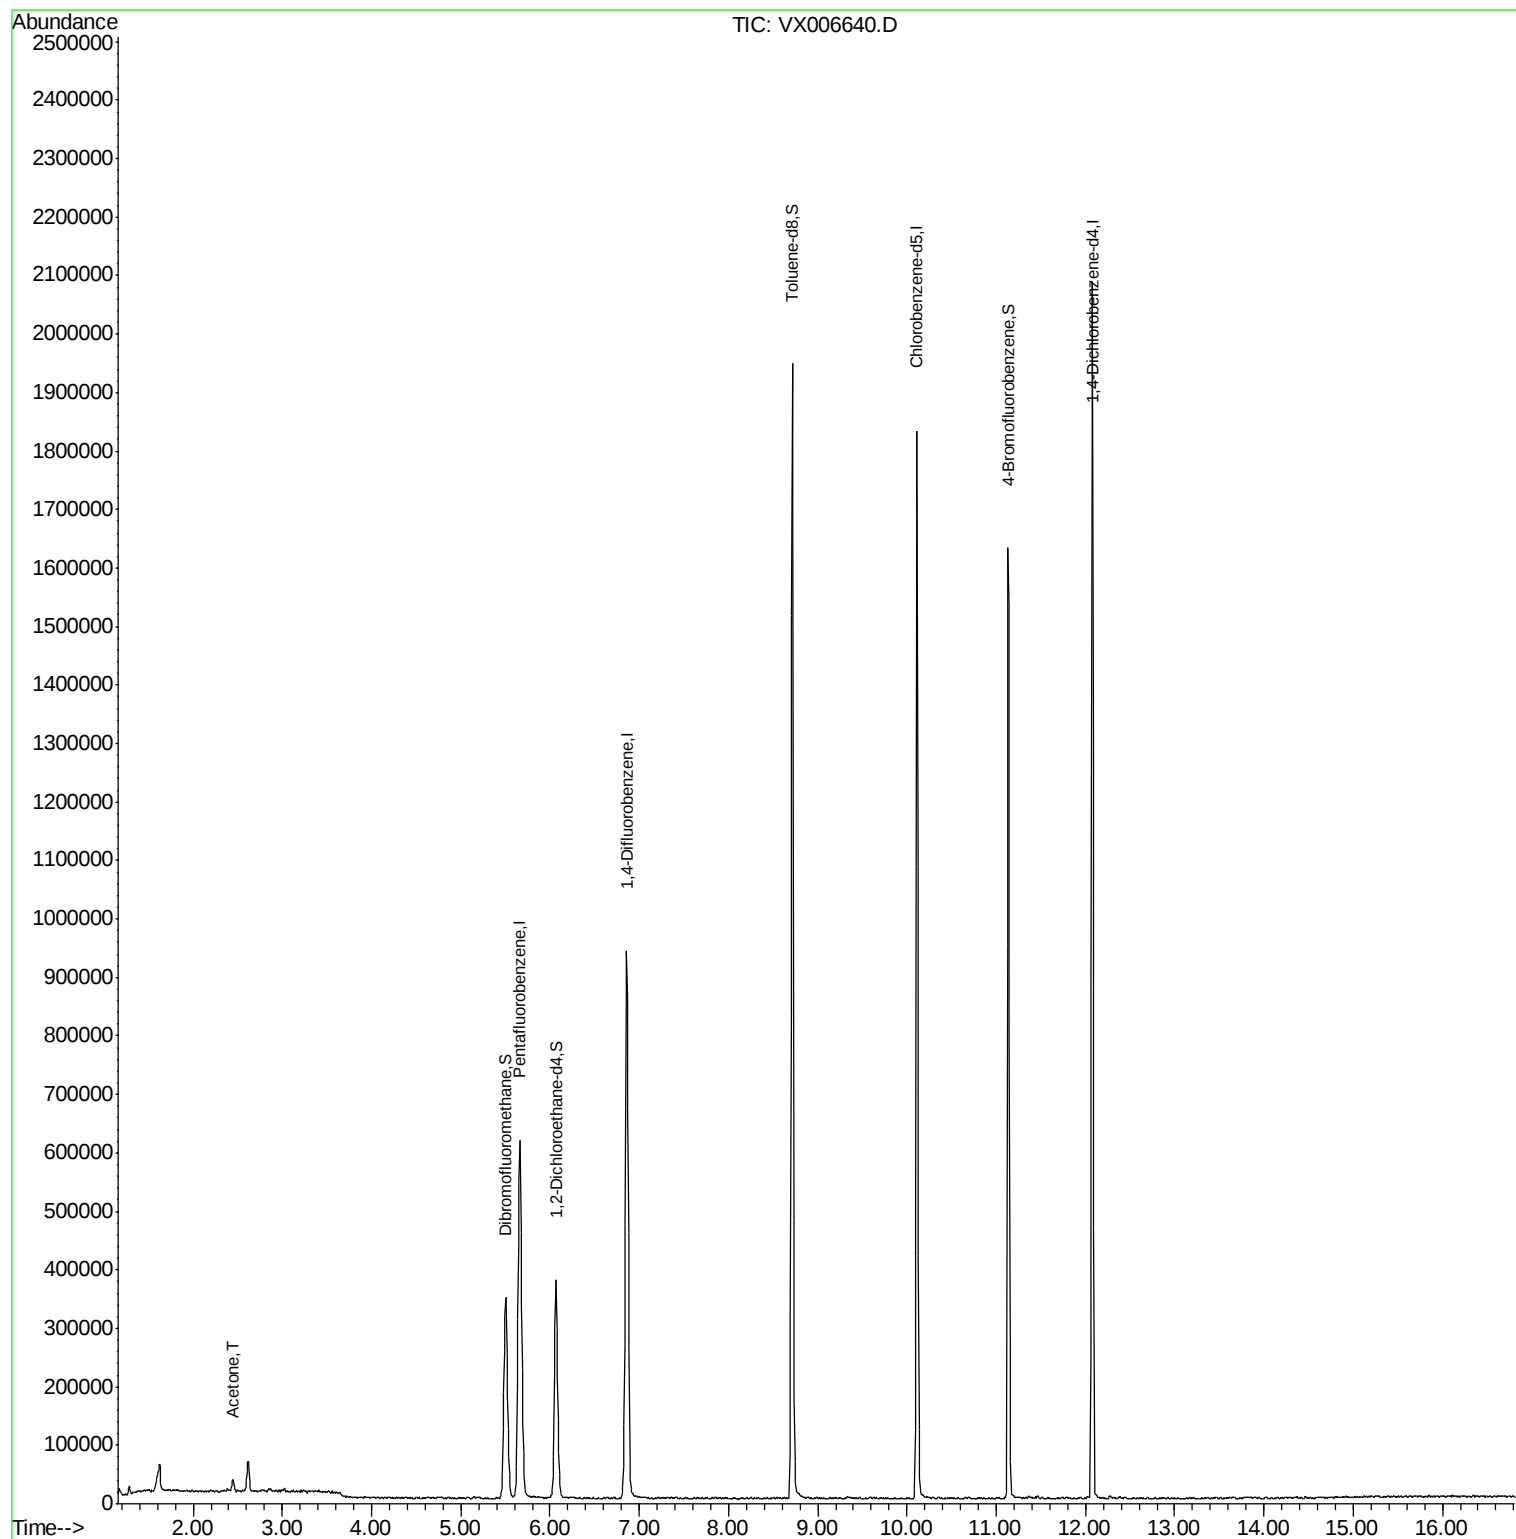

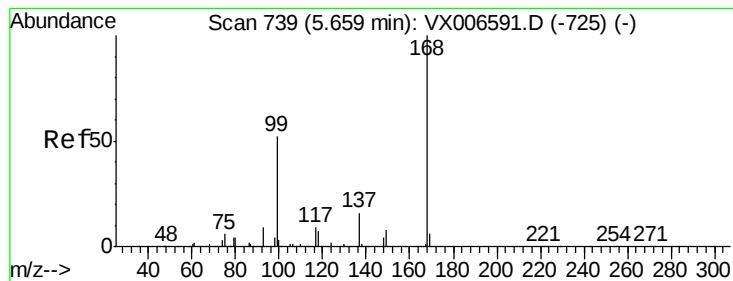

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.66 min Scan# 739

Delta R.T. 0.00 min

Lab File: VX006640.D

Acq: 19 Dec 2018 16:44

Instrument :

MSVOA_X

ClientSampleId :


TB-01-181218

Tot Ion:168 Resp: 628122

Ion Ratio Lower Upper

168 100

99 53.4 41.8 62.8

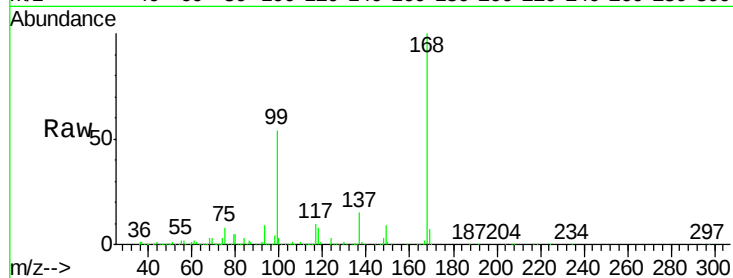

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.66

250000

200000



150000

100000

50000

0

Time-->

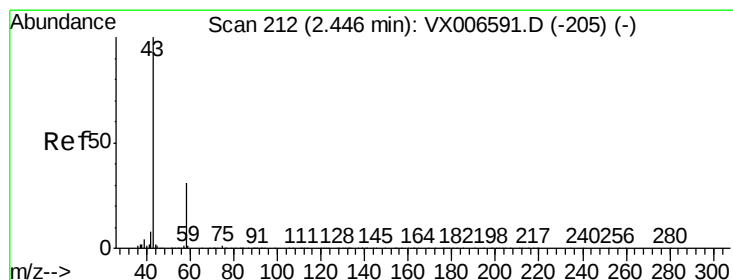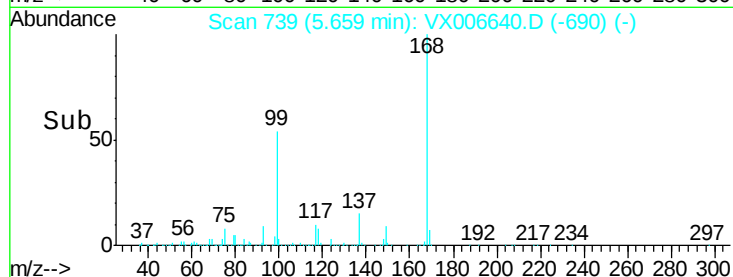

#16

Acetone

Concen: 7.301 ug/l

RT: 2.45 min Scan# 212

Delta R.T. 0.00 min

Lab File: VX006640.D


Acq: 19 Dec 2018 16:44

Tgt Ion: 43 Resp: 22707

Ion Ratio Lower Upper

43 100

58 31.3 25.0 37.6

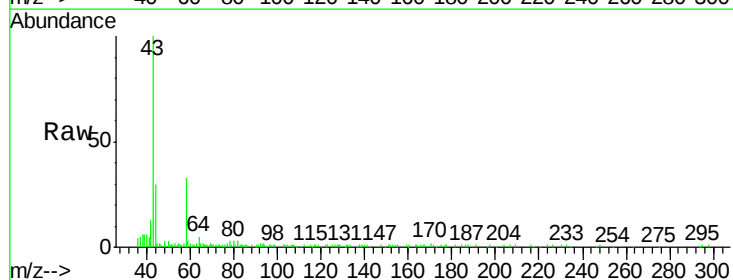

Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0


2.45


10000

5000

0

Time-->

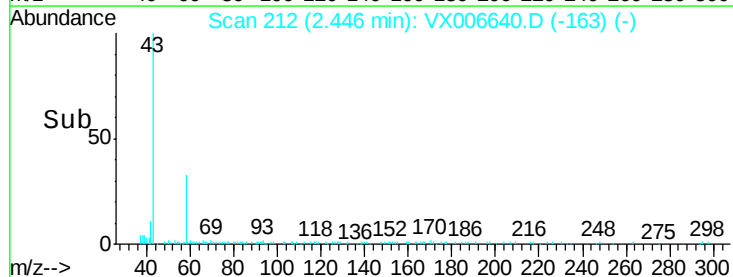

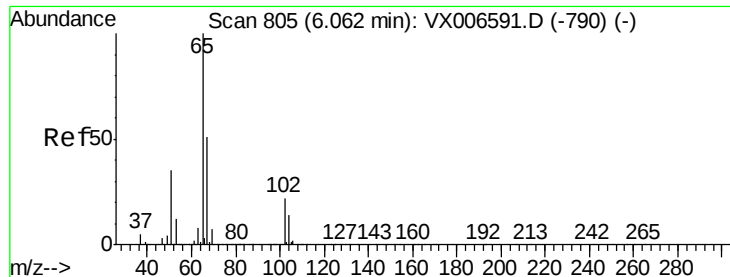

#33

1,2-Dichloroethane-d4

Concen: 51.267 ug/l

RT: 6.07 min Scan# 806

Delta R.T. 0.01 min

Lab File: VX006640.D

Acq: 19 Dec 2018 16:44

Instrument :

MSVOA_X

ClientSampleId :


TB-01-181218

Tot Ion: 65 Resp: 347060

Ion Ratio Lower Upper

65 100

67 53.2 0.0 105.0

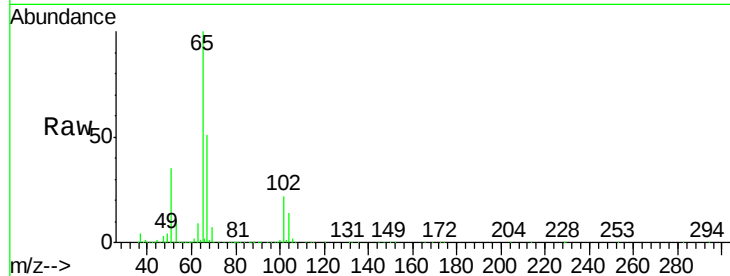

Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

6.07



150000

100000

50000

0

Time--> 5.90 6.00 6.10 6.20

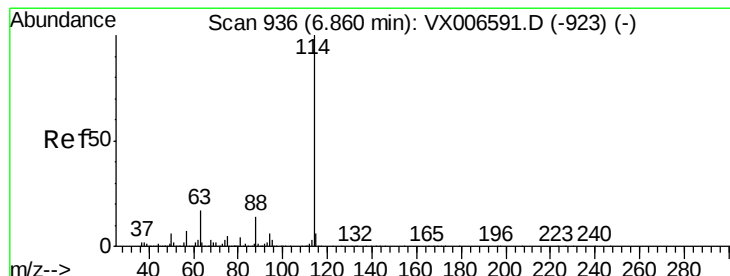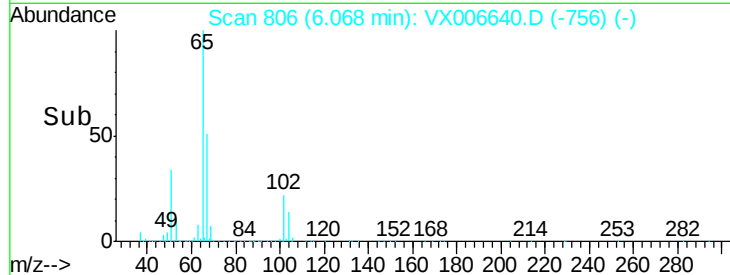

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.86 min Scan# 936

Delta R.T. 0.00 min

Lab File: VX006640.D

Acq: 19 Dec 2018 16:44


Tgt Ion: 114 Resp: 1007989

Ion Ratio Lower Upper

114 100

63 17.8 0.0 34.8

88 15.0 0.0 28.8

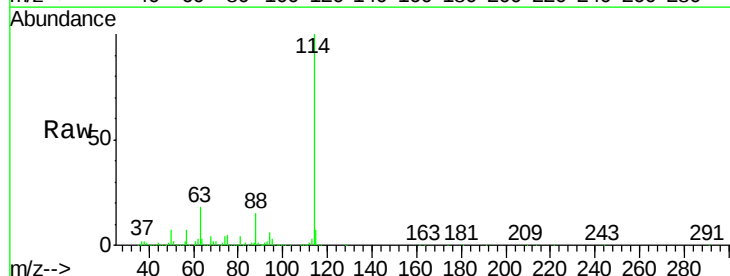

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

6.86

600000

500000

400000


300000


200000

100000

0

Time--> 6.70 6.80 6.90 7.00 7.10

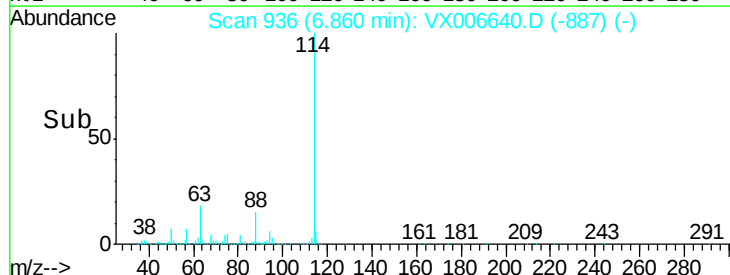

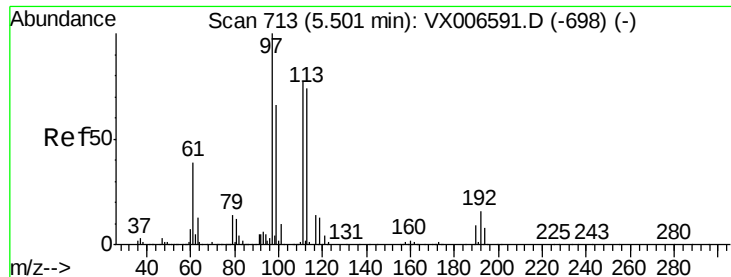

#35

Dibromofluoromethane

Concen: 47.199 ug/l

RT: 5.51 min Scan# 714

Delta R.T. 0.01 min

Lab File: VX006640.D

Acq: 19 Dec 2018 16:44

Instrument :

MSVOA_X

ClientSampleId :

TB-01-181218


Tot Ion:113 Resp: 300863

Ion Ratio Lower Upper

113 100

111 100.8 81.6 122.4




192 20.2 16.7 25.1

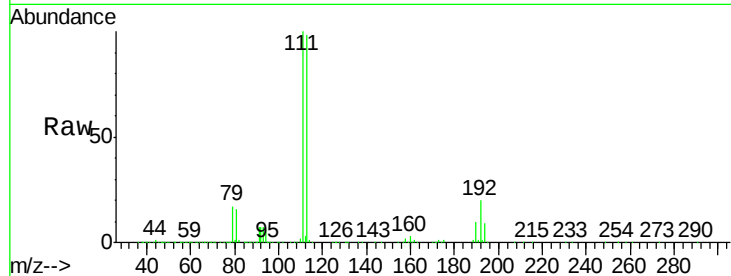

Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

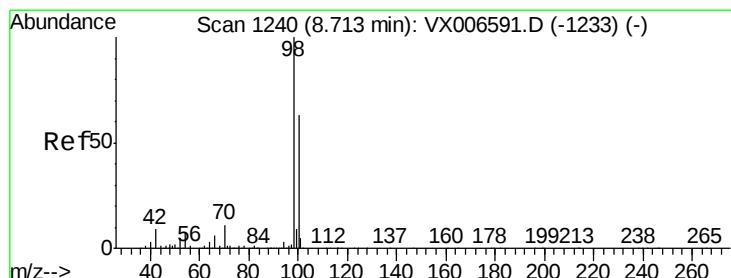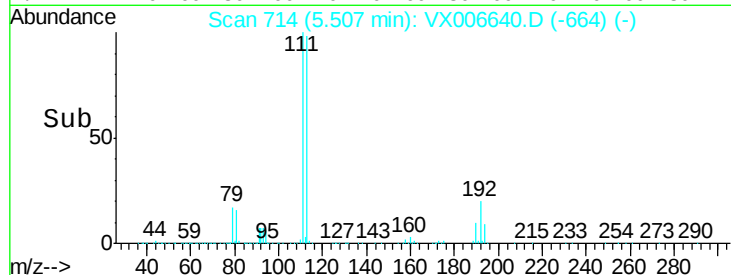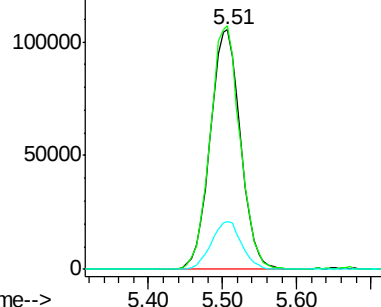

#50

Toluene-d8

Concen: 49.494 ug/l

RT: 8.71 min Scan# 1240

Delta R.T. 0.00 min

Lab File: VX006640.D


Acq: 19 Dec 2018 16:44

Tgt Ion: 98 Resp: 1189421

Ion Ratio Lower Upper



98 100


100 64.2 52.0 78.0

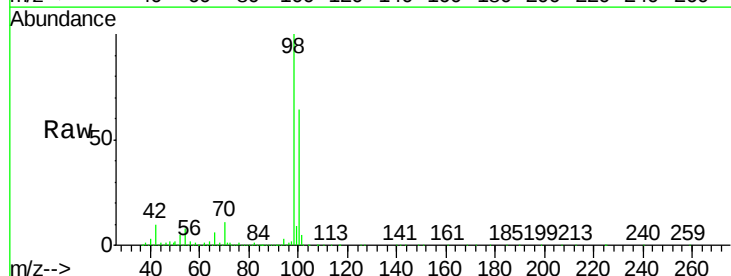

Abundance Ion 98.00 (97.70 to 98.70): VX0

Ion 100.00 (99.70 to 100.70): VX0

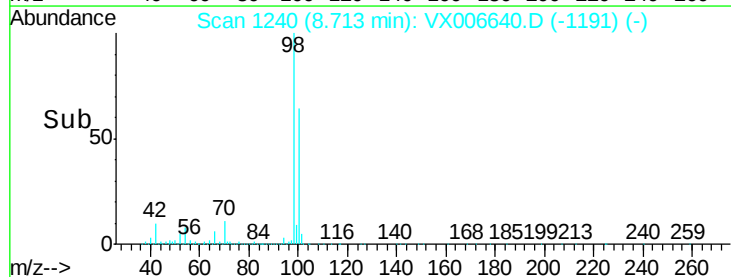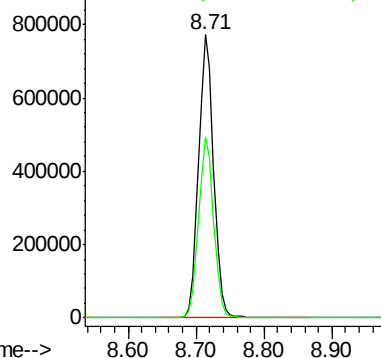

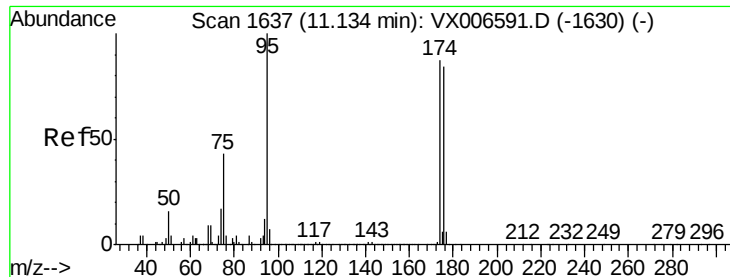

#62

4-Bromofluorobenzene

Concen: 48.890 ug/l

RT: 11.13 min Scan# 1637

Delta R.T. 0.00 min

Lab File: VX006640.D

Acq: 19 Dec 2018 16:44

Instrument :

MSVOA_X

ClientSampleId :

TB-01-181218


Tot Ion: 95 Resp: 430297

Ion Ratio Lower Upper

95 100

174 85.8 0.0 182.2




176 82.8 0.0 178.8

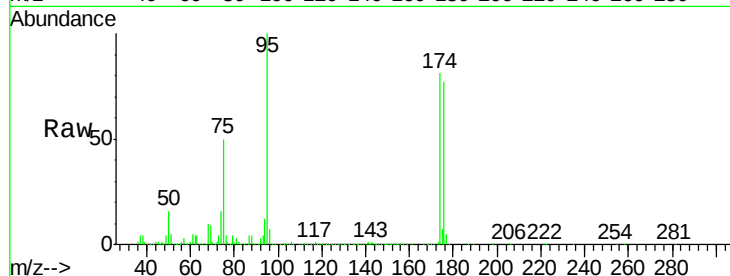

Abundance Ion 94.90 (94.60 to 95.60): VX0

Ion 173.80 (173.50 to 174.50): V

Ion 175.80 (175.50 to 176.50): V

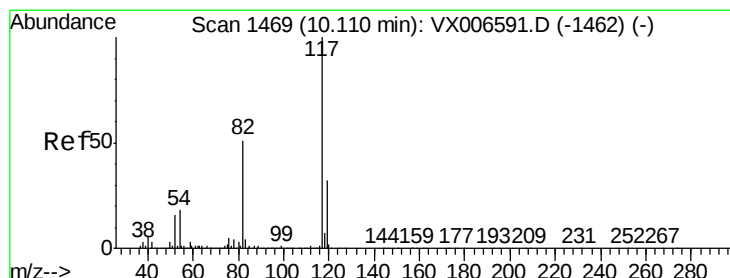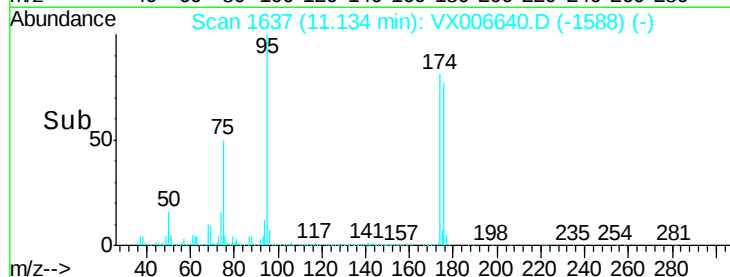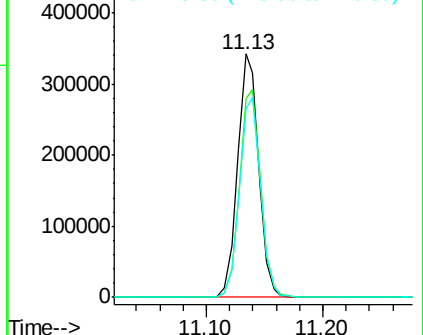

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.12 min Scan# 1470

Delta R.T. 0.01 min

Lab File: VX006640.D

Acq: 19 Dec 2018 16:44


Tgt Ion: 117 Resp: 918543

Ion Ratio Lower Upper

117 100

82 50.5 41.0 61.6



119 32.2 25.4 38.0

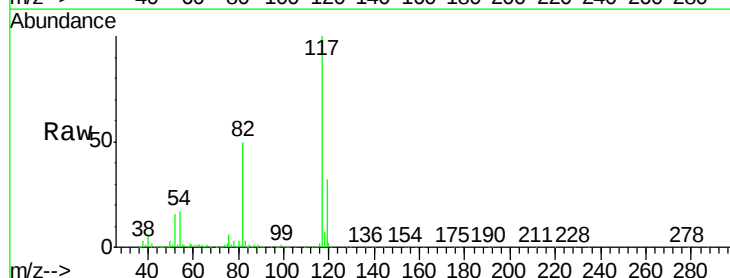


Abundance Ion 116.90 (116.60 to 117.60): V

Ion 82.00 (81.70 to 82.70): VX0

Ion 118.90 (118.60 to 119.60): V

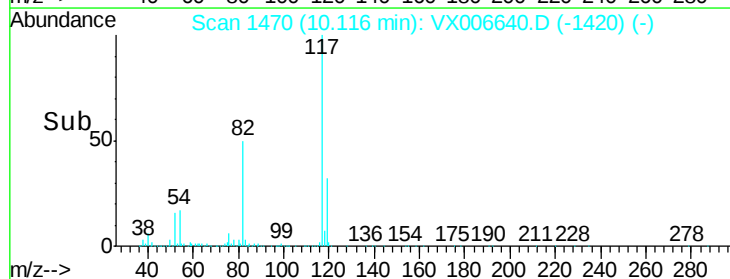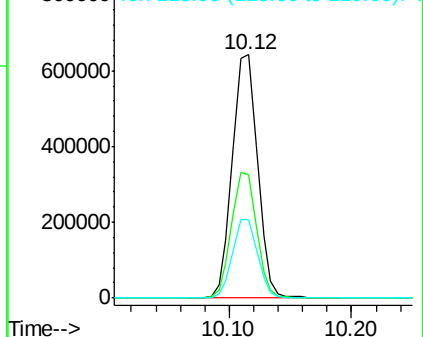

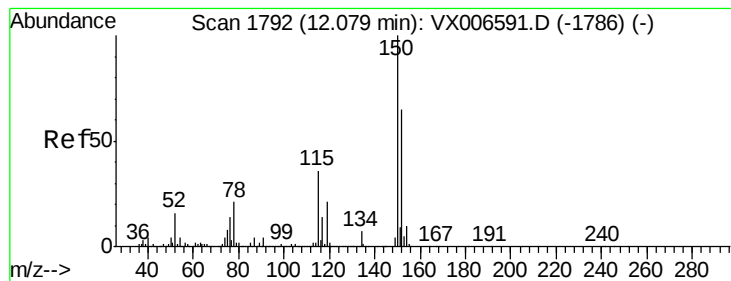

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.08 min Scan# 1792

Delta R.T. 0.00 min

Lab File: VX006640.D

Acq: 19 Dec 2018 16:44

Instrument :

MSVOA_X

ClientSampleId :

TB-01-181218


Tot Ion:152 Resp: 436658

Ion Ratio Lower Upper

152 100

115 56.6 39.1 117.2

150 156.7 0.0 344.8

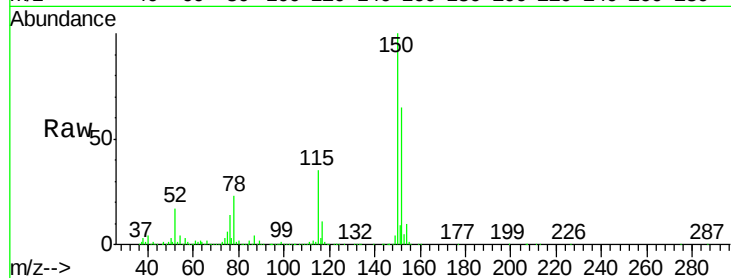

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

