


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX121918\  
Data File : VX006634.D  
Acq On : 19 Dec 2018 13:50  
Operator : JC/MD  
Sample : BFB  
Misc : 5.0mL/MSVOA X/WATER  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82X121818W.M  
Title : SW846 8260  
Last Update : Wed Dec 19 15:20:58 2018

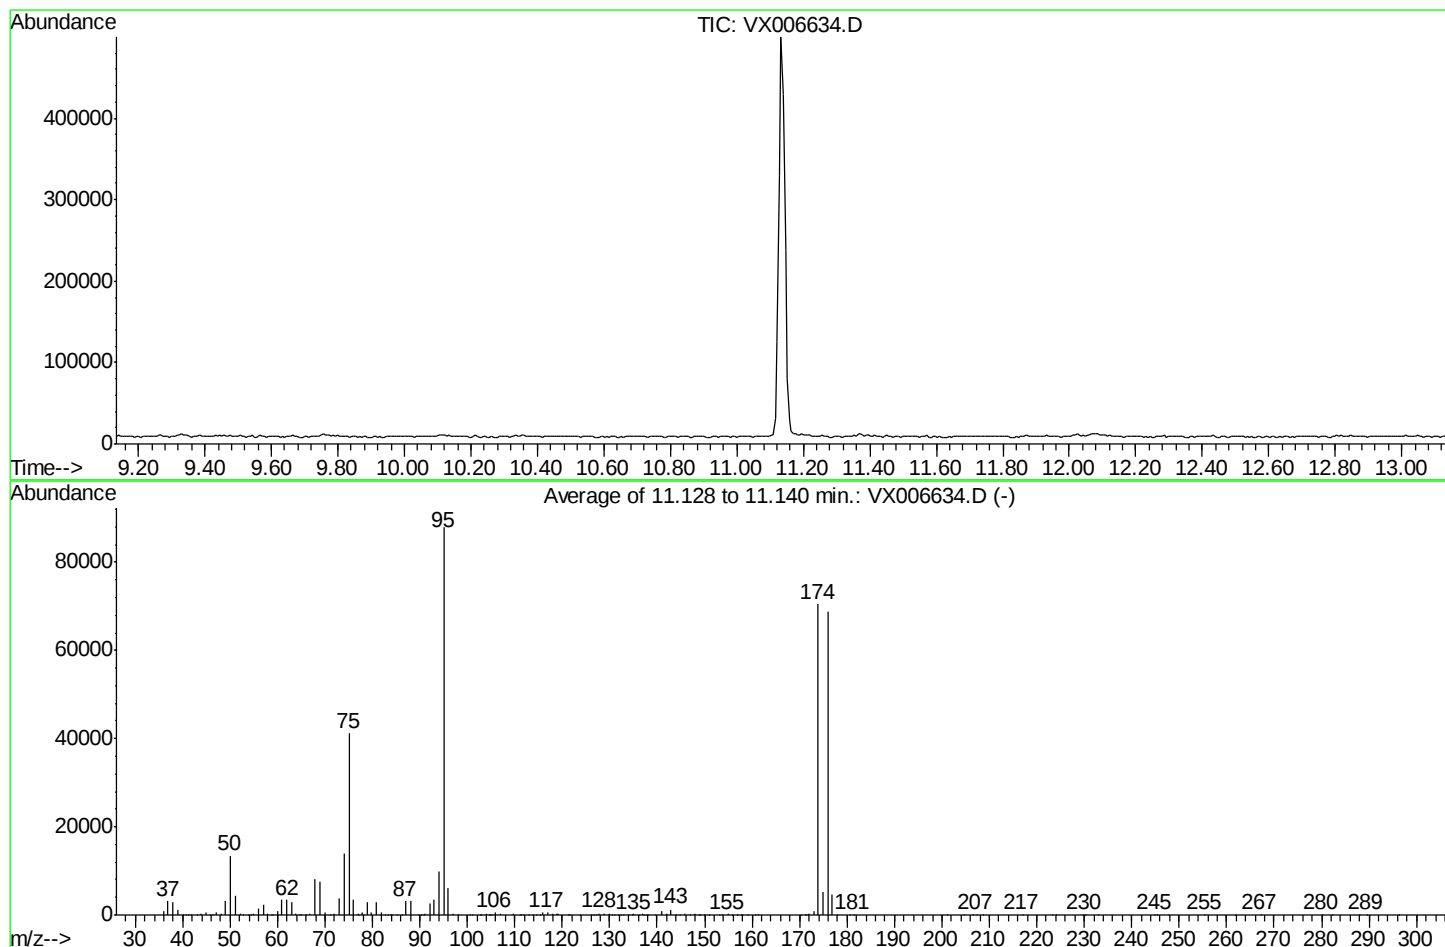

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1629

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 15           | 40           | 15.3      | 13423   | PASS             |
| 75          | 95           | 30           | 60           | 46.9      | 41185   | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 87893   | PASS             |
| 96          | 95           | 5            | 9            | 6.9       | 6081    | PASS             |
| 173         | 174          | 0.00         | 2            | 1.4       | 1005    | PASS             |
| 174         | 95           | 50           | 100          | 80.2      | 70493   | PASS             |
| 175         | 174          | 5            | 9            | 7.3       | 5163    | PASS             |
| 176         | 174          | 95           | 101          | 97.6      | 68834   | PASS             |
| 177         | 176          | 5            | 9            | 6.6       | 4565    | PASS             |