

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX121919\
 Data File : VX014151.D
 Acq On : 20 Dec 2019 04:29
 Operator : JC/SP
 Sample : K6372-10
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-4

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X121319W.M

Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.070	26	30	43	rBV	2267848	2633155	100.00%	15.995%
2	1.271	59	63	69	rBV	46681	61139	2.32%	0.371%
3	1.594	108	116	119	rVB9	29297	52970	2.01%	0.322%
4	2.588	274	279	289	rBV	80619	149775	5.69%	0.910%
5	5.490	746	755	767	rBV	292051	820390	31.16%	4.983%
6	5.655	769	782	795	rVV	536502	1474059	55.98%	8.954%
7	6.051	839	847	865	rVB	325964	872715	33.14%	5.301%
8	6.850	968	978	990	rBV	830209	1906090	72.39%	11.578%
9	8.709	1274	1283	1291	rBV	1707137	2619973	99.50%	15.915%
10	9.331	1379	1385	1391	rBV4	18838	32362	1.23%	0.197%
11	10.105	1507	1512	1521	rBV	1595711	2203934	83.70%	13.387%
12	11.129	1675	1680	1691	rBV	1262552	1672329	63.51%	10.158%
13	12.074	1830	1835	1841	rBV	1615703	1963746	74.58%	11.929%


Sum of corrected areas: 16462637

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX121919\
Data File : VX014151.D
Acq On : 20 Dec 2019 04:29
Operator : JC/SP
Sample : K6372-10
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-4

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X121319W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

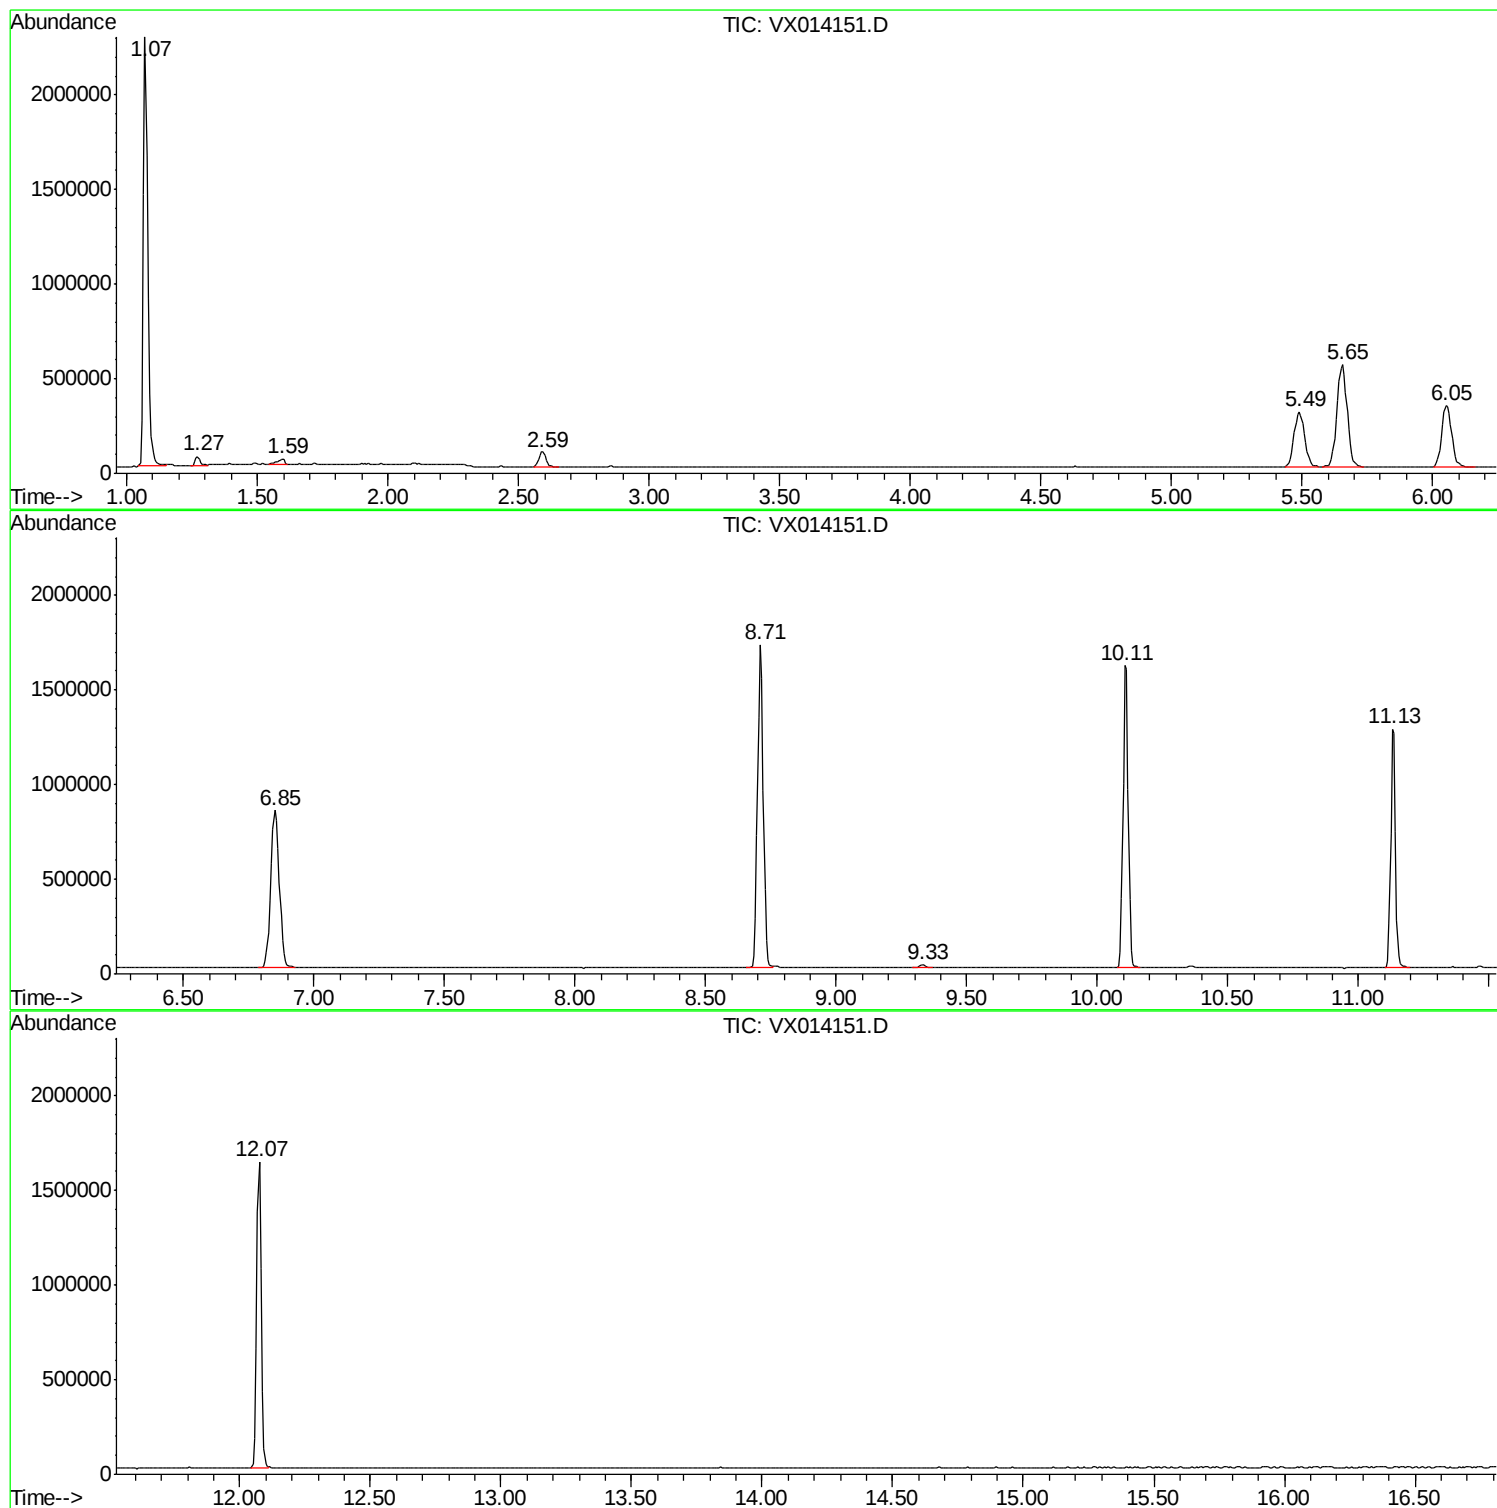

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX121919\
Data File : VX014151.D
Acq On : 20 Dec 2019 04:29
Operator : JC/SP
Sample : K6372-10
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-4










Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X121319W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Isopropyl Alcohol Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.59	5.08 ug/l	149775	Pentafluorobenzene	5.65

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Isopropyl Alcohol	60	C3H8O	000067-63-0	80
2		Propane, 2-ethoxy-	88	C5H12O	000625-54-7	56
3		2-Hexanol, 3-methyl-	116	C7H16O	002313-65-7	9
4		(R)-(-)-2-Pentanol	88	C5H12O	031087-44-2	9
5		2-Pentanol	88	C5H12O	006032-29-7	9

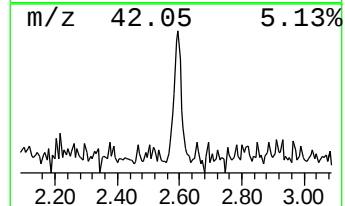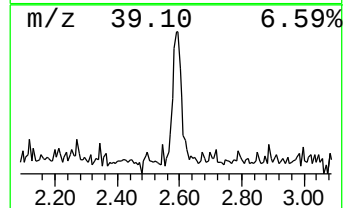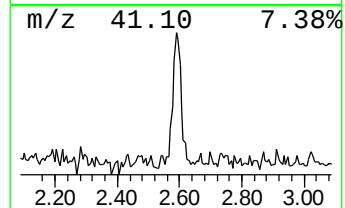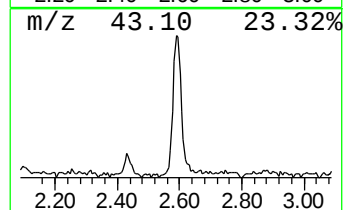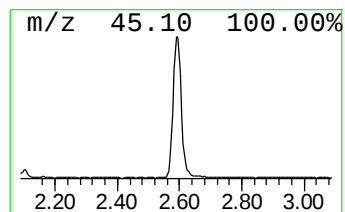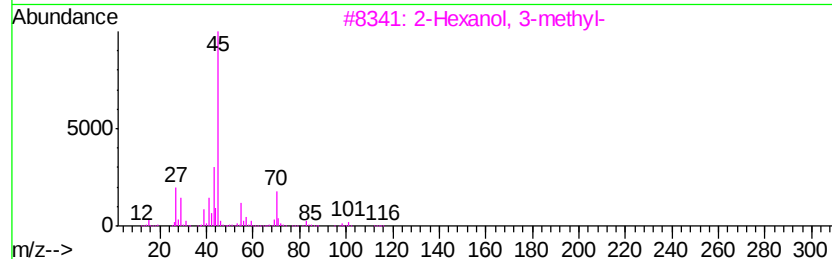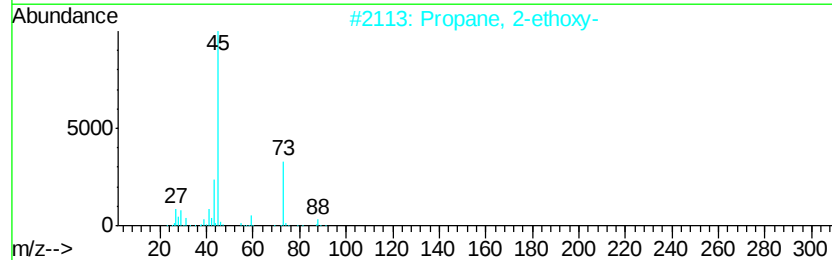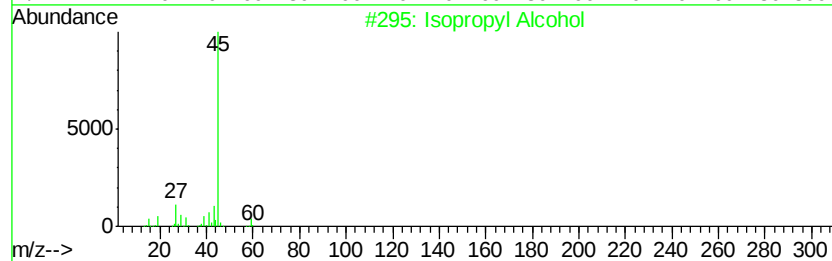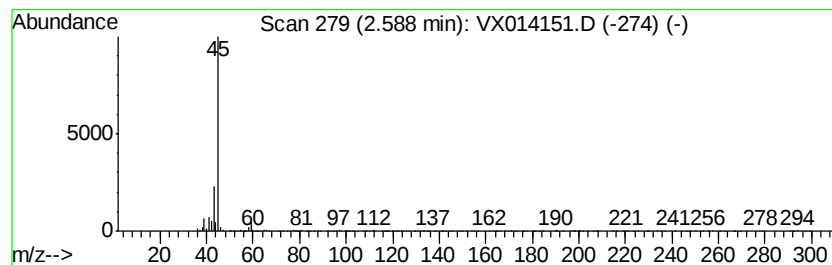

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX121919\
Data File : VX014151.D
Acq On : 20 Dec 2019 04:29
Operator : JC/SP
Sample : K6372-10
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-4

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X121319W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Isopropyl Alcohol	2.59	5.1	ug/l	149775	1	5.65	1474060	50.0