


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX121919\
 Data File : VX014110.D
 Acq On : 19 Dec 2019 10:02
 Operator : JC/SP
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\624X121219W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Fri Dec 13 01:35:34 2019

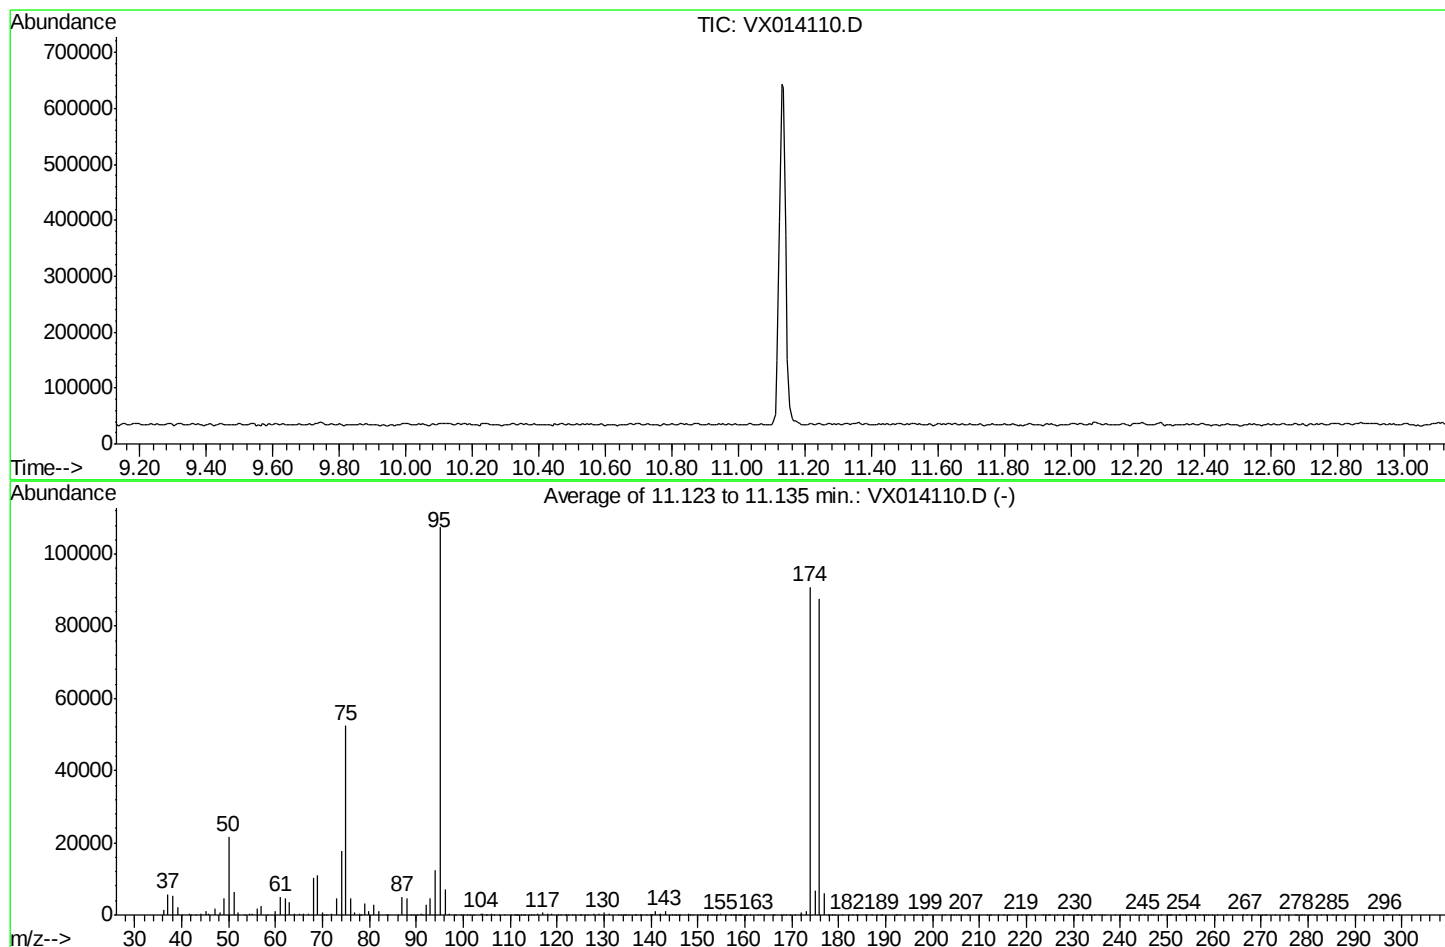

AutoFind: Scans 1679, 1680, 1681; Background Corrected with Scan 1673

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.2	21650	PASS
75	95	30	60	48.8	52477	PASS
95	95	100	100	100.0	107425	PASS
96	95	5	9	6.8	7278	PASS
173	174	0.00	2	1.2	1117	PASS
174	95	50	100	84.7	90984	PASS
175	174	5	9	7.3	6673	PASS
176	174	95	101	96.5	87775	PASS
177	176	5	9	6.9	6025	PASS