


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121919\
Data File : VX014138.D
Acq On : 19 Dec 2019 22:26
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X121319W.M
Title : SW846 8260
Last Update : Tue Dec 17 03:01:07 2019

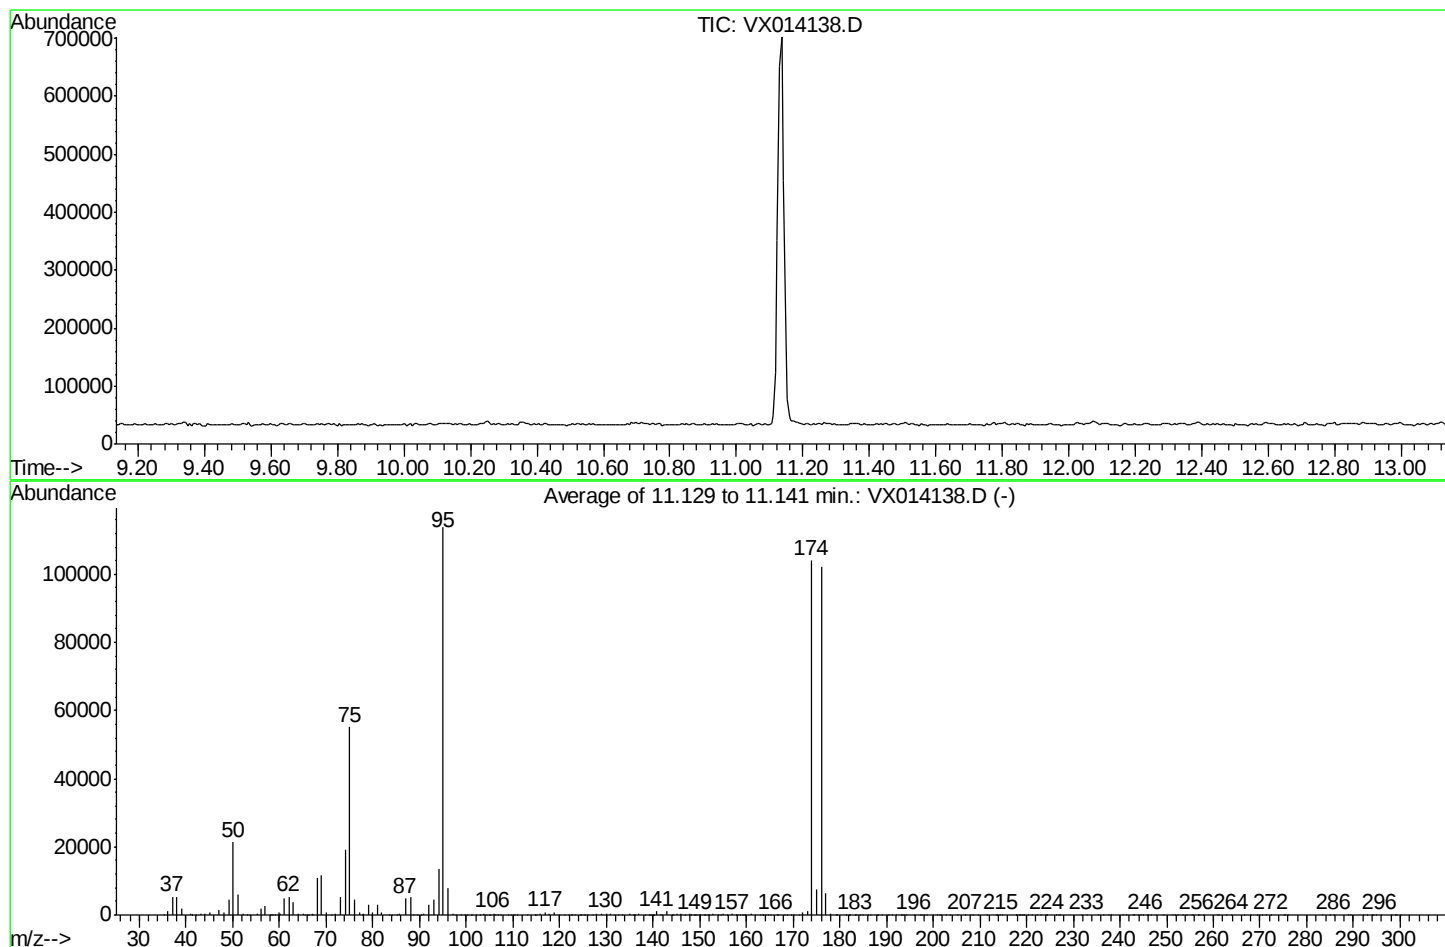

AutoFind: Scans 1680, 1681, 1682; Background Corrected with Scan 1670

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.7	21246	PASS
75	95	30	60	48.5	55212	PASS
95	95	100	100	100.0	113771	PASS
96	95	5	9	6.8	7749	PASS
173	174	0.00	2	1.0	1038	PASS
174	95	50	100	91.4	104018	PASS
175	174	5	9	7.2	7514	PASS
176	174	95	101	98.1	102066	PASS
177	176	5	9	6.3	6473	PASS