

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121920\
 Data File : VX020173.D
 Acq On : 19 Dec 2020 16:01
 Operator : JC/MD
 Sample : L5053-21DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 RE120D2-20201210DL

Integration Parameters: RTEINT.P
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X121820W.M
 Title : Sw846 8260

Signal : TIC: VX020173.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.368	204	210	218	rVB2	18626	35862	2.26%	0.387%
2	2.995	304	313	323	rVB	9071	21266	1.34%	0.230%
3	5.465	706	718	733	rBV	179378	511273	32.19%	5.521%
4	5.629	733	745	761	rVV	318645	875748	55.14%	9.457%
5	6.025	800	810	823	rBV	203533	536730	33.79%	5.796%
6	6.830	931	942	955	rBV	488374	1156832	72.83%	12.492%
7	7.184	990	1000	1019	rBV	449244	959527	60.41%	10.362%
8	8.696	1240	1248	1262	rBV	1029774	1588334	100.00%	17.152%
9	10.092	1471	1477	1496	rBV	1002946	1369937	86.25%	14.793%
10	11.122	1640	1646	1663	rBV	766985	995872	62.70%	10.754%
11	12.061	1794	1800	1809	rBV	989661	1209067	76.12%	13.056%




Sum of corrected areas: 9260448

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121920\
Data File : VX020173.D
Acq On : 19 Dec 2020 16:01
Operator : JC/MD
Sample : L5053-21DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE120D2-20201210DL

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X121820W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

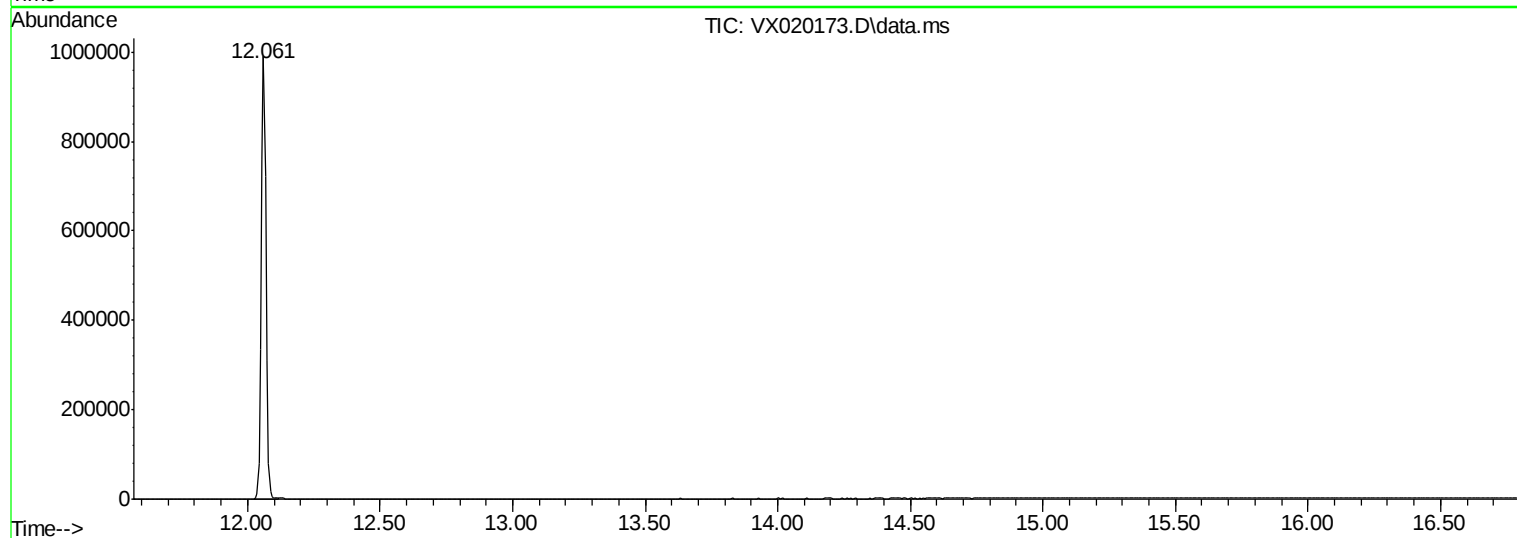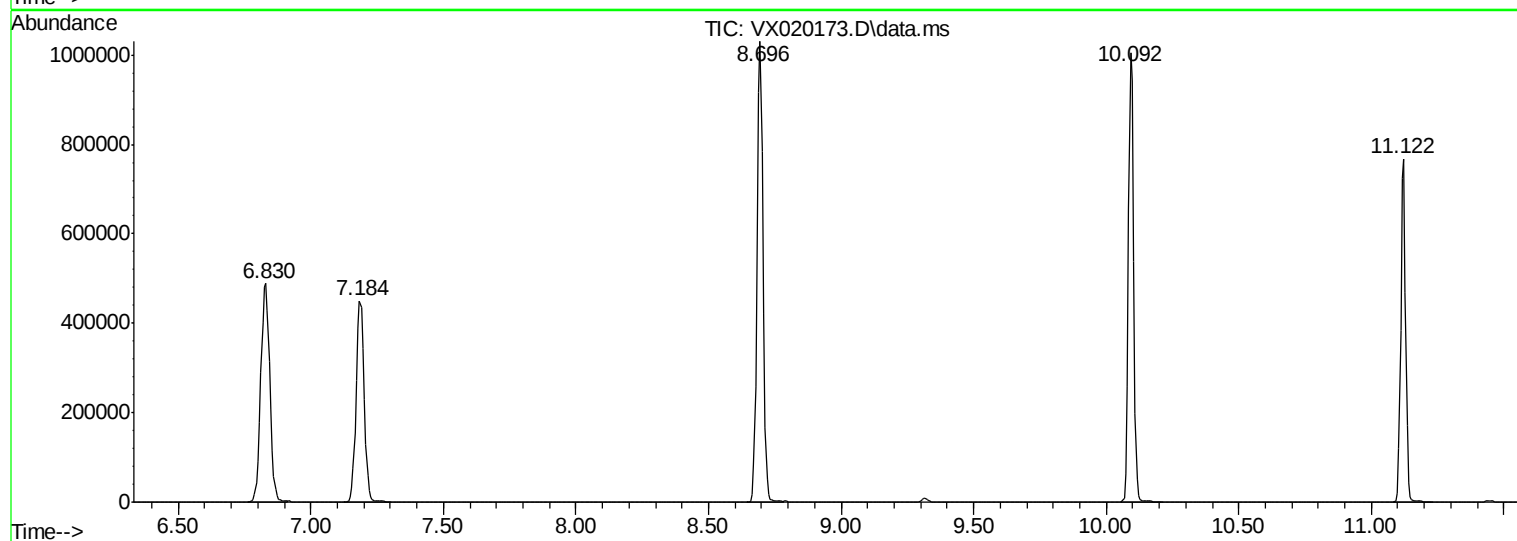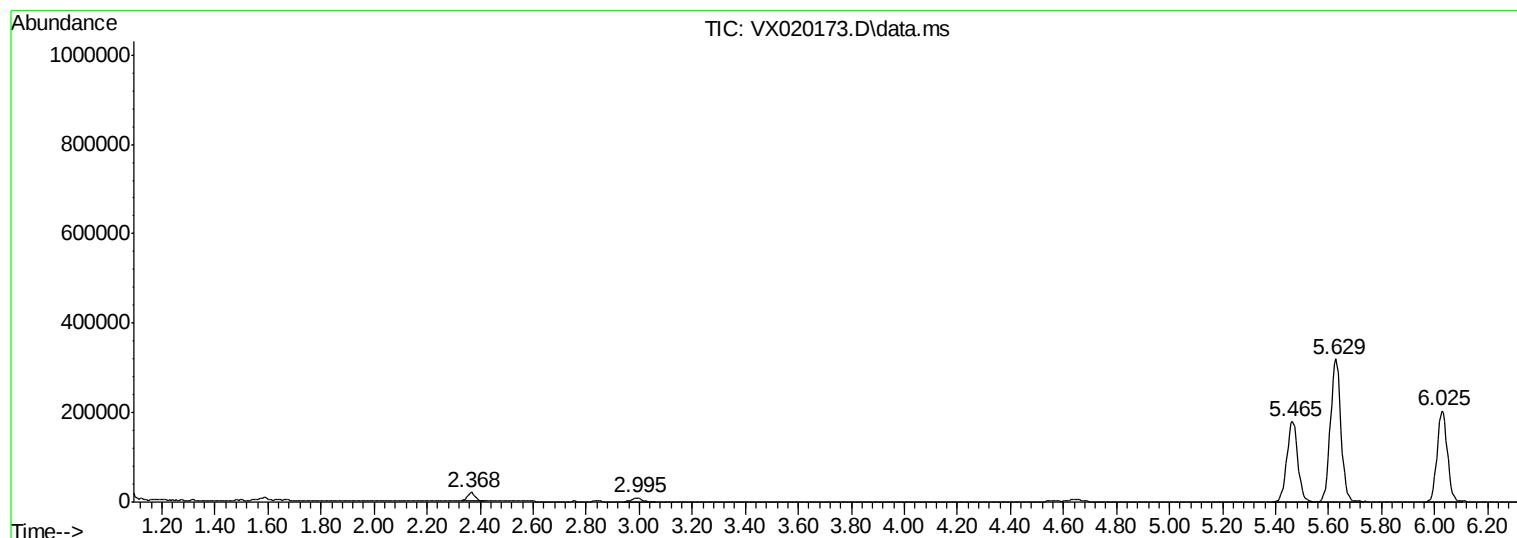

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121920\
Data File : VX020173.D
Acq On : 19 Dec 2020 16:01
Operator : JC/MD
Sample : L5053-21DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE120D2-20201210DL

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X121820W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121920\
Data File : VX020173.D
Acq On : 19 Dec 2020 16:01
Operator : JC/MD
Sample : L5053-21DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE120D2-20201210DL

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X121820W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
				#	RT Resp Conc