


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121920\
Data File : VX020165.D
Acq On : 19 Dec 2020 11:54
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X121820W.M
Title : SW846 8260
Last Update : Fri Dec 18 13:09:49 2020

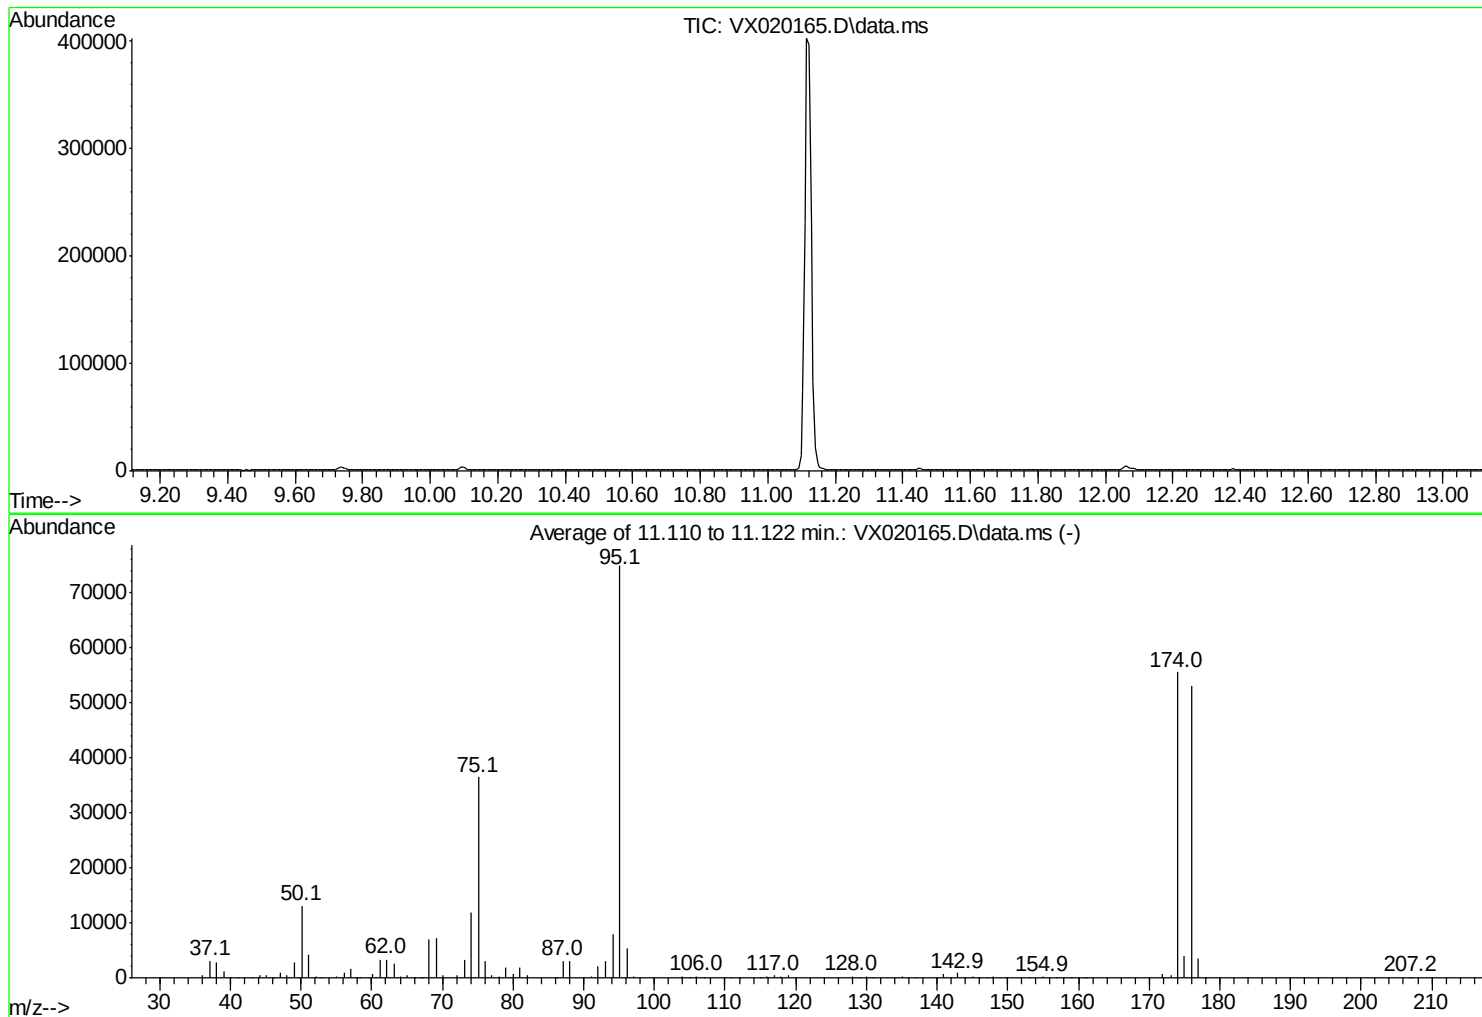

AutoFind: Scans 1644, 1645, 1646; Background Corrected with Scan 1637

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.5	13112	PASS
75	95	30	60	48.7	36475	PASS
95	95	100	100	100.0	74869	PASS
96	95	5	9	7.0	5245	PASS
173	174	0.00	2	0.9	482	PASS
174	95	50	100	74.1	55512	PASS
175	174	5	9	7.1	3942	PASS
176	174	95	101	95.7	53136	PASS
177	176	5	9	6.5	3464	PASS