


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121920\
Data File : VX020217.D
Acq On : 20 Dec 2020 10:12
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 56 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X121820W.M
Title : SW846 8260
Last Update : Fri Dec 18 13:09:49 2020

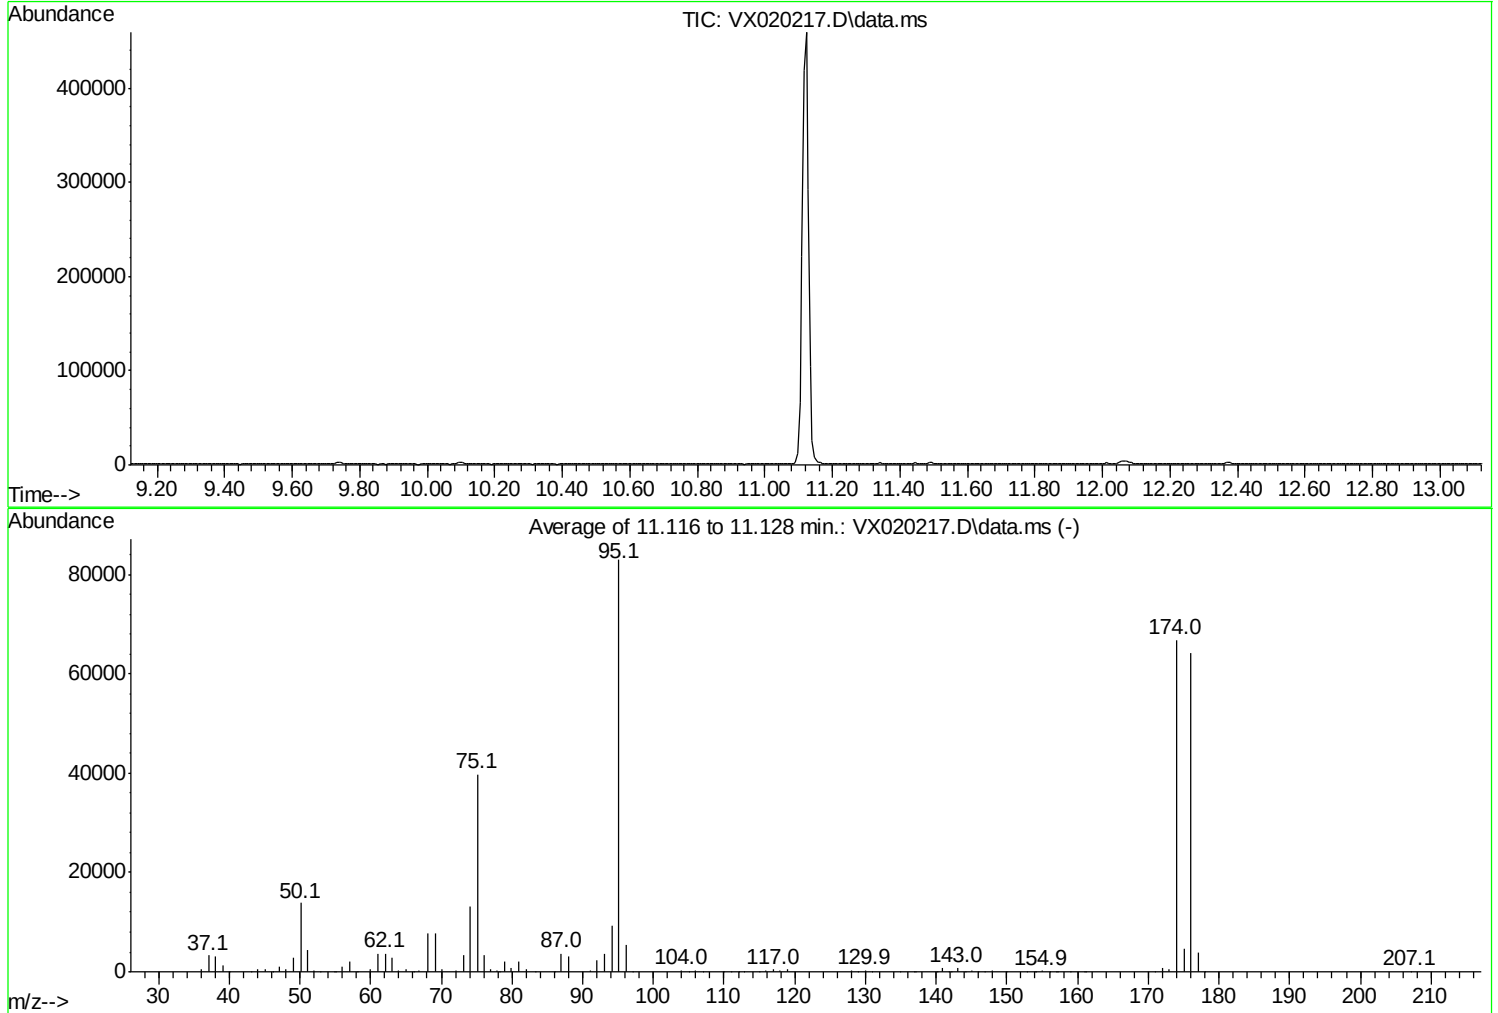

AutoFind: Scans 1645, 1646, 1647; Background Corrected with Scan 1638

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.7	13889	PASS
75	95	30	60	48.0	39789	PASS
95	95	100	100	100.0	82949	PASS
96	95	5	9	6.7	5522	PASS
173	174	0.00	2	0.8	542	PASS
174	95	50	100	80.6	66856	PASS
175	174	5	9	7.0	4666	PASS
176	174	95	101	96.2	64283	PASS
177	176	5	9	6.2	3996	PASS