

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121921\
 Data File : VX025903.D
 Acq On : 18 Dec 2021 11:38
 Operator : JC/MD
 Sample : VX1219MBL01
 Misc : 5.0g/10mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX1219MBL01

Quant Time: Dec 19 05:53:41 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X121321W.M
 Quant Title : SW846 8260
 QLast Update : Tue Dec 14 07:02:11 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	139351	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	245319	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	219640	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	89067	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	106210	52.97	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	= 105.94%	
35) Dibromofluoromethane	5.385	113	87195	50.96	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 101.92%	
50) Toluene-d8	8.647	98	318519	51.10	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	= 102.20%	
62) 4-Bromofluorobenzene	11.079	95	107137	45.25	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	= 90.50%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121921\
Data File : VX025903.D
Acq On : 18 Dec 2021 11:38
Operator : JC/MD
Sample : VX1219MBL01
Misc : 5.0g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX1219MBL01


Quant Time: Dec 19 05:53:41 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X121321W.M
Quant Title : SW846 8260
QLast Update : Tue Dec 14 07:02:11 2021
Response via : Initial Calibration

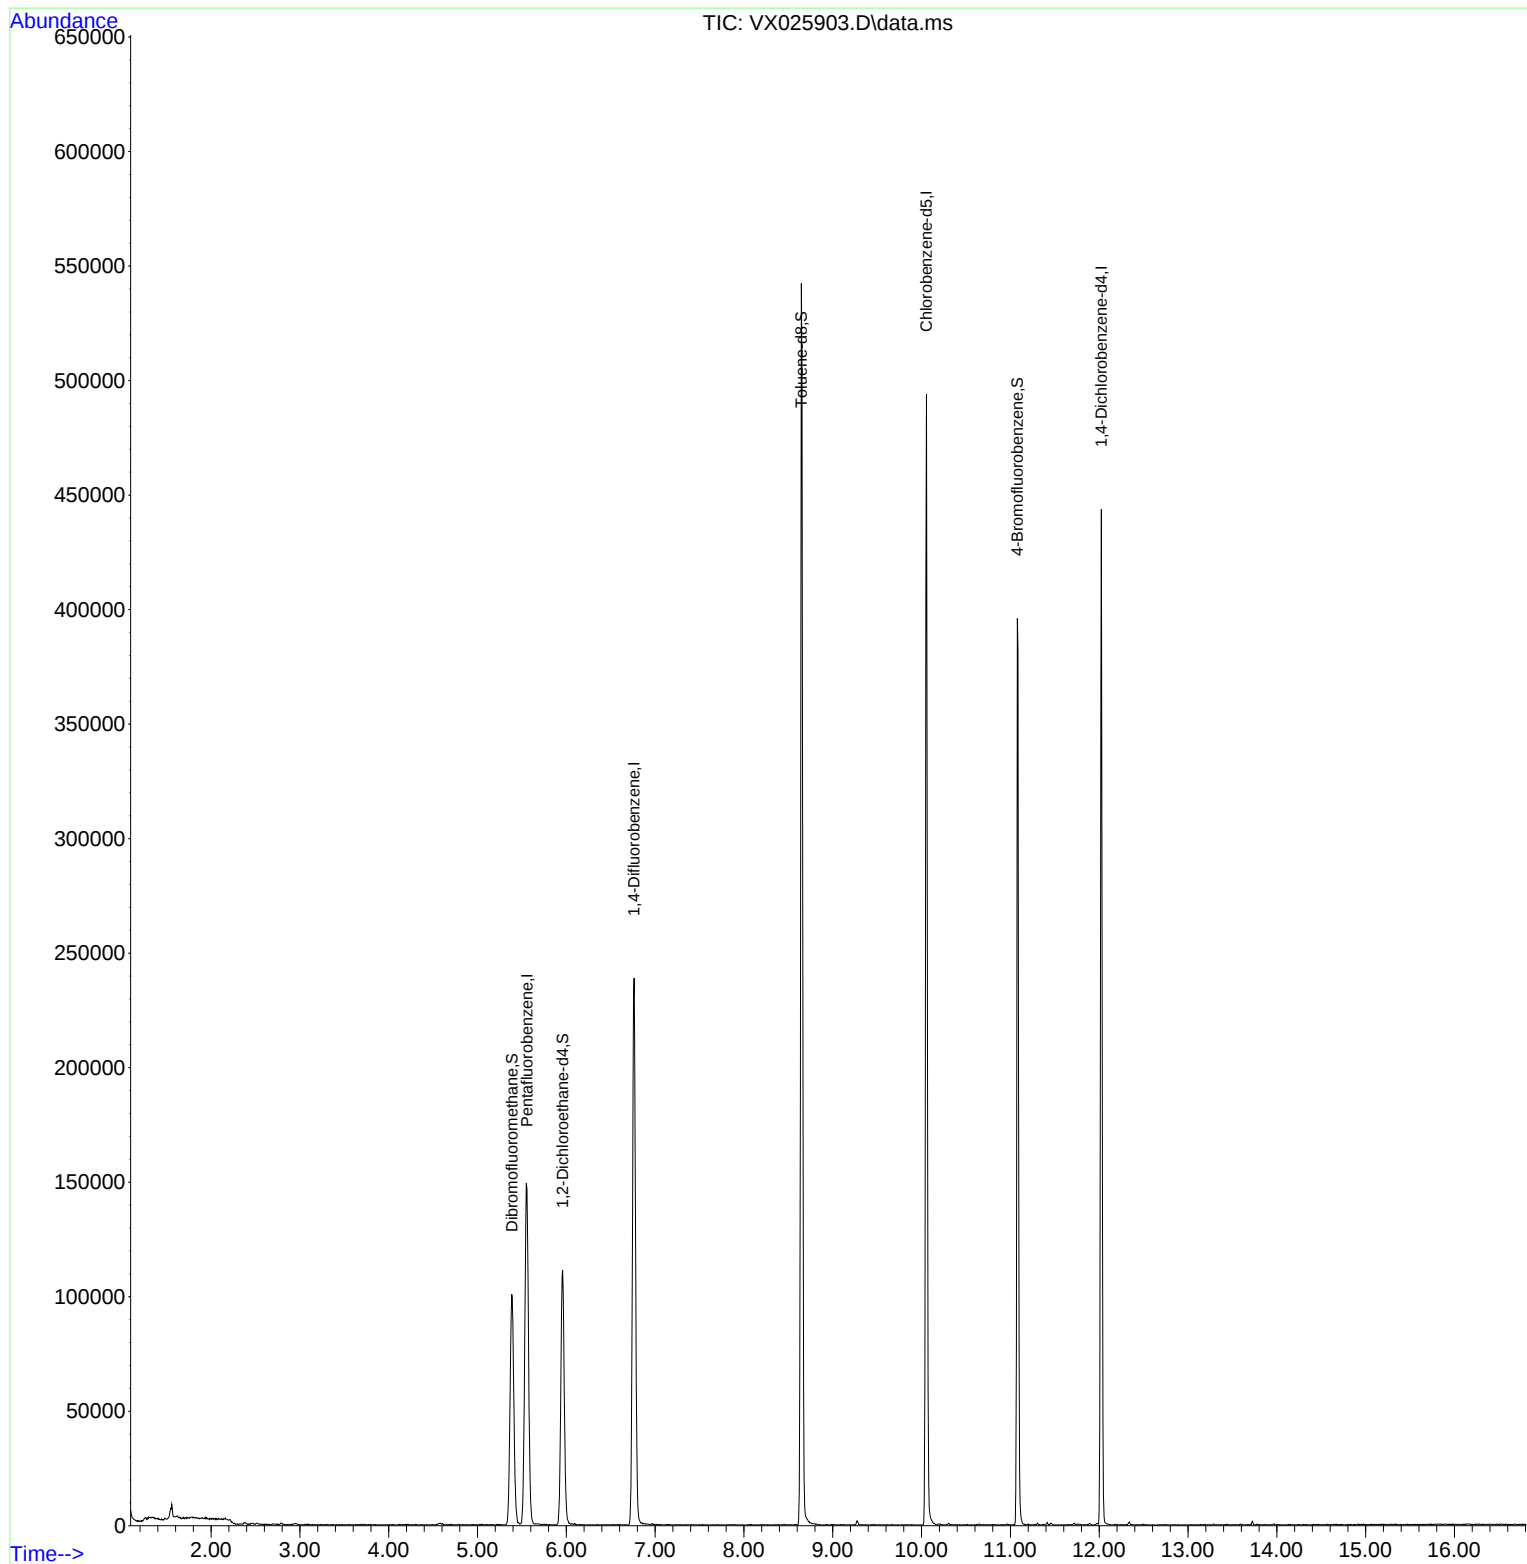



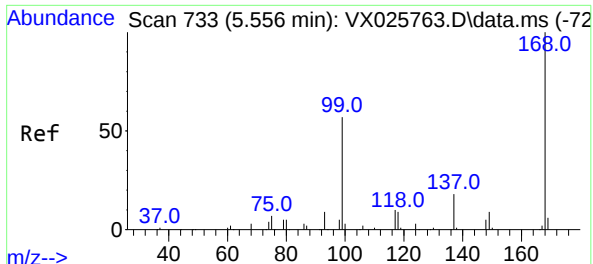


#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 5.556 min Scan# 733
Delta R.T. -0.000 min
Lab File: VX025903.D
Acq: 18 Dec 2021 11:38

Instrument :
MSVOA_X
ClientSampleId :
VX1219MBL01



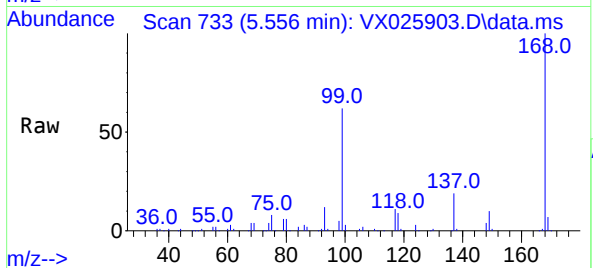



Tgt Ion:168 Resp: 139351
Ion Ratio Lower Upper
168 100
99 62.2 45.8 68.8

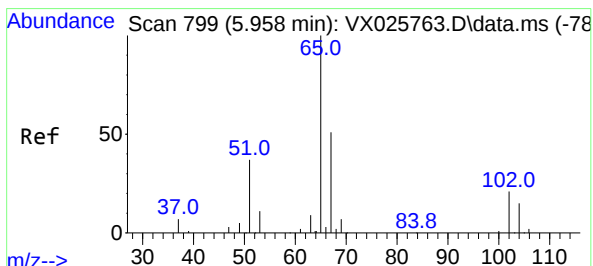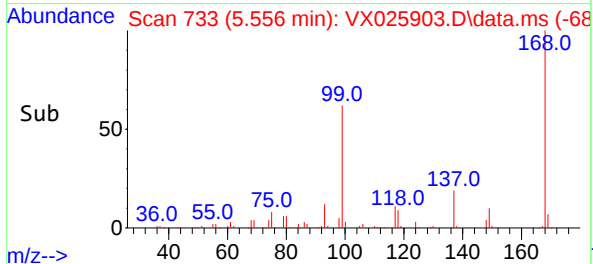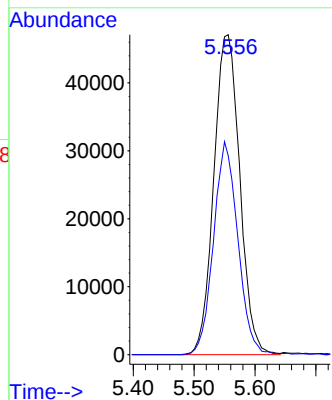

#33
1,2-Dichloroethane-d4
Concen: 52.97 ug/l
RT: 5.958 min Scan# 799
Delta R.T. -0.000 min
Lab File: VX025903.D
Acq: 18 Dec 2021 11:38

Tgt Ion: 65 Resp: 106210
Ion Ratio Lower Upper
65 100
67 51.7 0.0 103.4

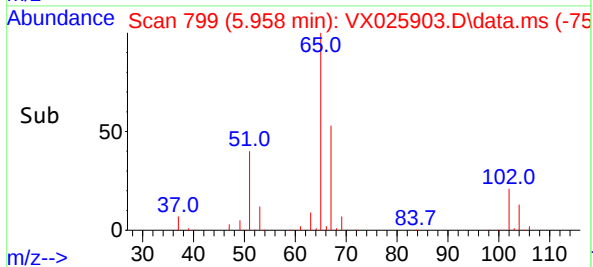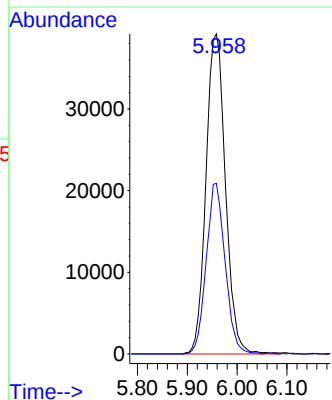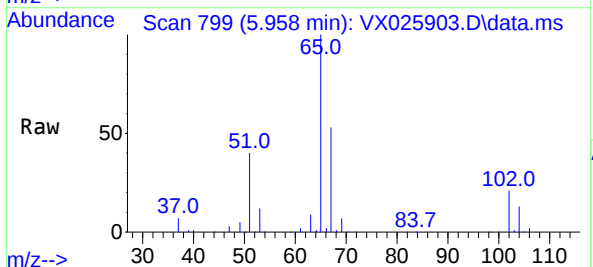

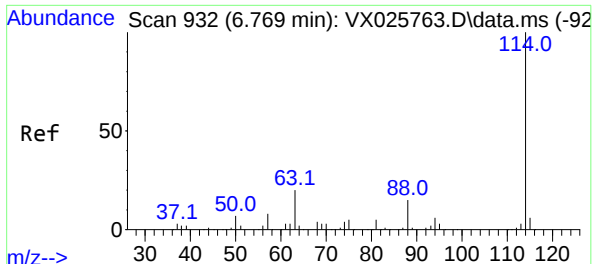

#34

1,4-Difluorobenzene

Concen: 50.00 ug/l

RT: 6.763 min Scan# 91

Delta R.T. -0.006 min

Lab File: VX025903.D

Acq: 18 Dec 2021 11:38

Instrument :

MSVOA_X

ClientSampleId :

VX1219MBL01





Tgt Ion:114 Resp: 245319

Ion Ratio Lower Upper

114 100

63 19.5 0.0 40.0

88 14.9 0.0 30.6

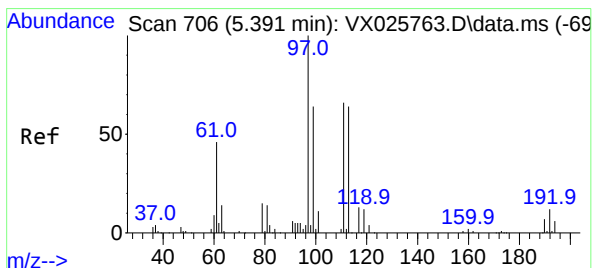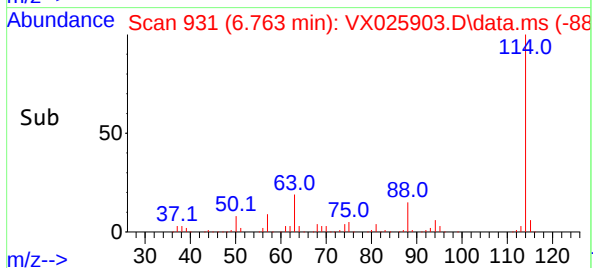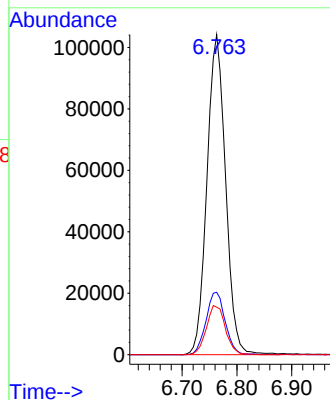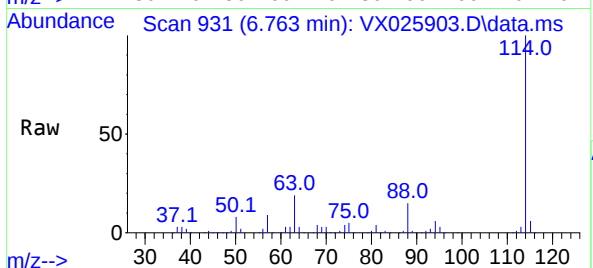

#35

Dibromofluoromethane

Concen: 50.96 ug/l

RT: 5.385 min Scan# 705

Delta R.T. -0.006 min

Lab File: VX025903.D

Acq: 18 Dec 2021 11:38




Tgt Ion:113 Resp: 87195


Ion Ratio Lower Upper

113 100

111 103.2 81.8 122.8

192 18.5 15.0 22.4


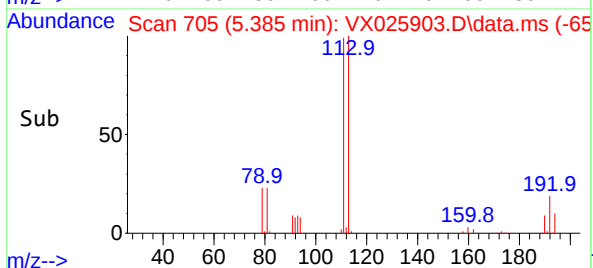
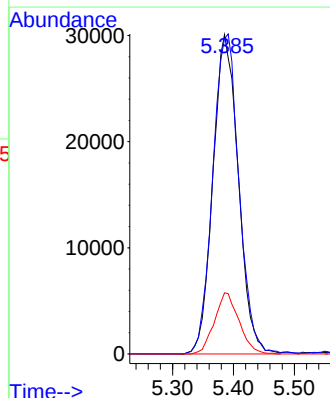
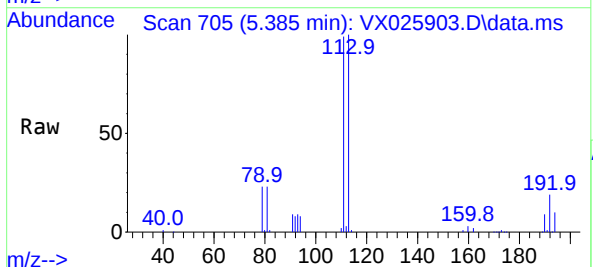


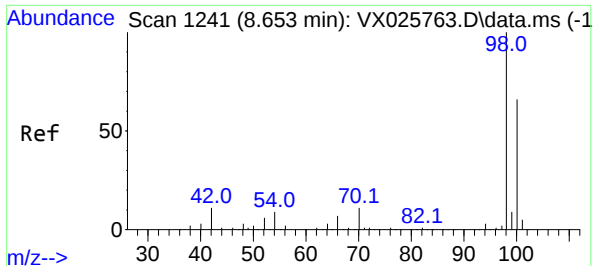

#50
Toluene-d8
Concen: 51.10 ug/l
RT: 8.647 min Scan# 11
Delta R.T. -0.006 min
Lab File: VX025903.D
Acq: 18 Dec 2021 11:38




Instrument :
MSVOA_X
ClientSampleId :
VX1219MBL01


Tgt Ion: 98 Resp: 318519
Ion Ratio Lower Upper
98 100
100 65.5 52.6 78.8

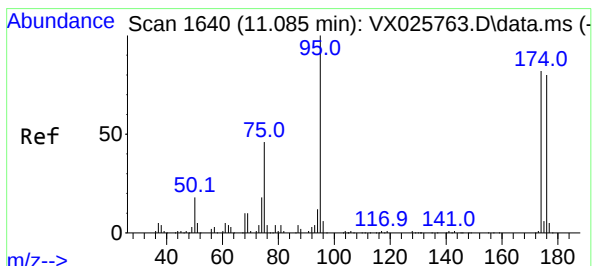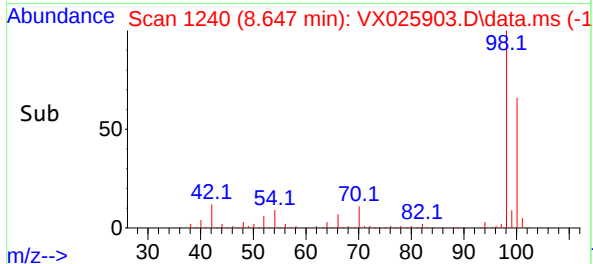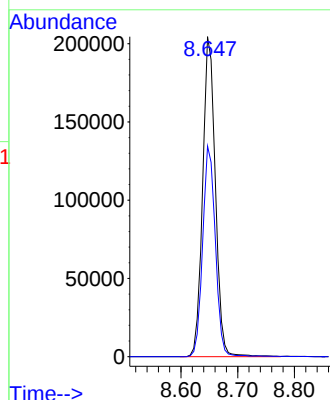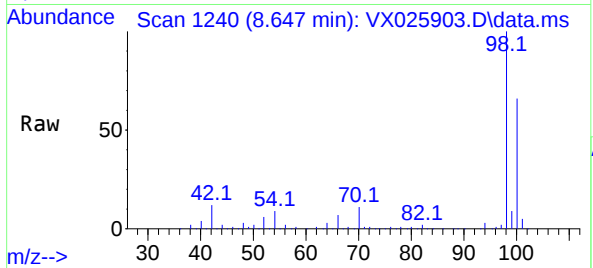

#62
4-Bromofluorobenzene
Concen: 45.25 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.006 min
Lab File: VX025903.D
Acq: 18 Dec 2021 11:38

Tgt Ion: 95 Resp: 107137
Ion Ratio Lower Upper
95 100
174 76.3 0.0 157.4
176 72.8 0.0 154.6


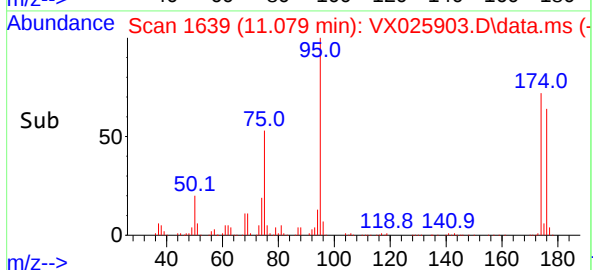
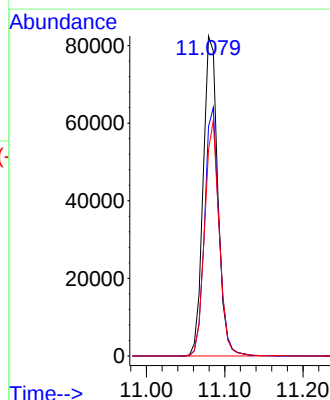
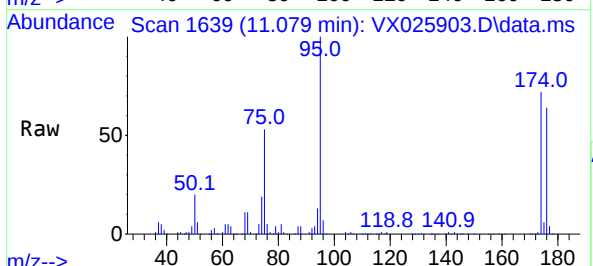


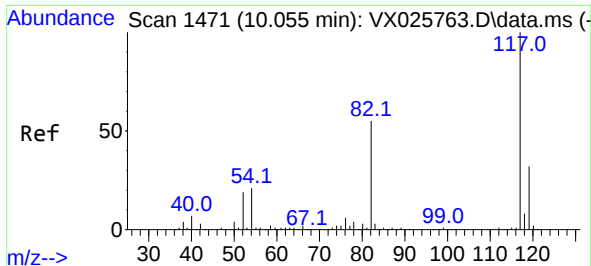

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX025903.D
Acq: 18 Dec 2021 11:38

Instrument :
MSVOA_X
ClientSampleId :
VX1219MBL01

Tgt Ion:117 Resp: 219640
Ion Ratio Lower Upper
117 100
82 54.9 43.8 65.6
119 32.2 25.2 37.8

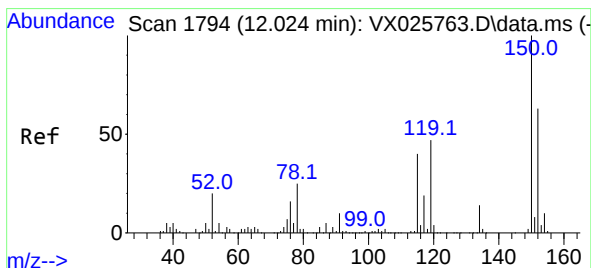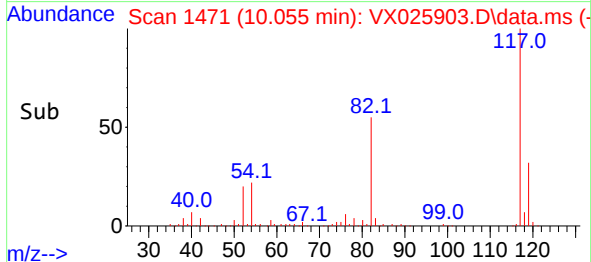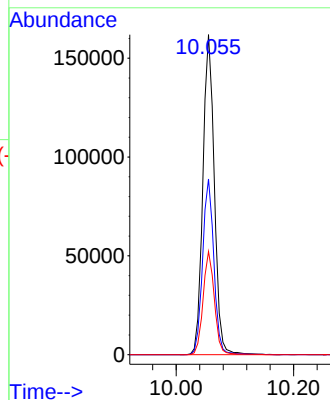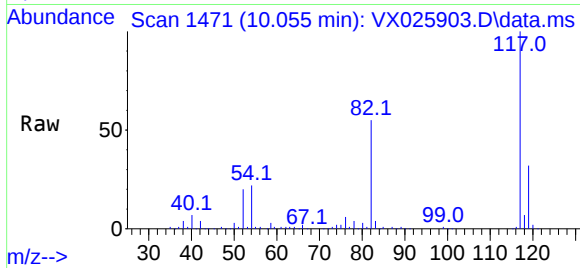

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. -0.000 min
Lab File: VX025903.D
Acq: 18 Dec 2021 11:38

Tgt Ion:152 Resp: 89067
Ion Ratio Lower Upper
152 100
115 61.1 41.3 123.9
150 158.2 0.0 351.8

