

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121922\
 Data File : VX033480.D
 Acq On : 19 Dec 2022 13:36
 Operator : JC/MD
 Sample : PB149705ZHE#04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 PB149705ZHE#04

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120722W.M
 Title : SW846 8260

Signal : TIC: VX033480.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.306	31	36	42	rBV2	3244	9177	1.07%	0.184%
2	2.386	208	213	221	rBV	5521	9881	1.16%	0.198%
3	2.794	273	280	291	rVB	11575	21592	2.53%	0.433%
4	4.714	587	595	609	rBV3	5573	16840	1.97%	0.337%
5	5.385	693	705	718	rBV	33837	97652	11.42%	1.956%
6	5.556	720	733	745	rBV2	85704	246073	28.79%	4.929%
7	5.958	789	799	811	rBV2	25017	64480	7.54%	1.292%
8	6.342	853	862	873	rBV	34426	88198	10.32%	1.767%
9	6.763	920	931	944	rBV	135298	340389	39.82%	6.818%
10	7.641	1069	1075	1080	rBV	19760	34987	4.09%	0.701%
11	7.696	1080	1084	1093	rVB	6748	11912	1.39%	0.239%
12	7.799	1093	1101	1114	rBV	500945	854747	100.00%	17.121%
13	8.549	1217	1224	1234	rBV	111319	172700	20.20%	3.459%
14	8.647	1234	1240	1251	rBV	100981	163031	19.07%	3.266%
15	8.951	1284	1290	1306	rVB	153219	218576	25.57%	4.378%
16	9.244	1332	1338	1344	rBV	164473	224068	26.21%	4.488%
17	9.305	1344	1348	1351	rVV	14380	20594	2.41%	0.413%
18	9.342	1351	1354	1356	rVV	23106	30283	3.54%	0.607%
19	9.378	1356	1360	1366	rVB	62517	90946	10.64%	1.822%
20	9.482	1372	1377	1388	rVV	277799	353003	41.30%	7.071%
21	9.579	1388	1393	1407	rVB	182149	233936	27.37%	4.686%
22	9.915	1442	1448	1460	rBV	517743	654726	76.60%	13.115%
23	10.055	1463	1471	1478	rBV	282957	386525	45.22%	7.742%
24	10.280	1503	1508	1516	rVB	6765	8864	1.04%	0.178%
25	10.506	1540	1545	1554	rBV	6559	8817	1.03%	0.177%
26	10.640	1562	1567	1571	rBV	44038	53532	6.26%	1.072%
27	10.683	1571	1574	1580	rVB	7815	10268	1.20%	0.206%
28	11.079	1634	1639	1651	rVB	176987	226794	26.53%	4.543%
29	12.024	1789	1794	1803	rVB	280597	339666	39.74%	6.804%


Sum of corrected areas: 4992257

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121922\
Data File : VX033480.D
Acq On : 19 Dec 2022 13:36
Operator : JC/MD
Sample : PB149705ZHE#04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
PB149705ZHE#04

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

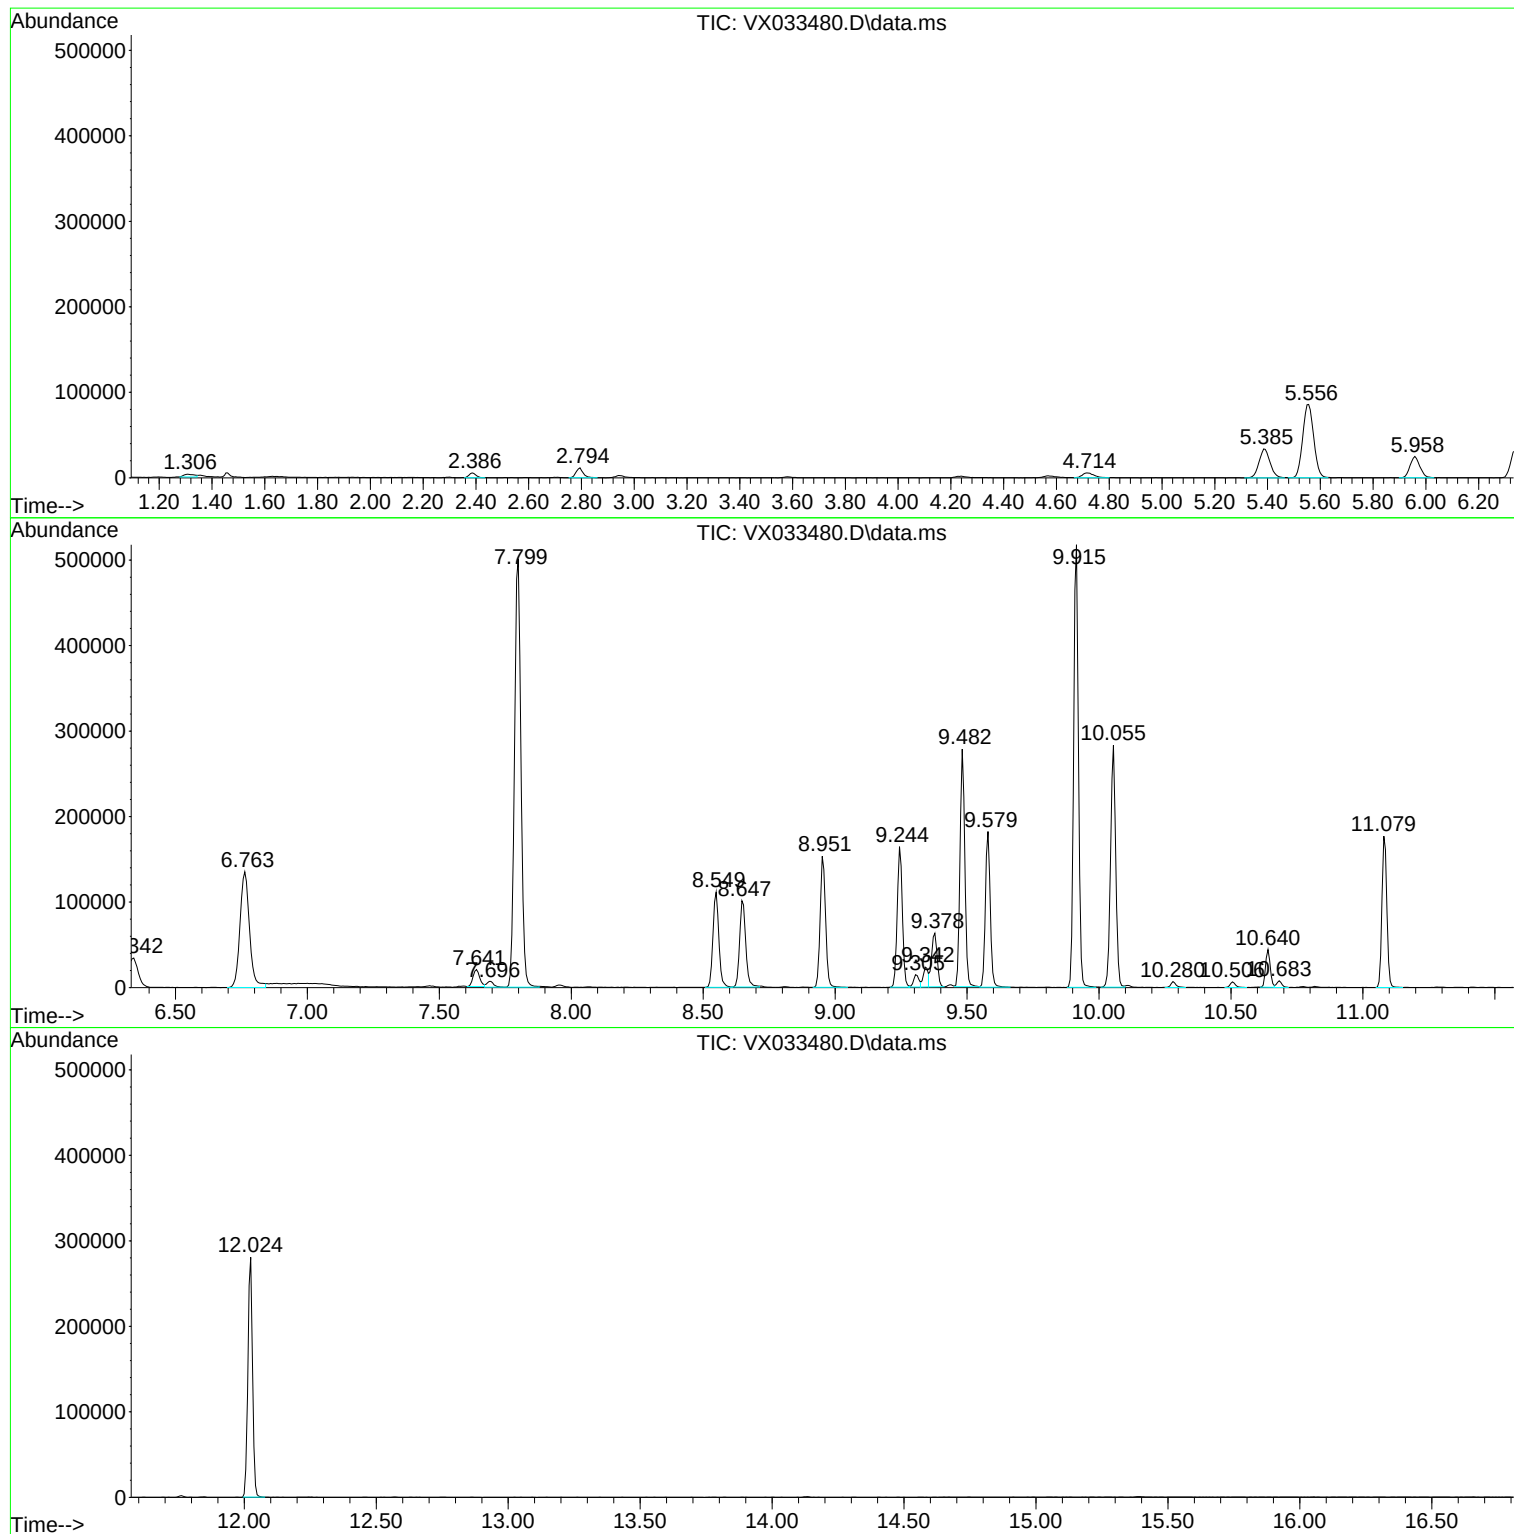

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121922\
Data File : VX033480.D
Acq On : 19 Dec 2022 13:36
Operator : JC/MD
Sample : PB149705ZHE#04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
PB149705ZHE#04

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121922\
Data File : VX033480.D
Acq On : 19 Dec 2022 13:36
Operator : JC/MD
Sample : PB149705ZHE#04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
PB149705ZHE#04

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------