




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
 Data File : VX039372.D
 Acq On : 19 Dec 2023 21:15
 Operator : JC/MD
 Sample : 05807-11ME
 Misc : 5.05g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0AZ3

Manual IntegrationsAPPROVED

Quant Time: Dec 20 02:20:45 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Dec 20 00:14:00 2023
 Response via : Initial Calibration

Reviewed By :John Carlone 12/20/2023
 Supervised By :Mahesh Dadoda 12/20/2023

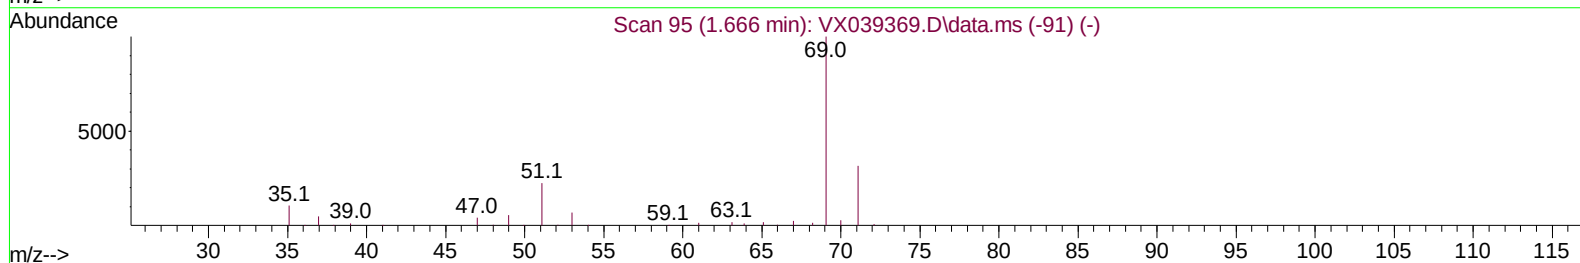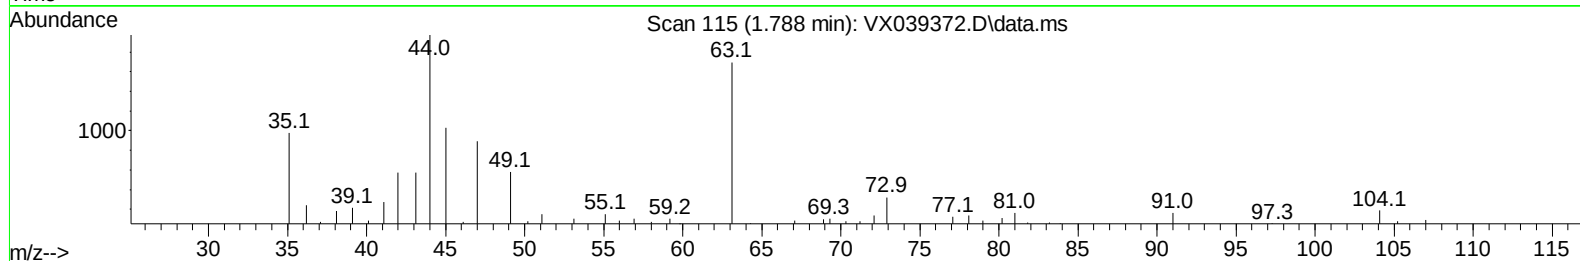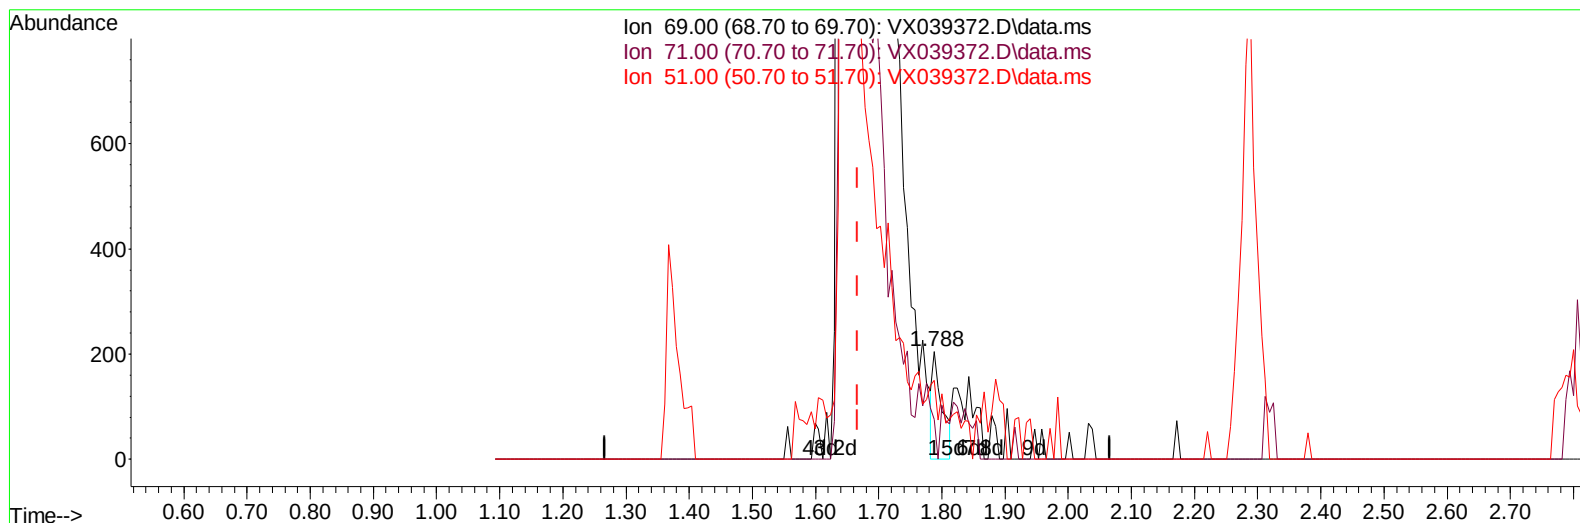

TIC: VX039372.D\data.ms

(7) Chloroethane-d5 (S)

1.788min (+ 0.122) 0.19 ug/L

response 215

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	32.10	41.40
51.00	27.90	30.23
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
 Data File : VX039372.D
 Acq On : 19 Dec 2023 21:15
 Operator : JC/MD
 Sample : 05807-11ME
 Misc : 5.05g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0AZ3

Manual IntegrationsAPPROVED

Quant Time: Dec 20 02:20:45 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Dec 20 00:14:00 2023
 Response via : Initial Calibration

Reviewed By :John Carlone 12/20/2023
 Supervised By :Mahesh Dadoda 12/20/2023

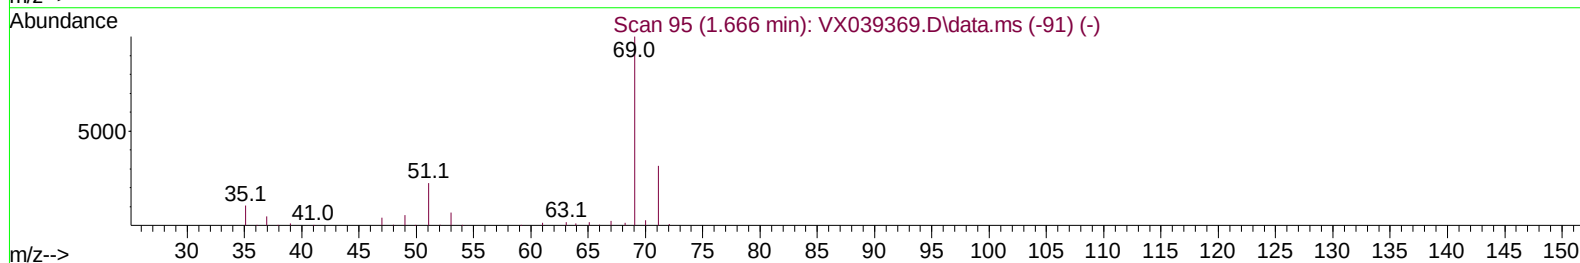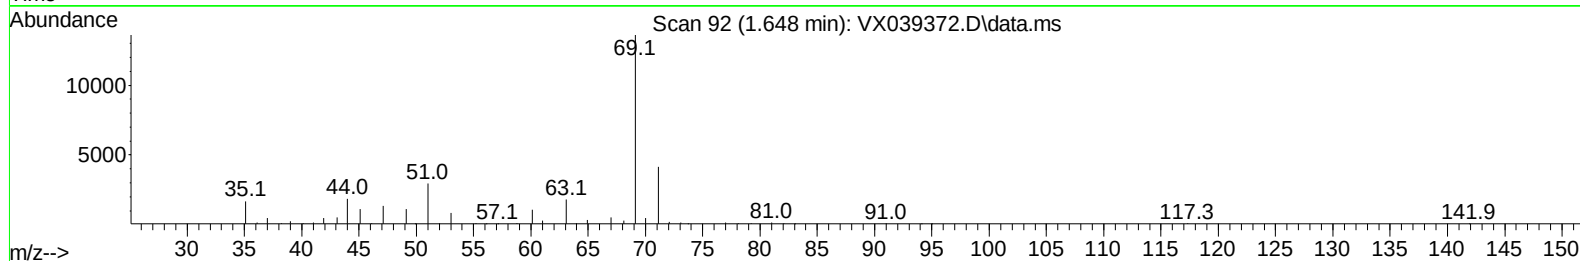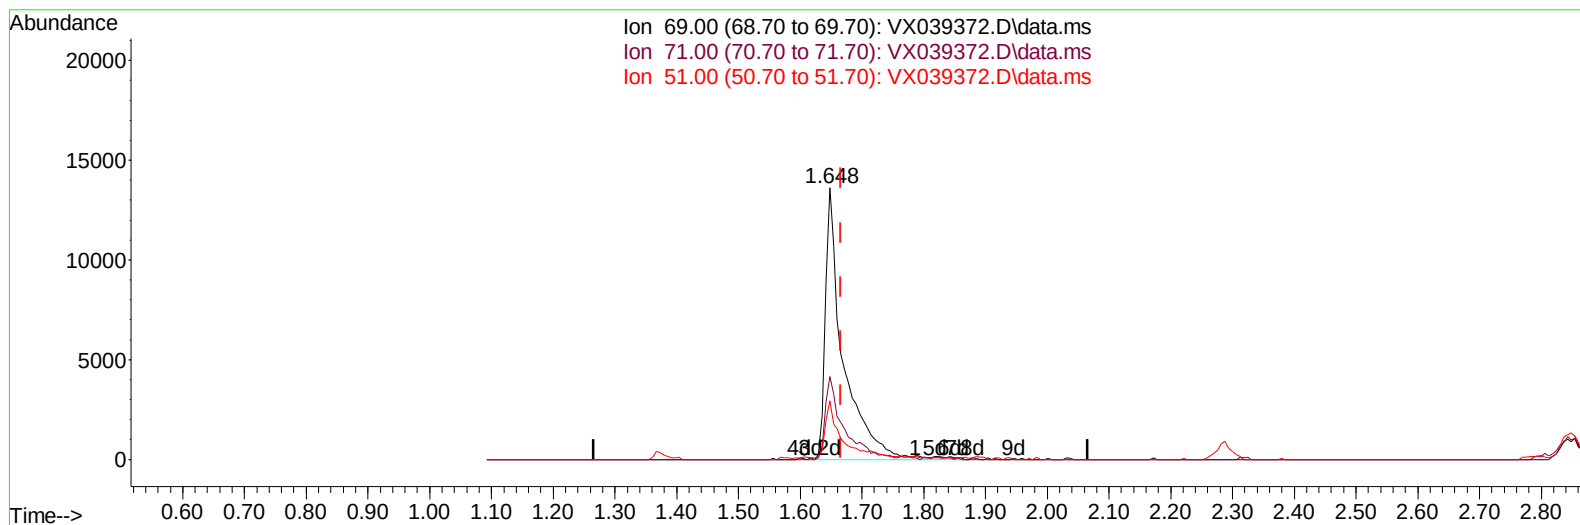

TIC: VX039372.D\data.ms

(7) Chloroethane-d5 (S)

1.648min (-0.019) 24.68 ug/L m

response 27614

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	32.10	0.32#
51.00	27.90	0.24#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
 Data File : VX039372.D
 Acq On : 19 Dec 2023 21:15
 Operator : JC/MD
 Sample : 05807-11ME
 Misc : 5.05g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0AZ3

Manual IntegrationsAPPROVED

Quant Time: Dec 20 02:20:45 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Dec 20 00:14:00 2023
 Response via : Initial Calibration

Reviewed By :John Carlone 12/20/2023
 Supervised By :Mahesh Dadoda 12/20/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	192962	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	176320	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	86417	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.373	65	70502	46.582	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	93.160%	
7) Chloroethane-d5	1.648	69	27614m	24.684	ug/L	-0.02
Spiked Amount 50.000	Range 70	- 130	Recovery	=	49.360%#	
11) 1,1-Dichloroethene-d2	2.288	65	33070	49.777	ug/L	-0.02
Spiked Amount 50.000	Range 60	- 125	Recovery	=	99.560%	
21) 2-Butanone-d5	4.483	46	124525	90.894	ug/L	0.04
Spiked Amount 100.000	Range 40	- 130	Recovery	=	90.890%	
24) Chloroform-d	5.062	84	126856	47.348	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	94.700%	
26) 1,2-Dichloroethane-d4	5.958	65	93395	53.825	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	107.660%	
32) Benzene-d6	5.970	84	273707	50.299	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	100.600%	
36) 1,2-Dichloropropane-d6	7.305	67	86721	49.521	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	99.040%	
41) Toluene-d8	8.646	98	238143	48.292	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	96.580%	
43) trans-1,3-Dichloroprop...	8.951	79	34942	39.209	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	78.420%	
47) 2-Hexanone-d5	9.396	63	90652	86.670	ug/L	0.01
Spiked Amount 100.000	Range 45	- 130	Recovery	=	86.670%	
56) 1,1,2,2-Tetrachloroeth...	11.195	84	111280	44.794	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	89.580%	
66) 1,2-Dichlorobenzene-d4	12.323	152	79421	48.622	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	97.240%	
Target Compounds						
					Qvalue	
33) Benzene	6.037	78	28504	5.087	ug/L	100
51) Chlorobenzene	10.079	112	523382	142.601	ug/L	95
64) 1,3-Dichlorobenzene	11.969	146	12423	4.596	ug/L	97
65) 1,4-Dichlorobenzene	12.042	146	119174	43.513	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
Data File : VX039372.D
Acq On : 19 Dec 2023 21:15
Operator : JC/MD
Sample : 05807-11ME
Misc : 5.05g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0AZ3

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 12/20/2023
Supervised By :Mahesh Dadoda 12/20/2023

Quant Time: Dec 20 02:20:45 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Dec 20 00:14:00 2023
Response via : Initial Calibration

