

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
 Data File : VX039372.D
 Acq On : 19 Dec 2023 21:15
 Operator : JC/MD
 Sample : 05807-11ME
 Misc : 5.05g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0AZ3

Quant Time: Dec 20 02:20:45 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Dec 20 00:14:00 2023
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By : John Carlone 12/20/2023
 Supervised By : Mahesh Dadoda 12/20/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	192962	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	176320	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	86417	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.373	65	70502	46.582	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	93.160%		
7) Chloroethane-d5	1.648	69	27614m	24.684	ug/L	-0.02
Spiked Amount 50.000	Range 70 - 130		Recovery =	49.360%#		
11) 1,1-Dichloroethene-d2	2.288	65	33070	49.777	ug/L	-0.02
Spiked Amount 50.000	Range 60 - 125		Recovery =	99.560%		
21) 2-Butanone-d5	4.483	46	124525	90.894	ug/L	0.04
Spiked Amount 100.000	Range 40 - 130		Recovery =	90.890%		
24) Chloroform-d	5.062	84	126856	47.348	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	94.700%		
26) 1,2-Dichloroethane-d4	5.958	65	93395	53.825	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	107.660%		
32) Benzene-d6	5.970	84	273707	50.299	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	100.600%		
36) 1,2-Dichloropropane-d6	7.305	67	86721	49.521	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	99.040%		
41) Toluene-d8	8.646	98	238143	48.292	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	96.580%		
43) trans-1,3-Dichloroprop...	8.951	79	34942	39.209	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	78.420%		
47) 2-Hexanone-d5	9.396	63	90652	86.670	ug/L	0.01
Spiked Amount 100.000	Range 45 - 130		Recovery =	86.670%		
56) 1,1,2,2-Tetrachloroeth...	11.195	84	111280	44.794	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	89.580%		
66) 1,2-Dichlorobenzene-d4	12.323	152	79421	48.622	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	97.240%		
Target Compounds						
					Qvalue	
33) Benzene	6.037	78	28504	5.087	ug/L	100
51) Chlorobenzene	10.079	112	523382	142.601	ug/L	95
64) 1,3-Dichlorobenzene	11.969	146	12423	4.596	ug/L	97
65) 1,4-Dichlorobenzene	12.042	146	119174	43.513	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
Data File : VX039372.D
Acq On : 19 Dec 2023 21:15
Operator : JC/MD
Sample : 05807-11ME
Misc : 5.05g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 32 Sample Multiplier: 1


Instrument :
MSVOA_X
ClientSampleId :
C0AZ3

Quant Time: Dec 20 02:20:45 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Dec 20 00:14:00 2023
Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By : John Carlone 12/20/2023
Supervised By : Mahesh Dadoda 12/20/2023

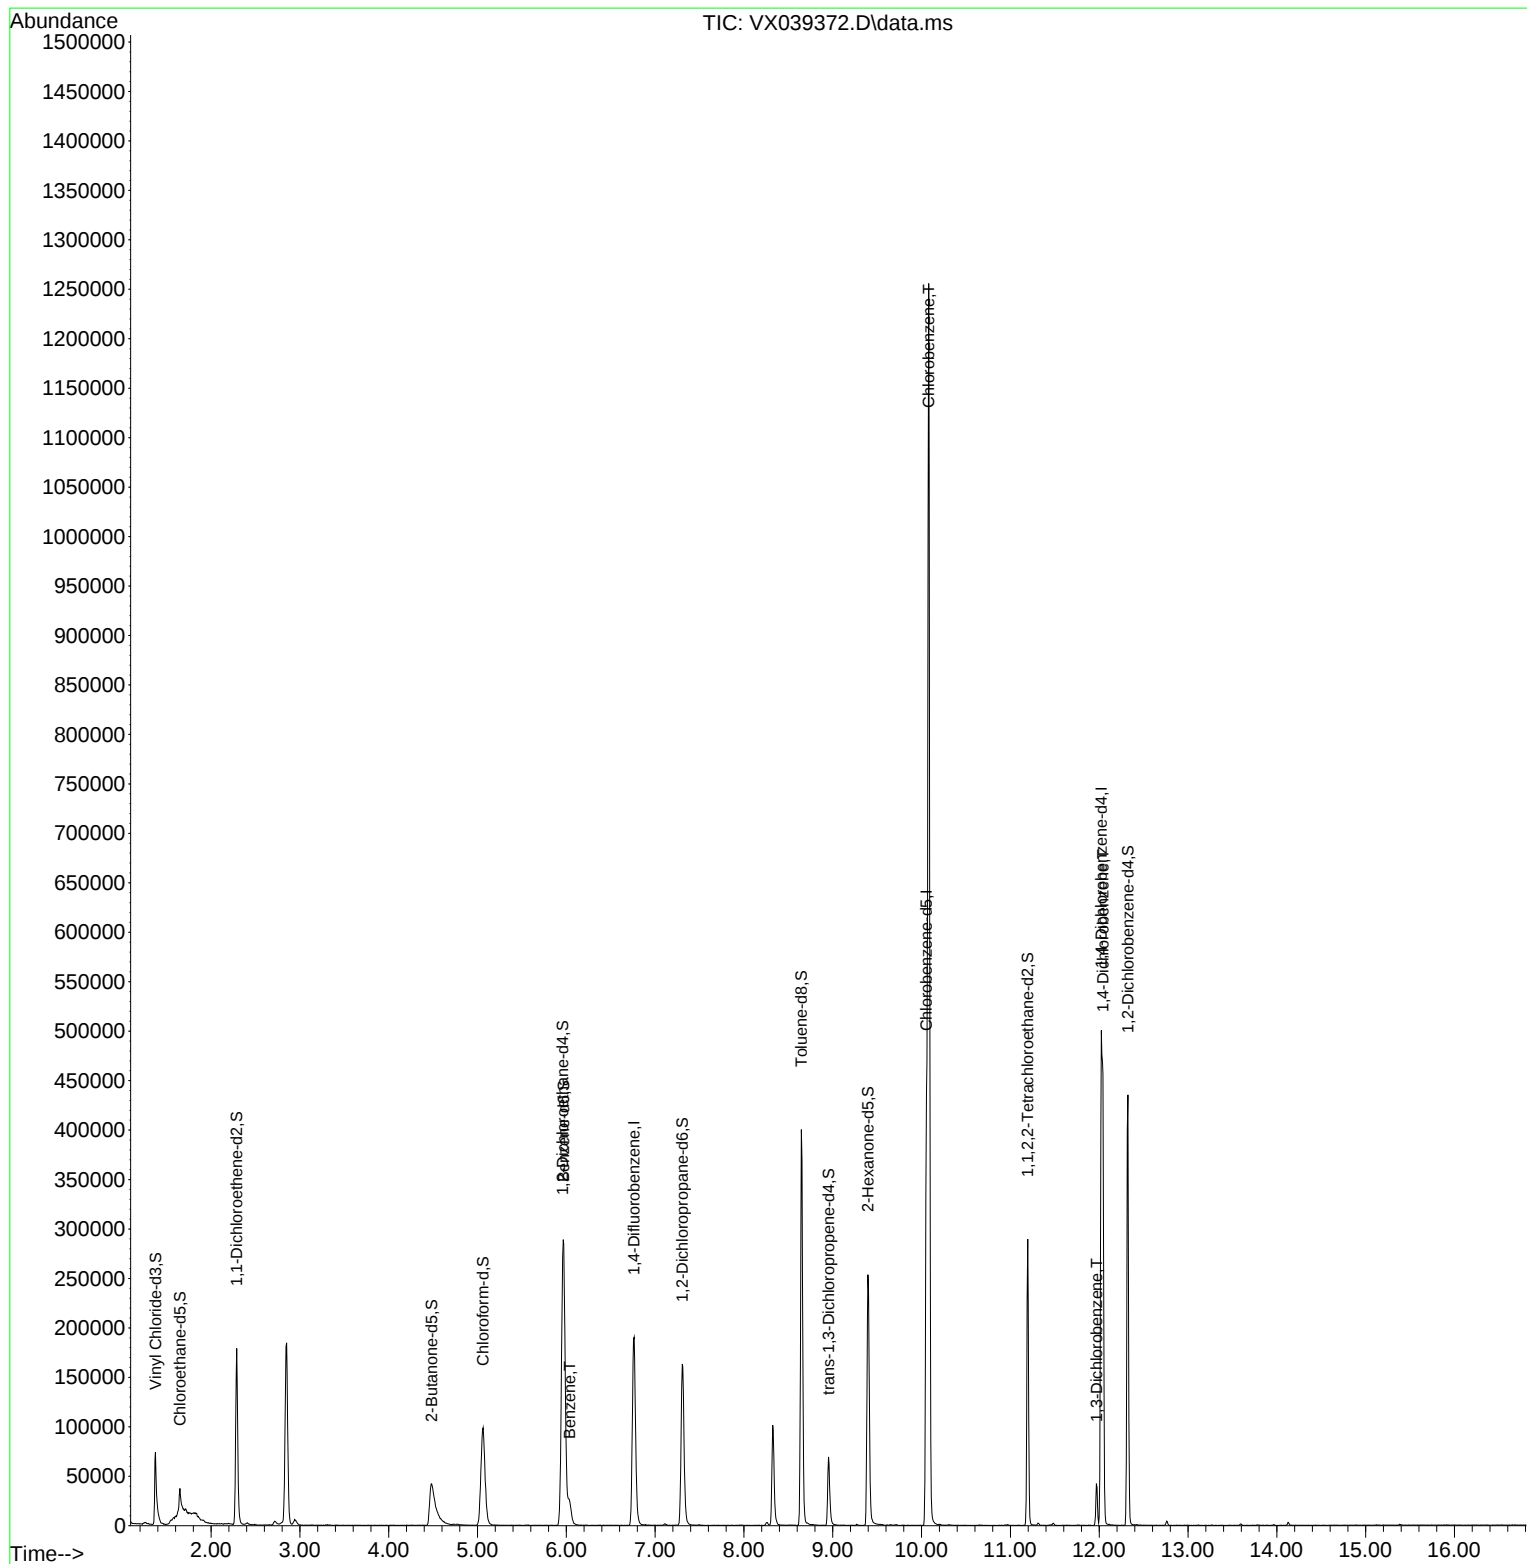

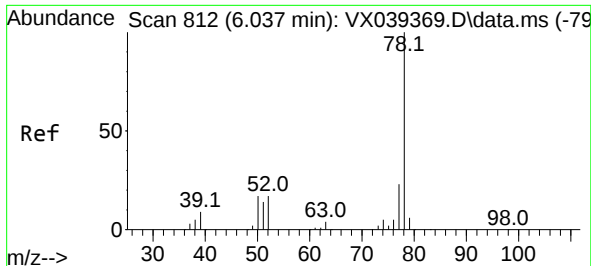





#33
Benzene
Concen: 5.087 ug/L
RT: 6.037 min Scan# 812
Delta R.T. -0.000 min
Lab File: VX039372.D
Acq: 19 Dec 2023 21:15

Instrument :
MSVOA_X
ClientSampleId :
C0AZ3

Tgt Ion: 78 Resp: 28504




Manual Integrations
APPROVED


Reviewed By :John Carlone 12/20/2023
Supervised By :Mahesh Dadoda 12/20/2023

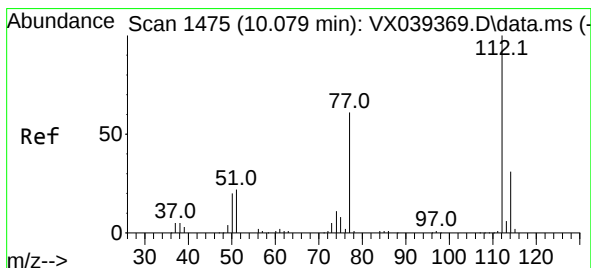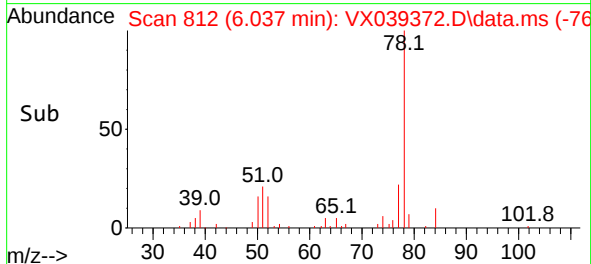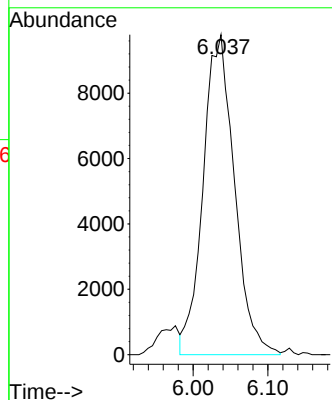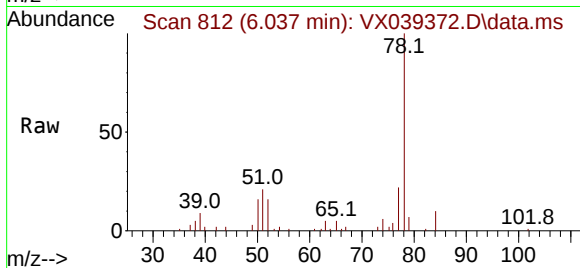

#51
Chlorobenzene
Concen: 142.601 ug/L
RT: 10.079 min Scan# 1475
Delta R.T. -0.000 min
Lab File: VX039372.D
Acq: 19 Dec 2023 21:15


Tgt Ion:112 Resp: 523382
Ion Ratio Lower Upper
112 100
114 31.8 21.8 40.4
77 66.1 49.0 73.6

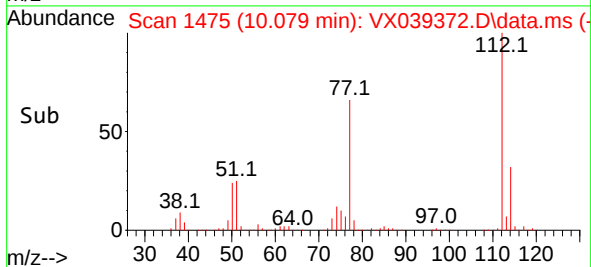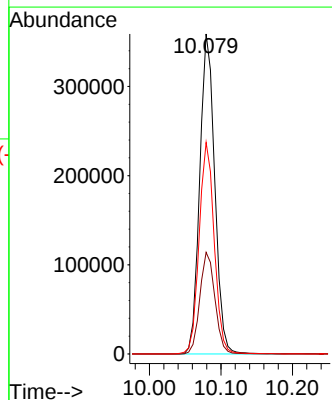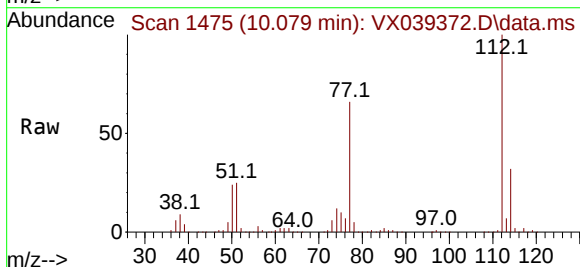

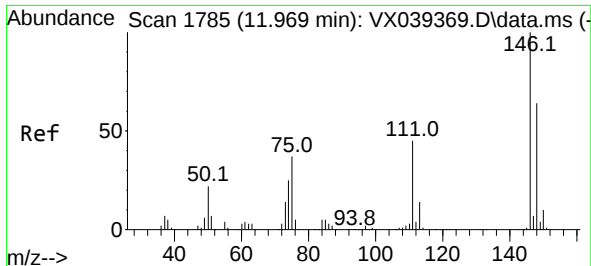

#64
1,3-Dichlorobenzene
Concen: 4.596 ug/L
RT: 11.969 min Scan# 1785
Delta R.T. -0.000 min
Lab File: VX039372.D
Acq: 19 Dec 2023 21:15




Instrument :
MSVOA_X
ClientSampleId :
C0AZ3

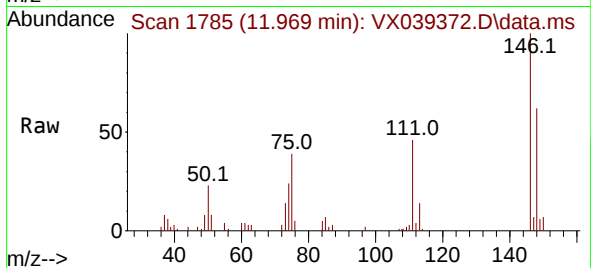


Tgt Ion:146 Resp: 1242
Ion Ratio Lower Upper
146 100
111 45.9 30.0 55.6
148 61.8 44.2 82.0

Manual Integrations
APPROVED

Reviewed By :John Carlone 12/20/2023
Supervised By :Mahesh Dadoda 12/20/2023

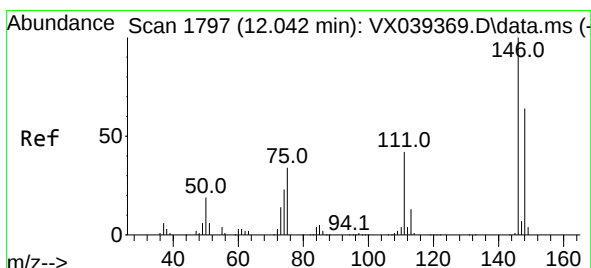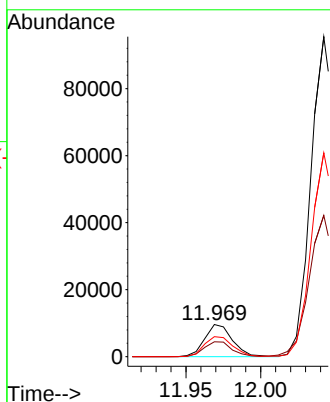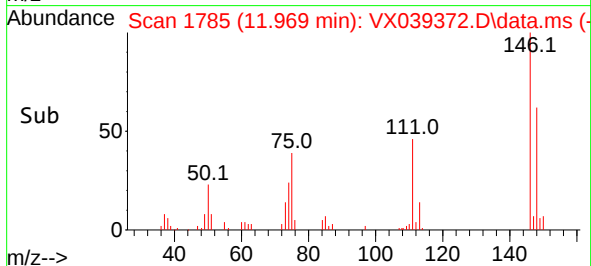

#65
1,4-Dichlorobenzene
Concen: 43.513 ug/L
RT: 12.042 min Scan# 1797
Delta R.T. -0.000 min
Lab File: VX039372.D
Acq: 19 Dec 2023 21:15

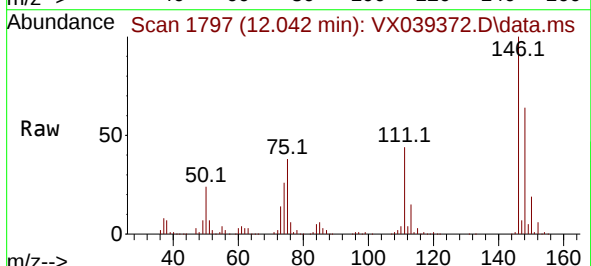

Tgt Ion:146 Resp: 119174
Ion Ratio Lower Upper
146 100
111 44.1 29.7 55.1
148 63.7 45.8 85.2

