

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
 Data File : VX039344.D
 Acq On : 19 Dec 2023 10:26
 Operator : JC/MD
 Sample : VX1219WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK652

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

Signal : TIC: VX039344.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	23	25	32	rBV4	1967	3754	0.40%	0.052%
2	1.368	42	46	56	rBV	118516	130316	14.01%	1.791%
3	1.666	91	95	110	rVB	72958	113077	12.16%	1.554%
4	2.307	194	200	211	rBV	208134	325523	35.00%	4.475%
5	2.514	230	234	238	rBV	923	1273	0.14%	0.018%
6	2.697	262	264	267	rBV2	249	250	0.03%	0.003%
7	2.745	270	272	275	rBV	180	239	0.03%	0.003%
8	2.788	275	279	284	rVV3	1452	2402	0.26%	0.033%
9	2.934	297	303	314	rVB2	2868	6263	0.67%	0.086%
10	3.099	328	330	331	rVV	377	350	0.04%	0.005%
11	3.142	335	337	343	rBV2	199	330	0.04%	0.005%
12	3.245	352	354	356	rBV2	198	236	0.03%	0.003%
13	3.587	409	410	414	rBV2	129	184	0.02%	0.003%
14	3.617	414	415	419	rVB2	199	214	0.02%	0.003%
15	4.081	487	491	493	rBV2	180	267	0.03%	0.004%
16	4.251	517	519	522	rVB	179	205	0.02%	0.003%
17	4.446	542	551	564	rBV	85334	242299	26.05%	3.331%
18	4.763	601	603	606	rBV3	182	191	0.02%	0.003%
19	4.879	620	622	624	rBV2	227	206	0.02%	0.003%
20	5.056	639	651	670	rBV	111482	366390	39.40%	5.037%
21	5.343	697	698	702	rBV2	279	252	0.03%	0.003%
22	5.422	709	711	712	rBV	402	240	0.03%	0.003%
23	5.513	725	726	729	rBV	182	193	0.02%	0.003%
24	5.550	729	732	735	rVB2	240	214	0.02%	0.003%
25	5.721	758	760	763	rVB2	236	196	0.02%	0.003%
26	5.964	788	800	824	rBV2	305107	930026	100.00%	12.785%
27	6.227	842	843	846	rVB2	264	249	0.03%	0.003%
28	6.428	873	876	878	rBV	207	194	0.02%	0.003%
29	6.458	879	881	884	rVV	339	302	0.03%	0.004%
30	6.580	899	901	904	rVB2	306	266	0.03%	0.004%
31	6.757	921	930	946	rBV	228860	545465	58.65%	7.499%
32	6.958	961	963	965	rBV2	314	260	0.03%	0.004%
33	7.111	983	988	994	rBV6	1523	3517	0.38%	0.048%
34	7.306	1011	1020	1033	rBV	192943	420277	45.19%	5.778%
35	7.641	1073	1075	1077	rVB	193	185	0.02%	0.003%
36	7.952	1122	1126	1127	rBV2	288	271	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
 Data File : VX039344.D
 Acq On : 19 Dec 2023 10:26
 Operator : JC/MD
 Sample : VX1219WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK652

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
 Title : VOC Analysis

37	8.086	1146	1148	1150	rVB2	192	185	0.02%	0.003%
38	8.324	1180	1187	1200	rBV	130625	220266	23.68%	3.028%
39	8.574	1225	1228	1232	rBV3	582	921	0.10%	0.013%
40	8.647	1233	1240	1260	rVV	478444	741763	79.76%	10.197%
41	8.946	1284	1289	1301	rBV	96557	146193	15.72%	2.010%
42	9.165	1323	1325	1327	rVB2	231	210	0.02%	0.003%
43	9.244	1337	1338	1341	rVB	363	186	0.02%	0.003%
44	9.281	1341	1344	1347	rBV2	354	357	0.04%	0.005%
45	9.378	1355	1360	1384	rBV	396516	575334	61.86%	7.909%
46	9.616	1395	1399	1402	rBV2	342	533	0.06%	0.007%
47	9.689	1410	1411	1417	rVB3	445	687	0.07%	0.009%
48	9.787	1425	1427	1430	rBV	198	209	0.02%	0.003%
49	9.921	1447	1449	1453	rBV	248	328	0.04%	0.005%
50	10.049	1465	1470	1489	rVB	484395	680942	73.22%	9.361%
51	10.183	1489	1492	1493	rBV2	390	334	0.04%	0.005%
52	10.250	1501	1503	1509	rVB2	324	428	0.05%	0.006%
53	10.317	1509	1514	1516	rBV4	651	1079	0.12%	0.015%
54	10.640	1565	1567	1569	rBV	538	620	0.07%	0.009%
55	10.781	1588	1590	1592	rBV2	202	187	0.02%	0.003%
56	10.811	1592	1595	1597	rVB2	201	194	0.02%	0.003%
57	10.976	1617	1622	1623	rBV2	487	734	0.08%	0.010%
58	11.031	1627	1631	1633	rVB2	222	333	0.04%	0.005%
59	11.085	1639	1640	1642	rBV	439	208	0.02%	0.003%
60	11.189	1652	1657	1669	rVB	351580	449507	48.33%	6.179%
61	11.354	1681	1684	1688	rBV2	219	238	0.03%	0.003%
62	11.457	1698	1701	1704	rBV3	653	730	0.08%	0.010%
63	11.567	1717	1719	1722	rBV	254	244	0.03%	0.003%
64	11.598	1722	1724	1727	rBV	203	200	0.02%	0.003%
65	11.750	1746	1749	1754	rBV3	577	871	0.09%	0.012%
66	11.902	1772	1774	1777	rBV2	144	194	0.02%	0.003%
67	11.969	1783	1785	1788	rBV3	922	818	0.09%	0.011%
68	12.018	1788	1793	1807	rBV	530175	694921	74.72%	9.553%
69	12.207	1821	1824	1825	rBV	301	272	0.03%	0.004%
70	12.317	1837	1842	1856	rVV	515601	644338	69.28%	8.858%
71	12.512	1871	1874	1875	rBV2	175	194	0.02%	0.003%
72	12.542	1878	1879	1882	rBV2	253	210	0.02%	0.003%
73	12.762	1911	1915	1920	rVB3	864	1117	0.12%	0.015%
74	13.073	1961	1966	1968	rVB2	153	232	0.02%	0.003%
75	13.116	1968	1973	1976	rBV2	489	709	0.08%	0.010%
76	13.177	1981	1983	1986	rBV2	186	218	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
 Data File : VX039344.D
 Acq On : 19 Dec 2023 10:26
 Operator : JC/MD
 Sample : VX1219WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK652

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

77	13.591	2048	2051	2056	rVV2	679	953	0.10%	0.013%
78	13.713	2068	2071	2072	rBV	266	227	0.02%	0.003%
79	13.780	2078	2082	2085	rBV2	901	1389	0.15%	0.019%
80	13.823	2088	2089	2094	rVB2	308	331	0.04%	0.005%
81	13.963	2110	2112	2115	rVB4	690	762	0.08%	0.010%
82	14.128	2134	2139	2145	rVV	1535	2209	0.24%	0.030%
83	14.268	2160	2162	2165	rVV	246	188	0.02%	0.003%
84	14.317	2168	2170	2172	rVB	274	197	0.02%	0.003%
85	14.359	2175	2177	2179	rBV	267	225	0.02%	0.003%
86	14.585	2211	2214	2218	rVB2	325	561	0.06%	0.008%
87	14.627	2218	2221	2222	rBV	227	195	0.02%	0.003%
88	14.676	2227	2229	2231	rVB	223	189	0.02%	0.003%
89	14.798	2247	2249	2251	rVB	369	265	0.03%	0.004%
90	14.932	2269	2271	2272	rBV	337	272	0.03%	0.004%
91	15.268	2322	2326	2329	rBV2	322	292	0.03%	0.004%
92	15.365	2339	2342	2343	rBV	240	254	0.03%	0.003%
93	15.670	2389	2392	2393	rBV	235	257	0.03%	0.004%
94	15.682	2393	2394	2397	rVV2	312	249	0.03%	0.003%
95	15.871	2422	2425	2426	rVV2	359	242	0.03%	0.003%
96	15.908	2429	2431	2434	rBV2	353	317	0.03%	0.004%
97	16.030	2450	2451	2455	rBV2	344	388	0.04%	0.005%
98	16.255	2486	2488	2491	rBV2	348	468	0.05%	0.006%
99	16.310	2495	2497	2499	rVB	320	195	0.02%	0.003%
100	16.743	2566	2568	2572	rBV3	233	321	0.03%	0.004%




Sum of corrected areas: 7274266

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
Data File : VX039344.D
Acq On : 19 Dec 2023 10:26
Operator : JC/MD
Sample : VX1219WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK652

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

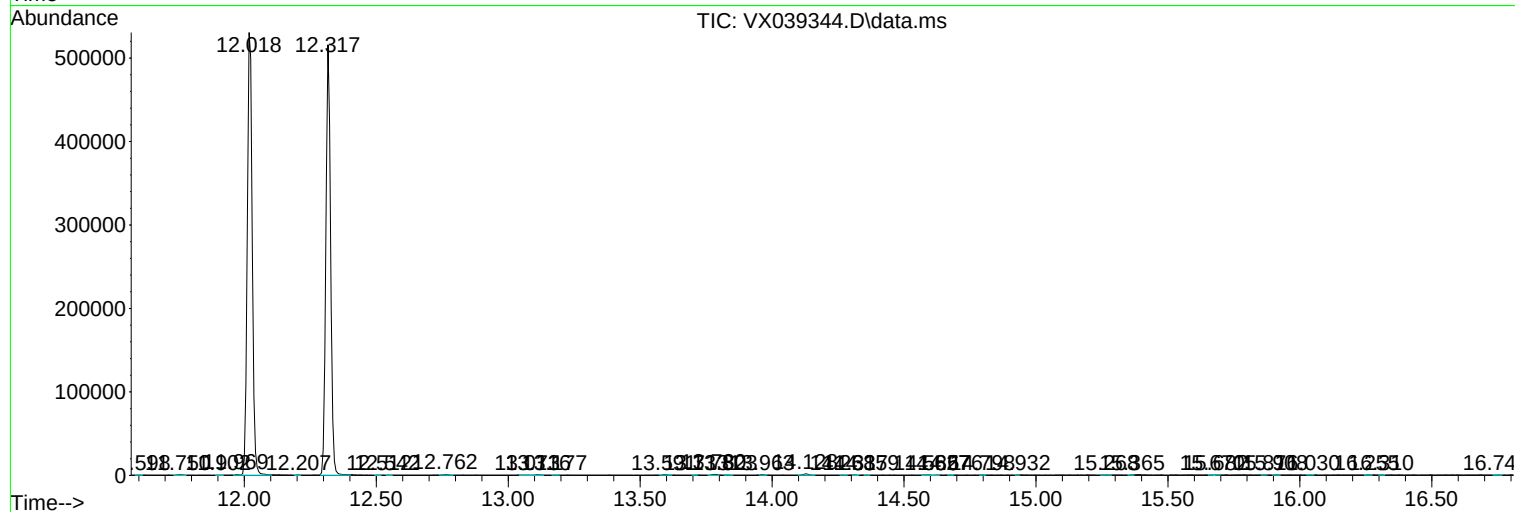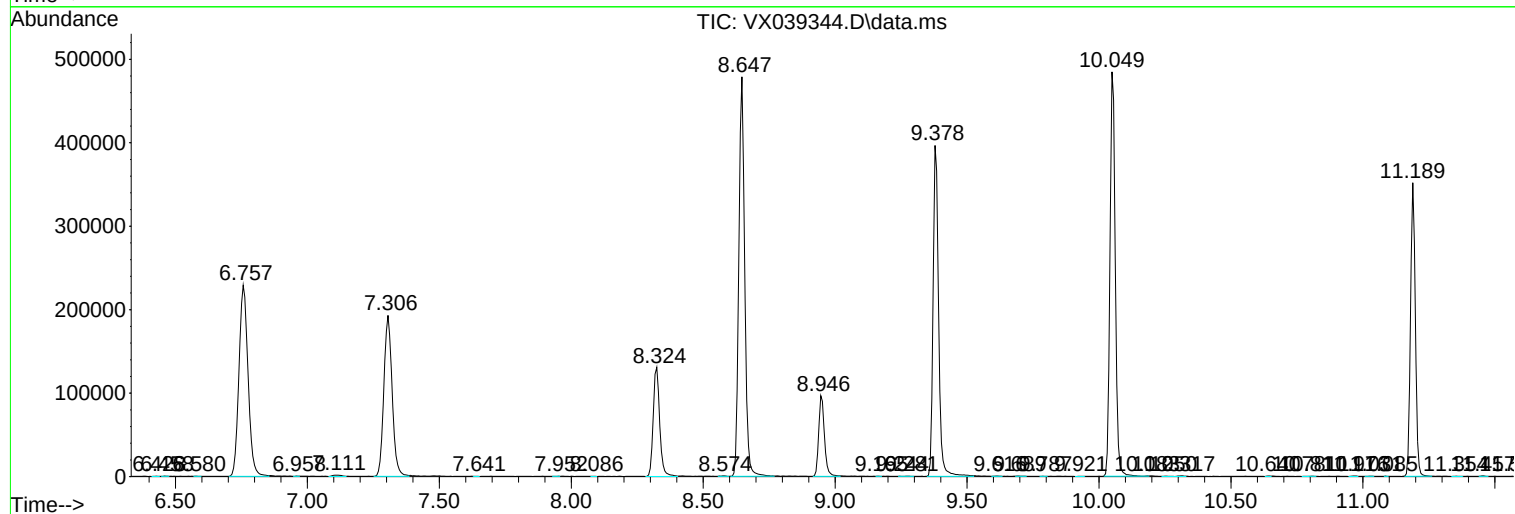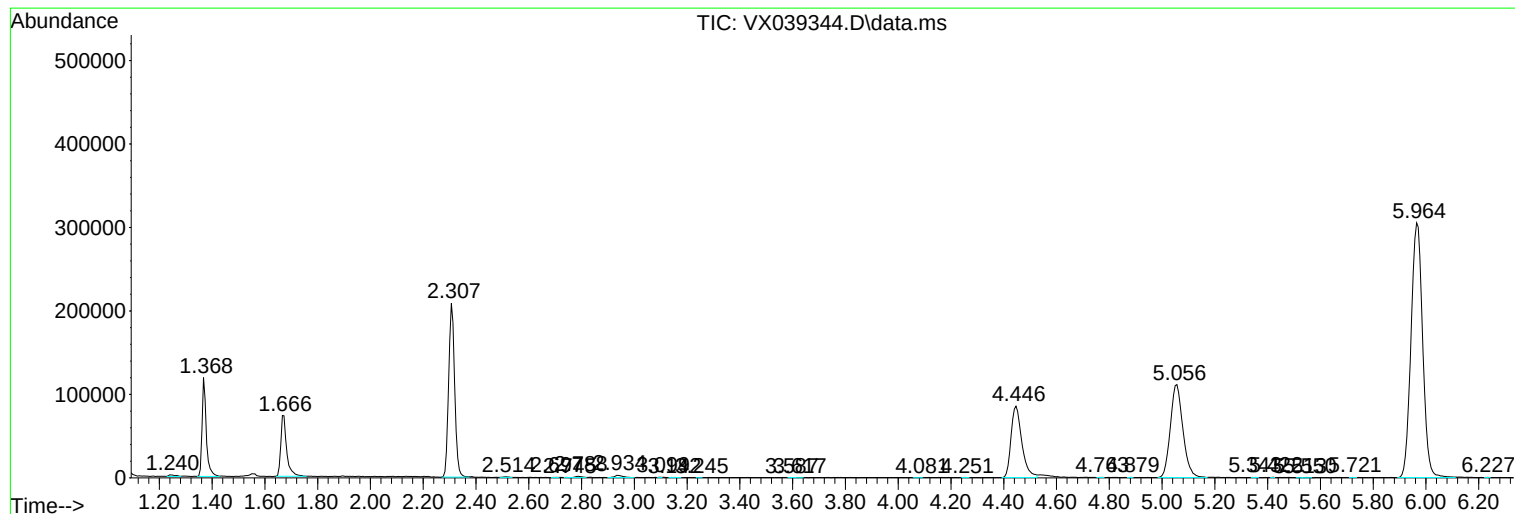

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
Data File : VX039344.D
Acq On : 19 Dec 2023 10:26
Operator : JC/MD
Sample : VX1219WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK652

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
Data File : VX039344.D
Acq On : 19 Dec 2023 10:26
Operator : JC/MD
Sample : VX1219WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK652

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc