

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
 Data File : VX039347.D
 Acq On : 19 Dec 2023 11:45
 Operator : JC/MD
 Sample : 05835-08 20X
 Misc : 5.27g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0AQ0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

Signal : TIC: VX039347.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	43	46	57	rVB	107931	120566	5.25%	1.446%
2	1.666	90	95	108	rVB	66098	99225	4.32%	1.190%
3	2.307	194	200	218	rVB	189366	296715	12.91%	3.559%
4	2.709	261	266	269	rBV3	515	710	0.03%	0.009%
5	2.794	274	280	283	rBV4	1407	2537	0.11%	0.030%
6	2.941	296	304	313	rBV2	5027	11484	0.50%	0.138%
7	3.093	327	329	331	rBV3	199	170	0.01%	0.002%
8	3.221	348	350	351	rBV	247	165	0.01%	0.002%
9	3.251	354	355	358	rVB2	200	163	0.01%	0.002%
10	3.343	367	370	371	rVV2	174	173	0.01%	0.002%
11	3.508	396	397	400	rBV2	190	242	0.01%	0.003%
12	3.898	459	461	464	rBV2	144	201	0.01%	0.002%
13	3.965	469	472	473	rBV2	198	204	0.01%	0.002%
14	4.166	504	505	509	rVB2	181	208	0.01%	0.002%
15	4.446	543	551	567	rBV	73697	213623	9.30%	2.562%
16	4.934	629	631	632	rBV	442	225	0.01%	0.003%
17	5.056	639	651	668	rBV2	100824	324064	14.10%	3.887%
18	5.208	674	676	678	rBV2	269	290	0.01%	0.003%
19	5.367	701	702	705	rBV2	344	421	0.02%	0.005%
20	5.513	725	726	730	rBV2	178	266	0.01%	0.003%
21	5.727	759	761	763	rBV	405	304	0.01%	0.004%
22	5.964	788	800	822	rBV2	276622	878378	38.23%	10.536%
23	6.251	845	847	849	rBV2	175	226	0.01%	0.003%
24	6.312	855	857	860	rBV2	162	180	0.01%	0.002%
25	6.391	868	870	874	rVV2	215	299	0.01%	0.004%
26	6.757	920	930	946	rBV	201393	488224	21.25%	5.856%
27	7.117	981	989	996	rVV4	1326	3246	0.14%	0.039%
28	7.306	1012	1020	1039	rBV	171101	379576	16.52%	4.553%
29	7.470	1045	1047	1048	rBV	405	275	0.01%	0.003%
30	7.489	1048	1050	1054	rVB2	598	492	0.02%	0.006%
31	7.586	1064	1066	1069	rVB2	238	225	0.01%	0.003%
32	7.702	1082	1085	1086	rBV	288	218	0.01%	0.003%
33	7.836	1103	1107	1109	rBV2	144	207	0.01%	0.002%
34	8.007	1134	1135	1138	rVB2	286	236	0.01%	0.003%
35	8.324	1181	1187	1201	rBV	116581	190827	8.30%	2.289%
36	8.501	1214	1216	1217	rBV	362	283	0.01%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
 Data File : VX039347.D
 Acq On : 19 Dec 2023 11:45
 Operator : JC/MD
 Sample : 05835-08 20X
 Misc : 5.27g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0AQ0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
 Title : VOC Analysis

37	8.568	1226	1227	1229	rBV	225	195	0.01%	0.002%
38	8.647	1234	1240	1251	rBV	423541	665876	28.98%	7.987%
39	8.854	1272	1274	1276	rBV2	270	192	0.01%	0.002%
40	8.952	1284	1290	1299	rBV	82072	125161	5.45%	1.501%
41	9.135	1315	1320	1323	rVB3	271	370	0.02%	0.004%
42	9.275	1339	1343	1347	rVB2	371	659	0.03%	0.008%
43	9.385	1355	1361	1376	rBV	341507	501288	21.82%	6.013%
44	9.634	1400	1402	1406	rVB	315	279	0.01%	0.003%
45	9.671	1406	1408	1410	rBV	207	162	0.01%	0.002%
46	9.702	1410	1413	1417	rVV	704	824	0.04%	0.010%
47	9.769	1420	1424	1427	rBV3	252	365	0.02%	0.004%
48	9.817	1430	1432	1435	rBV2	163	204	0.01%	0.002%
49	9.964	1453	1456	1458	rBV2	242	228	0.01%	0.003%
50	10.012	1461	1464	1465	rBV2	185	203	0.01%	0.002%
51	10.080	1465	1475	1491	rBV2	1198831	2297792	100.00%	27.561%
52	10.305	1509	1512	1519	rVB3	609	1105	0.05%	0.013%
53	10.360	1519	1521	1522	rBV	218	185	0.01%	0.002%
54	10.537	1549	1550	1552	rBV2	207	179	0.01%	0.002%
55	10.604	1559	1561	1563	rBV2	189	198	0.01%	0.002%
56	10.659	1565	1570	1571	rVV2	428	686	0.03%	0.008%
57	10.903	1608	1610	1613	rBV	224	221	0.01%	0.003%
58	10.970	1616	1621	1624	rVV3	444	567	0.02%	0.007%
59	11.092	1638	1641	1645	rBV2	453	515	0.02%	0.006%
60	11.189	1652	1657	1668	rBV	327255	401089	17.46%	4.811%
61	11.305	1674	1676	1682	rBV3	274	257	0.01%	0.003%
62	11.366	1682	1686	1691	rVB	5732	6985	0.30%	0.084%
63	11.457	1697	1701	1705	rBV2	2172	3102	0.13%	0.037%
64	11.756	1745	1750	1755	rBV3	530	875	0.04%	0.010%
65	11.841	1762	1764	1767	rVB2	246	249	0.01%	0.003%
66	11.969	1781	1785	1789	rBV	18224	22965	1.00%	0.275%
67	12.018	1789	1793	1804	rVB2	480026	700992	30.51%	8.408%
68	12.140	1811	1813	1816	rBV3	239	229	0.01%	0.003%
69	12.195	1820	1822	1826	rBV3	298	342	0.01%	0.004%
70	12.317	1837	1842	1853	rBV	449132	576612	25.09%	6.916%
71	12.530	1876	1877	1880	rBV	192	166	0.01%	0.002%
72	12.597	1885	1888	1891	rBV2	198	242	0.01%	0.003%
73	12.731	1908	1910	1911	rBV2	207	191	0.01%	0.002%
74	12.762	1912	1915	1919	rVB	983	985	0.04%	0.012%
75	12.908	1935	1939	1942	rBV	198	308	0.01%	0.004%
76	12.994	1950	1953	1955	rVV2	170	208	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
 Data File : VX039347.D
 Acq On : 19 Dec 2023 11:45
 Operator : JC/MD
 Sample : 05835-08 20X
 Misc : 5.27g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0AQ0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
 Title : VOC Analysis

77	13.012	1955	1956	1959	rVB	227	185	0.01%	0.002%
78	13.122	1971	1974	1976	rVB2	368	347	0.02%	0.004%
79	13.353	2010	2012	2014	rBV	253	223	0.01%	0.003%
80	13.396	2018	2019	2023	rVB	259	209	0.01%	0.003%
81	13.500	2034	2036	2038	rBV	220	194	0.01%	0.002%
82	13.597	2049	2052	2055	rVB2	652	702	0.03%	0.008%
83	13.664	2060	2063	2064	rBV2	191	197	0.01%	0.002%
84	13.786	2080	2083	2085	rBV2	389	430	0.02%	0.005%
85	13.896	2098	2101	2105	rVB2	223	369	0.02%	0.004%
86	13.969	2111	2113	2115	rBV2	398	334	0.01%	0.004%
87	14.054	2125	2127	2128	rBV	258	166	0.01%	0.002%
88	14.128	2135	2139	2142	rVV2	1151	1658	0.07%	0.020%
89	14.158	2142	2144	2146	rVV2	246	183	0.01%	0.002%
90	14.567	2210	2211	2212	rBV	331	184	0.01%	0.002%
91	14.829	2253	2254	2257	rBV2	235	192	0.01%	0.002%
92	14.963	2274	2276	2278	rBV2	210	196	0.01%	0.002%
93	15.030	2285	2287	2289	rVB2	265	199	0.01%	0.002%
94	15.127	2297	2303	2304	rBV3	293	584	0.03%	0.007%
95	15.207	2312	2316	2317	rBV3	259	377	0.02%	0.005%
96	15.371	2341	2343	2344	rBV	287	215	0.01%	0.003%
97	15.383	2344	2345	2351	rVB2	560	820	0.04%	0.010%
98	15.572	2375	2376	2378	rVB	452	214	0.01%	0.003%
99	16.042	2450	2453	2456	rBV2	224	335	0.01%	0.004%
100	16.682	2556	2558	2560	rBV2	296	352	0.02%	0.004%




Sum of corrected areas: 8336964

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
Data File : VX039347.D
Acq On : 19 Dec 2023 11:45
Operator : JC/MD
Sample : 05835-08 20X
Misc : 5.27g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0AQ0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

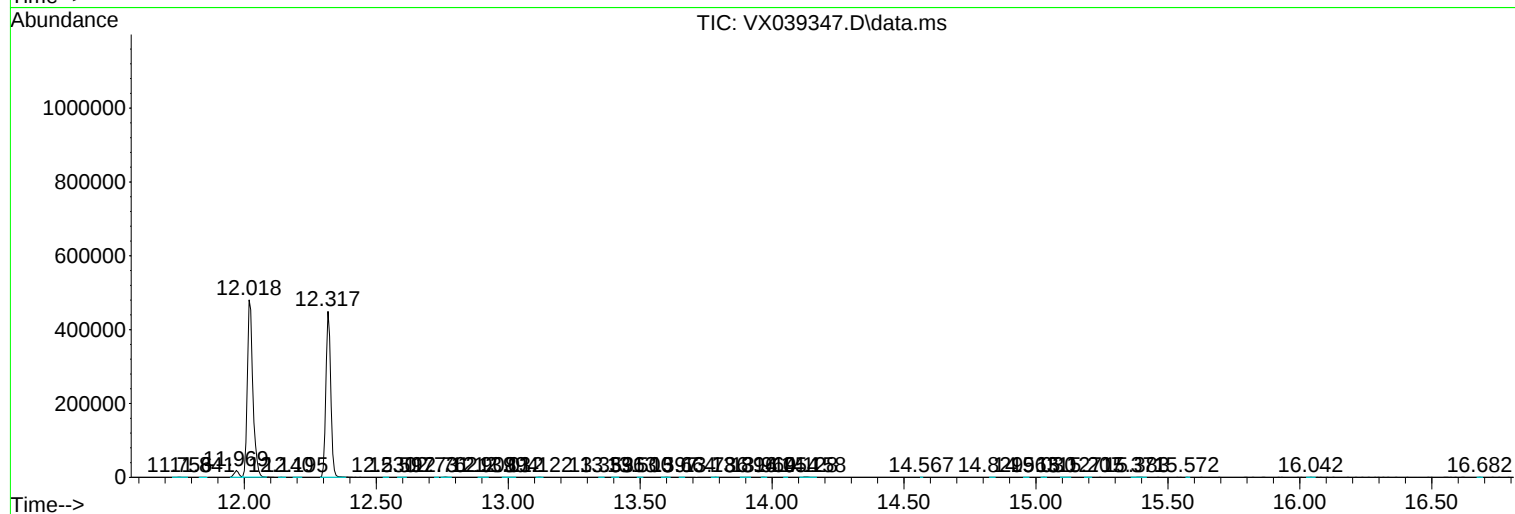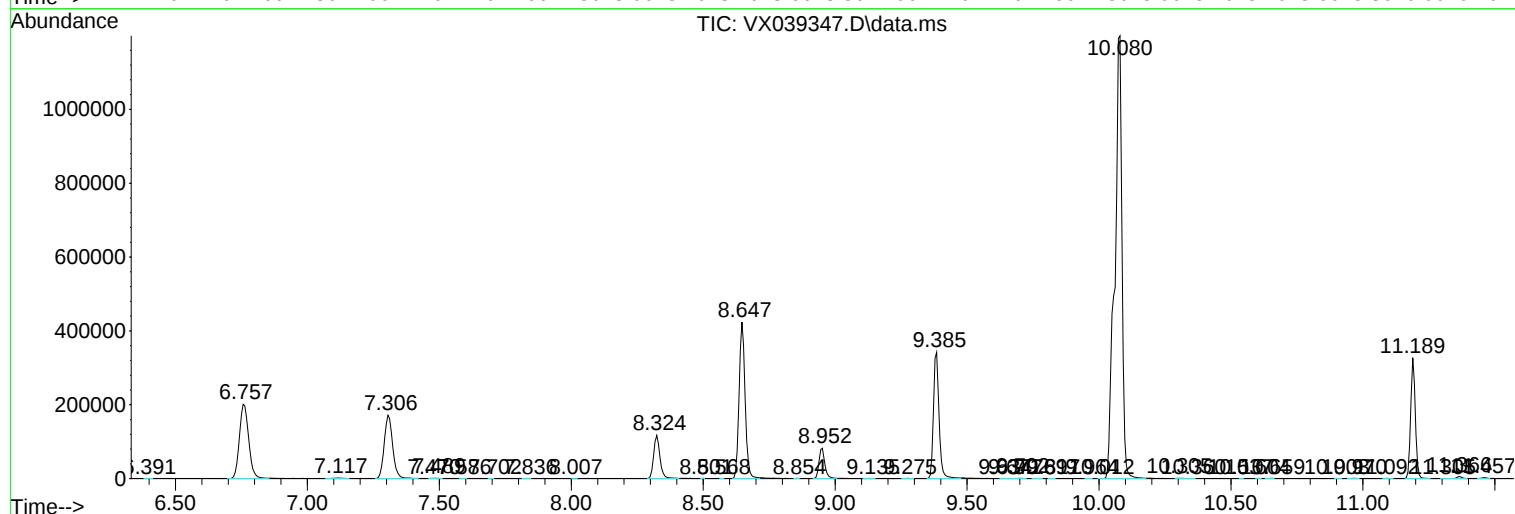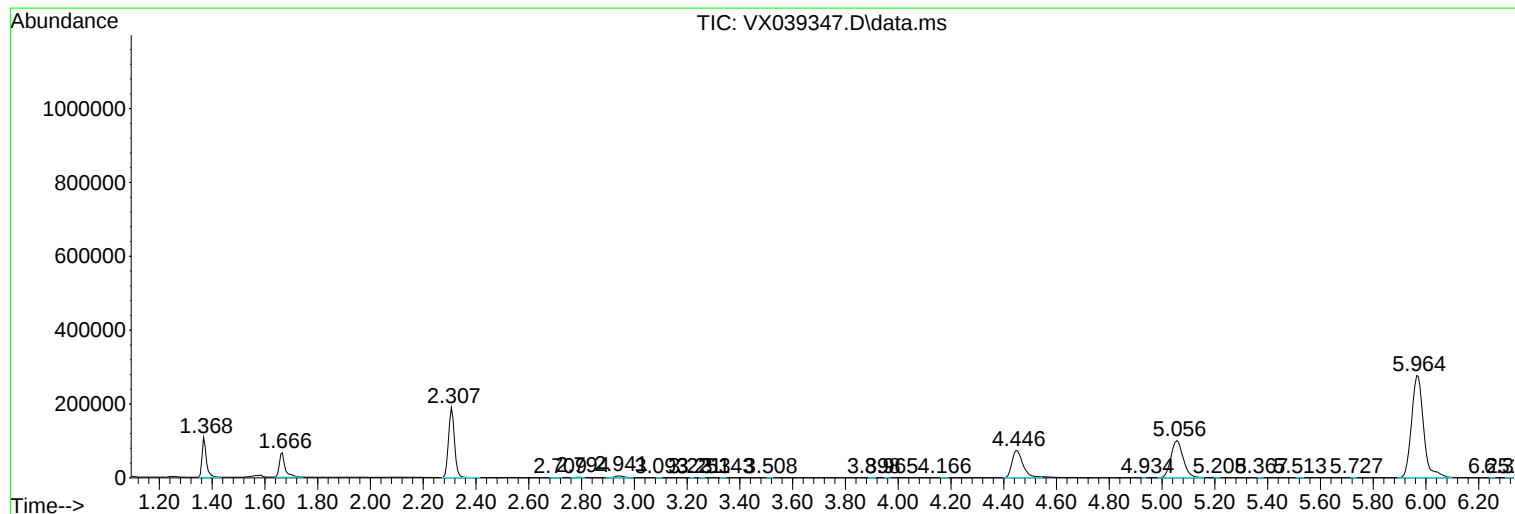

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
Data File : VX039347.D
Acq On : 19 Dec 2023 11:45
Operator : JC/MD
Sample : 05835-08 20X
Misc : 5.27g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0AQ0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
Data File : VX039347.D
Acq On : 19 Dec 2023 11:45
Operator : JC/MD
Sample : 05835-08 20X
Misc : 5.27g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0AQ0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc