

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
 Data File : VX039350.D
 Acq On : 19 Dec 2023 12:54
 Operator : JC/MD
 Sample : 05835-10 10X
 Misc : 3.22g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0AQ7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

Signal : TIC: VX039350.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	57	rBV	106641	117167	13.96%	1.810%
2	1.660	90	94	100	rBV	65521	86933	10.36%	1.343%
3	2.307	194	200	209	rBV	186689	296094	35.28%	4.573%
4	2.544	238	239	243	rVB3	429	321	0.04%	0.005%
5	2.703	260	265	270	rVB3	974	1807	0.22%	0.028%
6	2.782	275	278	285	rVB2	1347	2569	0.31%	0.040%
7	2.941	297	304	314	rVB	5892	13221	1.58%	0.204%
8	3.483	389	393	396	rBV2	207	197	0.02%	0.003%
9	3.526	399	400	403	rBV2	246	265	0.03%	0.004%
10	3.599	411	412	415	rBV2	251	224	0.03%	0.003%
11	3.733	433	434	437	rBV2	217	214	0.03%	0.003%
12	3.861	453	455	458	rVB2	222	222	0.03%	0.003%
13	3.922	463	465	468	rBV	251	262	0.03%	0.004%
14	4.446	541	551	569	rBV	69849	206966	24.66%	3.197%
15	4.904	625	626	630	rBV2	192	231	0.03%	0.004%
16	4.946	630	633	635	rBV	273	264	0.03%	0.004%
17	5.056	639	651	669	rBV	102073	324473	38.66%	5.011%
18	5.257	681	684	688	rVB3	284	359	0.04%	0.006%
19	5.373	702	703	706	rBV	249	225	0.03%	0.003%
20	5.471	717	719	720	rVB	354	225	0.03%	0.003%
21	5.568	733	735	738	rBV	170	204	0.02%	0.003%
22	5.629	742	745	747	rBV2	174	216	0.03%	0.003%
23	5.678	752	753	758	rVB2	291	314	0.04%	0.005%
24	5.751	762	765	767	rBV	221	210	0.03%	0.003%
25	5.885	784	787	788	rBV2	229	213	0.03%	0.003%
26	5.971	789	801	821	rBV2	275177	839314	100.00%	12.963%
27	6.190	835	837	840	rBV2	230	299	0.04%	0.005%
28	6.556	893	897	898	rBV2	326	438	0.05%	0.007%
29	6.586	900	902	906	rVB	280	246	0.03%	0.004%
30	6.623	906	908	914	rBV2	186	330	0.04%	0.005%
31	6.672	914	916	920	rVB	231	265	0.03%	0.004%
32	6.757	922	930	942	rBV	200041	479463	57.13%	7.405%
33	7.117	983	989	995	rBV4	1490	2879	0.34%	0.044%
34	7.306	1012	1020	1037	rBV	169235	375190	44.70%	5.795%
35	7.422	1037	1039	1040	rVV	552	376	0.04%	0.006%
36	7.446	1040	1043	1045	rVV2	354	439	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
 Data File : VX039350.D
 Acq On : 19 Dec 2023 12:54
 Operator : JC/MD
 Sample : 05835-10 10X
 Misc : 3.22g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0AQ7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

37	7.495	1047	1051	1055	rVV3	769	1159	0.14%	0.018%
38	7.763	1093	1095	1096	rBV	194	205	0.02%	0.003%
39	8.117	1151	1153	1156	rVB2	277	300	0.04%	0.005%
40	8.165	1159	1161	1166	rVV2	196	308	0.04%	0.005%
41	8.324	1181	1187	1200	rBV	113832	188971	22.51%	2.919%
42	8.507	1215	1217	1220	rBV	476	566	0.07%	0.009%
43	8.568	1225	1227	1229	rBV2	394	305	0.04%	0.005%
44	8.586	1229	1230	1234	rBV2	307	274	0.03%	0.004%
45	8.647	1234	1240	1253	rBV	418233	658782	78.49%	10.175%
46	8.952	1284	1290	1308	rBV	79944	124207	14.80%	1.918%
47	9.190	1325	1329	1331	rVB2	260	306	0.04%	0.005%
48	9.220	1331	1334	1336	rBV2	226	225	0.03%	0.003%
49	9.269	1340	1342	1345	rBV3	256	215	0.03%	0.003%
50	9.385	1355	1361	1376	rBV	332782	483696	57.63%	7.471%
51	9.567	1389	1391	1396	rVB3	513	707	0.08%	0.011%
52	9.702	1410	1413	1416	rVB2	340	394	0.05%	0.006%
53	10.055	1465	1471	1473	rBV	427767	653172	77.82%	10.088%
54	10.311	1511	1513	1516	rVB2	516	492	0.06%	0.008%
55	10.415	1528	1530	1531	rBV	237	207	0.02%	0.003%
56	10.500	1541	1544	1548	rVB	291	408	0.05%	0.006%
57	10.640	1566	1567	1571	rBV	211	288	0.03%	0.004%
58	10.695	1575	1576	1582	rVB2	223	267	0.03%	0.004%
59	10.823	1593	1597	1598	rBV	300	323	0.04%	0.005%
60	10.970	1619	1621	1623	rBV2	402	465	0.06%	0.007%
61	11.092	1638	1641	1645	rBV3	335	554	0.07%	0.009%
62	11.189	1652	1657	1670	rBV	314143	396910	47.29%	6.130%
63	11.317	1676	1678	1683	rBV2	279	374	0.04%	0.006%
64	11.372	1683	1687	1689	rVB3	221	304	0.04%	0.005%
65	11.457	1697	1701	1704	rBV3	407	607	0.07%	0.009%
66	11.659	1731	1734	1735	rBV	202	218	0.03%	0.003%
67	11.677	1735	1737	1740	rVV	266	238	0.03%	0.004%
68	11.750	1748	1749	1756	rVB3	314	554	0.07%	0.009%
69	11.970	1782	1785	1788	rVV2	807	830	0.10%	0.013%
70	12.018	1788	1793	1807	rBV	458865	617446	73.57%	9.536%
71	12.317	1836	1842	1853	rBV	444819	576699	68.71%	8.907%
72	12.463	1865	1866	1870	rBV2	276	267	0.03%	0.004%
73	12.512	1870	1874	1877	rBV3	199	387	0.05%	0.006%
74	12.762	1911	1915	1920	rBV2	597	914	0.11%	0.014%
75	12.829	1922	1926	1928	rVB	241	309	0.04%	0.005%
76	12.908	1935	1939	1943	rBV2	199	303	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
 Data File : VX039350.D
 Acq On : 19 Dec 2023 12:54
 Operator : JC/MD
 Sample : 05835-10 10X
 Misc : 3.22g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0AQ7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

77	13.244	1991	1994	1997	rBV2	254	375	0.04%	0.006%
78	13.652	2058	2061	2062	rBV	299	287	0.03%	0.004%
79	13.695	2066	2068	2070	rBV	234	231	0.03%	0.004%
80	13.780	2080	2082	2083	rBV	426	248	0.03%	0.004%
81	13.890	2096	2100	2102	rBV	185	226	0.03%	0.003%
82	13.969	2109	2113	2115	rVB2	422	496	0.06%	0.008%
83	14.054	2123	2127	2128	rBV2	235	302	0.04%	0.005%
84	14.128	2135	2139	2144	rVB	1645	2203	0.26%	0.034%
85	14.323	2168	2171	2172	rBV2	171	217	0.03%	0.003%
86	14.469	2194	2195	2197	rBV	373	233	0.03%	0.004%
87	14.682	2226	2230	2231	rBV	346	347	0.04%	0.005%
88	14.792	2246	2248	2250	rBV	390	336	0.04%	0.005%
89	14.932	2268	2271	2272	rBV2	182	217	0.03%	0.003%
90	15.085	2294	2296	2299	rBV3	243	266	0.03%	0.004%
91	15.432	2351	2353	2356	rBV2	230	218	0.03%	0.003%
92	15.463	2356	2358	2362	rBV2	261	297	0.04%	0.005%
93	15.676	2392	2393	2396	rVB2	413	331	0.04%	0.005%
94	15.707	2396	2398	2402	rBV2	251	334	0.04%	0.005%
95	16.072	2455	2458	2459	rBV2	349	386	0.05%	0.006%
96	16.115	2464	2465	2468	rVV	489	314	0.04%	0.005%
97	16.146	2468	2470	2472	rVV2	255	235	0.03%	0.004%
98	16.213	2479	2481	2483	rBV2	264	243	0.03%	0.004%
99	16.304	2495	2496	2499	rBV2	316	330	0.04%	0.005%
100	16.444	2517	2519	2521	rBV2	266	208	0.02%	0.003%




Sum of corrected areas: 6474671

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
Data File : VX039350.D
Acq On : 19 Dec 2023 12:54
Operator : JC/MD
Sample : 05835-10 10X
Misc : 3.22g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0AQ7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

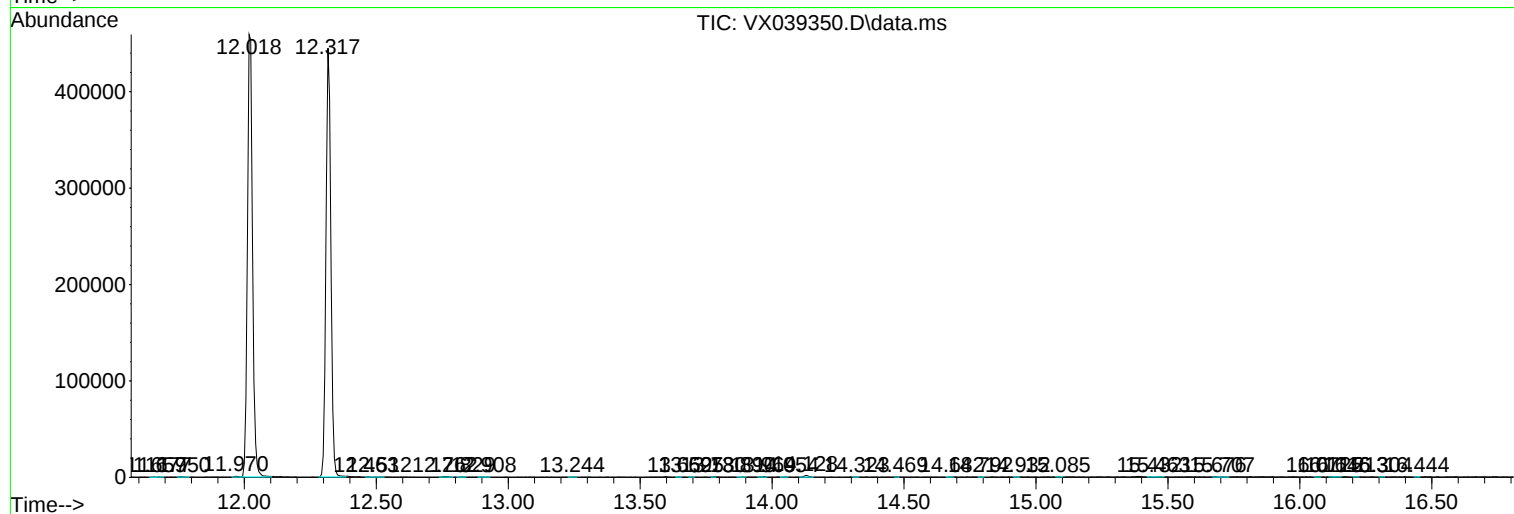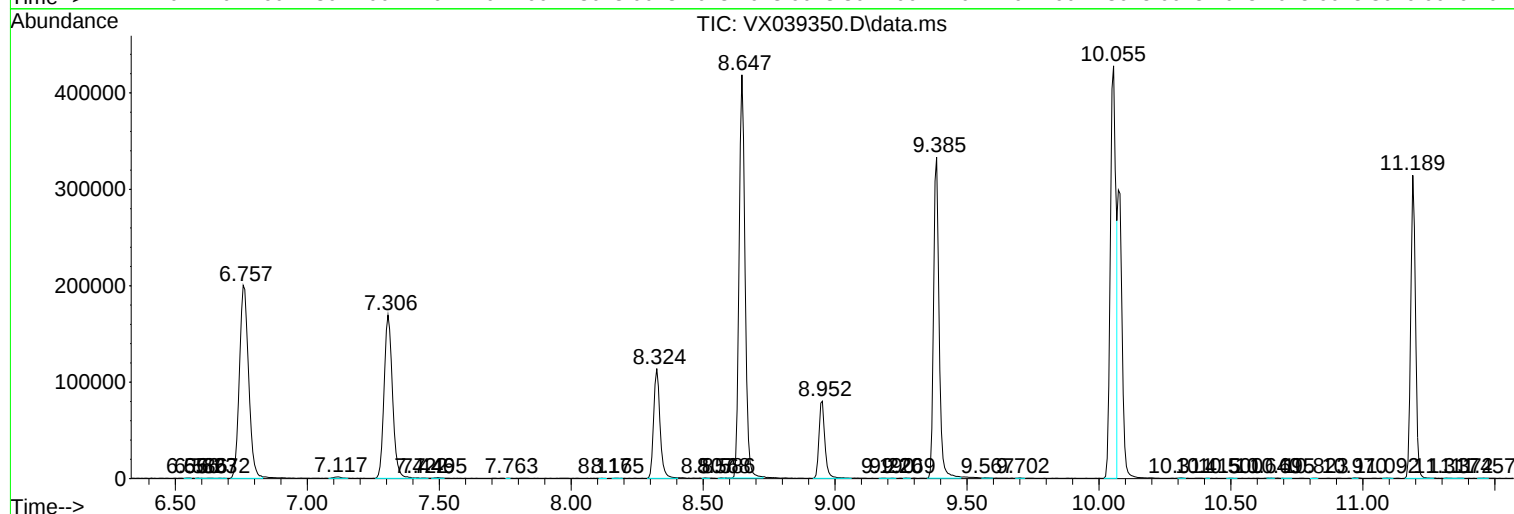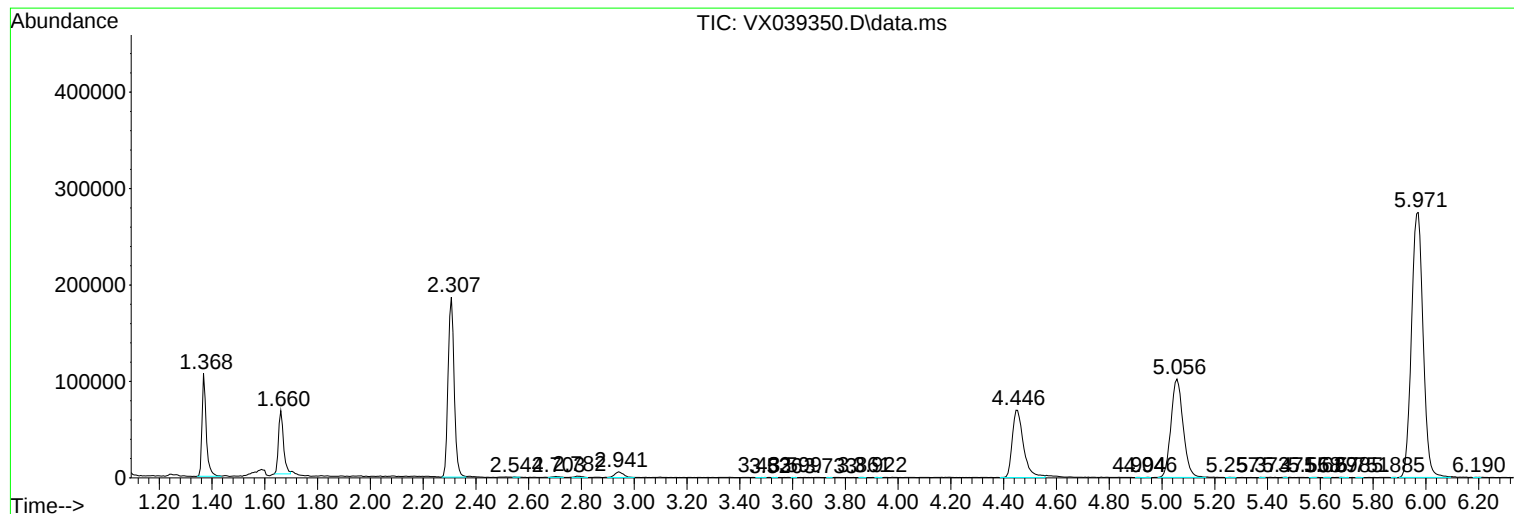

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
Data File : VX039350.D
Acq On : 19 Dec 2023 12:54
Operator : JC/MD
Sample : 05835-10 10X
Misc : 3.22g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0AQ7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
Data File : VX039350.D
Acq On : 19 Dec 2023 12:54
Operator : JC/MD
Sample : 05835-10 10X
Misc : 3.22g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0AQ7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc