

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
 Data File : VX039351.D
 Acq On : 19 Dec 2023 13:16
 Operator : JC/MD
 Sample : 05835-13
 Misc : 2.05g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0AR0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M

Title : VOC Analysis

Signal : TIC: VX039351.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	43	46	58	rBV	79861	118169	3.47%	1.284%
2	1.648	86	92	103	rBV2	32442	73086	2.15%	0.794%
3	2.288	191	197	209	rVB	182444	285994	8.41%	3.107%
4	2.398	210	215	223	rBV3	4929	11424	0.34%	0.124%
5	2.709	261	266	274	rBV	12594	25546	0.75%	0.278%
6	2.843	285	288	295	rVB6	1153	2233	0.07%	0.024%
7	2.941	297	304	314	rBV	5784	13741	0.40%	0.149%
8	3.203	346	347	351	rVB	326	307	0.01%	0.003%
9	3.239	351	353	356	rBV	194	200	0.01%	0.002%
10	3.410	379	381	384	rVV3	204	241	0.01%	0.003%
11	3.526	398	400	403	rVB	311	253	0.01%	0.003%
12	3.800	442	445	449	rBV	324	414	0.01%	0.004%
13	3.855	452	454	458	rVV2	245	222	0.01%	0.002%
14	3.995	474	477	478	rBV2	253	250	0.01%	0.003%
15	4.081	487	491	492	rBV	480	341	0.01%	0.004%
16	4.245	516	518	519	rBV2	399	375	0.01%	0.004%
17	4.367	535	538	540	rBV2	201	186	0.01%	0.002%
18	4.477	547	556	584	rBV2	46259	203704	5.99%	2.213%
19	5.056	639	651	673	rBV	96336	319041	9.38%	3.466%
20	5.269	685	686	689	rBV2	197	191	0.01%	0.002%
21	5.306	689	692	693	rVV	287	228	0.01%	0.002%
22	5.404	702	708	712	rVB4	356	661	0.02%	0.007%
23	5.458	715	717	723	rVB2	569	720	0.02%	0.008%
24	5.806	771	774	777	rBV2	179	266	0.01%	0.003%
25	5.964	787	800	824	rBV2	288525	833897	24.51%	9.059%
26	6.458	880	881	885	rBV2	229	234	0.01%	0.003%
27	6.544	893	895	896	rVB	339	178	0.01%	0.002%
28	6.757	921	930	944	rBV	192621	474045	13.94%	5.150%
29	6.995	968	969	971	rBV2	363	184	0.01%	0.002%
30	7.013	971	972	974	rBV2	282	188	0.01%	0.002%
31	7.117	983	989	996	rVB5	1215	2932	0.09%	0.032%
32	7.220	1003	1006	1007	rBV2	293	187	0.01%	0.002%
33	7.306	1011	1020	1038	rBV	167266	381249	11.21%	4.142%
34	7.470	1046	1047	1048	rBV	340	223	0.01%	0.002%
35	7.604	1066	1069	1070	rBV	233	270	0.01%	0.003%
36	7.702	1082	1085	1088	rVB2	208	226	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
 Data File : VX039351.D
 Acq On : 19 Dec 2023 13:16
 Operator : JC/MD
 Sample : 05835-13
 Misc : 2.05g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0AR0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
 Title : VOC Analysis

37	7.964	1122	1128	1138	rBV5	5151	12806	0.38%	0.139%
38	8.232	1169	1172	1173	rBV	171	208	0.01%	0.002%
39	8.324	1181	1187	1200	rBV	107735	183289	5.39%	1.991%
40	8.494	1214	1215	1216	rBV	325	215	0.01%	0.002%
41	8.580	1226	1229	1231	rBV3	227	231	0.01%	0.003%
42	8.598	1231	1232	1234	rBV2	316	240	0.01%	0.003%
43	8.647	1234	1240	1252	rBV	401196	655777	19.28%	7.124%
44	8.952	1284	1290	1302	rBV	75309	122315	3.60%	1.329%
45	9.244	1336	1338	1340	rBV	185	215	0.01%	0.002%
46	9.275	1340	1343	1346	rVV2	481	639	0.02%	0.007%
47	9.397	1357	1363	1383	rBV	267911	465212	13.68%	5.054%
48	9.635	1400	1402	1405	rVB2	248	248	0.01%	0.003%
49	9.720	1413	1416	1421	rVB6	747	1309	0.04%	0.014%
50	9.763	1421	1423	1425	rBV	324	219	0.01%	0.002%
51	9.988	1458	1460	1462	rVB2	299	222	0.01%	0.002%
52	10.080	1465	1475	1492	rBV2	2003794	3401719	100.00%	36.955%
53	10.573	1553	1556	1558	rVB2	171	185	0.01%	0.002%
54	10.726	1578	1581	1583	rBV2	210	232	0.01%	0.003%
55	10.756	1583	1586	1590	rVV2	182	272	0.01%	0.003%
56	10.878	1605	1606	1608	rBV2	235	212	0.01%	0.002%
57	10.957	1615	1619	1627	rBV	15635	22182	0.65%	0.241%
58	11.092	1638	1641	1642	rBV2	278	305	0.01%	0.003%
59	11.195	1652	1658	1665	rBV	300699	382743	11.25%	4.158%
60	11.451	1698	1700	1704	rBV3	471	588	0.02%	0.006%
61	11.488	1704	1706	1708	rBV2	371	346	0.01%	0.004%
62	11.561	1716	1718	1721	rBV2	218	241	0.01%	0.003%
63	11.610	1724	1726	1729	rVV2	192	213	0.01%	0.002%
64	11.695	1738	1740	1743	rVB	213	254	0.01%	0.003%
65	11.720	1743	1744	1747	rBV	206	214	0.01%	0.002%
66	11.762	1747	1751	1760	rVB4	913	2236	0.07%	0.024%
67	11.860	1765	1767	1769	rBV	314	306	0.01%	0.003%
68	11.976	1781	1786	1788	rBV2	3393	4173	0.12%	0.045%
69	12.024	1789	1794	1810	rVB	469101	612942	18.02%	6.659%
70	12.171	1815	1818	1823	rBV2	253	372	0.01%	0.004%
71	12.232	1825	1828	1830	rBV3	831	1045	0.03%	0.011%
72	12.317	1837	1842	1852	rBV	426723	566457	16.65%	6.154%
73	12.683	1900	1902	1905	rBV2	170	192	0.01%	0.002%
74	12.762	1910	1915	1920	rVB3	861	1364	0.04%	0.015%
75	12.872	1930	1933	1934	rBV2	616	542	0.02%	0.006%
76	13.597	2049	2052	2054	rVB3	376	473	0.01%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
 Data File : VX039351.D
 Acq On : 19 Dec 2023 13:16
 Operator : JC/MD
 Sample : 05835-13
 Misc : 2.05g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0AR0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

77	13.719	2070	2072	2075	rBV2	191	203	0.01%	0.002%
78	13.786	2080	2083	2084	rBV	510	512	0.02%	0.006%
79	13.884	2097	2099	2102	rVV2	304	279	0.01%	0.003%
80	13.914	2103	2104	2110	rVB2	211	222	0.01%	0.002%
81	13.963	2110	2112	2117	rBV3	404	498	0.01%	0.005%
82	14.030	2120	2123	2126	rVV2	159	192	0.01%	0.002%
83	14.128	2134	2139	2145	rVB	2428	3109	0.09%	0.034%
84	14.341	2171	2174	2177	rBV2	237	305	0.01%	0.003%
85	14.597	2213	2216	2217	rBV	214	186	0.01%	0.002%
86	14.762	2241	2243	2245	rBV3	196	208	0.01%	0.002%
87	14.847	2256	2257	2260	rBV2	275	264	0.01%	0.003%
88	15.152	2305	2307	2309	rVB2	222	199	0.01%	0.002%
89	15.176	2309	2311	2313	rBV2	204	264	0.01%	0.003%
90	15.262	2324	2325	2328	rBV2	321	322	0.01%	0.003%
91	15.304	2330	2332	2335	rVV2	287	356	0.01%	0.004%
92	15.384	2342	2345	2352	rVB3	710	1315	0.04%	0.014%
93	15.463	2356	2358	2360	rBV2	275	260	0.01%	0.003%
94	15.621	2381	2384	2386	rBV2	226	222	0.01%	0.002%
95	15.694	2394	2396	2400	rVV2	245	309	0.01%	0.003%
96	15.847	2419	2421	2423	rVB2	279	190	0.01%	0.002%
97	15.902	2428	2430	2431	rBV2	352	277	0.01%	0.003%
98	16.426	2514	2516	2519	rBV2	267	338	0.01%	0.004%
99	16.591	2542	2543	2546	rVB2	261	202	0.01%	0.002%
100	16.743	2566	2568	2569	rVB	544	227	0.01%	0.002%


Sum of corrected areas: 9205018

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
Data File : VX039351.D
Acq On : 19 Dec 2023 13:16
Operator : JC/MD
Sample : 05835-13
Misc : 2.05g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0AR0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

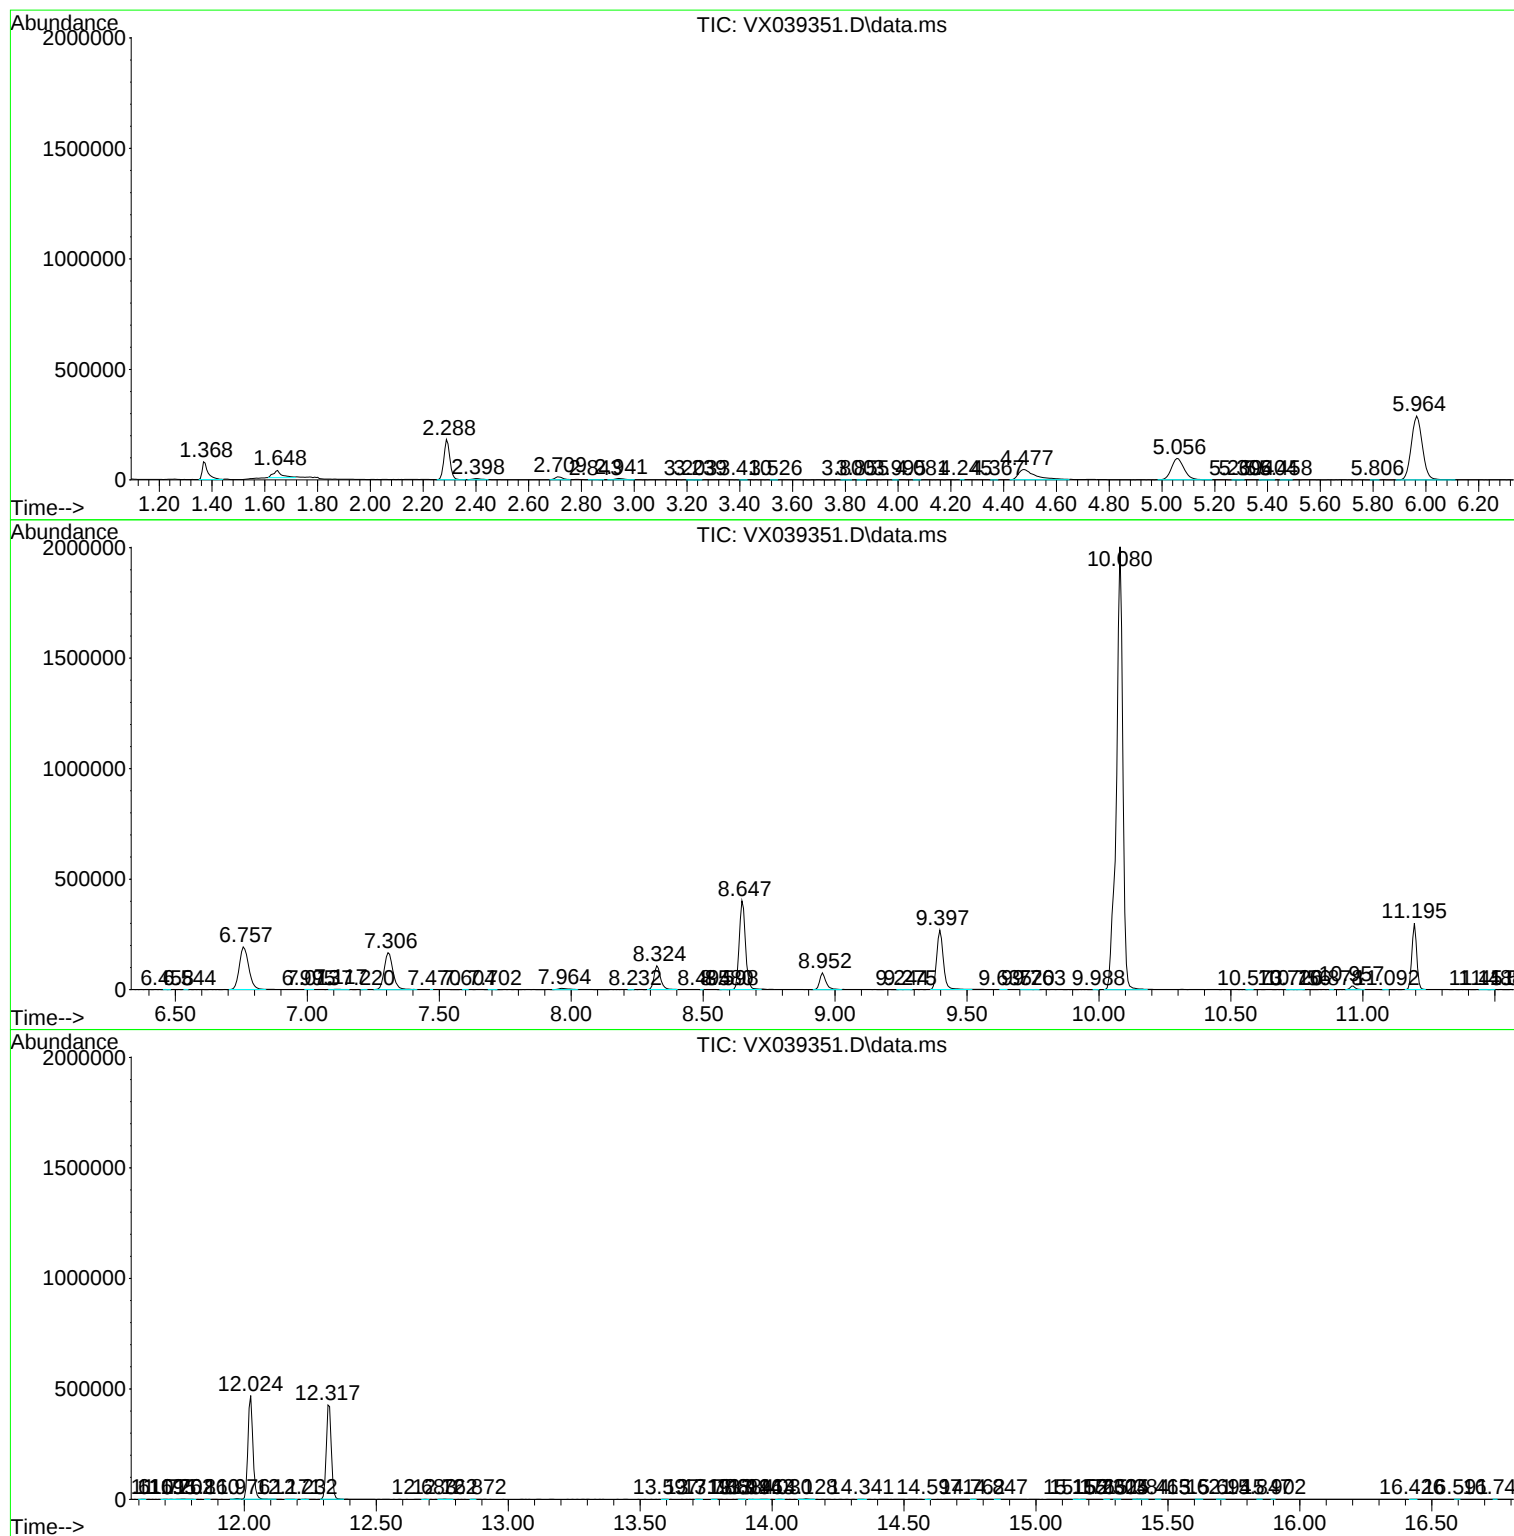

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
Data File : VX039351.D
Acq On : 19 Dec 2023 13:16
Operator : JC/MD
Sample : 05835-13
Misc : 2.05g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0AR0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
Data File : VX039351.D
Acq On : 19 Dec 2023 13:16
Operator : JC/MD
Sample : 05835-13
Misc : 2.05g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0AR0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc