

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
 Data File : VX039354.D
 Acq On : 19 Dec 2023 14:25
 Operator : JC/MD
 Sample : VIBLK626
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK626

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

Signal : TIC: VX039354.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	43	46	58	rVB	99200	108984	13.26%	1.720%
2	1.673	91	96	110	rVB	66197	99064	12.06%	1.563%
3	2.307	194	200	211	rVB	180280	282222	34.34%	4.453%
4	2.526	231	236	238	rBV4	492	800	0.10%	0.013%
5	2.630	251	253	254	rVB	290	193	0.02%	0.003%
6	2.648	254	256	258	rBV2	277	292	0.04%	0.005%
7	2.788	275	279	285	rVB4	2005	3990	0.49%	0.063%
8	2.837	285	287	289	rBV	279	243	0.03%	0.004%
9	2.941	298	304	311	rVV2	2505	5522	0.67%	0.087%
10	3.166	338	341	342	rBV2	165	191	0.02%	0.003%
11	3.251	354	355	359	rVB2	350	249	0.03%	0.004%
12	3.556	403	405	407	rVB	277	191	0.02%	0.003%
13	3.587	407	410	413	rBV2	244	250	0.03%	0.004%
14	3.629	415	417	420	rBV2	200	196	0.02%	0.003%
15	3.892	458	460	463	rVB	275	198	0.02%	0.003%
16	4.081	489	491	494	rVB	298	203	0.02%	0.003%
17	4.160	501	504	505	rBV2	200	211	0.03%	0.003%
18	4.190	505	509	510	rBV2	142	187	0.02%	0.003%
19	4.446	543	551	566	rBV	72577	211378	25.72%	3.335%
20	4.891	621	624	628	rVB	263	335	0.04%	0.005%
21	4.934	628	631	634	rBV2	185	288	0.04%	0.005%
22	5.056	638	651	670	rBV2	99700	323032	39.31%	5.097%
23	5.227	677	679	680	rVB	358	239	0.03%	0.004%
24	5.355	698	700	703	rBV2	197	305	0.04%	0.005%
25	5.477	717	720	725	rVB2	343	440	0.05%	0.007%
26	5.617	742	743	745	rBV	275	200	0.02%	0.003%
27	5.696	754	756	759	rVB2	170	197	0.02%	0.003%
28	5.971	787	801	819	rBV2	271672	821744	100.00%	12.966%
29	6.190	836	837	840	rBV	327	269	0.03%	0.004%
30	6.385	863	869	870	rBV	221	340	0.04%	0.005%
31	6.440	875	878	879	rBV	295	232	0.03%	0.004%
32	6.623	905	908	911	rBV2	255	342	0.04%	0.005%
33	6.763	921	931	952	rBV	197335	479645	58.37%	7.568%
34	6.952	960	962	964	rVB	399	199	0.02%	0.003%
35	7.117	985	989	995	rVB5	1192	2417	0.29%	0.038%
36	7.306	1011	1020	1034	rBV	166261	369246	44.93%	5.826%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
 Data File : VX039354.D
 Acq On : 19 Dec 2023 14:25
 Operator : JC/MD
 Sample : VIBLK626
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK626

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

37	7.464	1044	1046	1047	rBV	290	229	0.03%	0.004%
38	7.635	1072	1074	1077	rVB2	210	198	0.02%	0.003%
39	8.104	1149	1151	1155	rVB2	217	191	0.02%	0.003%
40	8.165	1158	1161	1163	rVB2	221	216	0.03%	0.003%
41	8.269	1175	1178	1181	rBV	197	277	0.03%	0.004%
42	8.324	1181	1187	1202	rVV	116277	188698	22.96%	2.977%
43	8.574	1225	1228	1233	rBV2	320	538	0.07%	0.008%
44	8.647	1233	1240	1253	rBV	401311	646109	78.63%	10.195%
45	8.952	1284	1290	1299	rBV	79099	122910	14.96%	1.939%
46	9.202	1328	1331	1332	rBV2	205	210	0.03%	0.003%
47	9.275	1341	1343	1346	rVB2	560	547	0.07%	0.009%
48	9.385	1355	1361	1375	rBV	332563	491802	59.85%	7.760%
49	9.604	1396	1397	1401	rVB2	404	357	0.04%	0.006%
50	9.695	1410	1412	1416	rBV4	461	450	0.05%	0.007%
51	9.848	1434	1437	1438	rBV	267	292	0.04%	0.005%
52	9.939	1449	1452	1453	rBV	239	196	0.02%	0.003%
53	9.994	1459	1461	1465	rVB	246	237	0.03%	0.004%
54	10.055	1465	1471	1481	rBV	413700	597486	72.71%	9.428%
55	10.305	1510	1512	1518	rVB3	528	567	0.07%	0.009%
56	10.397	1522	1527	1529	rBV	208	312	0.04%	0.005%
57	10.647	1565	1568	1572	rVV2	522	629	0.08%	0.010%
58	10.677	1572	1573	1576	rVV2	237	206	0.03%	0.003%
59	10.750	1583	1585	1588	rVB2	246	260	0.03%	0.004%
60	10.964	1617	1620	1623	rBV2	422	550	0.07%	0.009%
61	10.994	1623	1625	1630	rVV2	231	291	0.04%	0.005%
62	11.092	1638	1641	1644	rBV2	267	388	0.05%	0.006%
63	11.189	1652	1657	1669	rBV	314125	401644	48.88%	6.338%
64	11.274	1669	1671	1674	rVV	285	360	0.04%	0.006%
65	11.317	1674	1678	1681	rVB2	467	659	0.08%	0.010%
66	11.354	1681	1684	1685	rBV	223	196	0.02%	0.003%
67	11.378	1685	1688	1692	rBV2	137	198	0.02%	0.003%
68	11.457	1698	1701	1704	rBV4	473	584	0.07%	0.009%
69	11.585	1719	1722	1726	rBV2	140	204	0.02%	0.003%
70	11.756	1747	1750	1752	rVB	491	523	0.06%	0.008%
71	11.799	1755	1757	1759	rVB	265	206	0.03%	0.003%
72	12.018	1788	1793	1807	rBV	451716	595854	72.51%	9.402%
73	12.213	1821	1825	1826	rBV	202	195	0.02%	0.003%
74	12.317	1837	1842	1852	rBV	437843	556908	67.77%	8.787%
75	12.762	1910	1915	1920	rVB	1581	2187	0.27%	0.035%
76	12.841	1925	1928	1929	rBV2	276	234	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
 Data File : VX039354.D
 Acq On : 19 Dec 2023 14:25
 Operator : JC/MD
 Sample : VIBLK626
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK626

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

77	12.896	1933	1937	1939	rBV2	313	406	0.05%	0.006%
78	13.219	1987	1990	1991	rVB	279	210	0.03%	0.003%
79	13.292	2000	2002	2005	rBV2	206	219	0.03%	0.003%
80	13.408	2019	2021	2025	rVB2	320	301	0.04%	0.005%
81	13.591	2050	2051	2054	rBV2	411	307	0.04%	0.005%
82	13.640	2056	2059	2063	rVB2	212	323	0.04%	0.005%
83	13.695	2065	2068	2069	rBV2	275	246	0.03%	0.004%
84	13.780	2080	2082	2084	rBV2	372	298	0.04%	0.005%
85	13.969	2111	2113	2116	rBV2	219	210	0.03%	0.003%
86	14.030	2121	2123	2126	rBV2	147	211	0.03%	0.003%
87	14.128	2135	2139	2142	rBV	2144	2452	0.30%	0.039%
88	14.481	2195	2197	2200	rVB2	302	348	0.04%	0.005%
89	14.603	2215	2217	2219	rVB2	272	197	0.02%	0.003%
90	14.798	2248	2249	2252	rBV2	349	342	0.04%	0.005%
91	14.914	2267	2268	2271	rBV	341	272	0.03%	0.004%
92	14.981	2275	2279	2281	rVB2	316	350	0.04%	0.006%
93	15.054	2289	2291	2294	rVV3	256	246	0.03%	0.004%
94	15.109	2297	2300	2301	rBV2	277	222	0.03%	0.004%
95	15.158	2306	2308	2309	rBV	464	333	0.04%	0.005%
96	15.383	2343	2345	2351	rVB2	628	951	0.12%	0.015%
97	15.572	2371	2376	2377	rBV3	229	324	0.04%	0.005%
98	15.700	2395	2397	2398	rBV2	322	206	0.03%	0.003%
99	16.261	2488	2489	2492	rBV3	286	237	0.03%	0.004%
100	16.682	2556	2558	2559	rBV	297	197	0.02%	0.003%


Sum of corrected areas: 6337540

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
Data File : VX039354.D
Acq On : 19 Dec 2023 14:25
Operator : JC/MD
Sample : VIBLK626
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK626

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

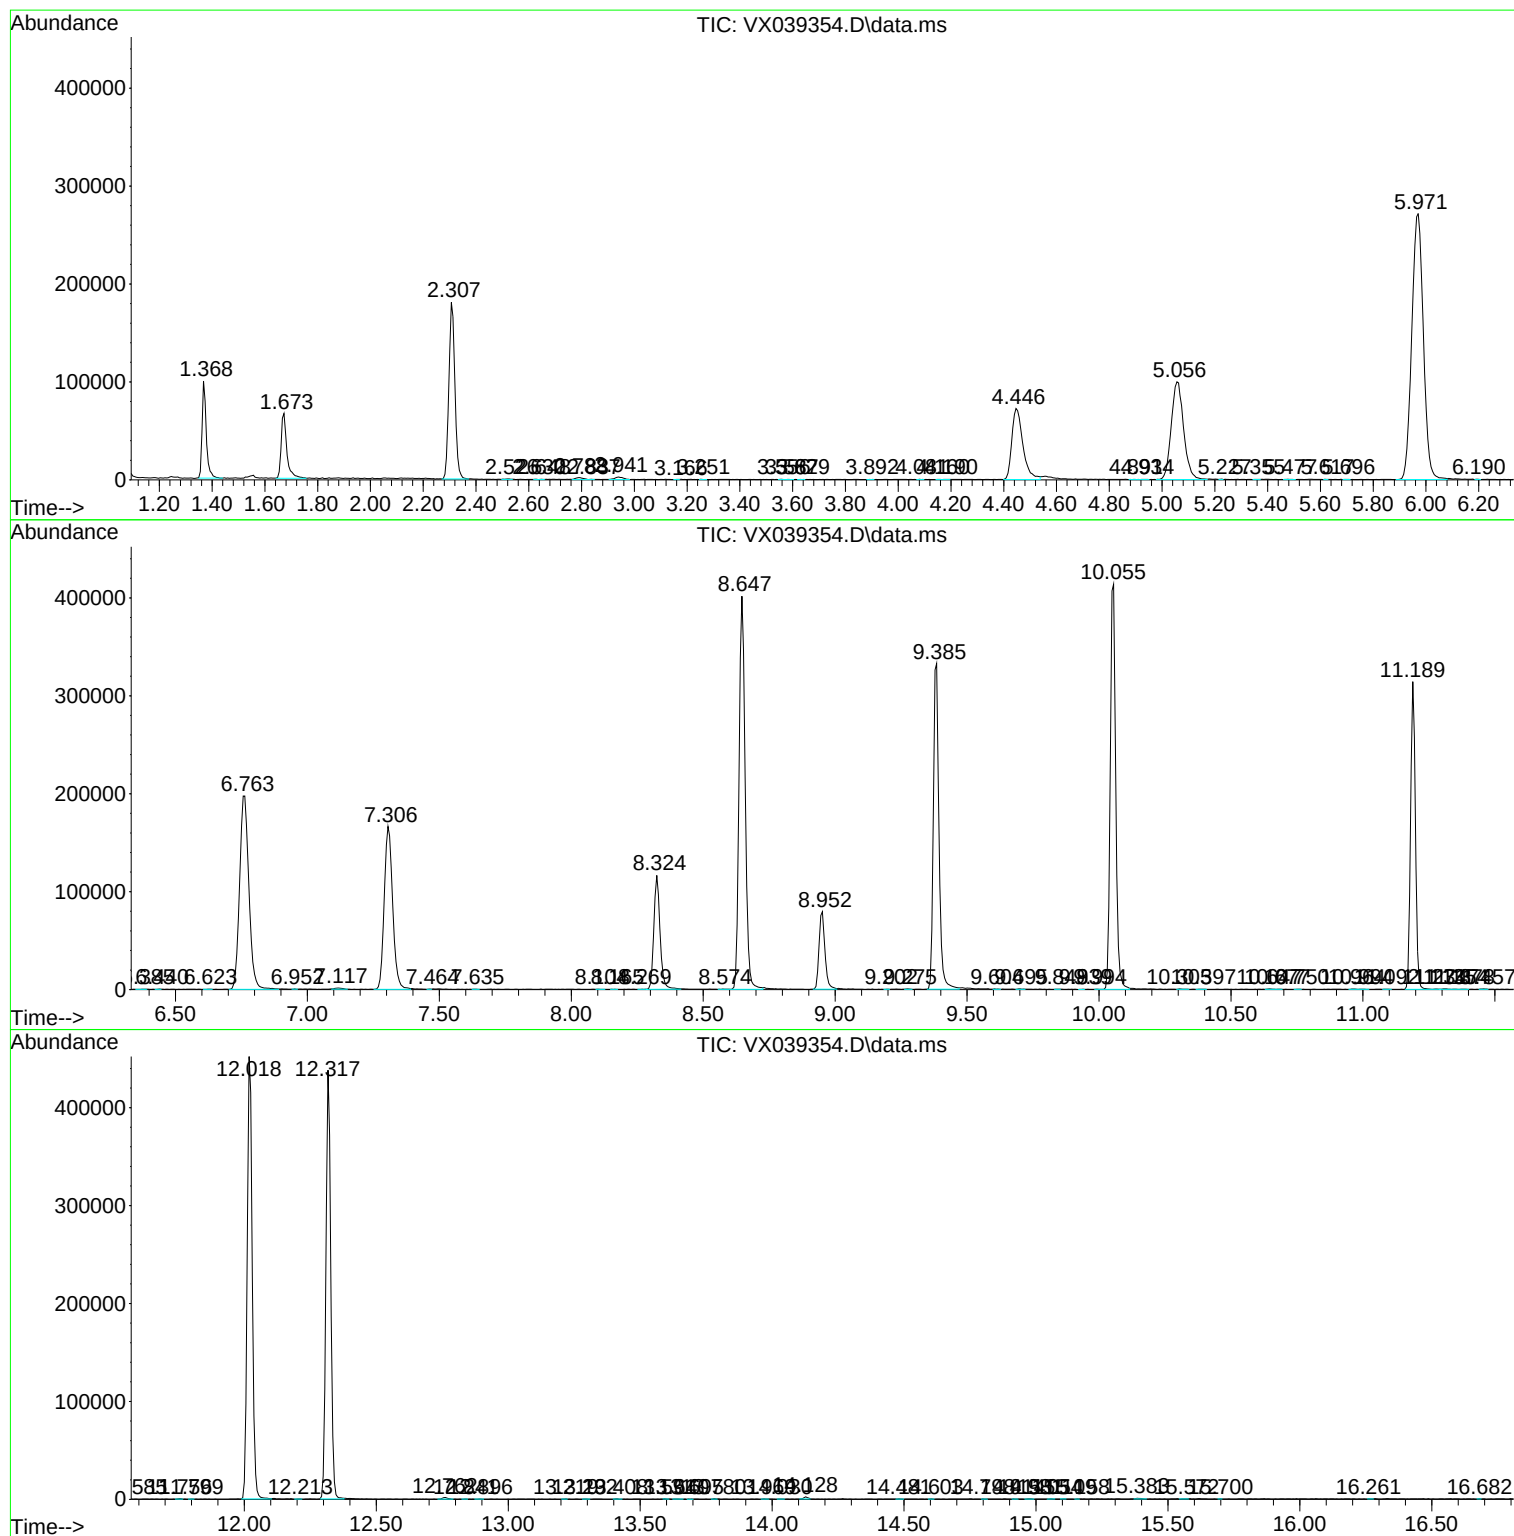

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
Data File : VX039354.D
Acq On : 19 Dec 2023 14:25
Operator : JC/MD
Sample : VIBLK626
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK626

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
Data File : VX039354.D
Acq On : 19 Dec 2023 14:25
Operator : JC/MD
Sample : VIBLK626
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK626

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------