

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
 Data File : VX039359.D
 Acq On : 19 Dec 2023 16:19
 Operator : JC/MD
 Sample : VIBLK627
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK627

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

Signal : TIC: VX039359.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.245	23	26	28	rBV	2050	2583	0.35%	0.043%
2	1.367	43	46	57	rBV	84535	93196	12.65%	1.539%
3	1.672	91	96	106	rBV	55848	84638	11.49%	1.398%
4	2.306	194	200	211	rBV	154770	247046	33.53%	4.080%
5	2.495	228	231	233	rBV3	315	455	0.06%	0.008%
6	2.788	275	279	288	rVB4	1920	3680	0.50%	0.061%
7	2.898	294	297	298	rBV	266	278	0.04%	0.005%
8	2.946	300	305	312	rVB3	1856	4073	0.55%	0.067%
9	3.105	329	331	336	rVV2	266	484	0.07%	0.008%
10	3.172	340	342	346	rVB	266	312	0.04%	0.005%
11	3.245	352	354	359	rVB2	209	197	0.03%	0.003%
12	3.397	376	379	382	rVB2	150	198	0.03%	0.003%
13	3.501	393	396	399	rBV2	197	233	0.03%	0.004%
14	4.324	528	531	532	rVB2	214	195	0.03%	0.003%
15	4.446	543	551	565	rBV	62446	182360	24.75%	3.012%
16	4.861	616	619	623	rVB2	181	247	0.03%	0.004%
17	4.946	629	633	634	rBV	174	203	0.03%	0.003%
18	5.062	639	652	667	rBV	88210	285520	38.75%	4.716%
19	5.287	685	689	690	rVB2	203	192	0.03%	0.003%
20	5.769	765	768	769	rBV2	209	185	0.03%	0.003%
21	5.970	787	801	818	rBV2	243375	736736	100.00%	12.168%
22	6.251	845	847	849	rVB2	268	248	0.03%	0.004%
23	6.275	849	851	852	rBV	223	201	0.03%	0.003%
24	6.342	860	862	863	rBV	355	183	0.02%	0.003%
25	6.549	893	896	899	rVB2	234	223	0.03%	0.004%
26	6.592	902	903	907	rBV2	211	235	0.03%	0.004%
27	6.763	922	931	951	rBV	207919	506259	68.72%	8.361%
28	6.891	951	952	954	rVB2	464	210	0.03%	0.003%
29	7.116	983	989	996	rVB5	1114	2506	0.34%	0.041%
30	7.232	1004	1008	1009	rVB	351	290	0.04%	0.005%
31	7.305	1011	1020	1038	rBV	148690	336038	45.61%	5.550%
32	7.482	1048	1049	1054	rVB4	325	221	0.03%	0.004%
33	7.793	1097	1100	1101	rBV	217	226	0.03%	0.004%
34	7.830	1105	1106	1111	rBV2	175	285	0.04%	0.005%
35	7.878	1111	1114	1116	rVB2	199	236	0.03%	0.004%
36	8.171	1159	1162	1163	rBV2	261	249	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
 Data File : VX039359.D
 Acq On : 19 Dec 2023 16:19
 Operator : JC/MD
 Sample : VIBLK627
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK627

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

37	8.238	1171	1173	1176	rVB	226	189	0.03%	0.003%
38	8.323	1181	1187	1202	rBV	100468	165542	22.47%	2.734%
39	8.512	1216	1218	1222	rBV2	411	515	0.07%	0.009%
40	8.567	1225	1227	1228	rBV	266	246	0.03%	0.004%
41	8.647	1234	1240	1251	rBV	370400	573350	77.82%	9.470%
42	8.951	1284	1290	1301	rBV	72458	109980	14.93%	1.816%
43	9.268	1340	1342	1343	rBV2	270	250	0.03%	0.004%
44	9.384	1355	1361	1377	rBV	294630	427279	58.00%	7.057%
45	9.701	1409	1413	1415	rBV2	523	745	0.10%	0.012%
46	9.744	1418	1420	1422	rBV2	173	193	0.03%	0.003%
47	9.823	1430	1433	1435	rBV2	198	225	0.03%	0.004%
48	9.854	1435	1438	1440	rBV	267	217	0.03%	0.004%
49	9.933	1445	1451	1454	rBV2	290	556	0.08%	0.009%
50	10.000	1460	1462	1465	rVB2	246	233	0.03%	0.004%
51	10.055	1465	1471	1482	rBV	450416	688345	93.43%	11.369%
52	10.311	1510	1513	1518	rBV2	373	670	0.09%	0.011%
53	10.835	1598	1599	1603	rBV2	140	183	0.02%	0.003%
54	10.957	1617	1619	1624	rBV3	389	682	0.09%	0.011%
55	11.189	1652	1657	1672	rVV	271639	351593	47.72%	5.807%
56	11.311	1674	1677	1683	rVB3	614	1026	0.14%	0.017%
57	11.457	1697	1701	1707	rVB2	515	797	0.11%	0.013%
58	11.512	1707	1710	1711	rBV2	245	250	0.03%	0.004%
59	11.676	1735	1737	1738	rVV	249	209	0.03%	0.003%
60	11.695	1738	1740	1741	rVV	389	304	0.04%	0.005%
61	11.762	1748	1751	1753	rVV	312	284	0.04%	0.005%
62	11.798	1755	1757	1760	rBV2	179	210	0.03%	0.003%
63	11.969	1781	1785	1788	rBV2	2867	3617	0.49%	0.060%
64	12.024	1788	1794	1809	rVB	482375	705420	95.75%	11.651%
65	12.122	1809	1810	1811	rBV	556	237	0.03%	0.004%
66	12.317	1837	1842	1853	rBV	379893	506223	68.71%	8.361%
67	12.500	1869	1872	1873	rBV	162	183	0.02%	0.003%
68	12.762	1909	1915	1920	rBV2	2827	3981	0.54%	0.066%
69	12.975	1947	1950	1952	rBV	327	322	0.04%	0.005%
70	13.054	1960	1963	1964	rBV2	332	338	0.05%	0.006%
71	13.115	1971	1973	1975	rBV3	324	197	0.03%	0.003%
72	13.371	2013	2015	2019	rBV	175	213	0.03%	0.004%
73	13.426	2019	2024	2025	rBV2	232	268	0.04%	0.004%
74	13.591	2047	2051	2055	rBV3	3194	4411	0.60%	0.073%
75	13.707	2067	2070	2073	rVB2	179	202	0.03%	0.003%
76	13.841	2088	2092	2095	rVB2	155	282	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
 Data File : VX039359.D
 Acq On : 19 Dec 2023 16:19
 Operator : JC/MD
 Sample : VIBLK627
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK627

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
 Title : VOC Analysis

77	13.877	2095	2098	2100	rVB	242	291	0.04%	0.005%
78	13.963	2108	2112	2117	rVB4	1826	2709	0.37%	0.045%
79	14.030	2120	2123	2127	rBV2	233	516	0.07%	0.009%
80	14.127	2135	2139	2144	rVB	3674	4915	0.67%	0.081%
81	14.219	2151	2154	2155	rBV2	271	219	0.03%	0.004%
82	14.274	2160	2163	2167	rBV2	205	290	0.04%	0.005%
83	14.408	2181	2185	2186	rBV2	187	222	0.03%	0.004%
84	14.499	2198	2200	2203	rBV2	224	305	0.04%	0.005%
85	14.700	2230	2233	2235	rBV2	217	249	0.03%	0.004%
86	14.731	2235	2238	2239	rVV2	241	245	0.03%	0.004%
87	14.749	2239	2241	2242	rVV2	301	211	0.03%	0.003%
88	14.786	2244	2247	2249	rVB	276	252	0.03%	0.004%
89	14.822	2249	2253	2256	rBV3	212	284	0.04%	0.005%
90	15.066	2289	2293	2294	rBV3	215	303	0.04%	0.005%
91	15.158	2306	2308	2311	rBV2	232	198	0.03%	0.003%
92	15.243	2321	2322	2323	rBV	502	296	0.04%	0.005%
93	15.718	2397	2400	2403	rBV3	242	394	0.05%	0.007%
94	15.822	2416	2417	2420	rBV2	373	297	0.04%	0.005%
95	15.877	2424	2426	2428	rVV2	330	270	0.04%	0.004%
96	15.993	2443	2445	2446	rVB	481	251	0.03%	0.004%
97	16.090	2459	2461	2464	rVB	379	289	0.04%	0.005%
98	16.218	2480	2482	2486	rVB2	577	417	0.06%	0.007%
99	16.413	2512	2514	2517	rBV2	334	418	0.06%	0.007%
100	16.657	2552	2554	2555	rBV	264	256	0.03%	0.004%




Sum of corrected areas: 6054685

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
Data File : VX039359.D
Acq On : 19 Dec 2023 16:19
Operator : JC/MD
Sample : VIBLK627
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK627

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

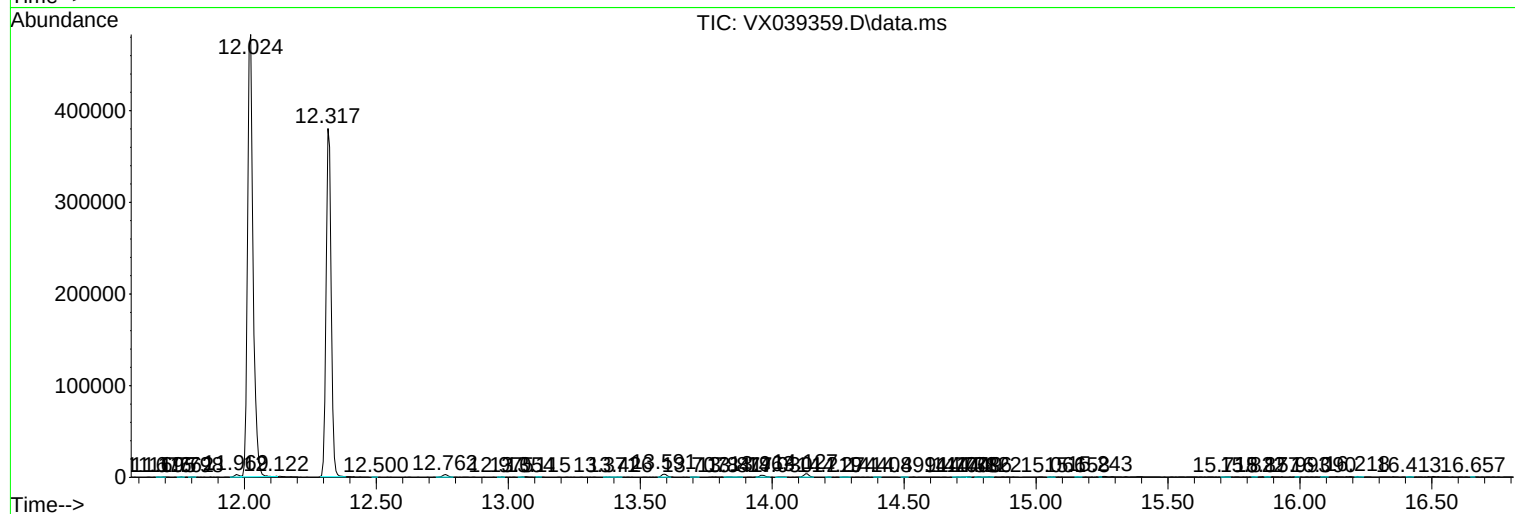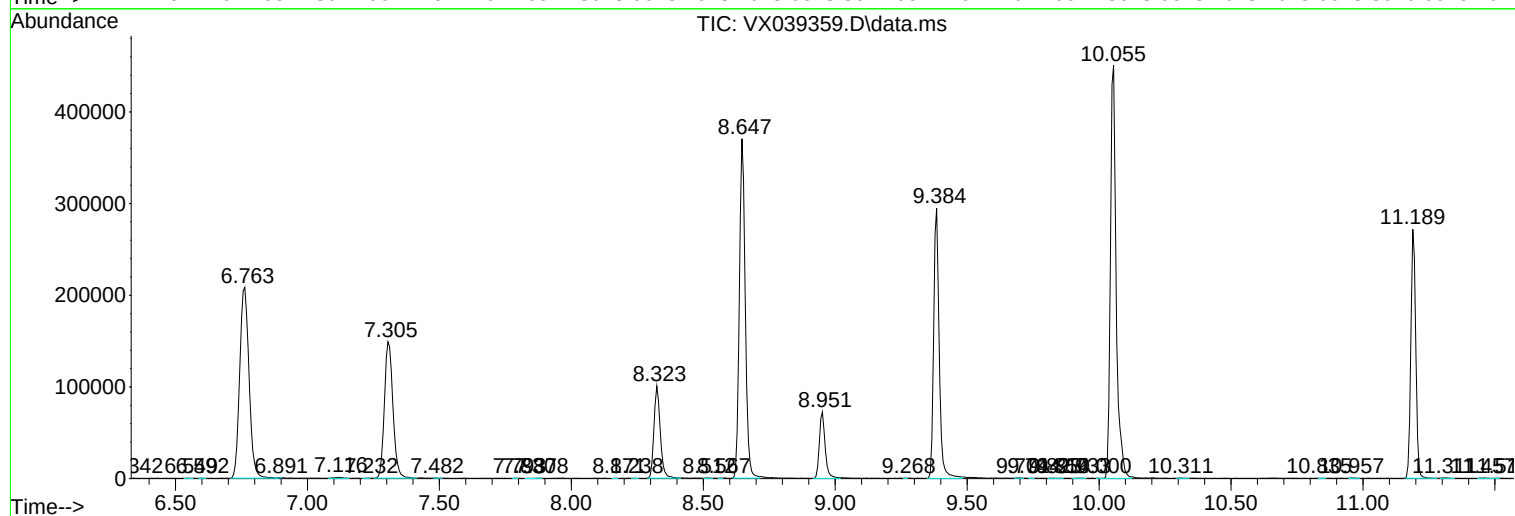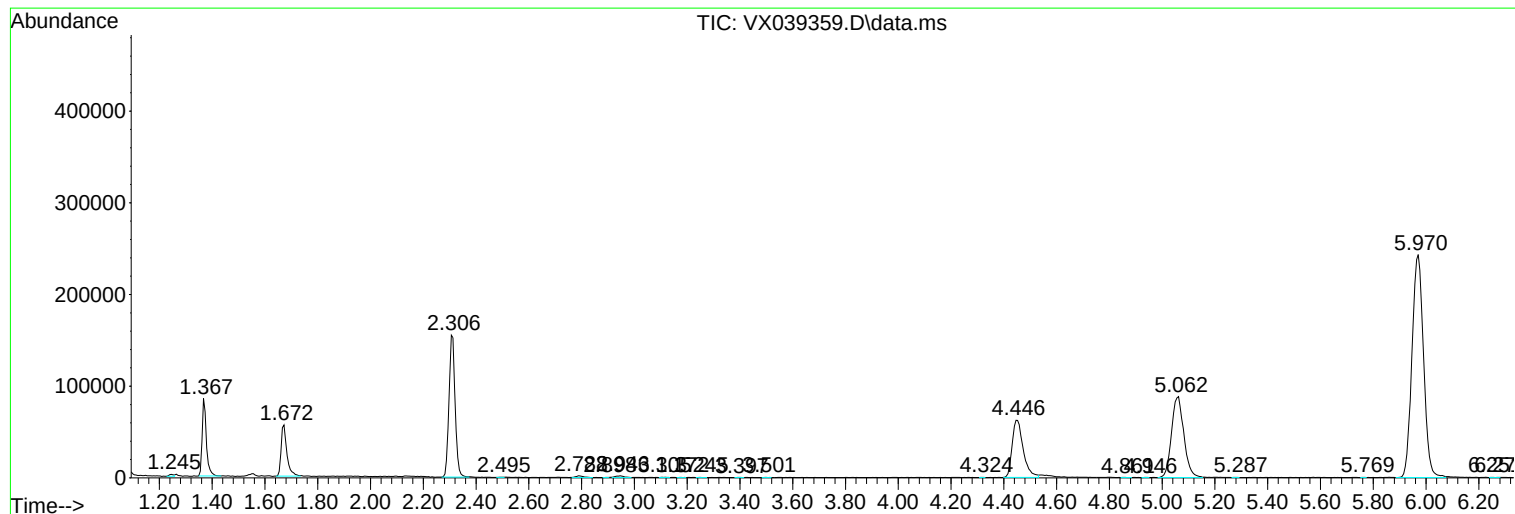

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
Data File : VX039359.D
Acq On : 19 Dec 2023 16:19
Operator : JC/MD
Sample : VIBLK627
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK627

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
Data File : VX039359.D
Acq On : 19 Dec 2023 16:19
Operator : JC/MD
Sample : VIBLK627
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK627

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------