

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
 Data File : VX039361.D
 Acq On : 19 Dec 2023 17:04
 Operator : JC/MD
 Sample : 05808-02ME
 Misc : 1.92g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COB23ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

Signal : TIC: VX039361.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.374	43	47	58	rBV	96412	152435	14.02%	1.833%
2	1.648	89	92	102	rVB	31354	50100	4.61%	0.602%
3	2.288	191	197	208	rVV	235175	370181	34.06%	4.451%
4	2.404	212	216	226	rVB	3245	7517	0.69%	0.090%
5	2.715	260	267	273	rBV	5790	12314	1.13%	0.148%
6	2.788	275	279	283	rVB2	1786	3351	0.31%	0.040%
7	2.941	298	304	315	rVB2	5249	13233	1.22%	0.159%
8	3.233	350	352	357	rVB	322	410	0.04%	0.005%
9	3.428	380	384	386	rBV2	405	665	0.06%	0.008%
10	3.587	407	410	411	rVB	251	214	0.02%	0.003%
11	3.855	451	454	455	rVB	314	245	0.02%	0.003%
12	3.940	466	468	470	rBV2	250	208	0.02%	0.003%
13	4.477	547	556	587	rBV	58360	262679	24.17%	3.158%
14	4.916	626	628	631	rVB2	300	251	0.02%	0.003%
15	4.971	634	637	638	rBV2	209	210	0.02%	0.003%
16	5.056	638	651	671	rBV	125628	411949	37.90%	4.953%
17	5.257	682	684	687	rVB	374	362	0.03%	0.004%
18	5.538	728	730	733	rBV3	279	331	0.03%	0.004%
19	5.964	788	800	807	rBV2	370676	1086962	100.00%	13.069%
20	6.367	860	866	870	rBV2	882	1938	0.18%	0.023%
21	6.690	916	919	921	rBV2	214	235	0.02%	0.003%
22	6.757	921	930	946	rBV	245604	614716	56.55%	7.391%
23	7.050	977	978	981	rVB	318	201	0.02%	0.002%
24	7.123	984	990	999	rBV7	1684	4828	0.44%	0.058%
25	7.220	999	1006	1010	rBV5	2004	4781	0.44%	0.057%
26	7.306	1010	1020	1038	rVB	210815	480450	44.20%	5.777%
27	7.476	1045	1048	1050	rBV2	518	723	0.07%	0.009%
28	7.562	1061	1062	1065	rVB	319	191	0.02%	0.002%
29	7.598	1065	1068	1072	rBV2	258	370	0.03%	0.004%
30	7.769	1094	1096	1098	rBV2	195	201	0.02%	0.002%
31	7.952	1123	1126	1129	rBV2	467	757	0.07%	0.009%
32	8.019	1136	1137	1143	rBV2	233	363	0.03%	0.004%
33	8.324	1180	1187	1200	rBV	136404	241421	22.21%	2.903%
34	8.580	1227	1229	1233	rBV2	347	507	0.05%	0.006%
35	8.647	1233	1240	1251	rBV	517624	844179	77.66%	10.150%
36	8.872	1274	1277	1279	rBV3	290	309	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
 Data File : VX039361.D
 Acq On : 19 Dec 2023 17:04
 Operator : JC/MD
 Sample : 05808-02ME
 Misc : 1.92g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COB23ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

37	8.952	1284	1290	1303	rBV2	95963	158504	14.58%	1.906%
38	9.092	1312	1313	1315	rBV	306	213	0.02%	0.003%
39	9.116	1315	1317	1321	rVV4	526	725	0.07%	0.009%
40	9.165	1324	1325	1326	rBV	375	212	0.02%	0.003%
41	9.287	1341	1345	1346	rBV	361	275	0.03%	0.003%
42	9.354	1353	1356	1357	rBV	294	310	0.03%	0.004%
43	9.397	1357	1363	1380	rBV	322475	603248	55.50%	7.253%
44	9.610	1397	1398	1401	rVB2	362	274	0.03%	0.003%
45	9.714	1411	1415	1418	rVB3	589	720	0.07%	0.009%
46	9.836	1433	1435	1439	rBV2	287	328	0.03%	0.004%
47	9.897	1442	1445	1446	rBV	261	264	0.02%	0.003%
48	10.055	1465	1471	1473	rBV	514056	782400	71.98%	9.407%
49	10.311	1510	1513	1520	rVB3	659	937	0.09%	0.011%
50	10.653	1565	1569	1576	rVB4	604	1166	0.11%	0.014%
51	10.762	1585	1587	1592	rBV2	334	540	0.05%	0.006%
52	10.799	1592	1593	1596	rVB	281	238	0.02%	0.003%
53	10.970	1613	1621	1624	rBV2	803	1245	0.11%	0.015%
54	11.195	1652	1658	1670	rBV	386262	491761	45.24%	5.912%
55	11.311	1673	1677	1681	rVB2	1977	2986	0.27%	0.036%
56	11.366	1683	1686	1692	rVB4	1884	2737	0.25%	0.033%
57	11.433	1692	1697	1698	rBV3	507	750	0.07%	0.009%
58	11.677	1735	1737	1741	rBV3	362	406	0.04%	0.005%
59	11.713	1741	1743	1745	rBV	481	242	0.02%	0.003%
60	11.756	1747	1750	1762	rBV6	679	1837	0.17%	0.022%
61	11.884	1768	1771	1775	rBV3	429	595	0.05%	0.007%
62	11.975	1782	1786	1789	rBV2	5592	7453	0.69%	0.090%
63	12.024	1789	1794	1808	rVB2	629159	890053	81.88%	10.701%
64	12.225	1823	1827	1834	rBV4	2318	4839	0.45%	0.058%
65	12.323	1837	1843	1856	rVB	568124	743918	68.44%	8.944%
66	12.573	1881	1884	1886	rVB3	544	483	0.04%	0.006%
67	12.597	1886	1888	1893	rBV2	321	608	0.06%	0.007%
68	12.762	1909	1915	1921	rBV	5098	7384	0.68%	0.089%
69	12.908	1937	1939	1943	rBV2	471	512	0.05%	0.006%
70	12.975	1949	1950	1952	rBV	308	208	0.02%	0.003%
71	13.109	1970	1972	1977	rVB3	526	671	0.06%	0.008%
72	13.164	1977	1981	1982	rBV2	316	391	0.04%	0.005%
73	13.304	2001	2004	2005	rBV2	204	260	0.02%	0.003%
74	13.335	2007	2009	2014	rVB3	895	1262	0.12%	0.015%
75	13.591	2046	2051	2058	rVB3	6888	8931	0.82%	0.107%
76	13.689	2065	2067	2073	rBV3	331	464	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
 Data File : VX039361.D
 Acq On : 19 Dec 2023 17:04
 Operator : JC/MD
 Sample : 05808-02ME
 Misc : 1.92g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0B23ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

77	13.750	2076	2077	2080	rBV2	577	387	0.04%	0.005%
78	13.780	2080	2082	2084	rBV	465	342	0.03%	0.004%
79	13.841	2089	2092	2095	rBV	300	304	0.03%	0.004%
80	13.884	2097	2099	2101	rVB	387	214	0.02%	0.003%
81	13.963	2108	2112	2117	rBV3	2764	3560	0.33%	0.043%
82	14.012	2119	2120	2124	rVB	207	210	0.02%	0.003%
83	14.128	2135	2139	2143	rVB2	4558	6177	0.57%	0.074%
84	14.384	2178	2181	2182	rBV2	215	205	0.02%	0.002%
85	14.487	2195	2198	2201	rBV2	300	352	0.03%	0.004%
86	14.627	2219	2221	2223	rBV2	238	190	0.02%	0.002%
87	14.731	2237	2238	2241	rVB	273	226	0.02%	0.003%
88	14.755	2241	2242	2243	rBV	366	210	0.02%	0.003%
89	14.902	2264	2266	2268	rBV2	389	455	0.04%	0.005%
90	15.140	2303	2305	2306	rVB	432	230	0.02%	0.003%
91	15.176	2306	2311	2312	rBV2	189	281	0.03%	0.003%
92	15.207	2314	2316	2317	rVV	350	199	0.02%	0.002%
93	15.249	2318	2323	2328	rVB3	6047	8310	0.76%	0.100%
94	15.658	2388	2390	2391	rBV2	296	235	0.02%	0.003%
95	15.871	2424	2425	2428	rBV2	296	225	0.02%	0.003%
96	16.060	2455	2456	2458	rVB	475	226	0.02%	0.003%
97	16.084	2458	2460	2462	rBV	349	246	0.02%	0.003%
98	16.267	2488	2490	2497	rVB4	1373	1688	0.16%	0.020%
99	16.377	2505	2508	2510	rBV2	389	473	0.04%	0.006%
100	16.505	2525	2529	2536	rVB3	1438	2234	0.21%	0.027%


Sum of corrected areas: 8317316

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
Data File : VX039361.D
Acq On : 19 Dec 2023 17:04
Operator : JC/MD
Sample : 05808-02ME
Misc : 1.92g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0B23ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

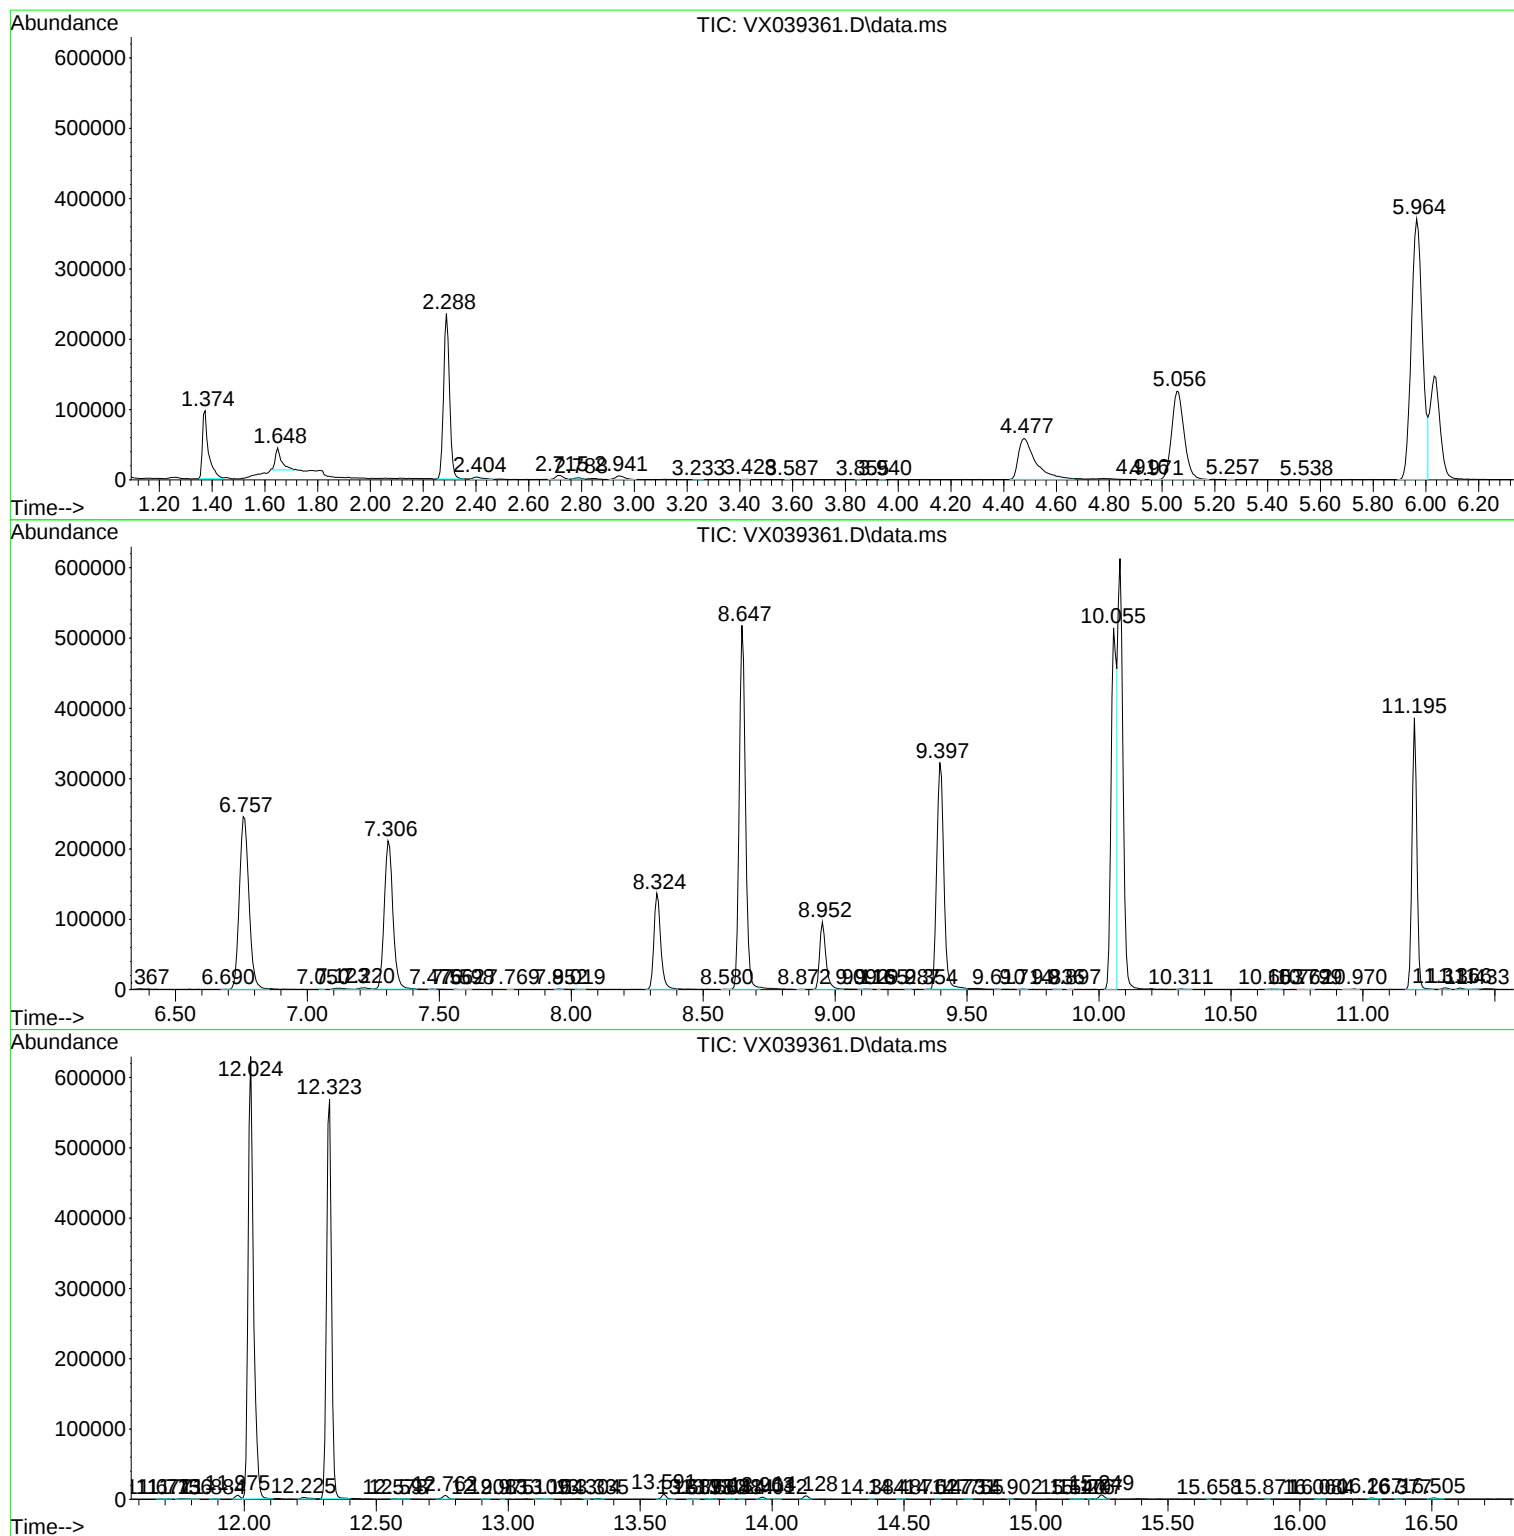

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
Data File : VX039361.D
Acq On : 19 Dec 2023 17:04
Operator : JC/MD
Sample : 05808-02ME
Misc : 1.92g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0B23ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
Data File : VX039361.D
Acq On : 19 Dec 2023 17:04
Operator : JC/MD
Sample : 05808-02ME
Misc : 1.92g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0B23ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc