

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
 Data File : VX039363.D
 Acq On : 19 Dec 2023 17:50
 Operator : JC/MD
 Sample : 05808-01 40X
 Misc : 2.75g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0B22

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
 Title : VOC Analysis

Signal : TIC: VX039363.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	23	25	27	rBV2	1883	1799	0.15%	0.025%
2	1.368	43	46	55	rVB	104999	115264	9.53%	1.607%
3	1.666	91	95	111	rVB	71168	101583	8.40%	1.416%
4	2.307	194	200	210	rBV	188350	292670	24.19%	4.080%
5	2.526	234	236	239	rVB	453	423	0.03%	0.006%
6	2.697	262	264	266	rBV	298	290	0.02%	0.004%
7	2.788	275	279	285	rBV4	1990	3183	0.26%	0.044%
8	2.947	298	305	311	rBV2	4771	10074	0.83%	0.140%
9	3.026	315	318	320	rBV2	242	312	0.03%	0.004%
10	3.111	329	332	333	rBV2	243	272	0.02%	0.004%
11	3.556	403	405	409	rBV2	242	318	0.03%	0.004%
12	3.666	420	423	426	rBV	173	323	0.03%	0.005%
13	3.788	439	443	444	rBV2	256	296	0.02%	0.004%
14	3.947	465	469	471	rBV	174	304	0.03%	0.004%
15	4.446	543	551	564	rBV	71279	204501	16.90%	2.851%
16	4.757	599	602	604	rBV2	229	264	0.02%	0.004%
17	4.776	604	605	609	rVB2	330	323	0.03%	0.005%
18	4.843	613	616	617	rBV2	248	274	0.02%	0.004%
19	4.898	624	625	628	rBV2	254	223	0.02%	0.003%
20	5.056	639	651	669	rBV2	103704	327300	27.05%	4.563%
21	5.312	690	693	696	rBV2	217	196	0.02%	0.003%
22	5.397	704	707	709	rBV2	382	413	0.03%	0.006%
23	5.556	731	733	736	rBV2	220	294	0.02%	0.004%
24	5.635	741	746	747	rBV	237	288	0.02%	0.004%
25	5.971	788	801	807	rBV2	282958	847512	70.06%	11.816%
26	6.275	850	851	853	rBV	262	222	0.02%	0.003%
27	6.617	905	907	910	rBV2	264	244	0.02%	0.003%
28	6.763	922	931	943	rBV	204885	502478	41.54%	7.005%
29	7.111	983	988	996	rVV4	1531	2976	0.25%	0.041%
30	7.306	1011	1020	1036	rVV	171543	382421	31.61%	5.332%
31	7.550	1057	1060	1063	rVB2	282	268	0.02%	0.004%
32	7.690	1081	1083	1084	rBV	203	187	0.02%	0.003%
33	7.739	1088	1091	1092	rBV2	232	217	0.02%	0.003%
34	7.763	1092	1095	1097	rBV2	204	297	0.02%	0.004%
35	7.995	1131	1133	1135	rVV	267	251	0.02%	0.003%
36	8.232	1168	1172	1174	rBV2	152	245	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
 Data File : VX039363.D
 Acq On : 19 Dec 2023 17:50
 Operator : JC/MD
 Sample : 05808-01 40X
 Misc : 2.75g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0B22

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

37	8.324	1181	1187	1199	rBV	115451	190931	15.78%	2.662%
38	8.519	1218	1219	1224	rVB3	371	334	0.03%	0.005%
39	8.586	1227	1230	1234	rBV2	250	314	0.03%	0.004%
40	8.647	1234	1240	1258	rVV	424709	669083	55.31%	9.328%
41	8.854	1272	1274	1276	rVB2	273	238	0.02%	0.003%
42	8.903	1279	1282	1283	rBV2	198	185	0.02%	0.003%
43	8.952	1284	1290	1301	rVV	79874	126009	10.42%	1.757%
44	9.171	1324	1326	1329	rVB2	262	187	0.02%	0.003%
45	9.208	1329	1332	1334	rBV2	197	187	0.02%	0.003%
46	9.287	1342	1345	1349	rVB2	228	251	0.02%	0.003%
47	9.385	1355	1361	1377	rBV	333102	489293	40.45%	6.822%
48	9.702	1410	1413	1421	rVB3	609	1084	0.09%	0.015%
49	9.787	1424	1427	1429	rBV	258	260	0.02%	0.004%
50	9.897	1442	1445	1446	rBV2	227	230	0.02%	0.003%
51	9.952	1452	1454	1458	rBV2	263	317	0.03%	0.004%
52	10.055	1465	1471	1473	rBV	450259	682111	56.38%	9.510%
53	10.202	1492	1495	1500	rVB4	646	1240	0.10%	0.017%
54	10.250	1500	1503	1506	rBV	337	405	0.03%	0.006%
55	10.311	1510	1513	1516	rBV2	568	552	0.05%	0.008%
56	10.427	1529	1532	1535	rBV2	195	202	0.02%	0.003%
57	10.537	1544	1550	1553	rBV2	154	317	0.03%	0.004%
58	10.610	1559	1562	1565	rVV2	141	226	0.02%	0.003%
59	10.640	1565	1567	1568	rVV2	353	227	0.02%	0.003%
60	10.970	1617	1621	1625	rBV3	521	712	0.06%	0.010%
61	11.104	1638	1643	1645	rBV3	234	368	0.03%	0.005%
62	11.189	1652	1657	1670	rVV	310345	397776	32.88%	5.546%
63	11.311	1674	1677	1681	rVB2	300	483	0.04%	0.007%
64	11.366	1683	1686	1690	rBV	1944	2502	0.21%	0.035%
65	11.457	1698	1701	1703	rBV3	707	804	0.07%	0.011%
66	11.585	1720	1722	1724	rBV	235	222	0.02%	0.003%
67	11.616	1724	1727	1728	rBV	318	237	0.02%	0.003%
68	11.756	1747	1750	1755	rBV3	384	490	0.04%	0.007%
69	11.969	1782	1785	1788	rBV2	1506	2093	0.17%	0.029%
70	12.024	1788	1794	1809	rVV2	540835	1209766	100.00%	16.866%
71	12.317	1837	1842	1855	rVV	448639	579849	47.93%	8.084%
72	12.695	1902	1904	1907	rVB2	188	215	0.02%	0.003%
73	12.762	1907	1915	1919	rBV3	1173	1928	0.16%	0.027%
74	12.921	1938	1941	1944	rVV2	203	204	0.02%	0.003%
75	12.982	1949	1951	1954	rVB	178	183	0.02%	0.003%
76	13.067	1964	1965	1968	rVV	365	247	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
 Data File : VX039363.D
 Acq On : 19 Dec 2023 17:50
 Operator : JC/MD
 Sample : 05808-01 40X
 Misc : 2.75g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0B22

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

77	13.116	1970	1973	1976	rVB2	431	501	0.04%	0.007%
78	13.591	2047	2051	2055	rVB4	1741	2329	0.19%	0.032%
79	13.683	2062	2066	2068	rBV2	191	218	0.02%	0.003%
80	13.780	2079	2082	2083	rBV2	291	281	0.02%	0.004%
81	13.963	2108	2112	2115	rVB2	687	924	0.08%	0.013%
82	14.128	2136	2139	2145	rVB2	1894	2568	0.21%	0.036%
83	14.176	2145	2147	2149	rBV2	201	229	0.02%	0.003%
84	14.213	2149	2153	2156	rBV	310	309	0.03%	0.004%
85	14.420	2185	2187	2190	rVB2	283	198	0.02%	0.003%
86	14.469	2193	2195	2197	rBV	250	205	0.02%	0.003%
87	14.554	2206	2209	2212	rVB2	213	274	0.02%	0.004%
88	14.609	2216	2218	2221	rVB2	242	232	0.02%	0.003%
89	14.749	2237	2241	2242	rBV2	204	223	0.02%	0.003%
90	15.073	2292	2294	2296	rVB	345	249	0.02%	0.003%
91	15.115	2300	2301	2303	rBV2	317	204	0.02%	0.003%
92	15.225	2316	2319	2320	rBV3	191	208	0.02%	0.003%
93	15.384	2341	2345	2350	rBV3	334	593	0.05%	0.008%
94	15.451	2354	2356	2357	rBV2	329	186	0.02%	0.003%
95	15.499	2362	2364	2365	rBV2	295	213	0.02%	0.003%
96	15.987	2441	2444	2445	rBV2	265	264	0.02%	0.004%
97	16.158	2471	2472	2475	rBV2	298	262	0.02%	0.004%
98	16.280	2489	2492	2495	rBV2	318	508	0.04%	0.007%
99	16.706	2559	2562	2564	rBV2	358	398	0.03%	0.006%
100	16.755	2567	2570	2573	rBV3	284	435	0.04%	0.006%




Sum of corrected areas: 7172778

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
Data File : VX039363.D
Acq On : 19 Dec 2023 17:50
Operator : JC/MD
Sample : 05808-01 40X
Misc : 2.75g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0B22

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

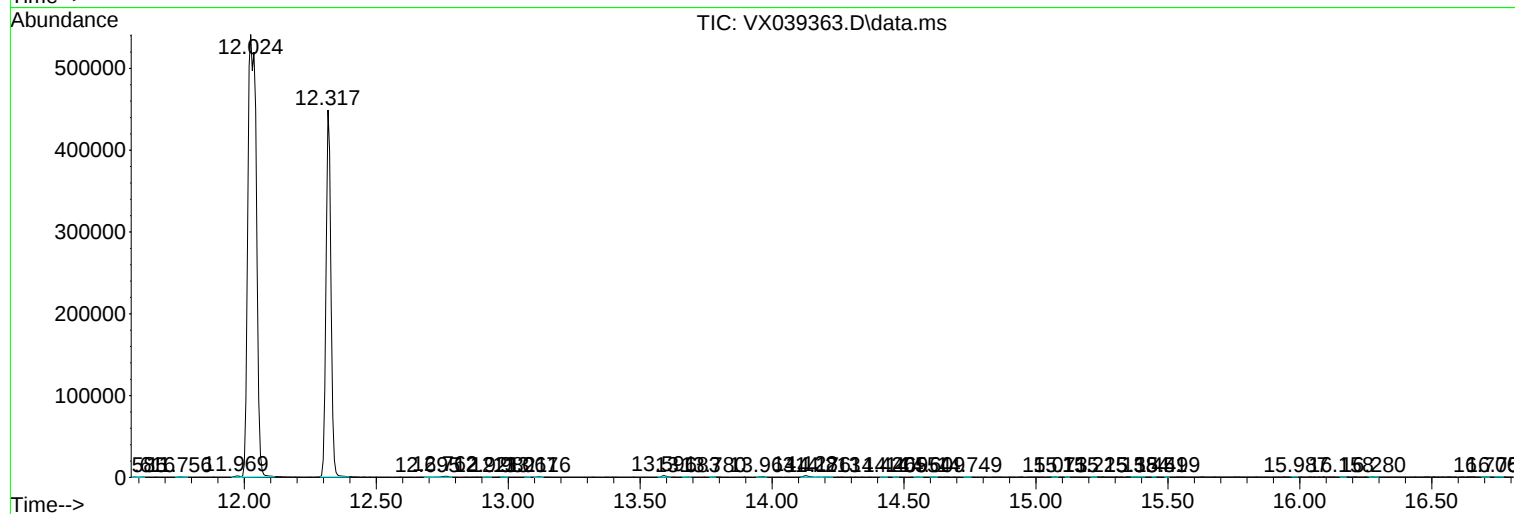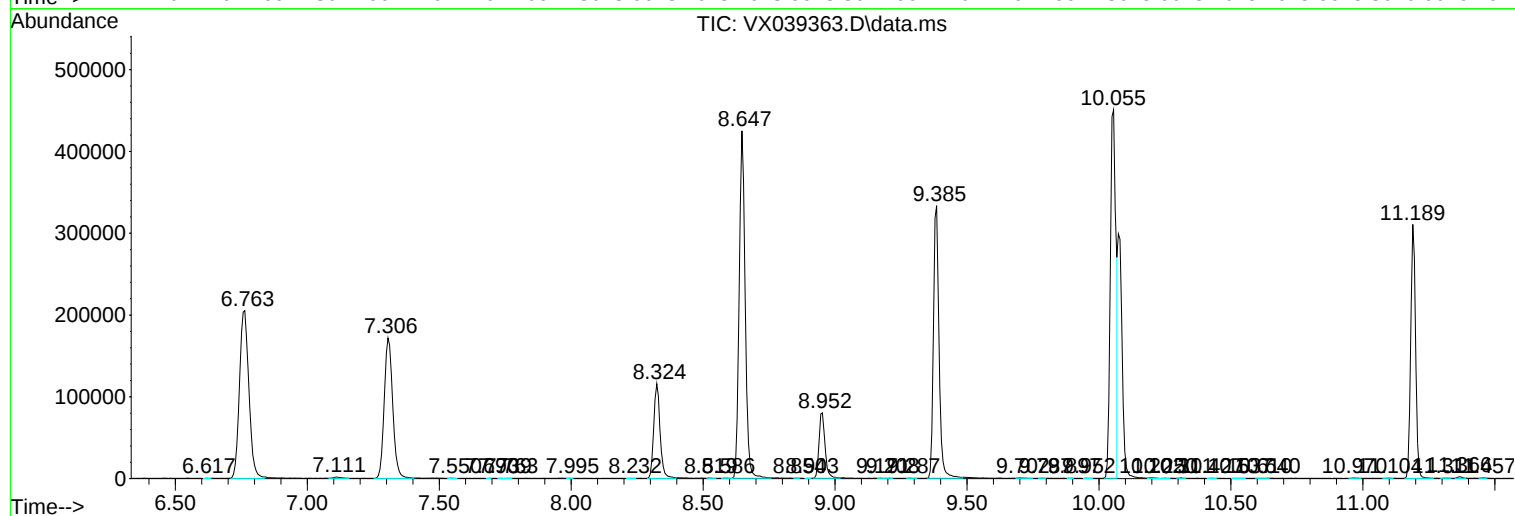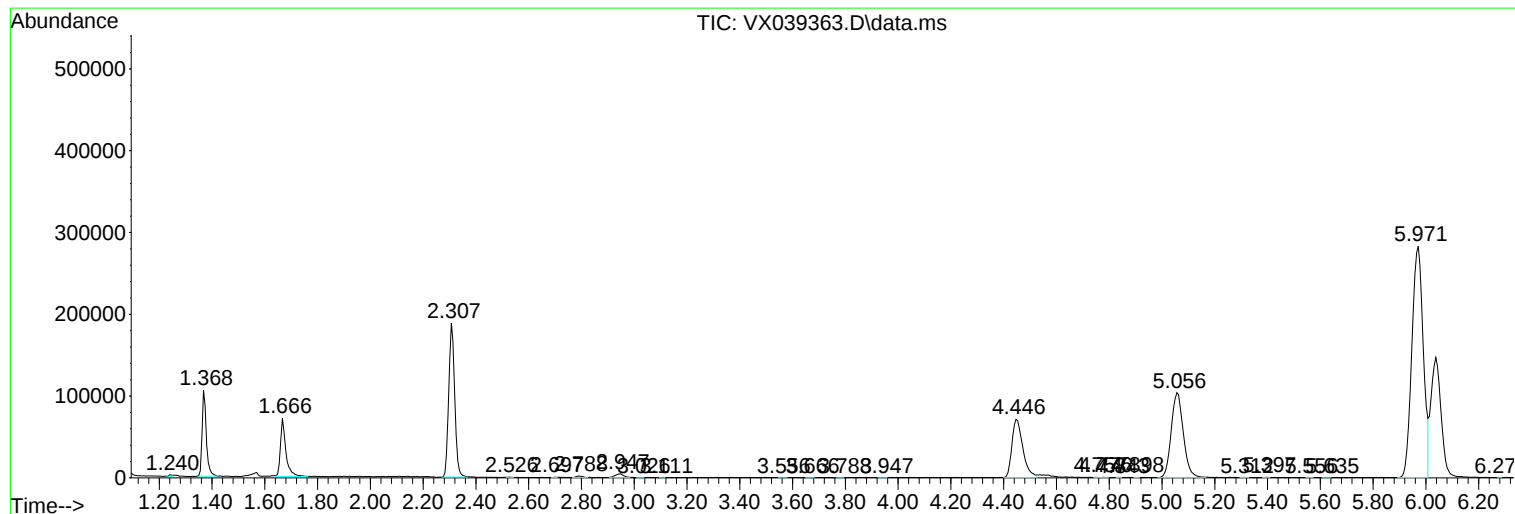

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
Data File : VX039363.D
Acq On : 19 Dec 2023 17:50
Operator : JC/MD
Sample : 05808-01 40X
Misc : 2.75g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0B22

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
Data File : VX039363.D
Acq On : 19 Dec 2023 17:50
Operator : JC/MD
Sample : 05808-01 40X
Misc : 2.75g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0B22

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
