

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
 Data File : VX039364.D
 Acq On : 19 Dec 2023 18:13
 Operator : JC/MD
 Sample : 05808-08 100X
 Misc : 4.19g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0B02

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

Signal : TIC: VX039364.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.367	43	46	56	rVB	101498	112223	13.44%	1.688%
2	1.672	91	96	107	rBV	67226	99366	11.90%	1.495%
3	2.306	194	200	210	rBV	180450	284782	34.11%	4.284%
4	2.788	275	279	286	rVV5	2064	4020	0.48%	0.060%
5	2.867	286	292	297	rVV3	1394	3033	0.36%	0.046%
6	2.940	298	304	312	rVB	4767	9997	1.20%	0.150%
7	3.093	327	329	331	rBV2	351	306	0.04%	0.005%
8	3.123	331	334	337	rVB2	375	493	0.06%	0.007%
9	3.343	364	370	371	rBV	363	340	0.04%	0.005%
10	3.611	411	414	417	rBV	189	226	0.03%	0.003%
11	3.763	434	439	442	rBV2	219	407	0.05%	0.006%
12	3.824	446	449	454	rBV2	239	232	0.03%	0.003%
13	3.971	470	473	474	rBV	223	184	0.02%	0.003%
14	4.099	491	494	498	rBV	277	286	0.03%	0.004%
15	4.446	543	551	564	rBV	71651	207696	24.88%	3.124%
16	4.855	615	618	619	rBV2	222	184	0.02%	0.003%
17	5.056	639	651	672	rVV	102802	324327	38.85%	4.879%
18	5.208	674	676	679	rVV2	333	279	0.03%	0.004%
19	5.391	703	706	709	rBV3	332	573	0.07%	0.009%
20	5.470	717	719	720	rBV	356	206	0.02%	0.003%
21	5.550	726	732	735	rBV3	407	820	0.10%	0.012%
22	5.970	785	801	817	rBV2	277914	834835	100.00%	12.559%
23	6.202	836	839	842	rBV2	226	249	0.03%	0.004%
24	6.251	846	847	851	rVB2	275	244	0.03%	0.004%
25	6.312	855	857	862	rVB2	254	323	0.04%	0.005%
26	6.635	908	910	912	rVB	253	189	0.02%	0.003%
27	6.665	912	915	917	rBV2	181	203	0.02%	0.003%
28	6.763	921	931	947	rBV	197736	483692	57.94%	7.276%
29	7.116	983	989	996	rVV3	1610	3107	0.37%	0.047%
30	7.305	1012	1020	1036	rBV	175949	379145	45.42%	5.704%
31	7.476	1047	1048	1049	rBV	387	196	0.02%	0.003%
32	7.525	1054	1056	1059	rBV2	213	247	0.03%	0.004%
33	7.708	1084	1086	1089	rVV	306	253	0.03%	0.004%
34	7.750	1091	1093	1096	rVB2	225	216	0.03%	0.003%
35	8.043	1137	1141	1142	rBV2	235	184	0.02%	0.003%
36	8.141	1156	1157	1160	rBV2	221	213	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
 Data File : VX039364.D
 Acq On : 19 Dec 2023 18:13
 Operator : JC/MD
 Sample : 05808-08 100X
 Misc : 4.19g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0B02

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
 Title : VOC Analysis

37	8.323	1181	1187	1205	rBV	116729	190808	22.86%	2.870%
38	8.537	1220	1222	1225	rVB2	258	204	0.02%	0.003%
39	8.586	1225	1230	1233	rBV3	343	659	0.08%	0.010%
40	8.647	1233	1240	1258	rBV	404967	650354	77.90%	9.783%
41	8.951	1284	1290	1308	rVB	82980	125293	15.01%	1.885%
42	9.384	1355	1361	1371	rBV	335063	488055	58.46%	7.342%
43	9.646	1403	1404	1407	rBV2	267	330	0.04%	0.005%
44	9.756	1420	1422	1425	rVB3	250	209	0.03%	0.003%
45	9.909	1446	1447	1451	rBV	178	178	0.02%	0.003%
46	10.055	1465	1471	1486	rBV	422770	616189	73.81%	9.269%
47	10.201	1491	1495	1498	rVB2	586	719	0.09%	0.011%
48	10.238	1500	1501	1504	rBV2	282	281	0.03%	0.004%
49	10.305	1510	1512	1513	rBV2	359	330	0.04%	0.005%
50	10.646	1564	1568	1572	rBV3	361	536	0.06%	0.008%
51	10.963	1618	1620	1624	rVB2	264	332	0.04%	0.005%
52	11.128	1645	1647	1649	rBV2	255	195	0.02%	0.003%
53	11.189	1651	1657	1664	rBV	309029	397861	47.66%	5.985%
54	11.305	1672	1676	1677	rBV2	239	312	0.04%	0.005%
55	11.317	1677	1678	1681	rVV	465	328	0.04%	0.005%
56	11.353	1683	1684	1687	rVV2	275	212	0.03%	0.003%
57	11.414	1690	1694	1697	rVB2	278	334	0.04%	0.005%
58	11.451	1697	1700	1704	rBV3	306	522	0.06%	0.008%
59	11.573	1715	1720	1723	rBV2	278	448	0.05%	0.007%
60	11.872	1766	1769	1772	rBV2	221	269	0.03%	0.004%
61	11.975	1781	1786	1788	rBV2	4669	5931	0.71%	0.089%
62	12.024	1788	1794	1804	rVB	456529	630283	75.50%	9.482%
63	12.164	1813	1817	1819	rVB3	229	341	0.04%	0.005%
64	12.231	1825	1828	1831	rBV2	241	297	0.04%	0.004%
65	12.317	1837	1842	1852	rBV	438540	575040	68.88%	8.650%
66	12.426	1859	1860	1863	rVB	370	224	0.03%	0.003%
67	12.457	1863	1865	1871	rVB2	318	358	0.04%	0.005%
68	12.518	1871	1875	1876	rBV2	255	218	0.03%	0.003%
69	12.664	1897	1899	1901	rBV2	250	200	0.02%	0.003%
70	12.707	1901	1906	1909	rVB2	197	309	0.04%	0.005%
71	12.762	1911	1915	1919	rVV3	1097	1656	0.20%	0.025%
72	12.804	1919	1922	1924	rVV2	138	181	0.02%	0.003%
73	12.896	1932	1937	1938	rBV2	261	292	0.03%	0.004%
74	12.993	1951	1953	1956	rBV2	262	288	0.03%	0.004%
75	13.066	1962	1965	1967	rVV2	352	379	0.05%	0.006%
76	13.115	1970	1973	1976	rBV2	427	509	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
 Data File : VX039364.D
 Acq On : 19 Dec 2023 18:13
 Operator : JC/MD
 Sample : 05808-08 100X
 Misc : 4.19g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0B02

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

77	13.195	1982	1986	1989	rVV	221	275	0.03%	0.004%
78	13.347	2009	2011	2015	rVB2	253	274	0.03%	0.004%
79	13.524	2038	2040	2044	rVB2	245	252	0.03%	0.004%
80	13.585	2046	2050	2060	rVV	87750	113307	13.57%	1.705%
81	13.957	2107	2111	2121	rVB	27229	36861	4.42%	0.555%
82	14.042	2123	2125	2130	rVV2	203	258	0.03%	0.004%
83	14.127	2136	2139	2143	rVV	2082	2260	0.27%	0.034%
84	14.182	2145	2148	2149	rBV2	204	208	0.02%	0.003%
85	14.341	2172	2174	2177	rVB2	192	178	0.02%	0.003%
86	14.371	2177	2179	2181	rBV2	171	195	0.02%	0.003%
87	14.597	2215	2216	2218	rBV2	220	184	0.02%	0.003%
88	14.627	2218	2221	2224	rVB2	349	367	0.04%	0.006%
89	14.725	2235	2237	2239	rVV	246	180	0.02%	0.003%
90	14.780	2241	2246	2252	rBV4	4311	7451	0.89%	0.112%
91	14.956	2271	2275	2276	rBV2	356	379	0.05%	0.006%
92	14.975	2276	2278	2283	rVV2	259	398	0.05%	0.006%
93	15.078	2293	2295	2297	rBV	330	232	0.03%	0.003%
94	15.121	2299	2302	2304	rBV2	242	243	0.03%	0.004%
95	15.158	2304	2308	2310	rBV3	211	290	0.03%	0.004%
96	15.249	2318	2323	2328	rBV2	27747	37932	4.54%	0.571%
97	15.334	2335	2337	2339	rBV2	250	264	0.03%	0.004%
98	16.121	2465	2466	2467	rBV	263	188	0.02%	0.003%
99	16.340	2499	2502	2504	rBV2	452	389	0.05%	0.006%
100	16.450	2519	2520	2522	rBV	239	193	0.02%	0.003%




Sum of corrected areas: 6647498

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
Data File : VX039364.D
Acq On : 19 Dec 2023 18:13
Operator : JC/MD
Sample : 05808-08 100X
Misc : 4.19g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0B02

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

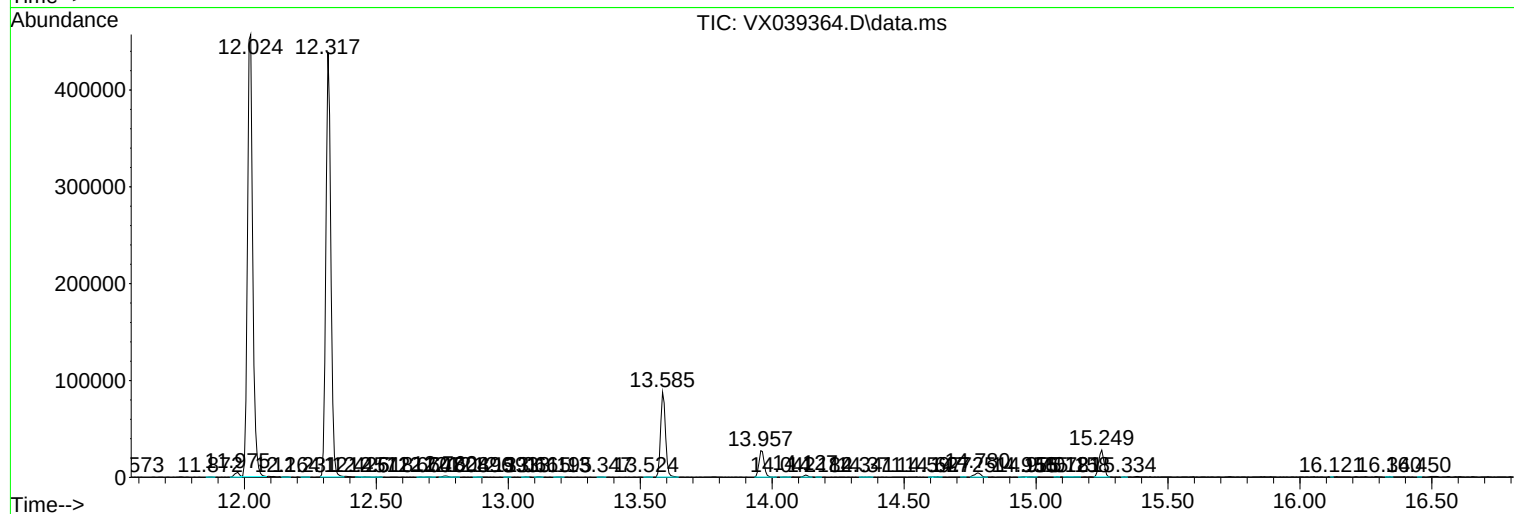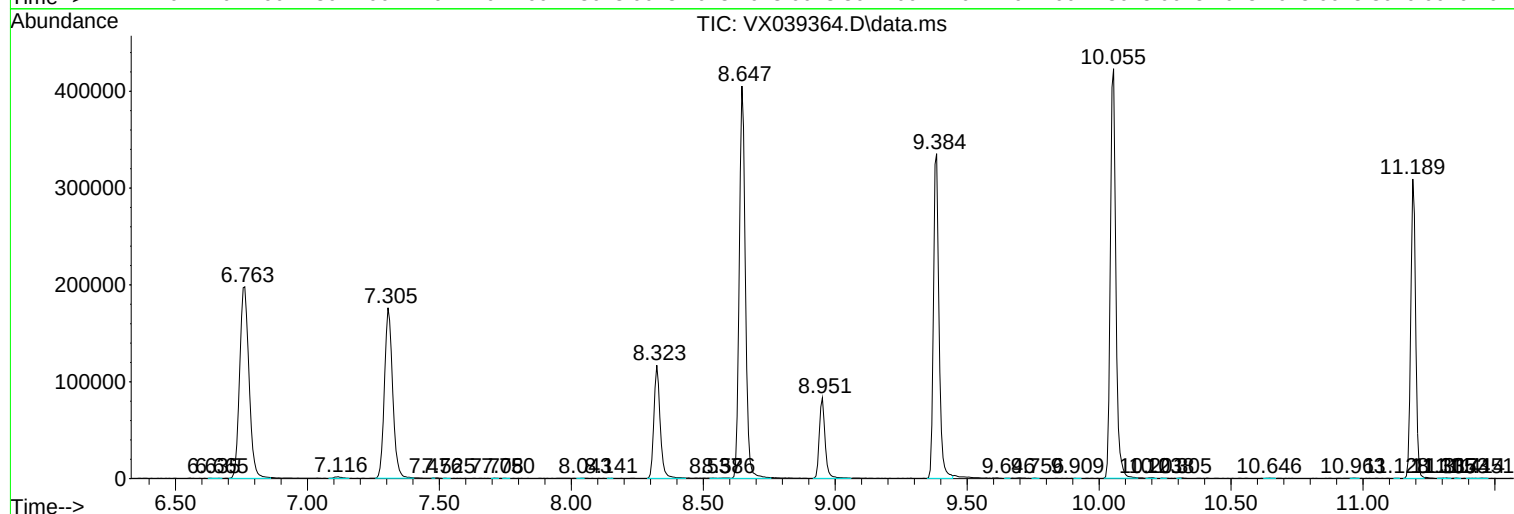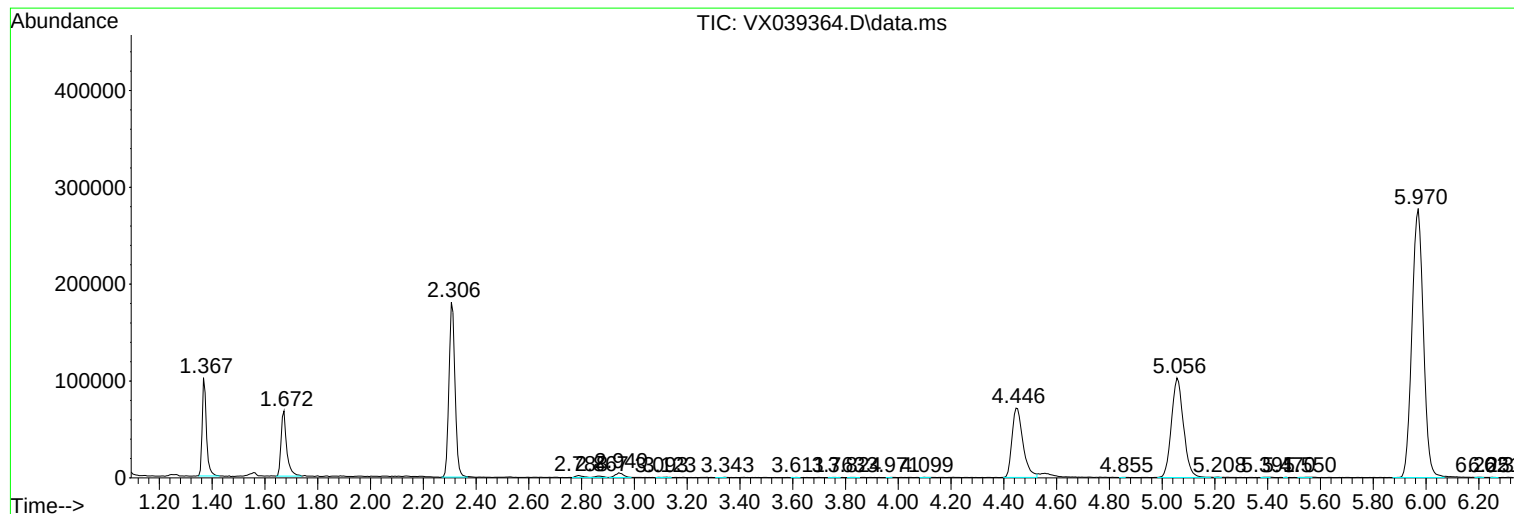

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
Data File : VX039364.D
Acq On : 19 Dec 2023 18:13
Operator : JC/MD
Sample : 05808-08 100X
Misc : 4.19g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0B02

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
Data File : VX039364.D
Acq On : 19 Dec 2023 18:13
Operator : JC/MD
Sample : 05808-08 100X
Misc : 4.19g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0B02

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc