

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
 Data File : VX039365.D
 Acq On : 19 Dec 2023 18:35
 Operator : JC/MD
 Sample : 05808-18 100X
 Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0B14

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M

Title : VOC Analysis

Signal : TIC: VX039365.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	43	46	56	rBV	101863	113019	14.04%	1.826%
2	1.672	91	96	106	rBV	63115	93448	11.61%	1.509%
3	2.306	194	200	211	rBV	174858	279950	34.79%	4.522%
4	2.569	241	243	245	rVB	421	289	0.04%	0.005%
5	2.794	274	280	286	rBV4	1841	3984	0.50%	0.064%
6	2.861	286	291	299	rVV2	2526	5602	0.70%	0.090%
7	2.947	299	305	314	rVB2	3445	7748	0.96%	0.125%
8	3.111	329	332	335	rVV3	289	352	0.04%	0.006%
9	3.367	372	374	376	rVB	241	168	0.02%	0.003%
10	3.459	387	389	391	rBV2	205	213	0.03%	0.003%
11	3.520	397	399	401	rBV2	278	228	0.03%	0.004%
12	3.550	401	404	405	rBV2	230	222	0.03%	0.004%
13	3.971	464	473	477	rBV2	244	610	0.08%	0.010%
14	4.013	477	480	481	rBV2	195	218	0.03%	0.004%
15	4.221	512	514	517	rBV2	150	198	0.02%	0.003%
16	4.446	543	551	565	rBV	71102	201001	24.98%	3.247%
17	4.751	600	601	604	rBV	228	201	0.02%	0.003%
18	4.879	620	622	624	rBV	418	221	0.03%	0.004%
19	5.056	639	651	669	rBV	101045	314280	39.05%	5.077%
20	5.385	704	705	707	rBV	184	191	0.02%	0.003%
21	5.678	752	753	758	rVB2	198	219	0.03%	0.004%
22	5.970	789	801	815	rBV2	264633	804792	100.00%	13.000%
23	6.287	850	853	854	rBV2	278	307	0.04%	0.005%
24	6.306	854	856	858	rVB	278	225	0.03%	0.004%
25	6.342	861	862	866	rVB	275	199	0.02%	0.003%
26	6.385	866	869	871	rBV2	221	271	0.03%	0.004%
27	6.464	879	882	883	rBV	201	183	0.02%	0.003%
28	6.495	886	887	891	rVB	279	244	0.03%	0.004%
29	6.604	903	905	908	rBV2	202	214	0.03%	0.003%
30	6.757	922	930	943	rBV	185613	450765	56.01%	7.281%
31	7.110	984	988	989	rBV4	1327	1600	0.20%	0.026%
32	7.306	1011	1020	1037	rBV	164062	366820	45.58%	5.925%
33	7.482	1045	1049	1051	rBV3	659	841	0.10%	0.014%
34	7.549	1058	1060	1061	rBV	332	172	0.02%	0.003%
35	7.623	1070	1072	1075	rBV2	134	196	0.02%	0.003%
36	7.744	1090	1092	1094	rVB	253	192	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
 Data File : VX039365.D
 Acq On : 19 Dec 2023 18:35
 Operator : JC/MD
 Sample : 05808-18 100X
 Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0B14

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
 Title : VOC Analysis

37	7.830	1103	1106	1107	rBV2	224	230	0.03%	0.004%
38	7.860	1110	1111	1113	rBV2	214	191	0.02%	0.003%
39	8.159	1158	1160	1163	rBV	156	176	0.02%	0.003%
40	8.263	1173	1177	1179	rBV2	208	198	0.02%	0.003%
41	8.324	1181	1187	1200	rVV	108519	181686	22.58%	2.935%
42	8.476	1211	1212	1215	rVB	261	227	0.03%	0.004%
43	8.525	1219	1220	1224	rVB	468	441	0.05%	0.007%
44	8.574	1224	1228	1229	rBV2	422	529	0.07%	0.009%
45	8.647	1234	1240	1256	rBV	397941	626957	77.90%	10.127%
46	8.848	1272	1273	1275	rBV	413	215	0.03%	0.003%
47	8.952	1284	1290	1304	rBV	75225	119738	14.88%	1.934%
48	9.110	1314	1316	1318	rBV2	237	240	0.03%	0.004%
49	9.238	1336	1337	1340	rBV2	295	333	0.04%	0.005%
50	9.384	1355	1361	1376	rBV	311145	472162	58.67%	7.627%
51	9.701	1409	1413	1415	rBV3	446	518	0.06%	0.008%
52	9.720	1415	1416	1421	rVB	273	201	0.02%	0.003%
53	10.012	1462	1464	1465	rBV2	239	171	0.02%	0.003%
54	10.055	1465	1471	1483	rBV	395679	574033	71.33%	9.273%
55	10.189	1491	1493	1496	rVB3	527	509	0.06%	0.008%
56	10.262	1503	1505	1510	rBV	276	311	0.04%	0.005%
57	10.311	1510	1513	1516	rBV2	382	513	0.06%	0.008%
58	10.463	1536	1538	1541	rBV	213	172	0.02%	0.003%
59	10.585	1554	1558	1560	rBV	218	175	0.02%	0.003%
60	10.616	1562	1563	1565	rBV	205	171	0.02%	0.003%
61	10.640	1565	1567	1568	rVV2	237	201	0.02%	0.003%
62	10.677	1570	1573	1575	rVV	146	198	0.02%	0.003%
63	10.720	1577	1580	1582	rBV2	257	246	0.03%	0.004%
64	10.781	1588	1590	1591	rBV	198	167	0.02%	0.003%
65	10.829	1594	1598	1599	rBV2	163	174	0.02%	0.003%
66	10.963	1618	1620	1626	rVB3	296	506	0.06%	0.008%
67	11.189	1652	1657	1672	rVB	303400	389698	48.42%	6.295%
68	11.421	1694	1695	1698	rBV2	248	202	0.03%	0.003%
69	11.451	1698	1700	1704	rVV2	378	451	0.06%	0.007%
70	11.640	1729	1731	1733	rBV2	144	158	0.02%	0.003%
71	11.689	1737	1739	1742	rBV	184	177	0.02%	0.003%
72	11.811	1757	1759	1762	rBV2	213	270	0.03%	0.004%
73	11.975	1782	1786	1788	rBV2	1442	1709	0.21%	0.028%
74	12.018	1788	1793	1804	rVV	411028	573184	71.22%	9.259%
75	12.317	1837	1842	1852	rBV	432003	546960	67.96%	8.835%
76	12.469	1865	1867	1870	rBV2	231	229	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
 Data File : VX039365.D
 Acq On : 19 Dec 2023 18:35
 Operator : JC/MD
 Sample : 05808-18 100X
 Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0B14

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

77	12.530	1873	1877	1879	rBV2	218	261	0.03%	0.004%
78	12.609	1886	1890	1891	rBV	194	229	0.03%	0.004%
79	12.756	1909	1914	1919	rBV4	1281	2047	0.25%	0.033%
80	12.823	1923	1925	1929	rVV2	219	297	0.04%	0.005%
81	12.914	1939	1940	1943	rVV	244	160	0.02%	0.003%
82	13.054	1962	1963	1967	rVB2	299	254	0.03%	0.004%
83	13.329	2007	2008	2010	rVV	297	179	0.02%	0.003%
84	13.371	2013	2015	2018	rBV	296	191	0.02%	0.003%
85	13.512	2035	2038	2042	rVB2	209	315	0.04%	0.005%
86	13.585	2046	2050	2058	rVB2	15330	20163	2.51%	0.326%
87	13.963	2108	2112	2118	rVB2	4954	6548	0.81%	0.106%
88	14.127	2135	2139	2145	rVB	1537	2257	0.28%	0.036%
89	14.323	2168	2171	2175	rBV	241	248	0.03%	0.004%
90	14.536	2204	2206	2209	rBV2	237	251	0.03%	0.004%
91	14.560	2209	2210	2212	rBV	260	212	0.03%	0.003%
92	14.780	2241	2246	2249	rVV4	606	1009	0.13%	0.016%
93	14.847	2254	2257	2258	rBV	195	196	0.02%	0.003%
94	15.024	2284	2286	2288	rBV2	190	195	0.02%	0.003%
95	15.207	2314	2316	2318	rBV2	247	240	0.03%	0.004%
96	15.249	2318	2323	2328	rVV3	7195	10272	1.28%	0.166%
97	15.304	2330	2332	2333	rBV2	211	160	0.02%	0.003%
98	16.194	2476	2478	2481	rBV2	283	279	0.03%	0.005%
99	16.426	2515	2516	2520	rBV2	248	334	0.04%	0.005%
100	16.560	2536	2538	2541	rBV3	316	384	0.05%	0.006%




Sum of corrected areas: 6190691

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
Data File : VX039365.D
Acq On : 19 Dec 2023 18:35
Operator : JC/MD
Sample : 05808-18 100X
Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0B14

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

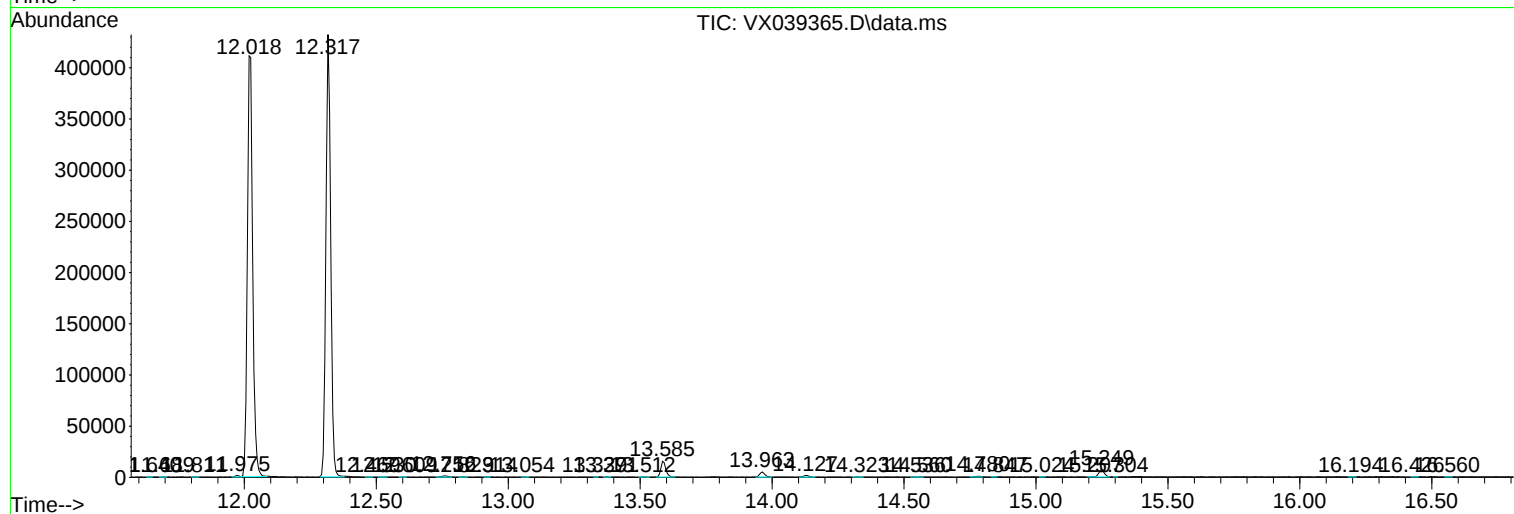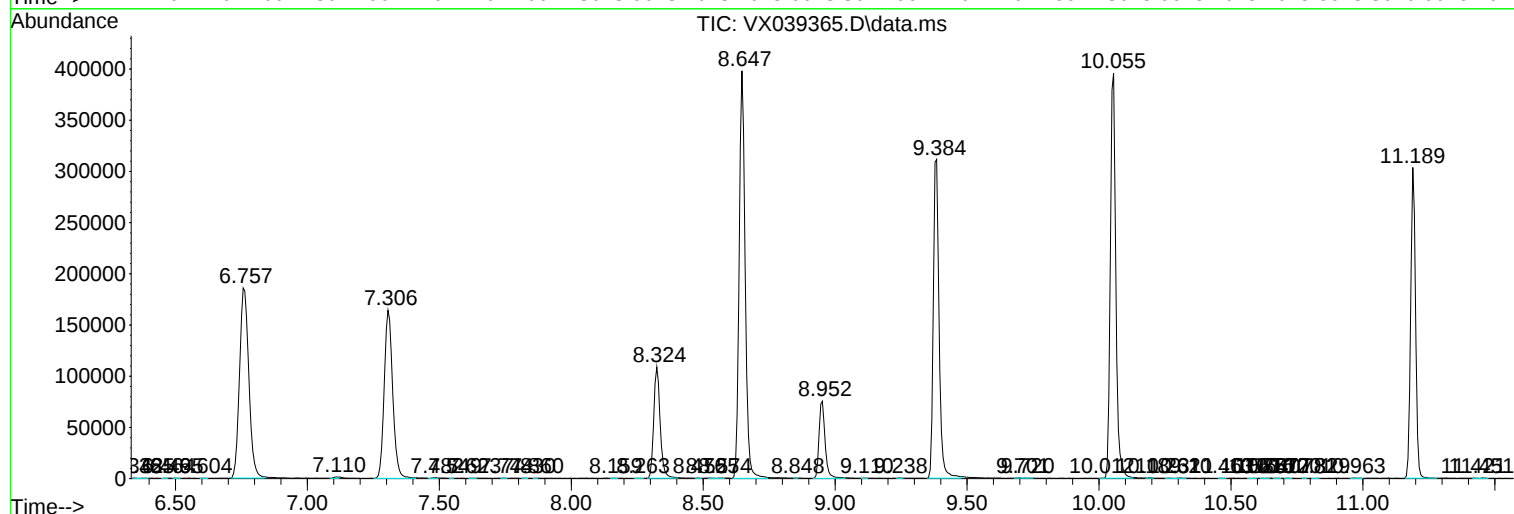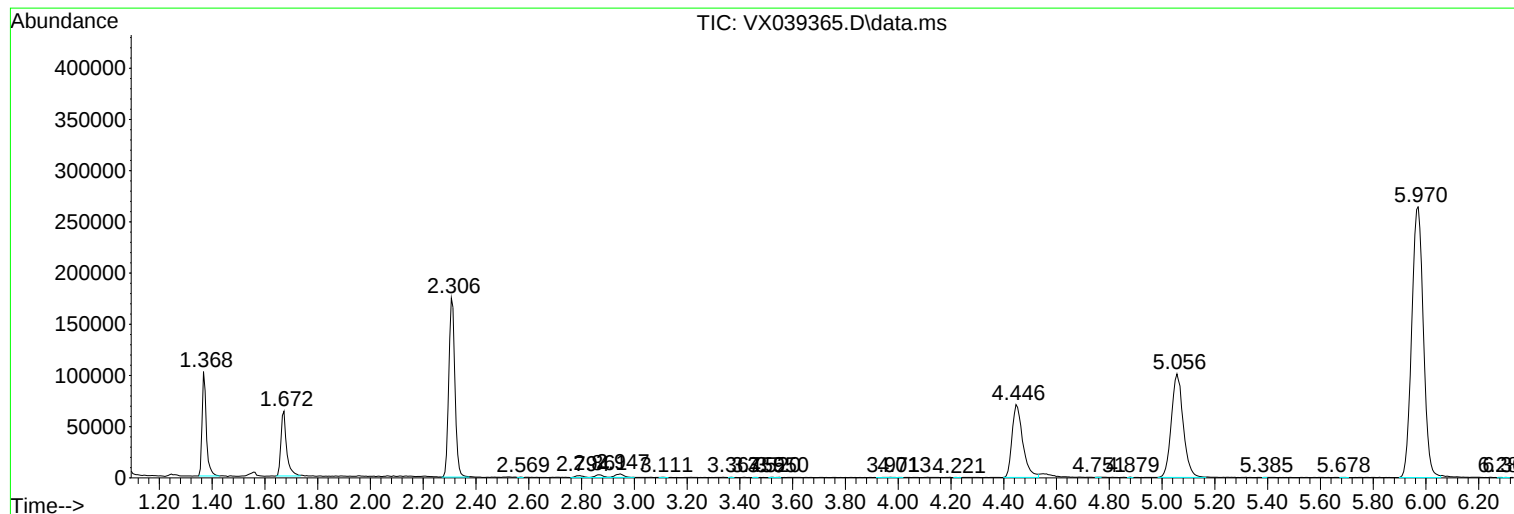

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
Data File : VX039365.D
Acq On : 19 Dec 2023 18:35
Operator : JC/MD
Sample : 05808-18 100X
Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0B14

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
Data File : VX039365.D
Acq On : 19 Dec 2023 18:35
Operator : JC/MD
Sample : 05808-18 100X
Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0B14

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc