

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
 Data File : VX039375.D
 Acq On : 19 Dec 2023 22:23
 Operator : JC/MD
 Sample : 05807-13 10X
 Misc : 1.26g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0AZ5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

Signal : TIC: VX039375.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	43	46	57	rVB	96460	103327	6.01%	1.286%
2	1.660	90	94	109	rVB	59804	93288	5.42%	1.161%
3	2.306	194	200	210	rBV	167504	263388	15.32%	3.278%
4	2.593	245	247	248	rBV2	169	152	0.01%	0.002%
5	2.697	263	264	271	rVB2	659	835	0.05%	0.010%
6	2.788	274	279	287	rBV3	2707	5398	0.31%	0.067%
7	2.855	287	290	291	rBV2	756	700	0.04%	0.009%
8	2.947	297	305	316	rVB2	7540	18524	1.08%	0.231%
9	3.038	318	320	322	rVB	233	140	0.01%	0.002%
10	3.562	404	406	409	rBV2	167	157	0.01%	0.002%
11	4.001	471	478	479	rBV	229	382	0.02%	0.005%
12	4.129	497	499	502	rBV	220	301	0.02%	0.004%
13	4.337	531	533	536	rBV2	142	178	0.01%	0.002%
14	4.446	541	551	569	rBV	66836	198999	11.57%	2.477%
15	4.769	601	604	607	rVB2	413	530	0.03%	0.007%
16	4.800	607	609	610	rBV	497	339	0.02%	0.004%
17	5.056	637	651	669	rBV	96282	306736	17.84%	3.818%
18	5.269	684	686	688	rBV	223	159	0.01%	0.002%
19	5.343	694	698	701	rBV2	151	185	0.01%	0.002%
20	5.385	704	705	708	rVB	306	221	0.01%	0.003%
21	5.556	731	733	735	rVB	286	171	0.01%	0.002%
22	5.611	740	742	743	rBV2	160	161	0.01%	0.002%
23	5.788	767	771	772	rBV	175	260	0.02%	0.003%
24	5.830	775	778	780	rBV2	126	179	0.01%	0.002%
25	5.964	788	800	822	rBV2	256737	788368	45.84%	9.812%
26	6.214	839	841	843	rBV3	251	194	0.01%	0.002%
27	6.263	846	849	850	rBV	322	259	0.02%	0.003%
28	6.397	869	871	874	rVB	191	179	0.01%	0.002%
29	6.446	877	879	882	rVV	249	258	0.02%	0.003%
30	6.501	886	888	891	rVB2	149	186	0.01%	0.002%
31	6.537	891	894	896	rBV2	337	362	0.02%	0.005%
32	6.641	908	911	913	rBV2	152	161	0.01%	0.002%
33	6.757	922	930	945	rBV	193704	461704	26.85%	5.746%
34	7.025	972	974	977	rBV3	260	345	0.02%	0.004%
35	7.062	978	980	982	rVB	329	172	0.01%	0.002%
36	7.117	985	989	993	rVV3	990	1592	0.09%	0.020%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
 Data File : VX039375.D
 Acq On : 19 Dec 2023 22:23
 Operator : JC/MD
 Sample : 05807-13 10X
 Misc : 1.26g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0AZ5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM120523WMA.M
 Title : VOC Analysis

37	7.251	1009	1011	1012	rBV	243	181	0.01%	0.002%
38	7.306	1012	1020	1039	rVV	159241	353720	20.57%	4.402%
39	8.141	1155	1157	1159	rBV2	194	194	0.01%	0.002%
40	8.324	1181	1187	1199	rBV	106936	175841	10.22%	2.188%
41	8.494	1211	1215	1218	rBV3	319	591	0.03%	0.007%
42	8.647	1233	1240	1257	rBV	381513	612138	35.59%	7.618%
43	8.952	1284	1290	1303	rBV	74234	113150	6.58%	1.408%
44	9.098	1312	1314	1317	rVB2	311	210	0.01%	0.003%
45	9.275	1340	1343	1344	rBV	270	330	0.02%	0.004%
46	9.336	1351	1353	1355	rBV2	152	175	0.01%	0.002%
47	9.384	1355	1361	1378	rBV	321220	469216	27.28%	5.840%
48	9.702	1410	1413	1416	rVV3	450	580	0.03%	0.007%
49	9.756	1420	1422	1424	rBV	182	203	0.01%	0.003%
50	9.915	1446	1448	1449	rVB2	222	153	0.01%	0.002%
51	9.951	1451	1454	1457	rBV2	185	182	0.01%	0.002%
52	10.006	1460	1463	1465	rBV	145	153	0.01%	0.002%
53	10.055	1465	1471	1472	rBV	436069	572917	33.31%	7.130%
54	10.305	1509	1512	1514	rBV2	435	450	0.03%	0.006%
55	10.342	1517	1518	1521	rBV	145	150	0.01%	0.002%
56	10.604	1559	1561	1563	rBV	143	151	0.01%	0.002%
57	10.732	1581	1582	1587	rBV2	227	185	0.01%	0.002%
58	10.781	1589	1590	1592	rVV	255	145	0.01%	0.002%
59	10.799	1592	1593	1597	rVV2	237	214	0.01%	0.003%
60	10.909	1608	1611	1614	rVB2	199	274	0.02%	0.003%
61	10.939	1614	1616	1617	rBV	188	146	0.01%	0.002%
62	10.963	1618	1620	1626	rVB2	399	581	0.03%	0.007%
63	11.043	1629	1633	1634	rBV2	144	183	0.01%	0.002%
64	11.189	1652	1657	1670	rVV	301869	387257	22.52%	4.820%
65	11.293	1672	1674	1675	rBV	178	173	0.01%	0.002%
66	11.317	1675	1678	1682	rVB3	591	741	0.04%	0.009%
67	11.396	1688	1691	1692	rBV	152	191	0.01%	0.002%
68	11.524	1710	1712	1714	rBV2	163	197	0.01%	0.002%
69	11.640	1729	1731	1734	rBV2	175	238	0.01%	0.003%
70	11.695	1739	1740	1743	rBB2	164	163	0.01%	0.002%
71	11.969	1780	1785	1789	rBV	86215	109152	6.35%	1.358%
72	12.036	1789	1796	1807	rVB2	898572	1719789	100.00%	21.404%
73	12.232	1826	1828	1829	rBV2	170	152	0.01%	0.002%
74	12.329	1837	1844	1861	rBV2	595830	1132516	65.85%	14.095%
75	12.695	1902	1904	1909	rBV3	239	345	0.02%	0.004%
76	12.762	1911	1915	1920	rVB	2561	3342	0.19%	0.042%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
 Data File : VX039375.D
 Acq On : 19 Dec 2023 22:23
 Operator : JC/MD
 Sample : 05807-13 10X
 Misc : 1.26g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0AZ5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
 Title : VOC Analysis

77	12.927	1938	1942	1946	rBV4	2790	3887	0.23%	0.048%
78	13.109	1969	1972	1978	rBV2	320	467	0.03%	0.006%
79	13.152	1978	1979	1983	rVV	240	207	0.01%	0.003%
80	13.201	1983	1987	1991	rVV3	1414	1678	0.10%	0.021%
81	13.585	2045	2050	2057	rBV	77477	98988	5.76%	1.232%
82	13.780	2079	2082	2089	rVB3	671	1053	0.06%	0.013%
83	13.963	2108	2112	2119	rBV3	10924	15179	0.88%	0.189%
84	14.128	2134	2139	2146	rVB	3404	4444	0.26%	0.055%
85	14.213	2151	2153	2155	rBV	208	181	0.01%	0.002%
86	14.396	2182	2183	2187	rBV2	196	148	0.01%	0.002%
87	14.463	2190	2194	2196	rVB2	254	337	0.02%	0.004%
88	14.506	2200	2201	2205	rBV	198	258	0.02%	0.003%
89	14.603	2214	2217	2220	rBV2	341	380	0.02%	0.005%
90	14.634	2220	2222	2224	rVB	361	187	0.01%	0.002%
91	14.658	2224	2226	2227	rBV	262	198	0.01%	0.002%
92	14.713	2234	2235	2240	rVV	185	217	0.01%	0.003%
93	15.024	2285	2286	2287	rBV	330	148	0.01%	0.002%
94	15.329	2334	2336	2337	rBV	263	181	0.01%	0.002%
95	15.627	2383	2385	2387	rBV	297	187	0.01%	0.002%
96	15.725	2399	2401	2402	rVB	354	148	0.01%	0.002%
97	15.847	2419	2421	2424	rBV	338	372	0.02%	0.005%
98	15.938	2435	2436	2438	rBV2	256	207	0.01%	0.003%
99	16.182	2475	2476	2479	rBV2	327	262	0.02%	0.003%
100	16.767	2568	2572	2575	rBV3	321	458	0.03%	0.006%




Sum of corrected areas: 8034931

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
Data File : VX039375.D
Acq On : 19 Dec 2023 22:23
Operator : JC/MD
Sample : 05807-13 10X
Misc : 1.26g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0AZ5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

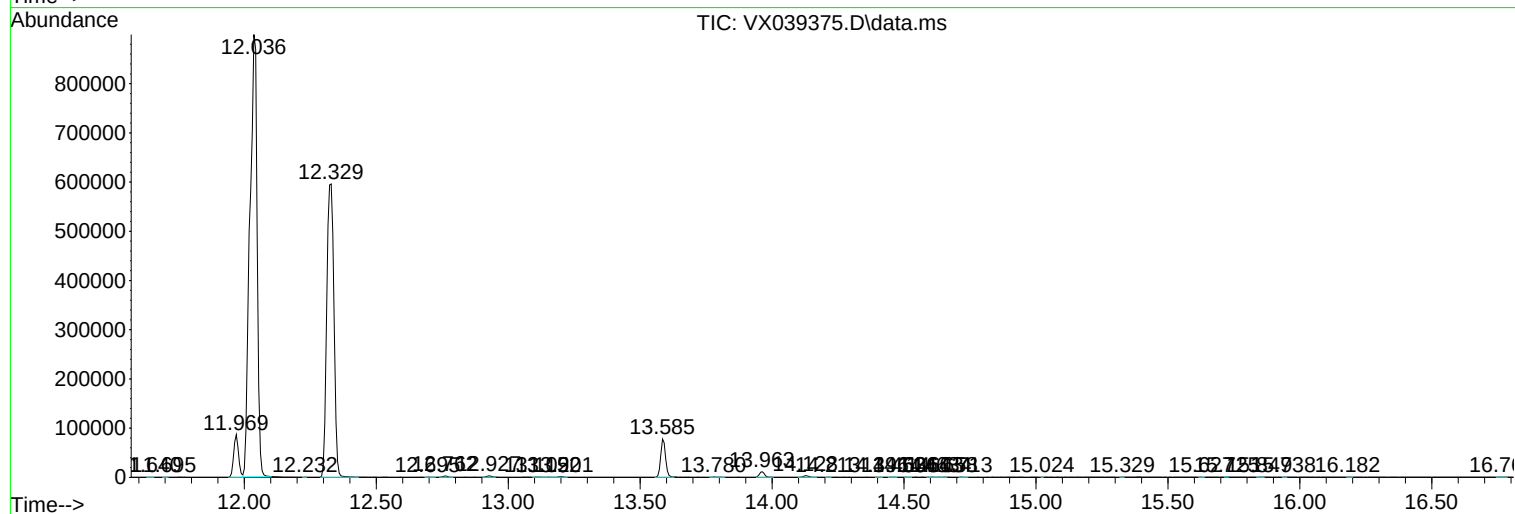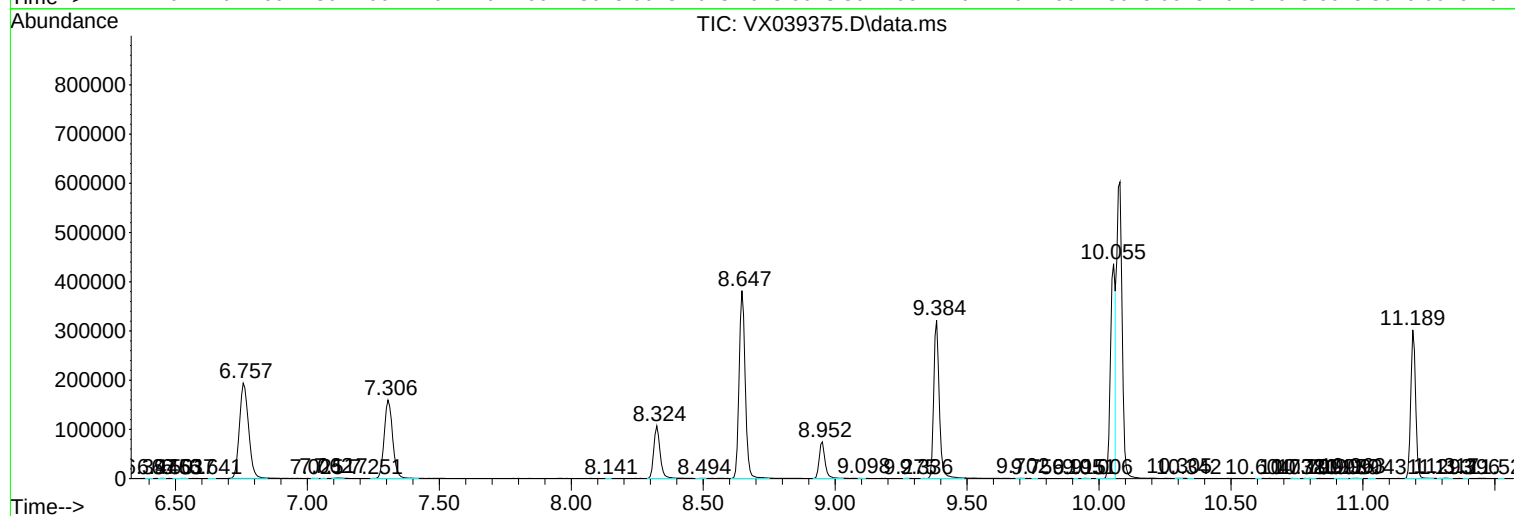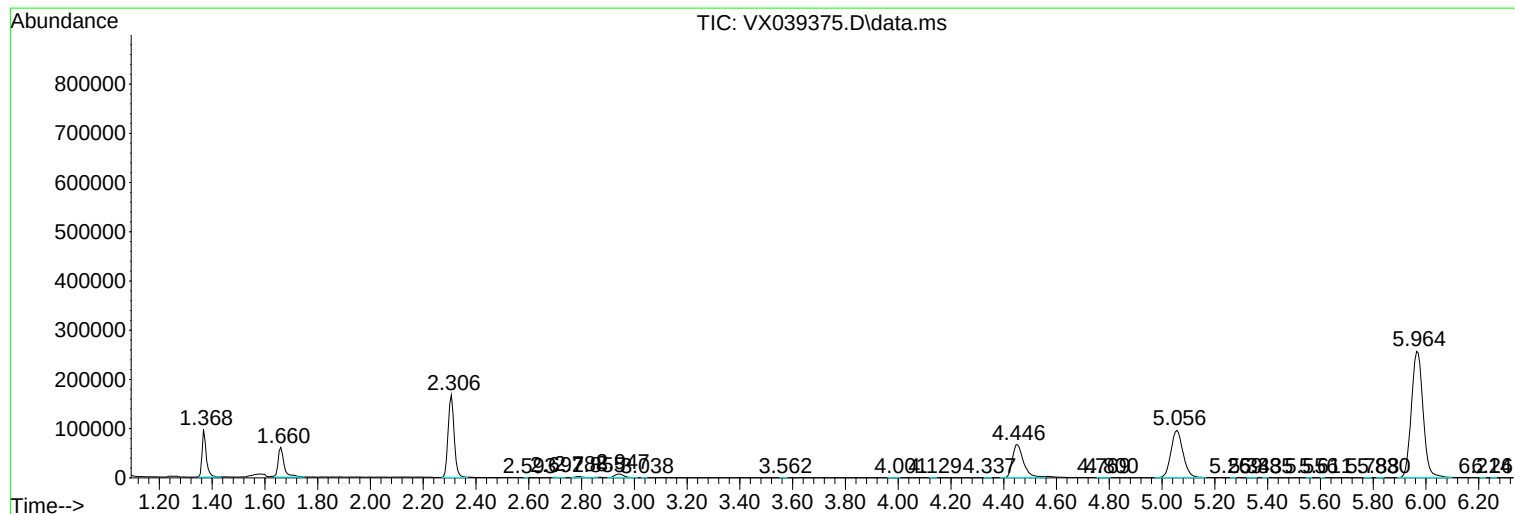

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
Data File : VX039375.D
Acq On : 19 Dec 2023 22:23
Operator : JC/MD
Sample : 05807-13 10X
Misc : 1.26g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0AZ5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121923\
Data File : VX039375.D
Acq On : 19 Dec 2023 22:23
Operator : JC/MD
Sample : 05807-13 10X
Misc : 1.26g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0AZ5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML120523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc